

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
 Data File : VX042823.D
 Acq On : 02 Aug 2024 04:15
 Operator : JC/MD
 Sample : P3430-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 927-K1-WPO-0-0.25-073124-FD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
 Title : SW846 8260

Signal : TIC: VX042823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	12	rBV	23942	19481	6.16%	1.057%
2	1.172	12	14	20	rVB	4606	5787	1.83%	0.314%
3	1.264	20	29	33	rVB5	3096	6045	1.91%	0.328%
4	1.374	42	47	52	rBV	7338	9455	2.99%	0.513%
5	1.642	87	91	95	rVB4	5452	8401	2.66%	0.456%
6	2.136	167	172	183	rVB2	6945	11628	3.68%	0.631%
7	4.489	548	558	568	rBV4	4522	12515	3.96%	0.679%
8	5.025	640	646	659	rBV4	2393	8084	2.56%	0.438%
9	5.385	694	705	722	rBV2	45640	133369	42.16%	7.234%
10	5.550	722	732	745	rBV	54479	152925	48.34%	8.295%
11	5.952	790	798	812	rBV	51176	136406	43.12%	7.399%
12	6.763	922	931	949	rBV	102178	245586	77.63%	13.321%
13	7.135	986	992	997	rBV2	2463	4827	1.53%	0.262%
14	8.647	1234	1240	1248	rBV	196901	316355	100.00%	17.159%
15	8.720	1248	1252	1259	rVB	7987	14119	4.46%	0.766%
16	10.055	1465	1471	1483	rBV	214154	296235	93.64%	16.068%
17	11.079	1634	1639	1652	rBV	164006	213844	67.60%	11.599%
18	12.024	1788	1794	1807	rBV	184671	244670	77.34%	13.271%
19	13.122	1971	1974	1979	rBV2	3263	3903	1.23%	0.212%




Sum of corrected areas: 1843635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042823.D
Acq On : 02 Aug 2024 04:15
Operator : JC/MD
Sample : P3430-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

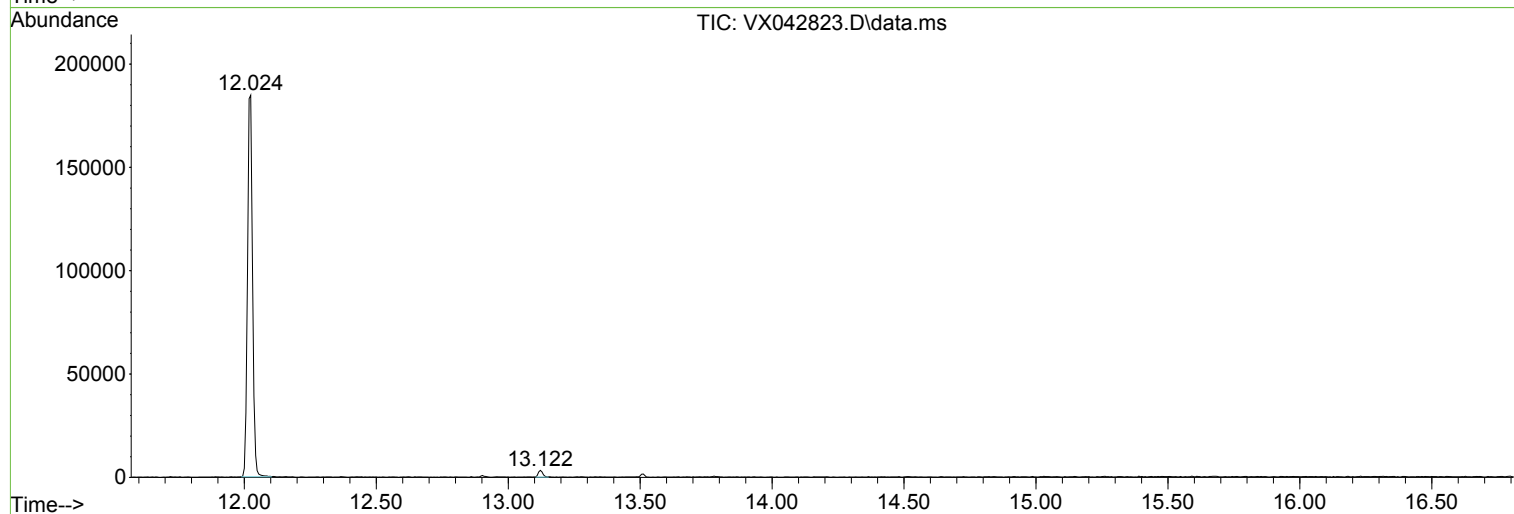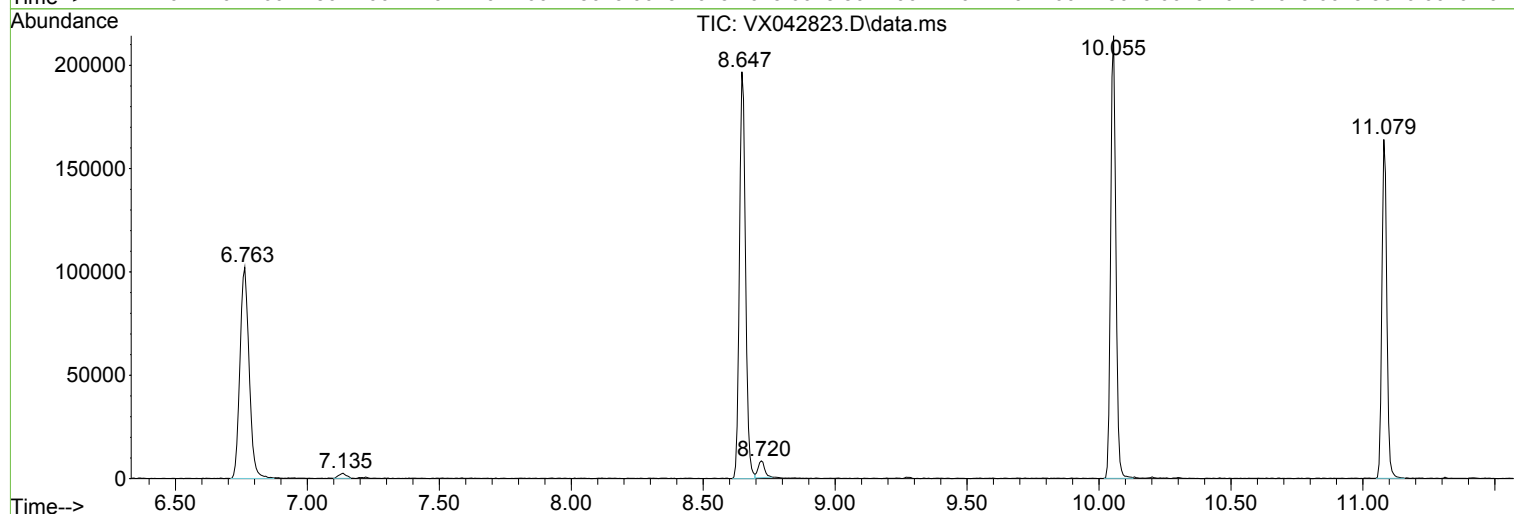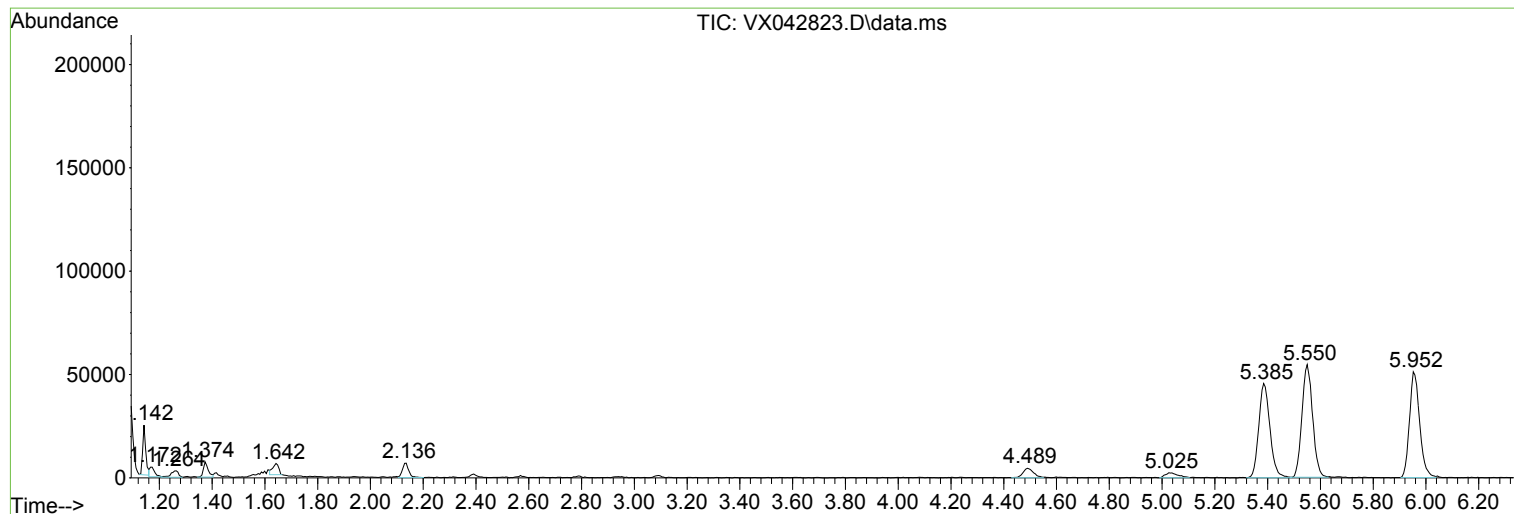

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042823.D
Acq On : 02 Aug 2024 04:15
Operator : JC/MD
Sample : P3430-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124-FD










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, chlorotrifluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.142	6.37 ug/l	19481	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethene, chlorotrifluoro-	116	C2ClF3	000079-38-9	95
2			5-Chloro-1-methylimidazole	116	C4H5ClN2	000872-49-1	9
3			Methylphosphonothionic difluoride	116	CH3F2PS	000753-72-0	5
4			1,2-Difluoroethane	66	C2H4F2	000624-72-6	5
5			1-Propene, 1-(ethylthio)-2-methyl-	116	C6H12S	027482-14-0	5

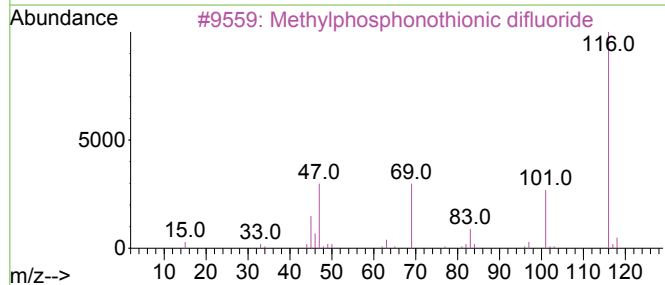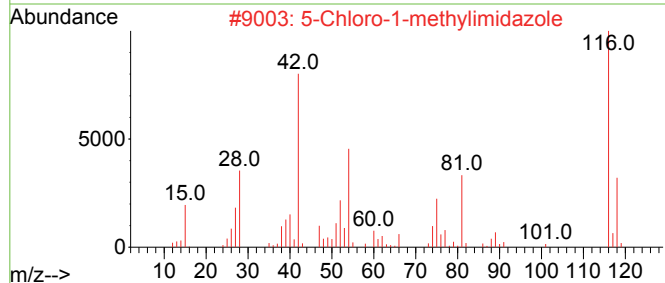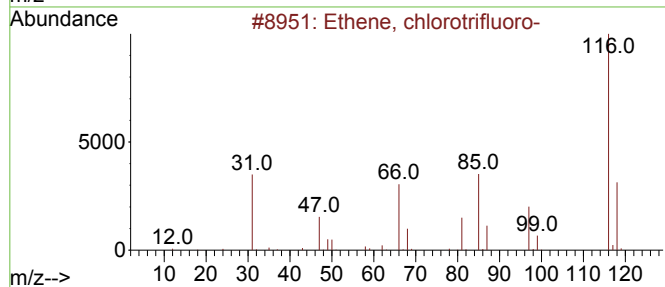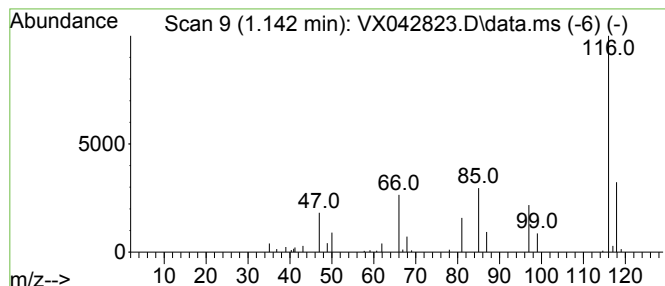

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042823.D
Acq On : 02 Aug 2024 04:15
Operator : JC/MD
Sample : P3430-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, chlorot...	1.142	6.4	ug/l	19481	1	5.550	152925	50.0