
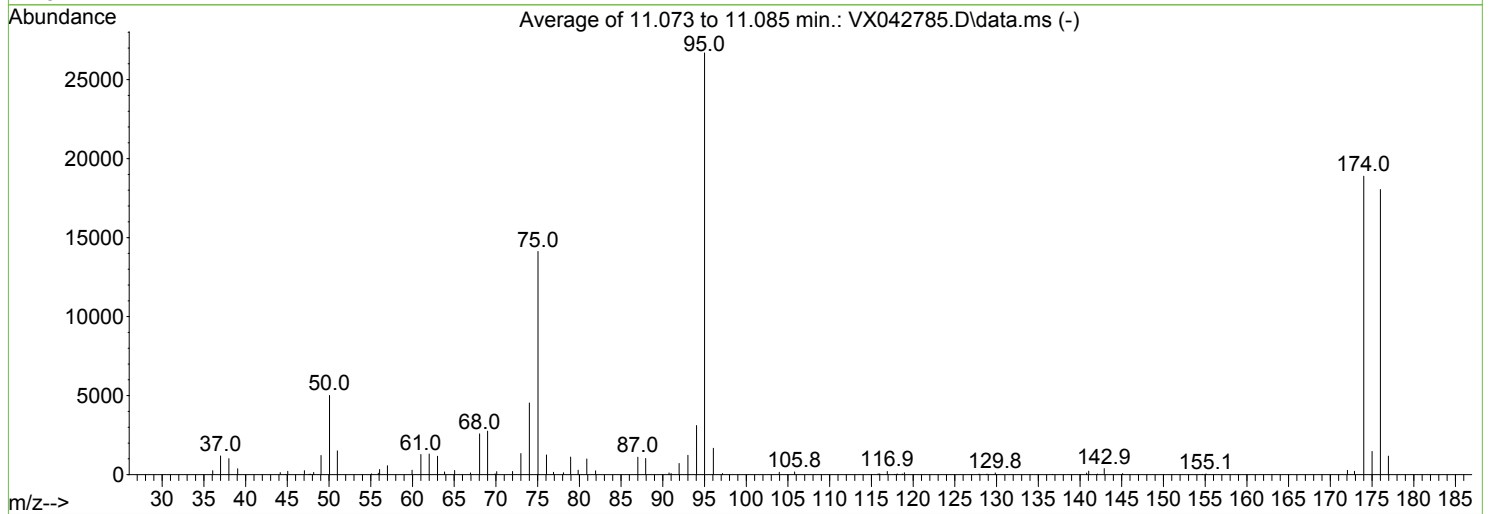


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042785.D
Acq On : 01 Aug 2024 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Title : SW846 8260
Last Update : Thu Aug 01 16:40:12 2024

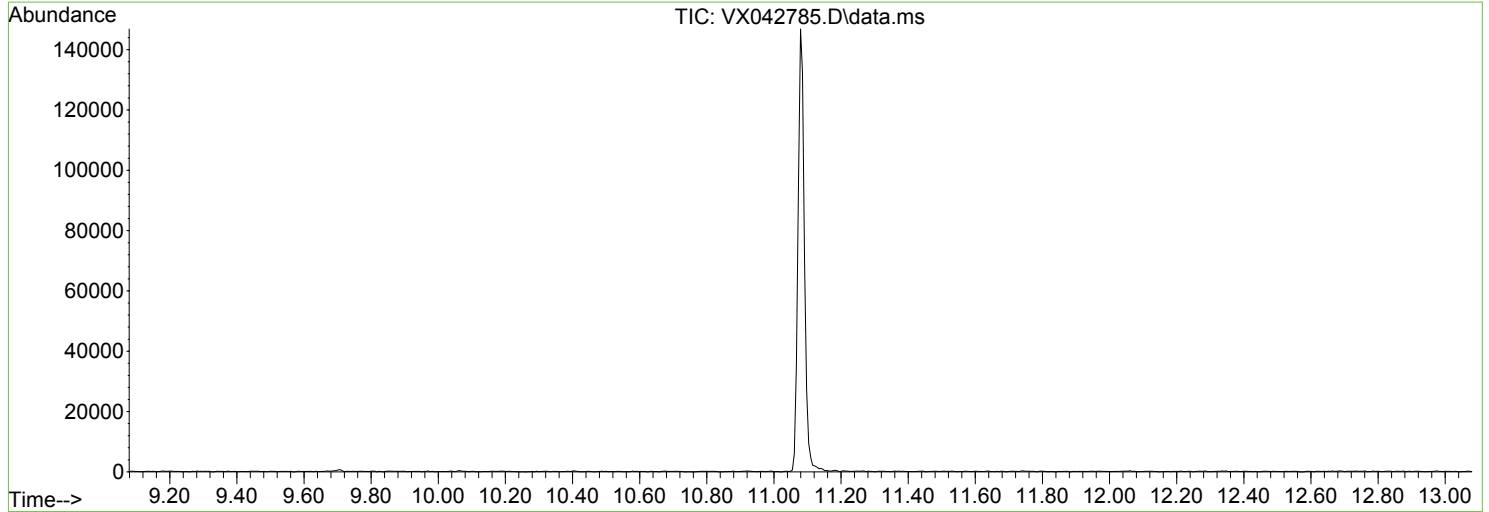

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	5016	PASS
75	95	30	60	52.9	14125	PASS
95	95	100	100	100.0	26693	PASS
96	95	5	9	6.3	1670	PASS
173	174	0.00	2	1.1	215	PASS
174	95	50	100	70.7	18882	PASS
175	174	5	9	7.8	1470	PASS
176	174	95	101	95.5	18041	PASS
177	176	5	9	6.5	1170	PASS