
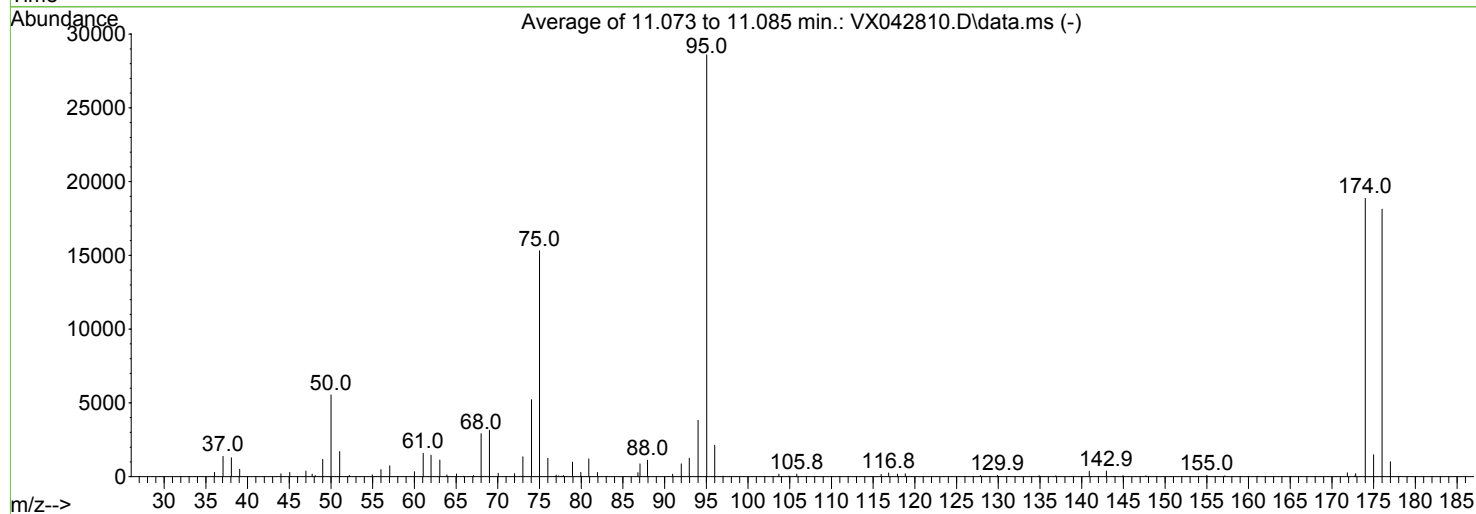


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042810.D
Acq On : 01 Aug 2024 22:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Title : SW846 8260
Last Update : Thu Aug 01 16:40:12 2024

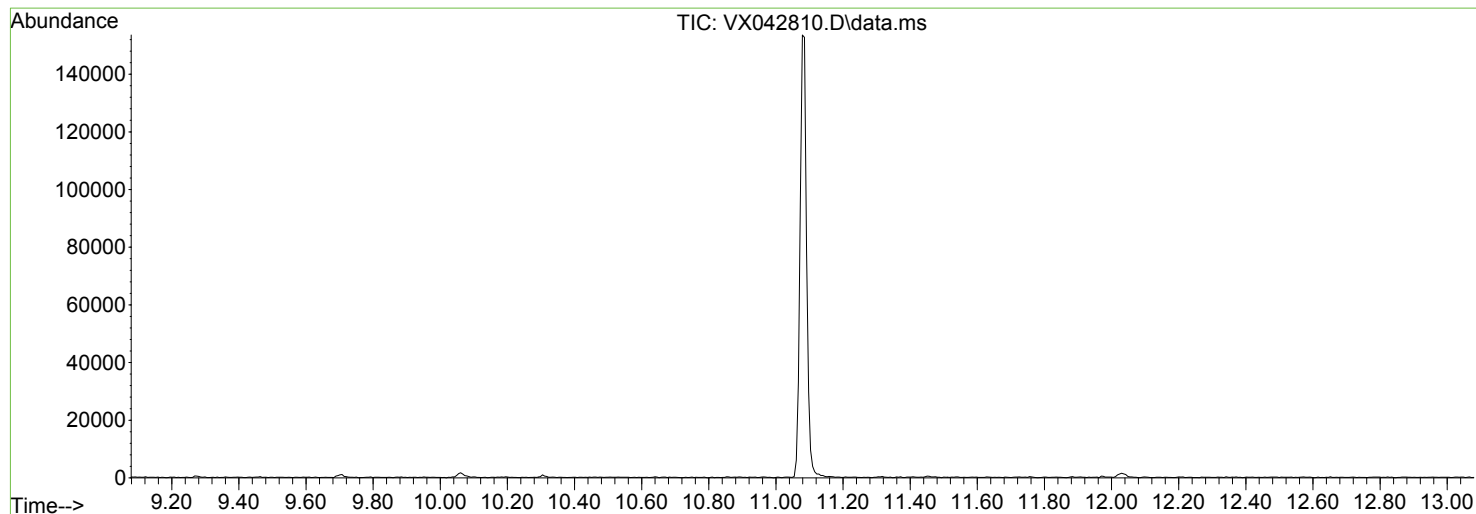

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	5539	PASS
75	95	30	60	53.6	15320	PASS
95	95	100	100	100.0	28595	PASS
96	95	5	9	7.4	2121	PASS
173	174	0.00	2	1.1	204	PASS
174	95	50	100	66.0	18865	PASS
175	174	5	9	7.9	1489	PASS
176	174	95	101	96.1	18136	PASS
177	176	5	9	5.6	1013	PASS