


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080218\
 Data File : VX003818.D
 Acq On : 02 Aug 2018 10:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X072718W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jul 27 16:17:43 2018

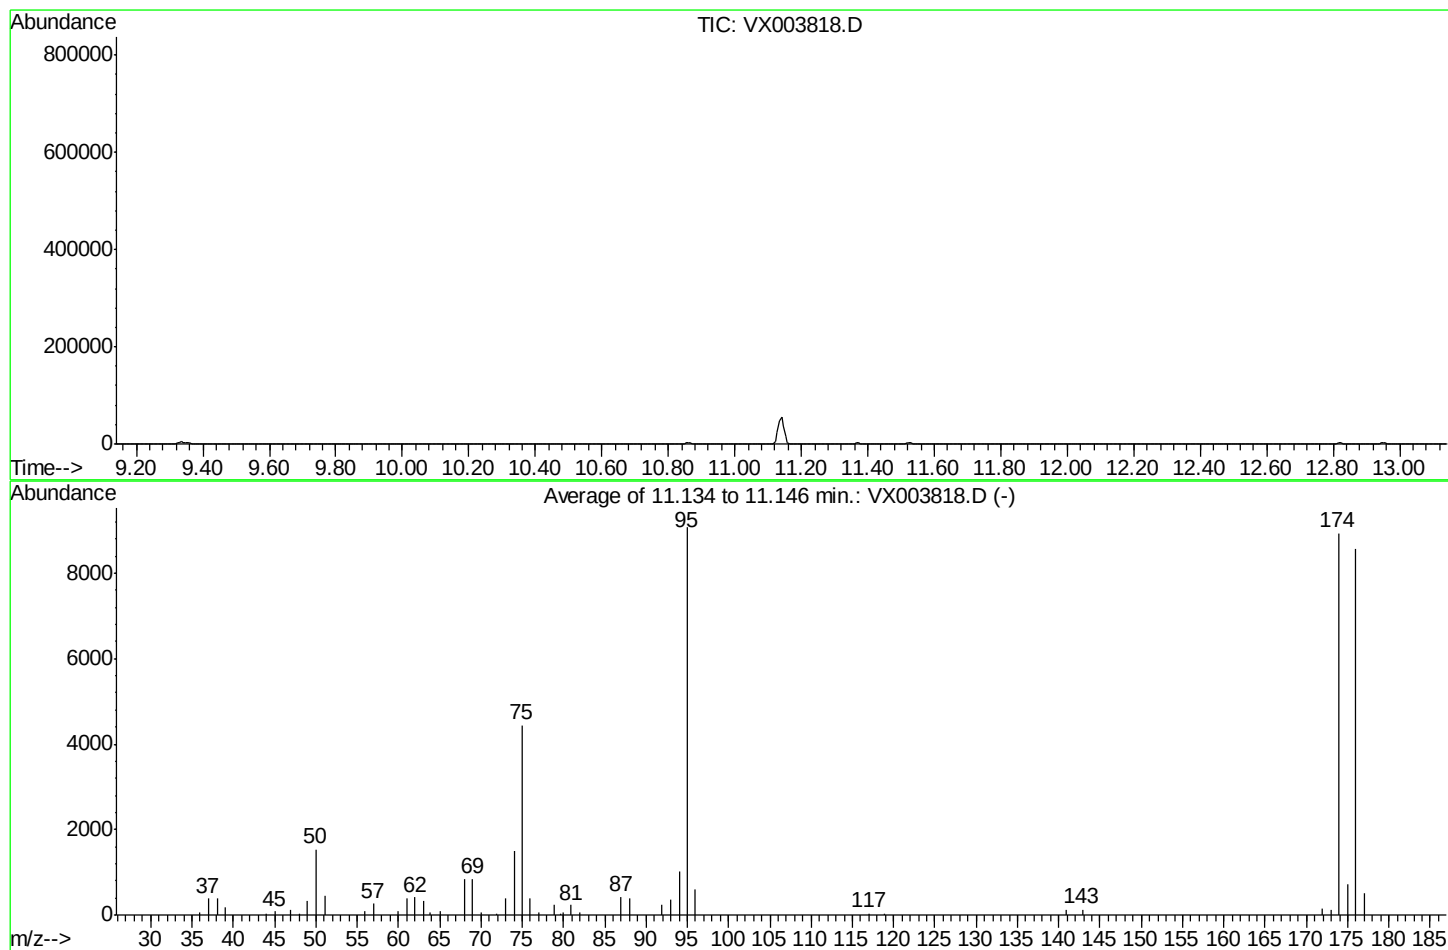

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	1539	PASS
75	95	30	60	48.9	4438	PASS
95	95	100	100	100.0	9073	PASS
96	95	5	9	6.6	603	PASS
173	174	0.00	2	1.3	116	PASS
174	95	50	100	98.4	8932	PASS
175	174	5	9	8.0	714	PASS
176	174	95	101	95.9	8566	PASS
177	176	5	9	6.0	515	PASS