

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080219\  
 Data File : VX011303.D  
 Acq On : 02 Aug 2019 14:33  
 Operator : JC/SP  
 Sample : K4119-12  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 Z3-TB-2019-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.270       | 16            | 19          | 27           | rBV      | 8446           | 12518         | 1.75%           | 0.326%        |
| 2         | 1.599       | 64            | 73          | 77           | rBV5     | 4983           | 10336         | 1.45%           | 0.269%        |
| 3         | 3.007       | 297           | 304         | 313          | rBV2     | 4117           | 10377         | 1.45%           | 0.270%        |
| 4         | 5.494       | 697           | 712         | 725          | rBV      | 85656          | 253260        | 35.48%          | 6.592%        |
| 5         | 5.653       | 727           | 738         | 753          | rVB      | 139596         | 397507        | 55.69%          | 10.346%       |
| 6         | 6.055       | 793           | 804         | 817          | rBV      | 84529          | 222044        | 31.11%          | 5.779%        |
| 7         | 6.854       | 925           | 935         | 946          | rBV      | 220279         | 516960        | 72.43%          | 13.456%       |
| 8         | 8.713       | 1233          | 1240        | 1249         | rBV      | 460867         | 713727        | 100.00%         | 18.577%       |
| 9         | 10.109      | 1463          | 1469        | 1478         | rBV      | 473832         | 623328        | 87.33%          | 16.224%       |
| 10        | 11.134      | 1630          | 1637        | 1646         | rBV      | 389635         | 493795        | 69.19%          | 12.853%       |
| 11        | 12.072      | 1785          | 1791        | 1801         | rBV      | 451766         | 588107        | 82.40%          | 15.307%       |


Sum of corrected areas: 3841959

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080219\  
Data File : VX011303.D  
Acq On : 02 Aug 2019 14:33  
Operator : JC/SP  
Sample : K4119-12  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampled :  
Z3-TB-2019-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

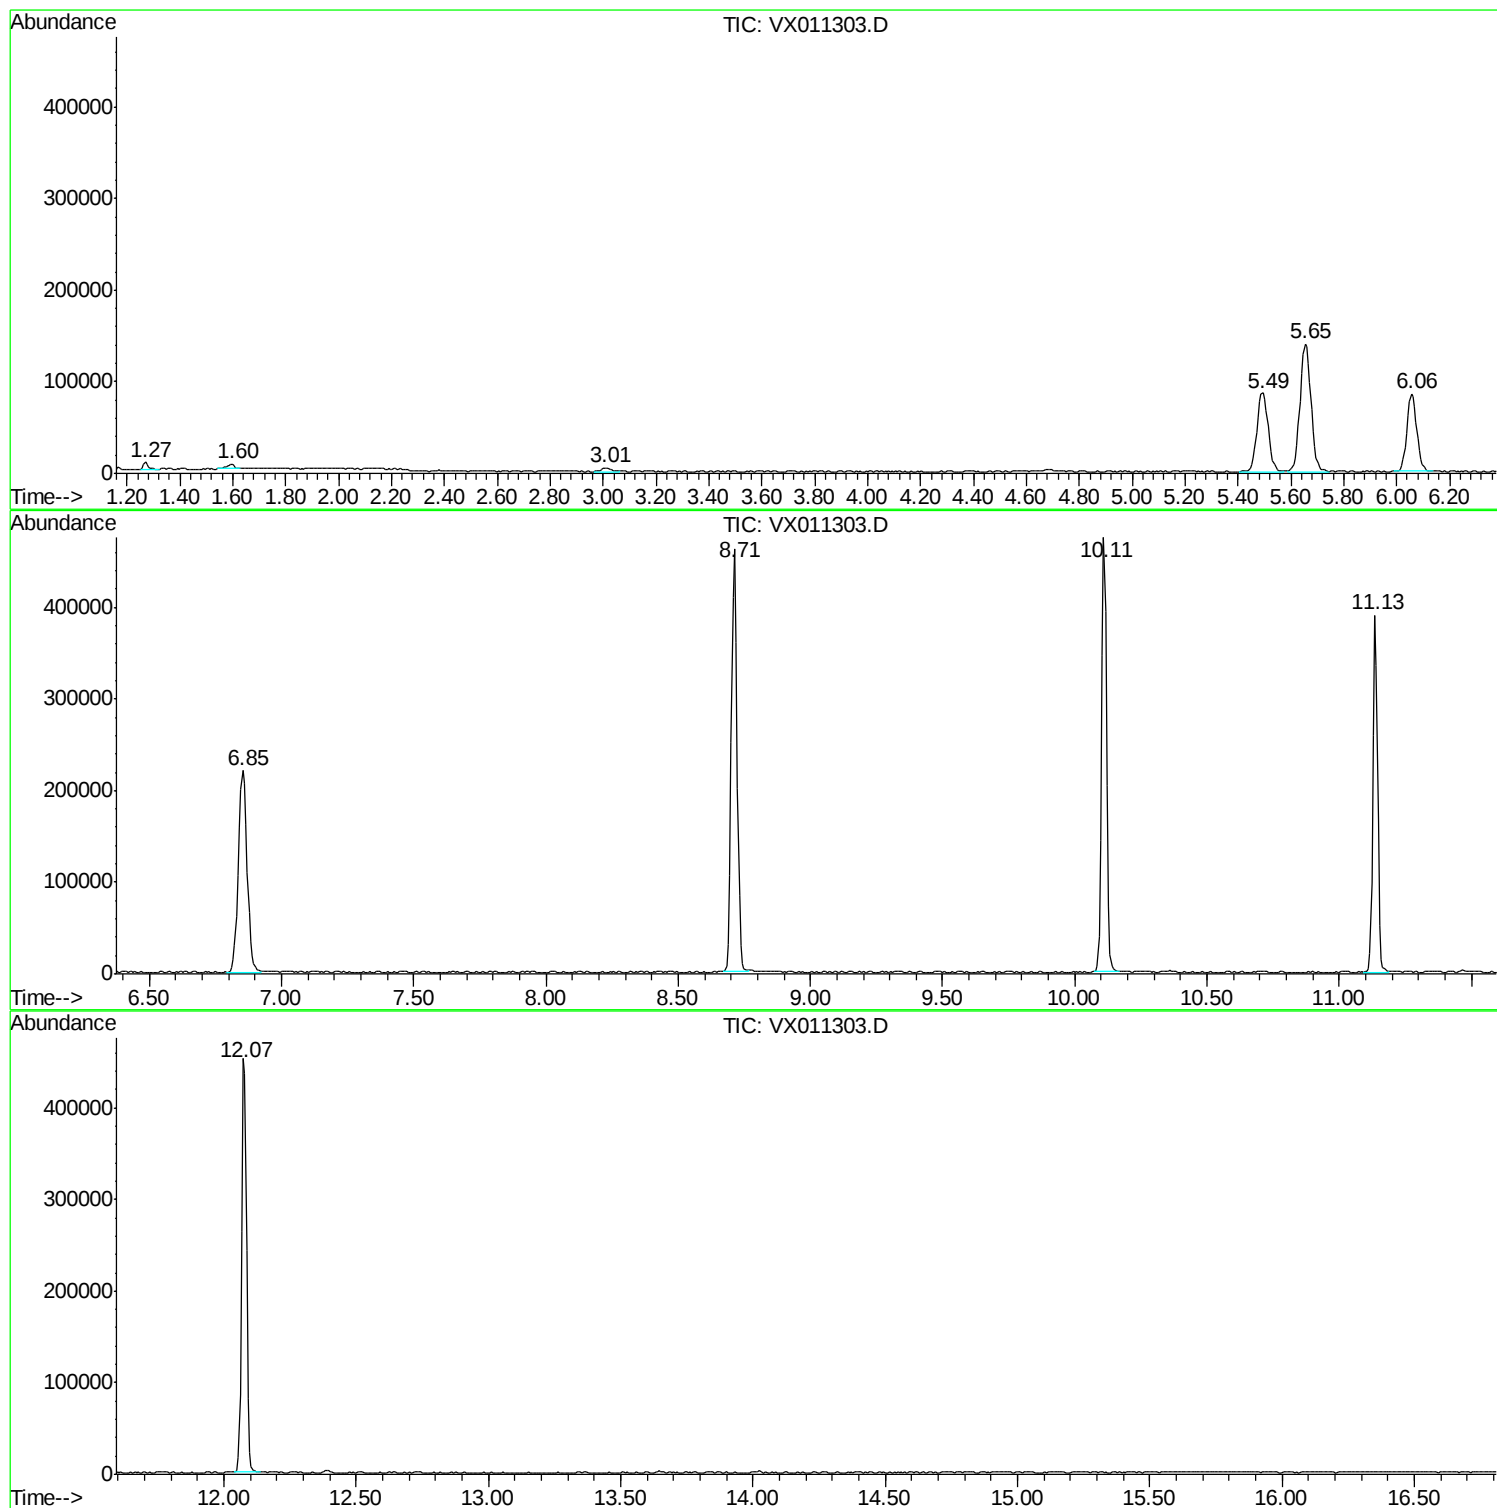

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX080219\  
Data File : VX011303.D  
Acq On : 02 Aug 2019 14:33  
Operator : JC/SP  
Sample : K4119-12  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
Z3-TB-2019-4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX080219\  
Data File : VX011303.D  
Acq On : 02 Aug 2019 14:33  
Operator : JC/SP  
Sample : K4119-12  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
Z3-TB-2019-4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X080119W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |