

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080219\
 Data File : VX011317.D
 Acq On : 02 Aug 2019 20:01
 Operator : JC/SP
 Sample : K4119-11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0690

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.269	15	19	28	rBV	64946	85623	12.17%	2.189%
2	1.398	37	40	45	rBV	17397	18727	2.66%	0.479%
3	1.593	67	72	77	rVB6	4716	8293	1.18%	0.212%
4	4.592	558	564	571	rBV9	3623	9141	1.30%	0.234%
5	5.494	700	712	722	rBV	87580	244637	34.76%	6.255%
6	5.653	728	738	751	rVB	132388	379019	53.86%	9.692%
7	6.055	796	804	814	rBV	80791	212499	30.20%	5.434%
8	6.141	814	818	824	rVB7	3726	8074	1.15%	0.206%
9	6.854	923	935	946	rBV	212317	497106	70.64%	12.711%
10	8.713	1232	1240	1254	rBV	449698	699681	99.43%	17.891%
11	10.109	1463	1469	1480	rBV2	454322	703719	100.00%	17.994%
12	11.134	1631	1637	1649	rBV	377169	479724	68.17%	12.267%
13	12.072	1786	1791	1803	rVB	434206	564551	80.22%	14.436%


Sum of corrected areas: 3910794

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080219\
Data File : VX011317.D
Acq On : 02 Aug 2019 20:01
Operator : JC/SP
Sample : K4119-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0690

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

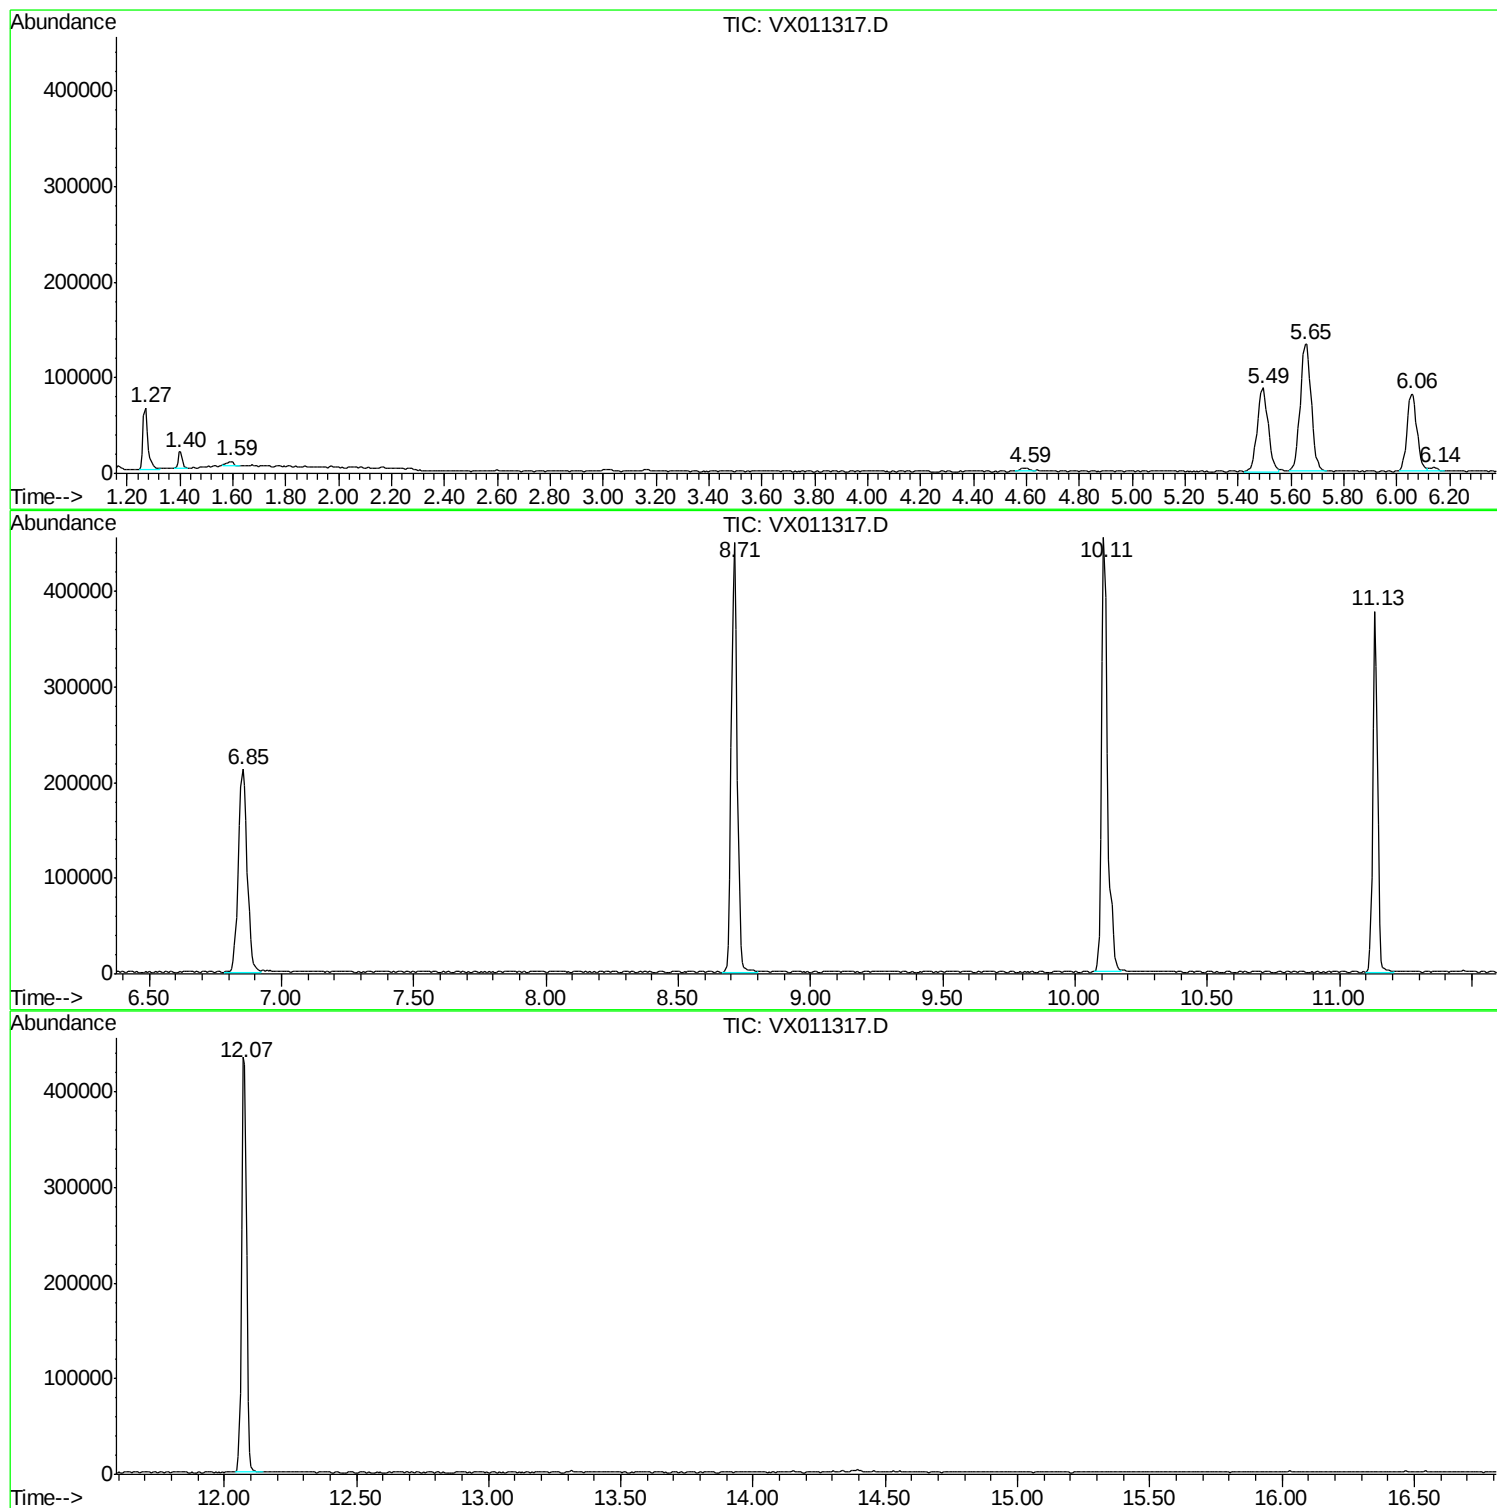

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080219\
Data File : VX011317.D
Acq On : 02 Aug 2019 20:01
Operator : JC/SP
Sample : K4119-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
Z3-0690

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
1.27	11.30 ug/l	85623	Pentafluorobenzene	5.65		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Sulfur dioxide	64	O2S	007446-09-5	83	
2	Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74	
3	L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9	
4	Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4	
5	Ethyl Chloride	64	C2H5Cl	000075-00-3	3	

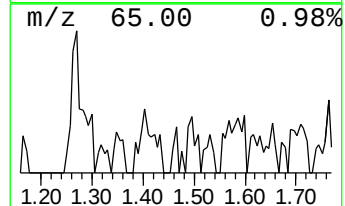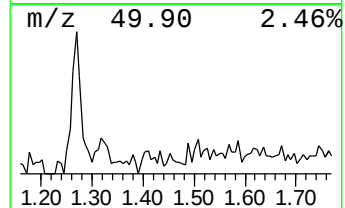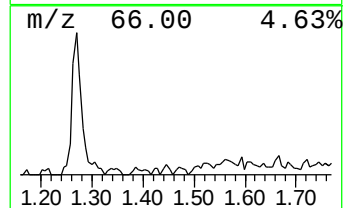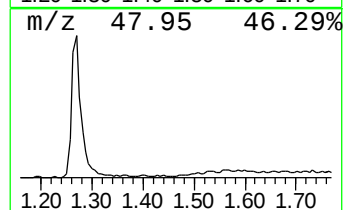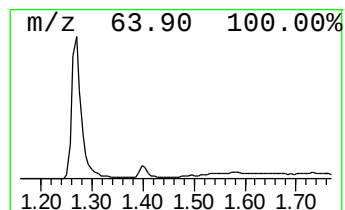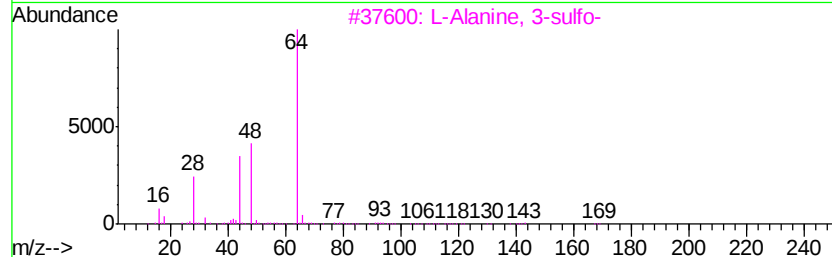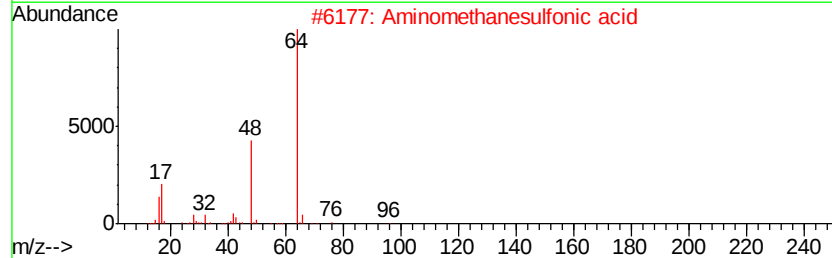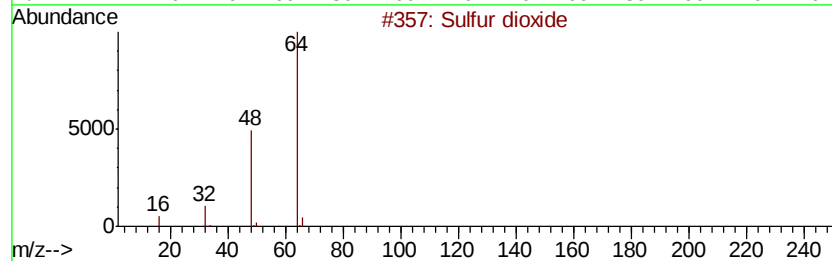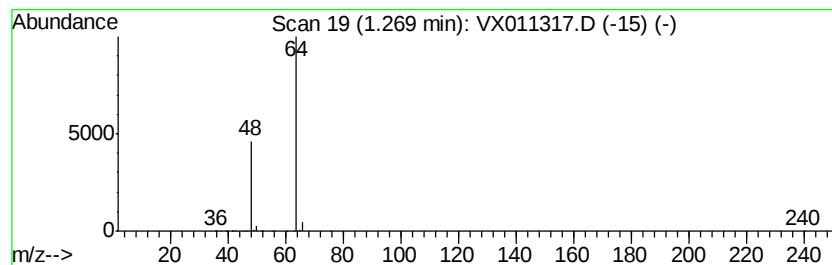

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080219\
Data File : VX011317.D
Acq On : 02 Aug 2019 20:01
Operator : JC/SP
Sample : K4119-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0690

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.27	11.3	ug/l	85623	1	5.65	379019	50.0