

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
 Data File : VX030356.D
 Acq On : 02 Aug 2022 16:41
 Operator : JC/MD
 Sample : PB146634ZHE#03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB146634ZHE#03

Quant Time: Aug 03 01:09:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 25 16:49:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	152881	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	278102	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	274728	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	153959	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	155911	50.739	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 101.480%			
35) Dibromofluoromethane	5.391	113	125118	47.063	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 94.120%			
50) Toluene-d8	8.653	98	467185	45.378	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 90.760%			
62) 4-Bromofluorobenzene	11.085	95	168935	44.213	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 88.420%			
Target Compounds					Qvalue	
5) Bromomethane	1.624	94	551	Below Cal	#	47
6) Chloroethane	1.733	64	660	0.459	ug/l #	41
8) Diethyl Ether	2.130	74	419	0.324	ug/l	90
10) Methyl Iodide	2.459	142	72	1.554	ug/l #	45
11) Tert butyl alcohol	2.947	59	9732	12.984	ug/l #	74
13) Acrolein	2.239	56	158	0.858	ug/l #	70
14) Allyl chloride	2.648	41	2071	0.420	ug/l #	61
16) Acetone	2.386	43	98516	62.621	ug/l	93
18) Methyl Acetate	2.715	43	4939	1.061	ug/l	92
20) Methylene Chloride	2.794	84	18061	4.384	ug/l	97
25) 2-Butanone	4.574	43	33911	12.827	ug/l	94
29) Tetrahydrofuran	5.025	42	12316	6.924	ug/l	93
31) Cyclohexane	5.550	56	3581	0.803	ug/l #	1
36) 1,1-Dichloropropene	5.562	75	12966	3.389	ug/l #	49
37) Ethyl Acetate	4.721	43	50885	9.392	ug/l	99
38) Carbon Tetrachloride	5.556	117	15469	4.331	ug/l #	16
41) Methacrylonitrile	5.019	41	6582	2.266	ug/l #	46
43) Isopropyl Acetate	6.354	43	215836	27.175	ug/l	98
48) Methyl methacrylate	7.805	41	185776	47.522	ug/l #	41
49) 1,4-Dioxane	7.671	88	413	4.574	ug/l #	25
51) 4-Methyl-2-Pentanone	8.555	43	170370	31.597	ug/l #	51
53) t-1,3-Dichloropropene	8.958	75	1743	0.407	ug/l #	42
54) cis-1,3-Dichloropropene	8.555	75	72871	15.629	ug/l #	60
57) 1,3-Dichloropropane	9.488	76	9881	1.914	ug/l #	42
59) 2-Hexanone	9.378	43	203688	47.882	ug/l #	24
67) Ethyl Benzene	10.195	91	333	Below Cal	#	43
74) N-amyl acetate	10.640	43	48295	8.268	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	82918	20.432	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	82918	61.294	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
Data File : VX030356.D
Acq On : 02 Aug 2022 16:41
Operator : JC/MD
Sample : PB146634ZHE#03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03

Quant Time: Aug 03 01:09:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 25 16:49:17 2022
Response via : Initial Calibration




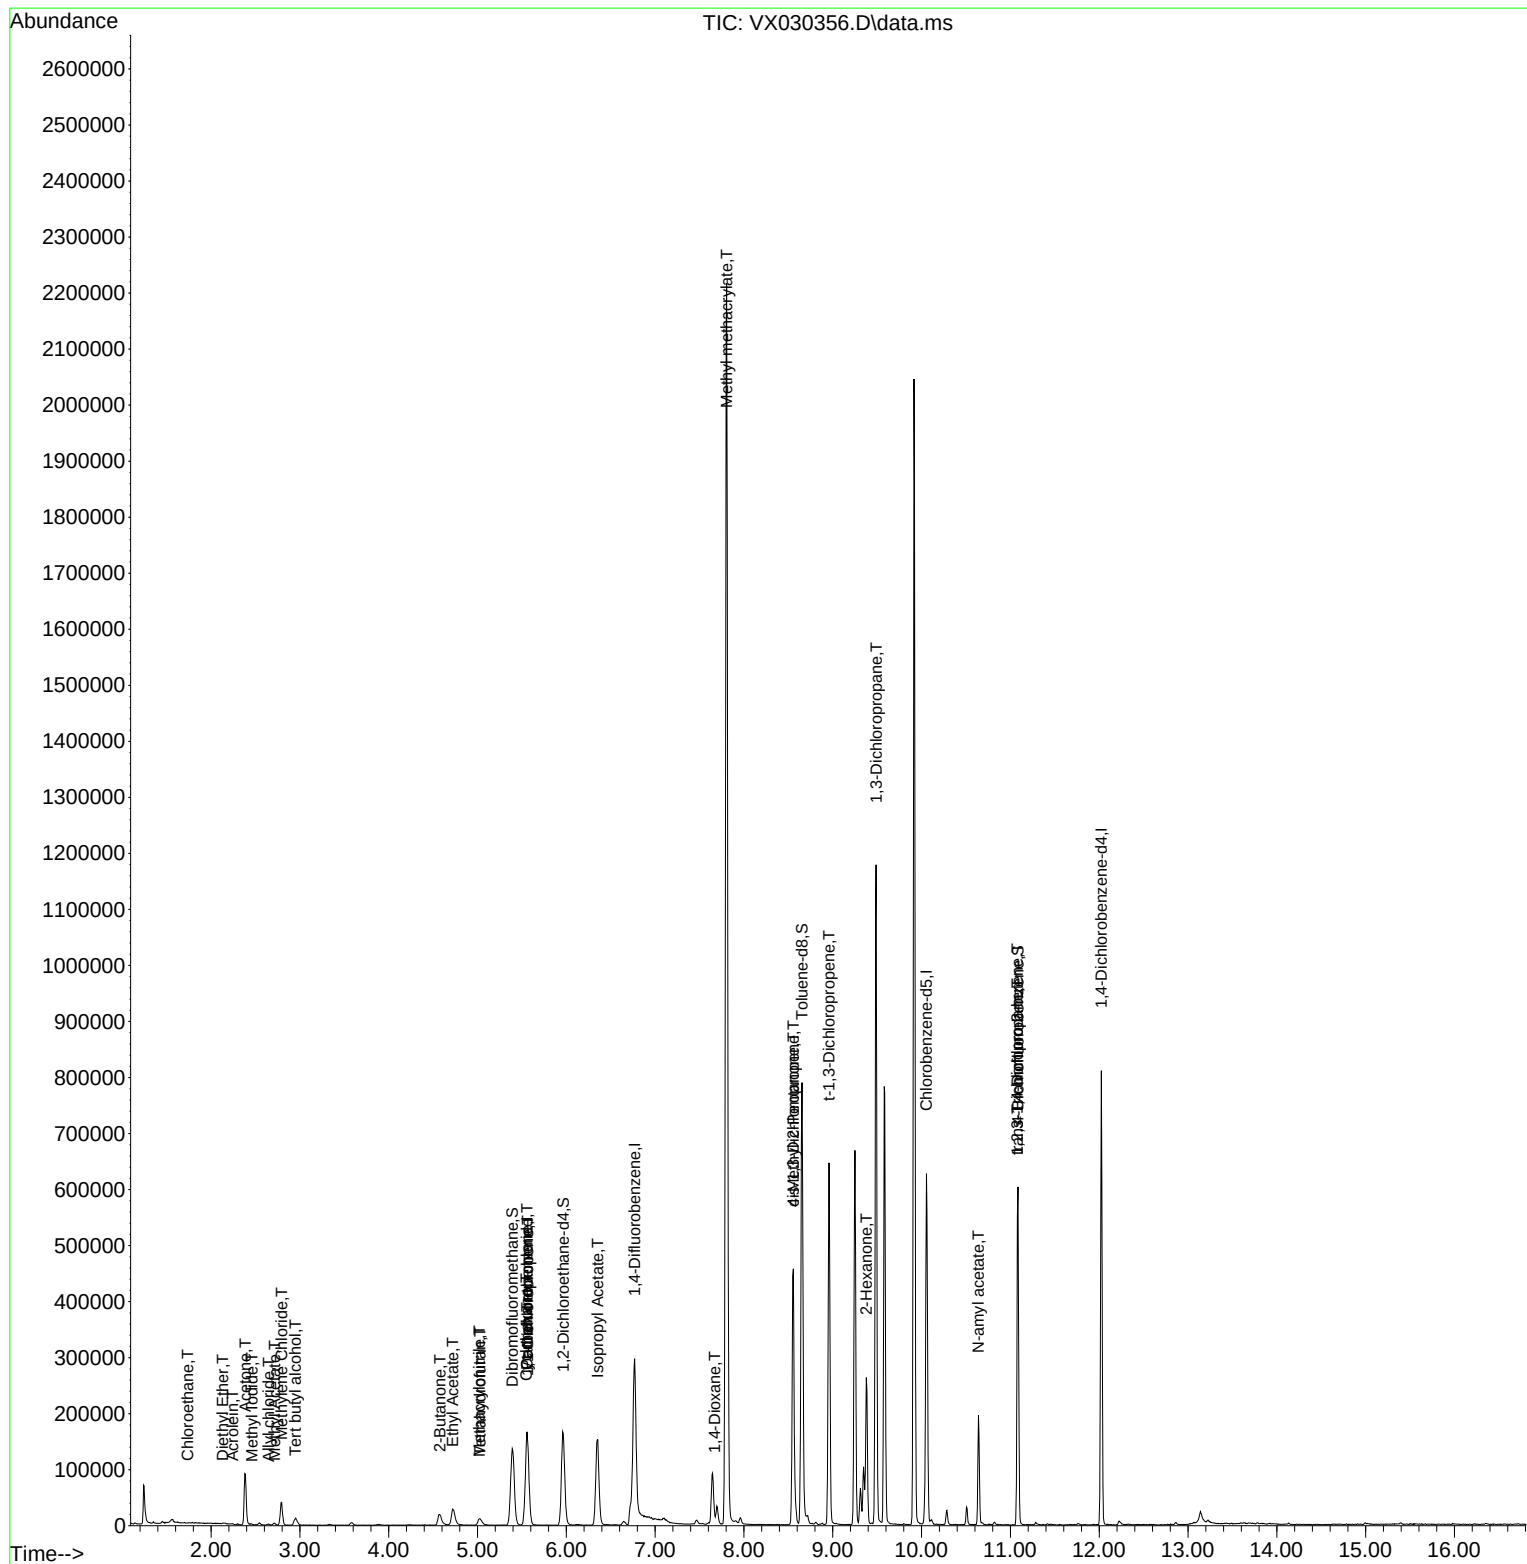




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion:168 Resp: 152881
Ion Ratio Lower Upper
168 100
99 59.6 44.0 66.0

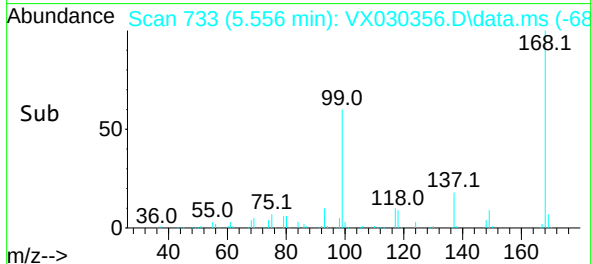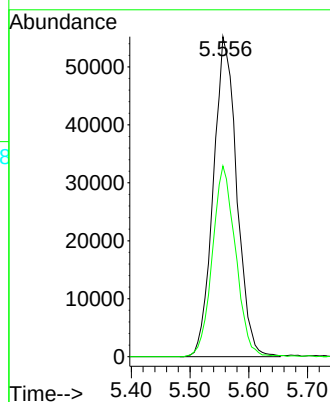

#5
Bromomethane
Concen: Below Cal
RT: 1.624 min Scan# 88
Delta R.T. 0.025 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion: 94 Resp: 551
Ion Ratio Lower Upper
94 100
96 44.1 76.9 115.3#


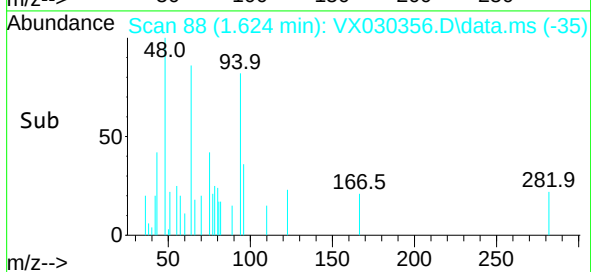
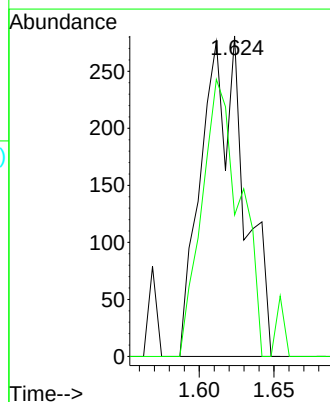



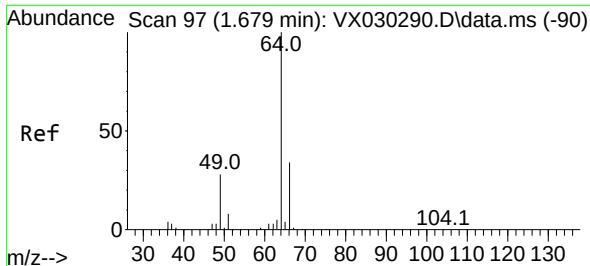

#6
Chloroethane
Concen: 0.459 ug/l
RT: 1.733 min Scan# 106
Delta R.T. 0.055 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion: 64 Resp: 660
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

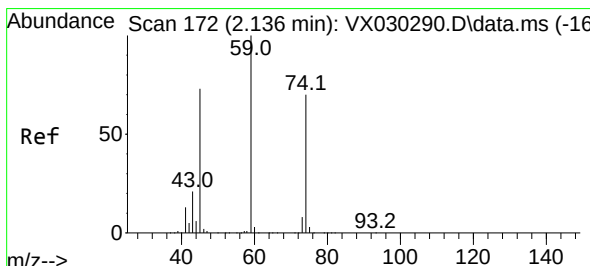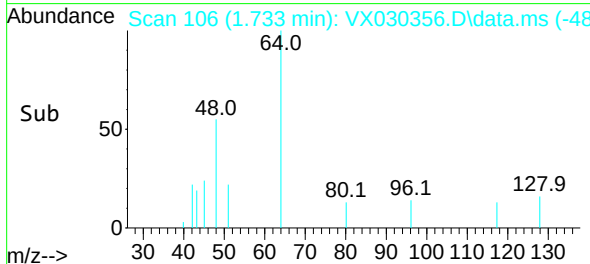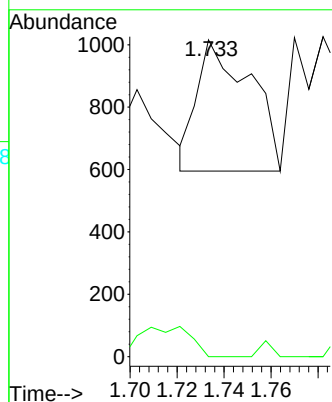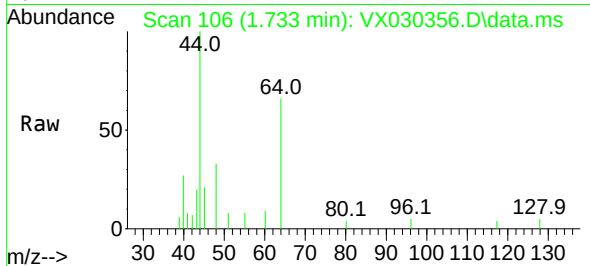

#8
Diethyl Ether
Concen: 0.324 ug/l
RT: 2.130 min Scan# 171
Delta R.T. -0.005 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41


Tgt Ion: 74 Resp: 419
Ion Ratio Lower Upper
74 100
45 93.1 51.5 154.7

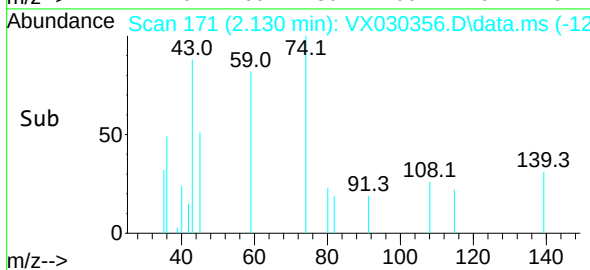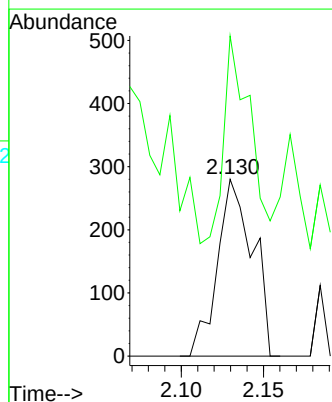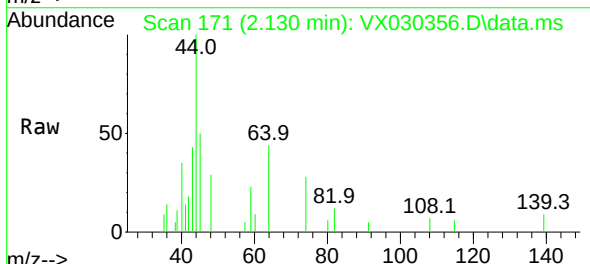



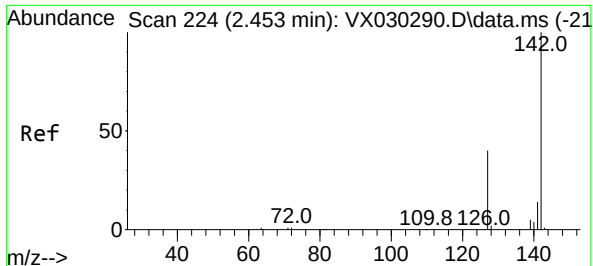


#10
Methyl Iodide
Concen: 1.554 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.013 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03



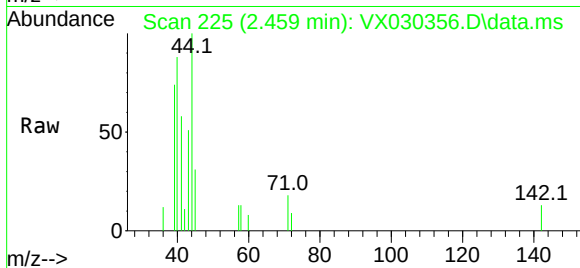



Tgt Ion:142 Resp: 72
Ion Ratio Lower Upper
142 100
127 0.0 30.2 45.2#
141 0.0 11.3 16.9#

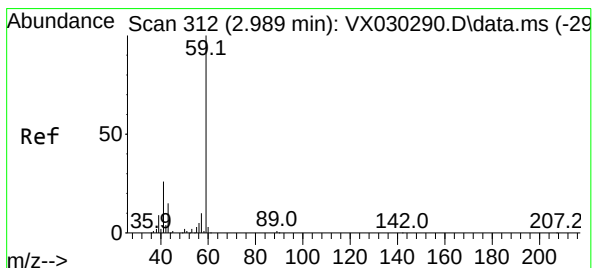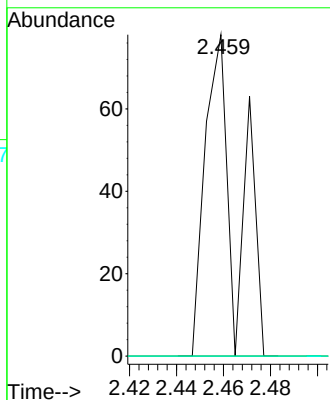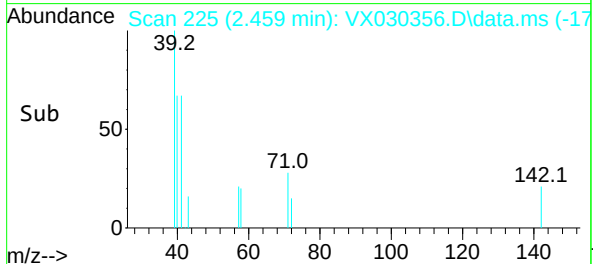

#11
Tert butyl alcohol
Concen: 12.984 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.030 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion: 59 Resp: 9732
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#


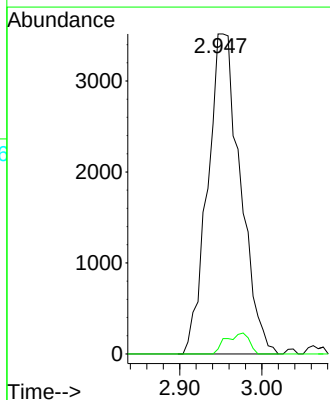
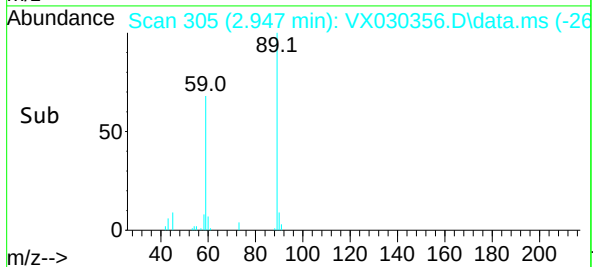
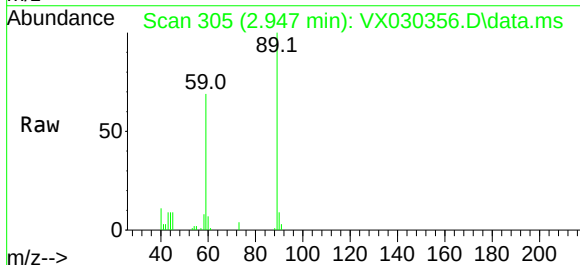




#13
Acrolein
Concen: 0.858 ug/l
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion: 56 Resp: 158
Ion Ratio Lower Upper
56 100
55 95.6 56.6 84.8#

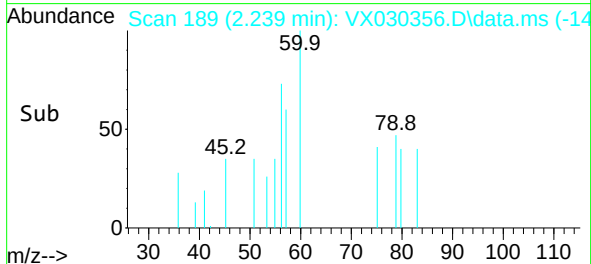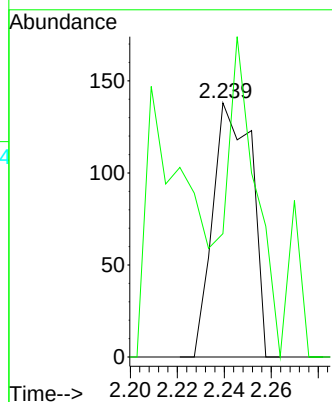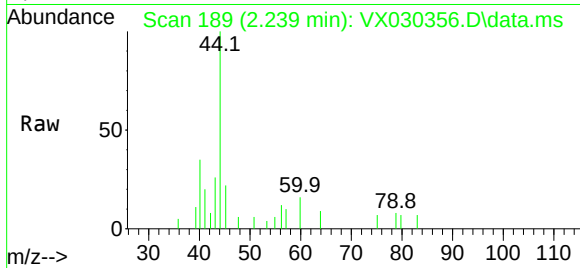

#14
Allyl chloride
Concen: 0.420 ug/l
RT: 2.648 min Scan# 256
Delta R.T. -0.018 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41


Tgt Ion: 41 Resp: 2071
Ion Ratio Lower Upper
41 100
39 39.4 48.9 73.3#
76 0.0 26.9 40.3#

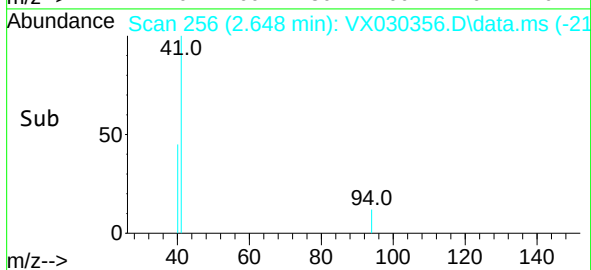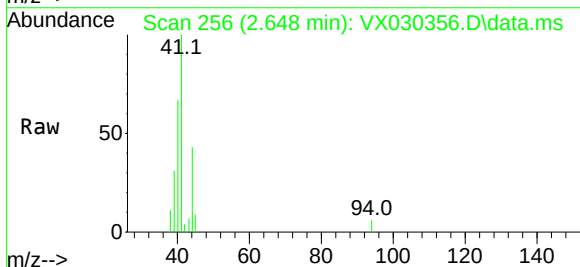



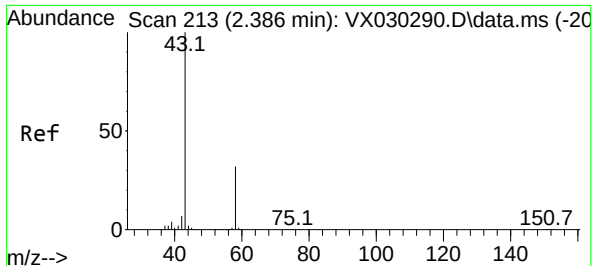


#16
Acetone
Concen: 62.621 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.001 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03



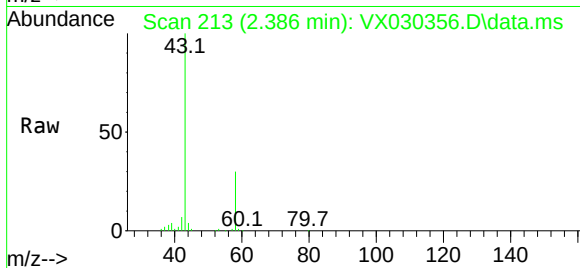



Tgt Ion: 43 Resp: 98516
Ion Ratio Lower Upper
43 100
58 30.4 27.7 41.5

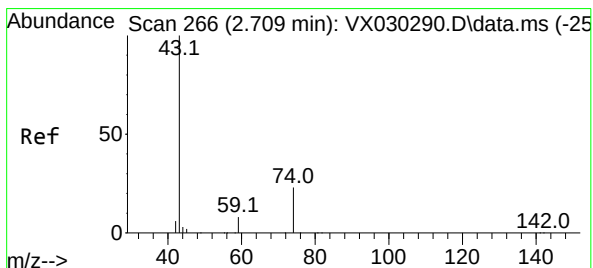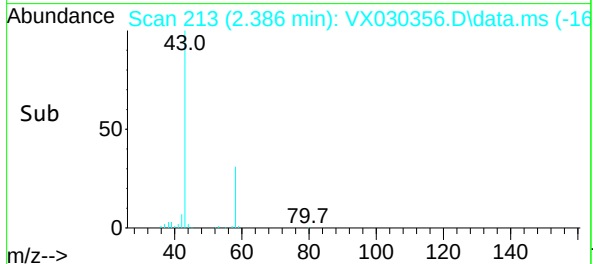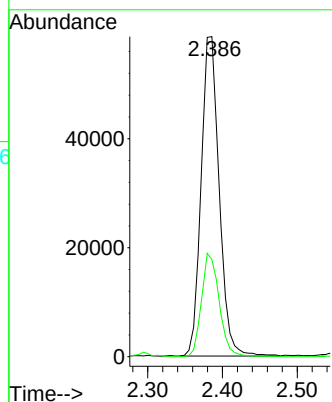

#18
Methyl Acetate
Concen: 1.061 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.007 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41


Tgt Ion: 43 Resp: 4939
Ion Ratio Lower Upper
43 100
74 20.3 19.4 29.2

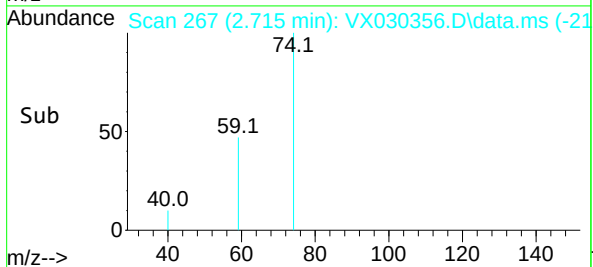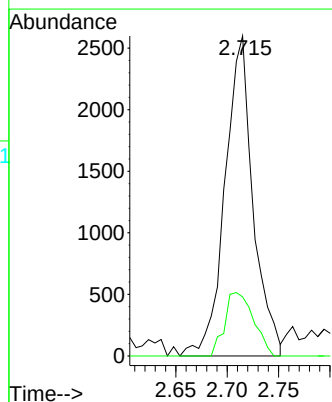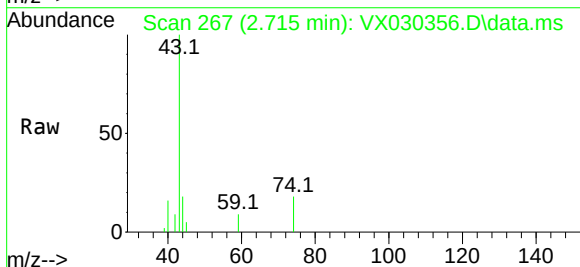





#20
Methylene Chloride
Concen: 4.384 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03







Tgt Ion:	84	Resp:	18061
Ion	Ratio	Lower	Upper
84	100		
49	118.3	93.8	140.6
51	35.1	29.4	44.0
86	58.1	51.0	76.4

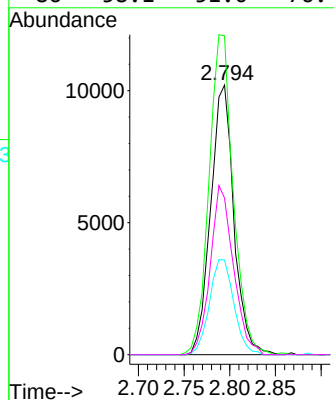

#25
2-Butanone
Concen: 12.827 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion:	43	Resp:	33911
Ion	Ratio	Lower	Upper
43	100		
72	24.2	21.7	32.5

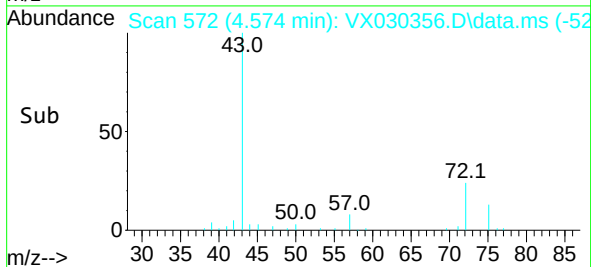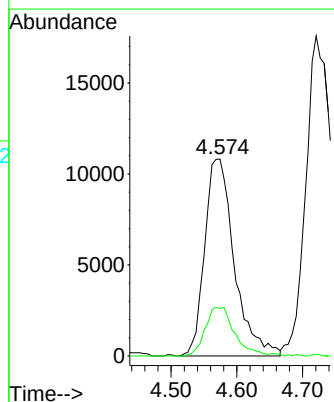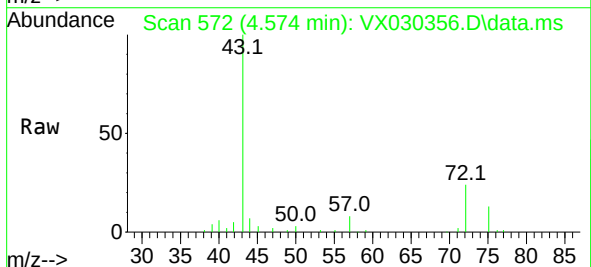

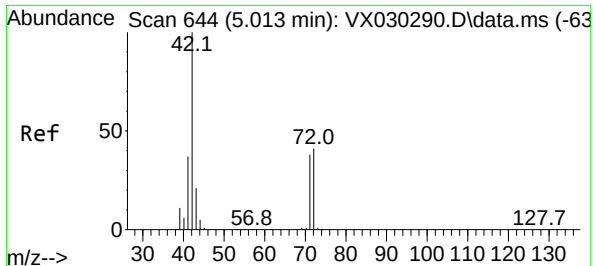

#29

Tetrahydrofuran

Concen: 6.924 ug/l

RT: 5.025 min Scan# 64

Delta R.T. 0.012 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41

Instrument :

MSVOA_X

ClientSampleId :

PB146634ZHE#03





Tgt Ion: 42 Resp: 12316

Ion Ratio Lower Upper

42 100

72 41.2 36.5 54.7

71 38.0 33.9 50.9

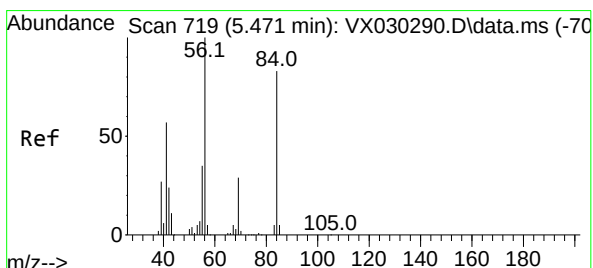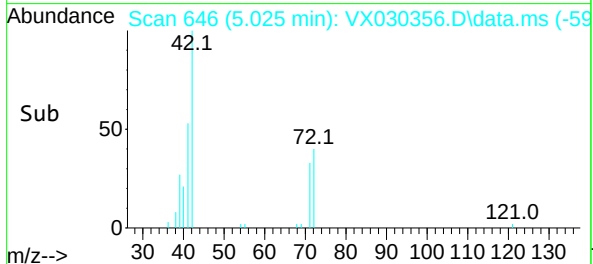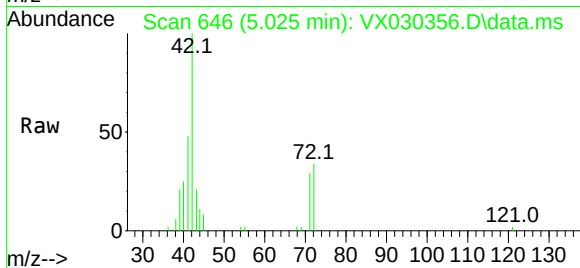

#31

Cyclohexane

Concen: 0.803 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.080 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41




Tgt Ion: 56 Resp: 3581


Ion Ratio Lower Upper

56 100

69 187.4 25.4 38.0#

84 158.6 68.9 103.3#

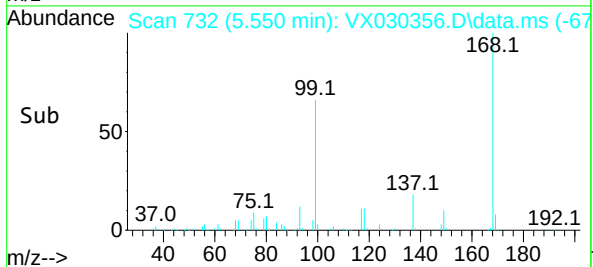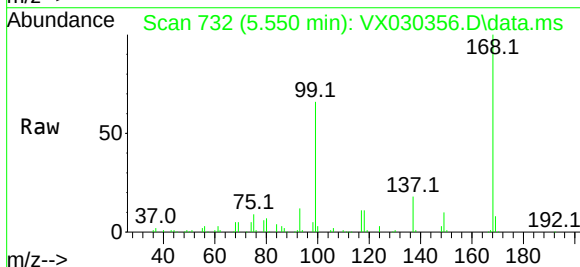



#33

1,2-Dichloroethane-d4

Concen: 50.739 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.000 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41

Instrument :

MSVOA_X

ClientSampleId :





PB146634ZHE#03

Tgt Ion: 65 Resp: 155911

Ion Ratio Lower Upper

65 100

67 54.6 0.0 109.6

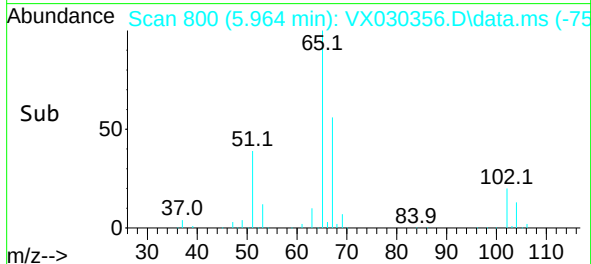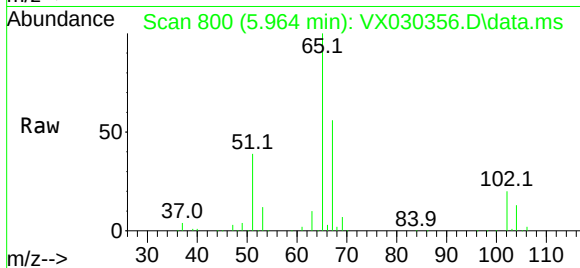

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41




Tgt Ion: 114 Resp: 278102


Ion Ratio Lower Upper

114 100

63 22.3 0.0 38.4

88 16.3 0.0 31.8


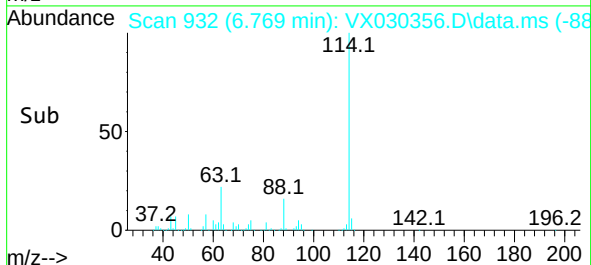
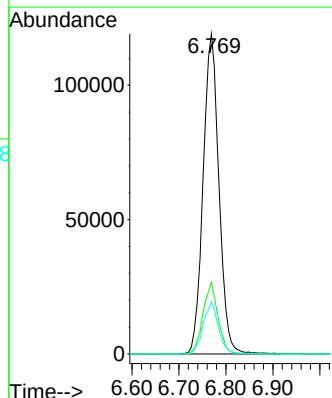
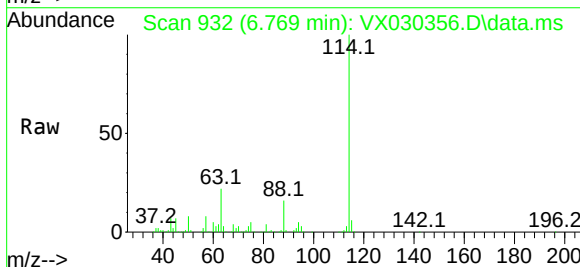




#35
Dibromofluoromethane
Concen: 47.063 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion:113 Resp: 125118
Ion Ratio Lower Upper
113 100
111 103.4 83.2 124.8
192 17.7 14.8 22.2

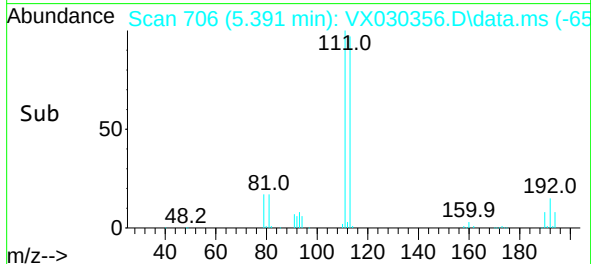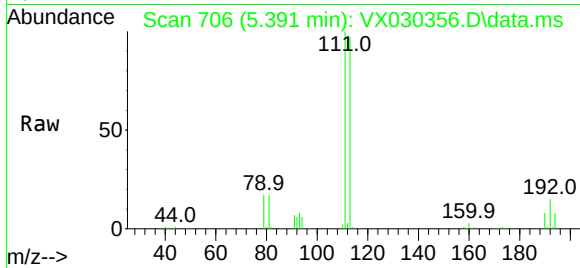

#36
1,1-Dichloropropene
Concen: 3.389 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.134 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion: 75 Resp: 12966
Ion Ratio Lower Upper
75 100
110 10.3 19.3 57.9#
77 0.0 24.4 36.6#

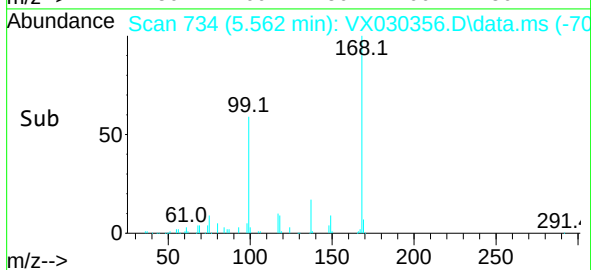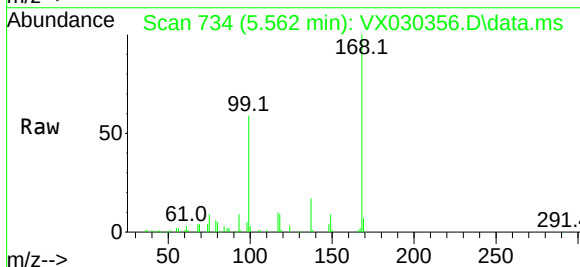



#37

Ethyl Acetate

Concen: 9.392 ug/l

RT: 4.721 min Scan# 595

Delta R.T. 0.001 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41

Instrument :

MSVOA_X

ClientSampleId :

PB146634ZHE#03





Tgt Ion: 43 Resp: 50885

Ion Ratio Lower Upper

43 100

61 14.8 11.7 17.5

70 10.7 9.3 13.9

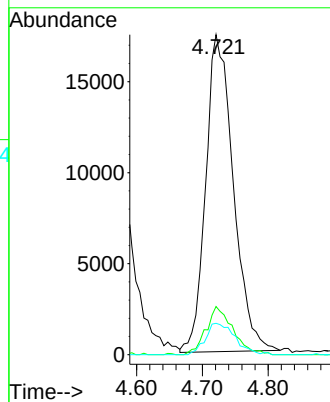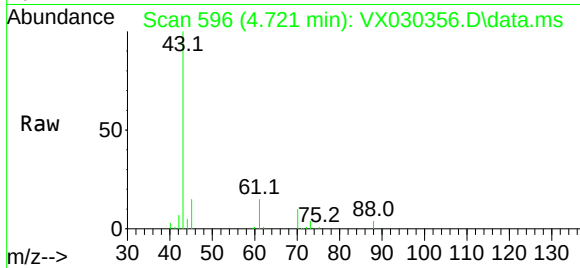

#38

Carbon Tetrachloride

Concen: 4.331 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.127 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41




Tgt Ion: 117 Resp: 15469


Ion Ratio Lower Upper

117 100

119 3.6 74.1 111.1#

121 0.0 25.8 38.8#


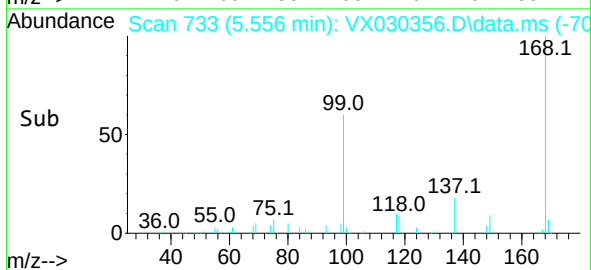
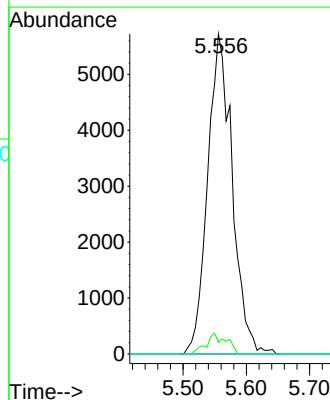
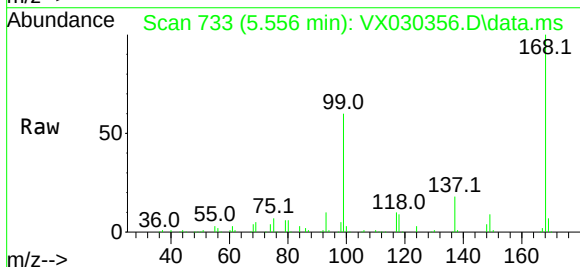




#41
Methacrylonitrile
Concen: 2.266 ug/l
RT: 5.019 min Scan# 641
Delta R.T. 0.091 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion:	41	Resp:	6582
Ion	Ratio	Lower	Upper
41	100		
39	50.0	42.9	64.3
67	0.0	60.1	90.1#
52	0.0	22.6	34.0#

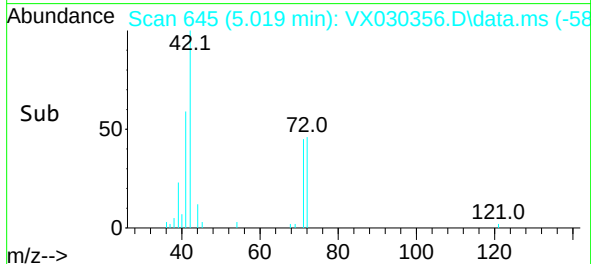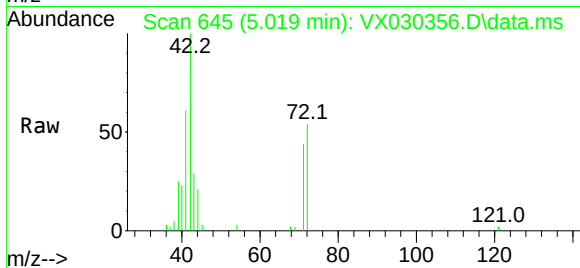

#43
Isopropyl Acetate
Concen: 27.175 ug/l
RT: 6.354 min Scan# 864
Delta R.T. 0.006 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion:	43	Resp:	215836
Ion	Ratio	Lower	Upper
43	100		
61	20.1	16.5	24.7
87	12.7	11.1	16.7

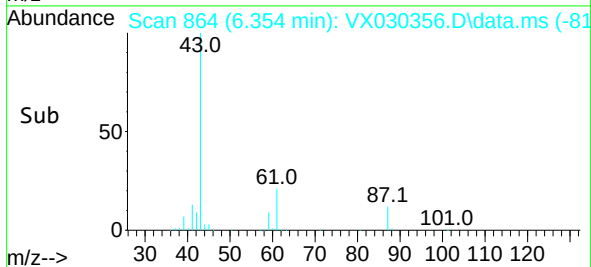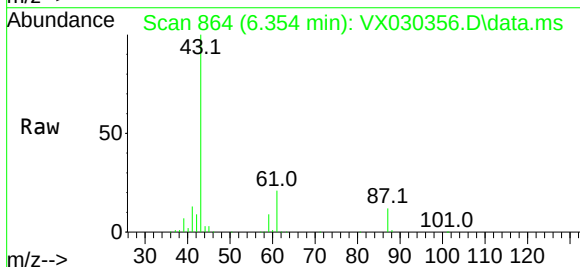



#48

Methyl methacrylate

Concen: 47.522 ug/l

RT: 7.805 min Scan# 1102

Delta R.T. 0.110 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41

Instrument :

MSVOA_X

ClientSampleId :

PB146634ZHE#03





Tgt Ion: 41 Resp: 185776

Ion Ratio Lower Upper

41 100

69 0.2 68.8 103.2#

39 50.7 44.6 66.8

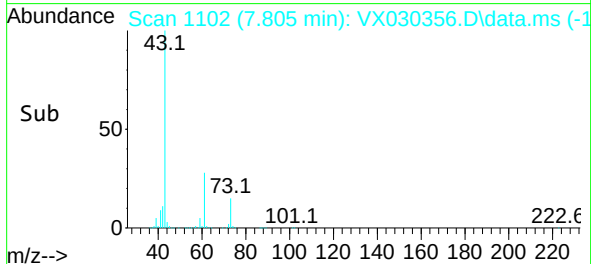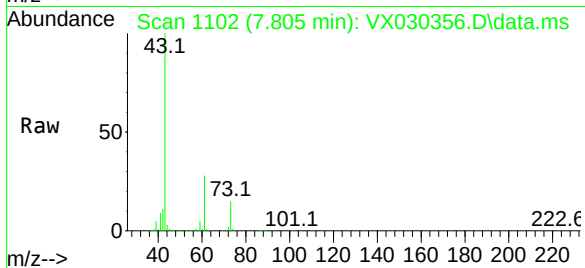

#49

1,4-Dioxane

Concen: 4.574 ug/l

RT: 7.671 min Scan# 1080

Delta R.T. 0.006 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41




Tgt Ion: 88 Resp: 413


Ion Ratio Lower Upper

88 100

43 0.0 23.8 35.8#

58 0.0 53.8 80.6#

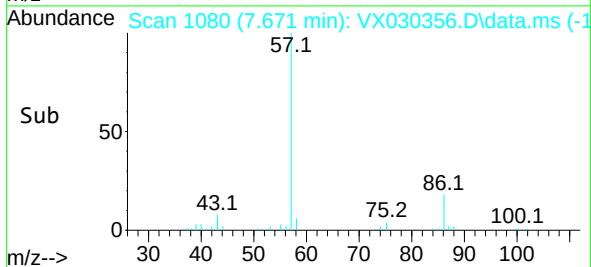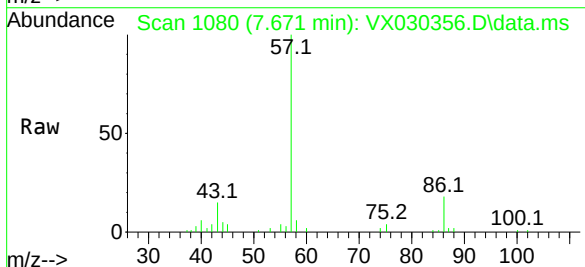

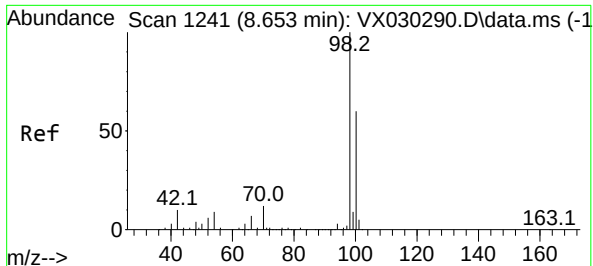

#50

Toluene-d8

Concen: 45.378 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.001 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41

Instrument :

MSVOA_X

ClientSampleId :





PB146634ZHE#03

Tgt Ion: 98 Resp: 467185

Ion Ratio Lower Upper

98 100

100 65.5 52.3 78.5

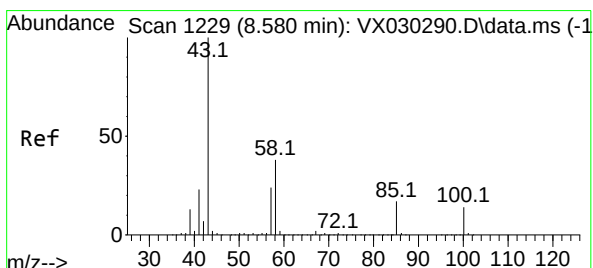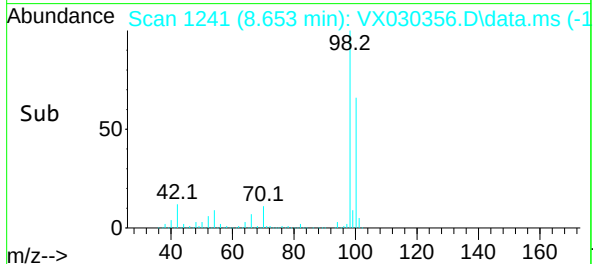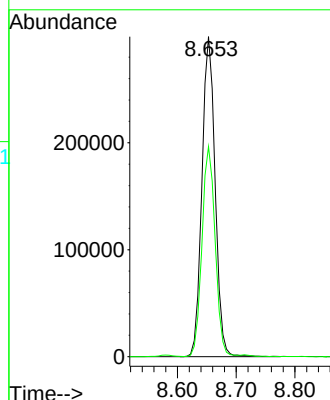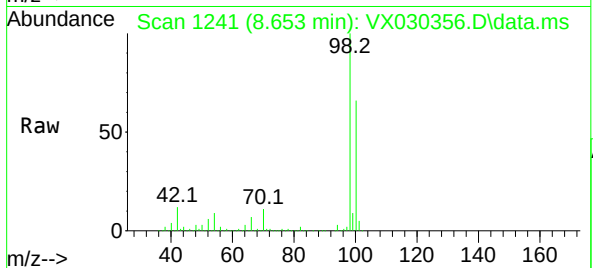

#51

4-Methyl-2-Pentanone

Concen: 31.597 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. -0.024 min

Lab File: VX030356.D




Acq: 02 Aug 2022 16:41


Tgt Ion: 43 Resp: 170370

Ion Ratio Lower Upper

43 100

58 9.4 31.4 47.2#


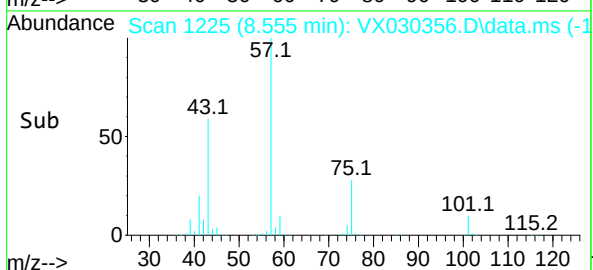
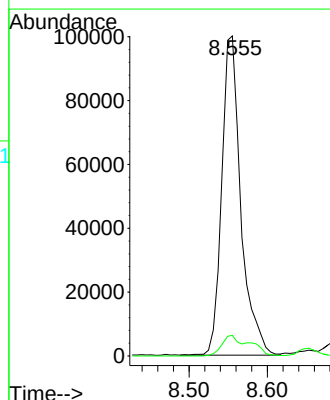
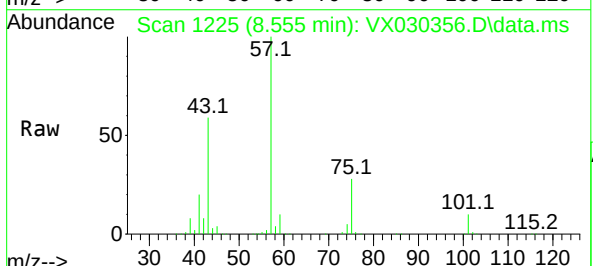


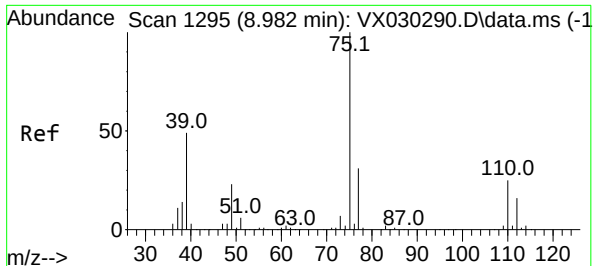

#53
 t-1,3-Dichloropropene
 Concen: 0.407 ug/l
 RT: 8.958 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX030356.D
 Acq: 02 Aug 2022 16:41




Instrument :
 MSVOA_X
 ClientSampleId :
 PB146634ZHE#03


Tgt Ion: 75 Resp: 1743
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.3 39.5#

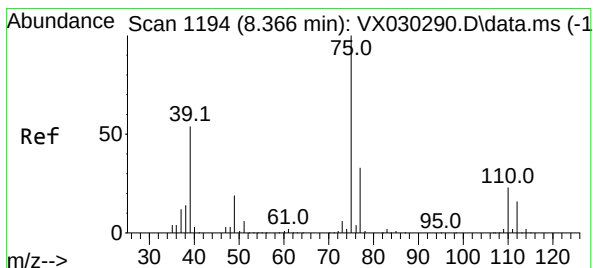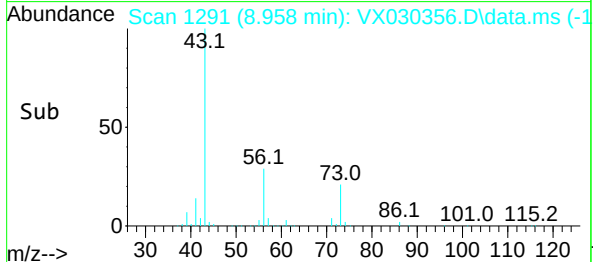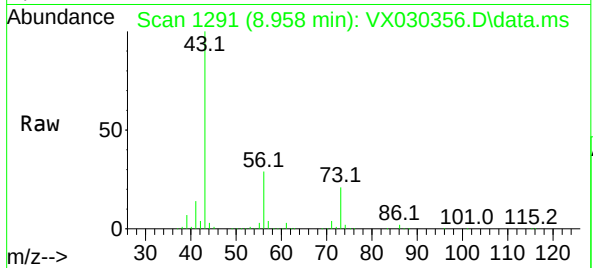

#54
 cis-1,3-Dichloropropene
 Concen: 15.629 ug/l
 RT: 8.555 min Scan# 1225
 Delta R.T. 0.183 min
 Lab File: VX030356.D
 Acq: 02 Aug 2022 16:41

Tgt Ion: 75 Resp: 72871
 Ion Ratio Lower Upper
 75 100
 77 0.4 25.0 37.4#
 39 27.5 37.5 56.3#

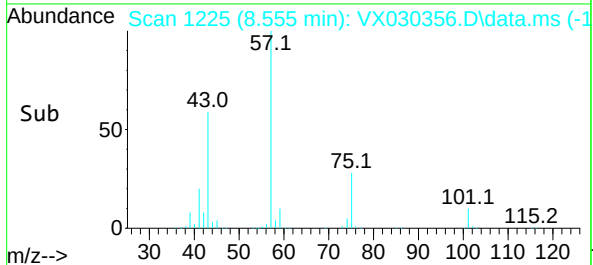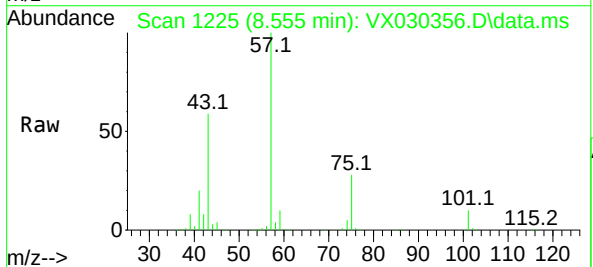

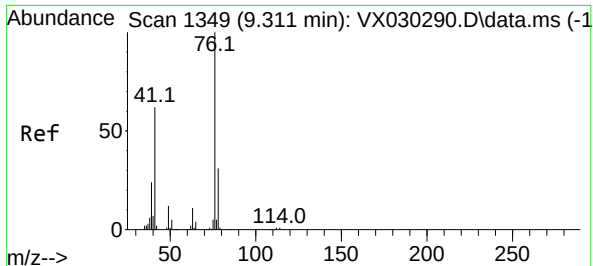

#57

1,3-Dichloropropane

Concen: 1.914 ug/l

RT: 9.488 min Scan# 1378

Delta R.T. 0.177 min

Lab File: VX030356.D

Acq: 02 Aug 2022 16:41

Instrument :

MSVOA_X

ClientSampleId :





PB146634ZHE#03

Tgt Ion: 76 Resp: 9881

Ion Ratio Lower Upper

76 100

78 0.0 25.9 38.9#

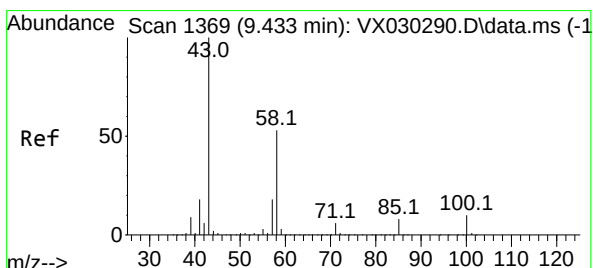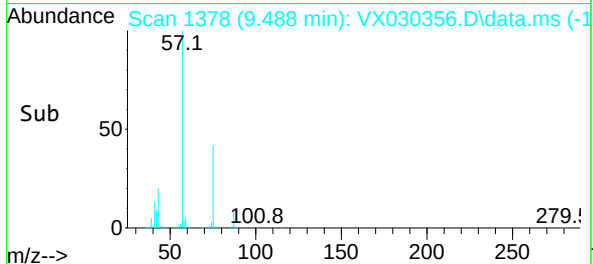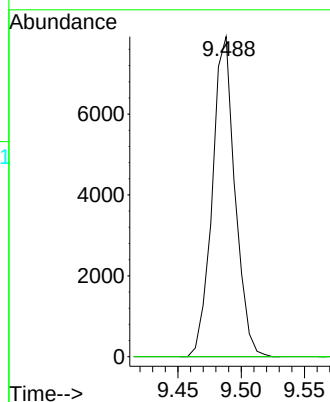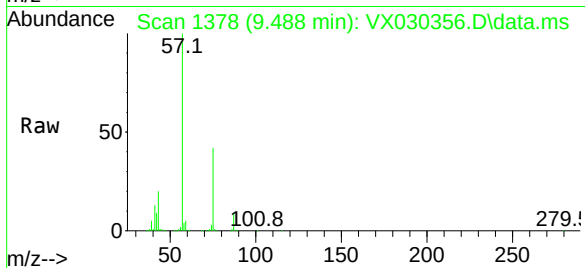

#59

2-Hexanone

Concen: 47.882 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.055 min

Lab File: VX030356.D




Acq: 02 Aug 2022 16:41


Tgt Ion: 43 Resp: 203688

Ion Ratio Lower Upper

43 100

58 0.0 27.6 82.8#


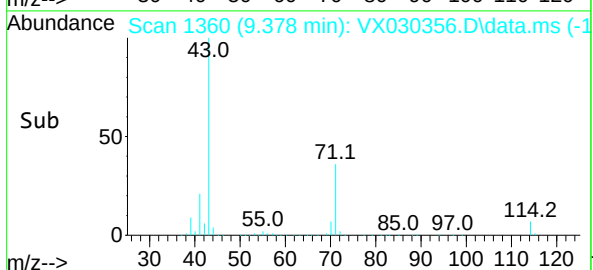
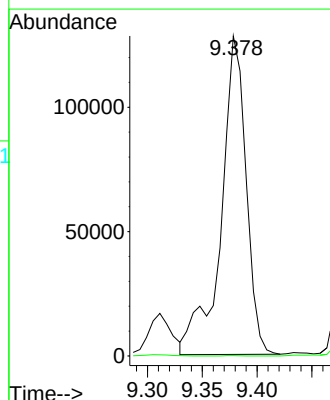
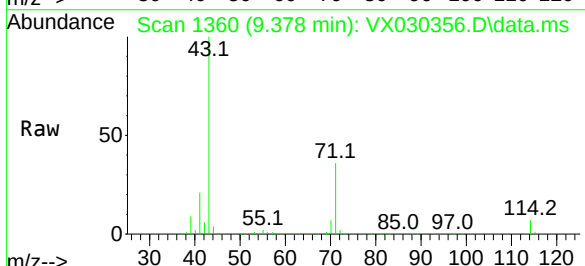




#62
4-Bromofluorobenzene
Concen: 44.213 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion: 95 Resp: 168935
Ion Ratio Lower Upper
95 100
174 70.5 0.0 149.0
176 67.9 0.0 146.0

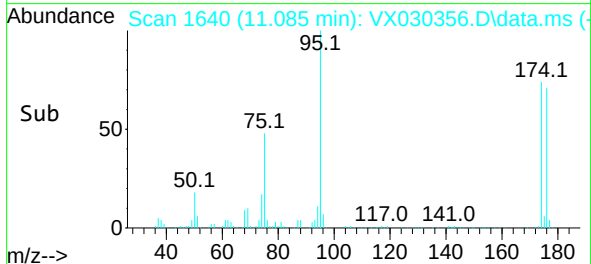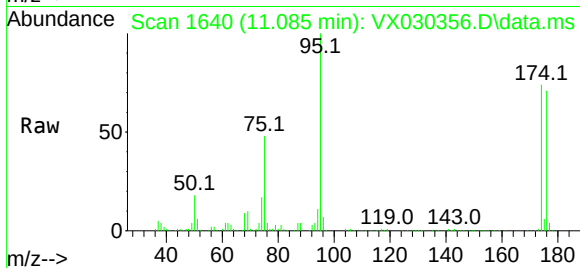

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion: 117 Resp: 274728
Ion Ratio Lower Upper
117 100
82 59.2 42.7 64.1
119 33.3 25.4 38.2


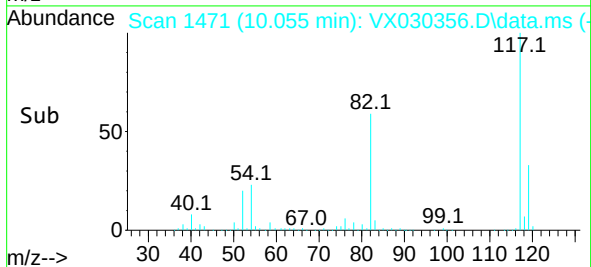

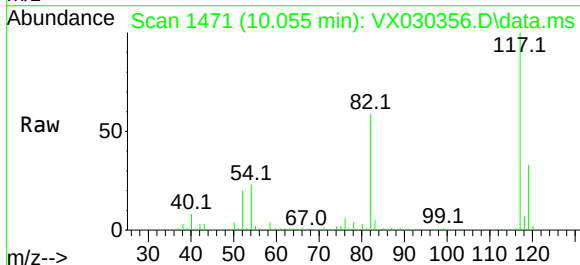




#67
Ethyl Benzene
Concen: Below Cal
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41




Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03


Tgt Ion: 91 Resp: 333
Ion Ratio Lower Upper
91 100
106 0.0 25.5 38.3#

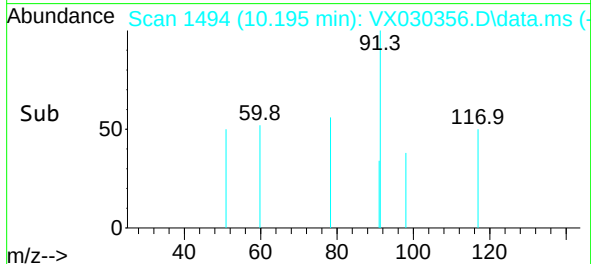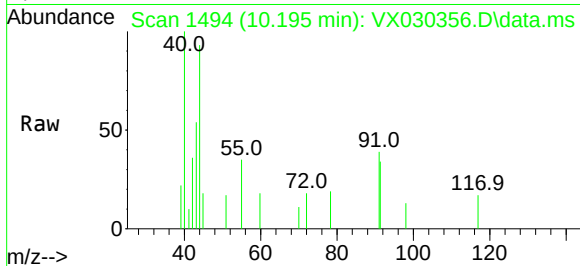

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41


Tgt Ion: 152 Resp: 153959
Ion Ratio Lower Upper
152 100
115 64.2 40.5 121.5
150 159.5 0.0 347.0

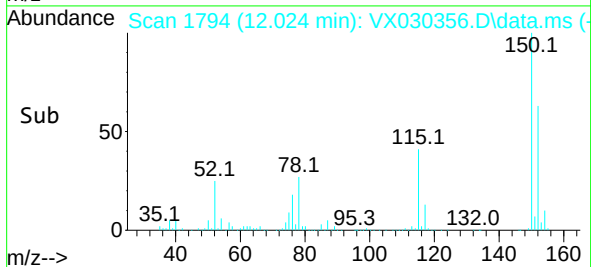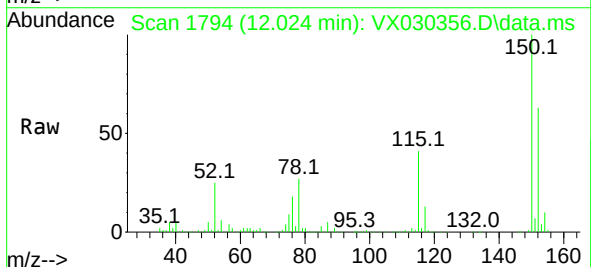






#74
N-ethyl acetate
Concen: 8.268 ug/l
RT: 10.640 min Scan# 1639
Delta R.T. -0.207 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Instrument :
MSVOA_X
ClientSampleId :
PB146634ZHE#03



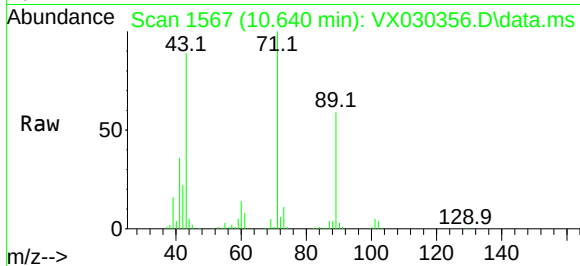



Tgt Ion:	43	Resp:	48295
Ion Ratio	100	Lower	Upper
43	100		
70	1.8	32.3	48.5#
55	4.2	18.4	27.6#
61	10.3	19.2	28.8#

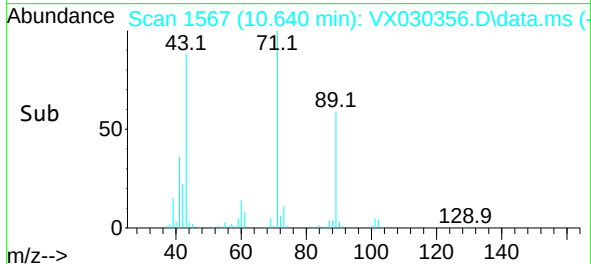

#76
1,2,3-Trichloropropane
Concen: 20.432 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.164 min
Lab File: VX030356.D
Acq: 02 Aug 2022 16:41

Tgt Ion:	75	Resp:	82918
Ion Ratio	100	Lower	Upper
75	100		
77	1.2	19.8	59.3#

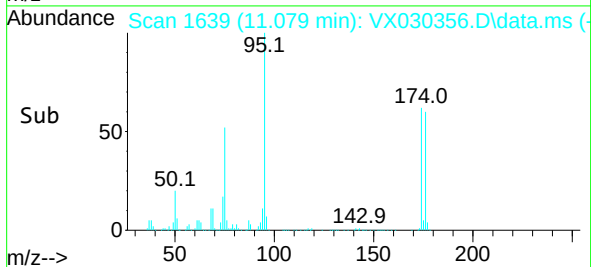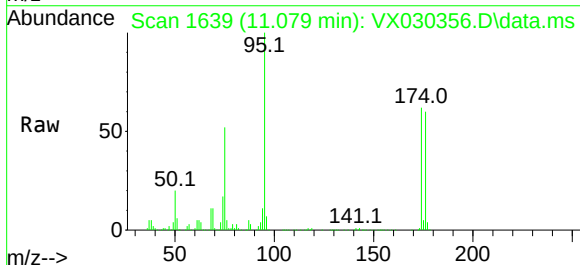

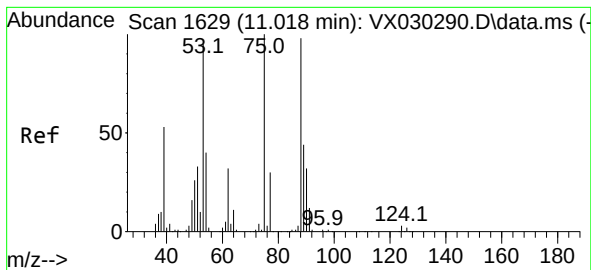

#81
 trans-1,4-Dichloro-2-butene
 Concen: 61.294 ug/l
 RT: 11.079 min Scan# 1
 Delta R.T. 0.055 min
 Lab File: VX030356.D
 Acq: 02 Aug 2022 16:41

Instrument :
 MSVOA_X
 ClientSampleId :
 PB146634ZHE#03

Tgt Ion: 75 Resp: 82918
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.2 111.4#
 89 0.0 34.8 52.2#

