

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
Data File : VX030342.D
Acq On : 02 Aug 2022 10:53
Operator : JC/MD
Sample : VX0802WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0802WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	21	28	40	rBV2	17130	42858	3.38%	0.745%
2	2.947	297	305	316	rBV	31095	73774	5.82%	1.282%
3	4.580	562	573	587	rBV3	8880	31287	2.47%	0.544%
4	5.391	695	706	719	rBV2	145346	416235	32.82%	7.235%
5	5.556	722	733	747	rVB	154876	437775	34.52%	7.610%
6	5.964	789	800	813	rBV2	173440	463148	36.52%	8.051%
7	6.763	921	931	942	rBV	245836	589904	46.51%	10.254%
8	8.653	1234	1241	1256	rBV	807215	1268287	100.00%	22.047%
9	10.055	1465	1471	1482	rBV	590265	775212	61.12%	13.476%
10	11.085	1634	1640	1650	rBV	577159	770997	60.79%	13.402%
11	12.024	1788	1794	1807	rBV	721930	883226	69.64%	15.353%




Sum of corrected areas: 5752703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
Data File : VX030342.D
Acq On : 02 Aug 2022 10:53
Operator : JC/MD
Sample : VX0802WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0802WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

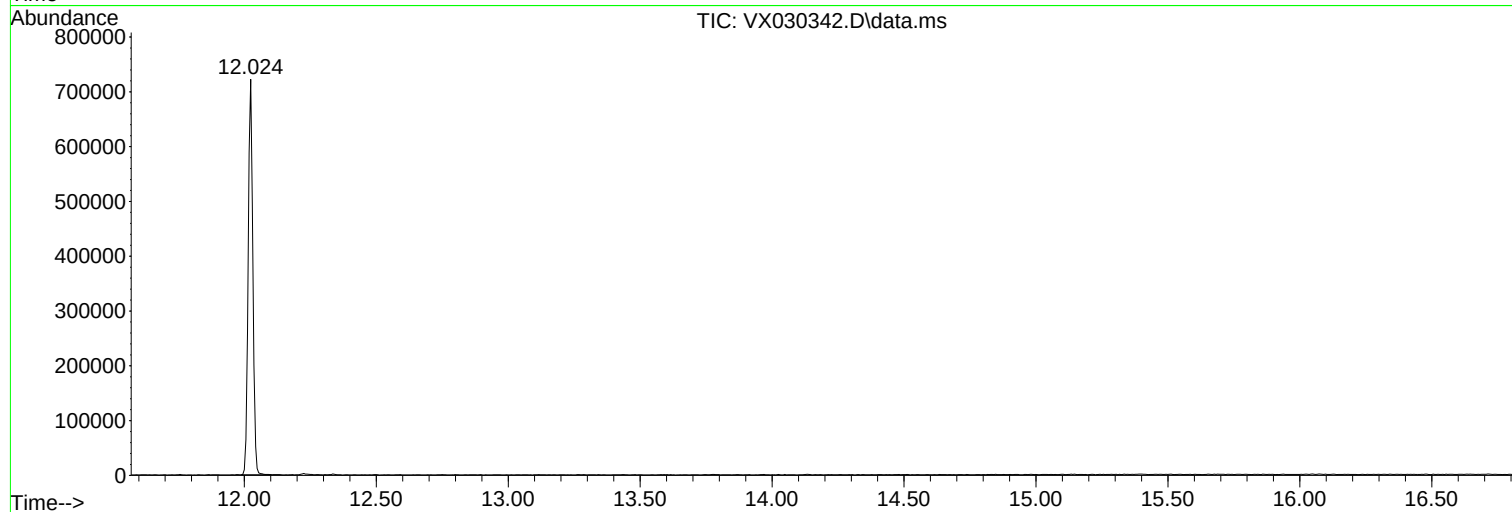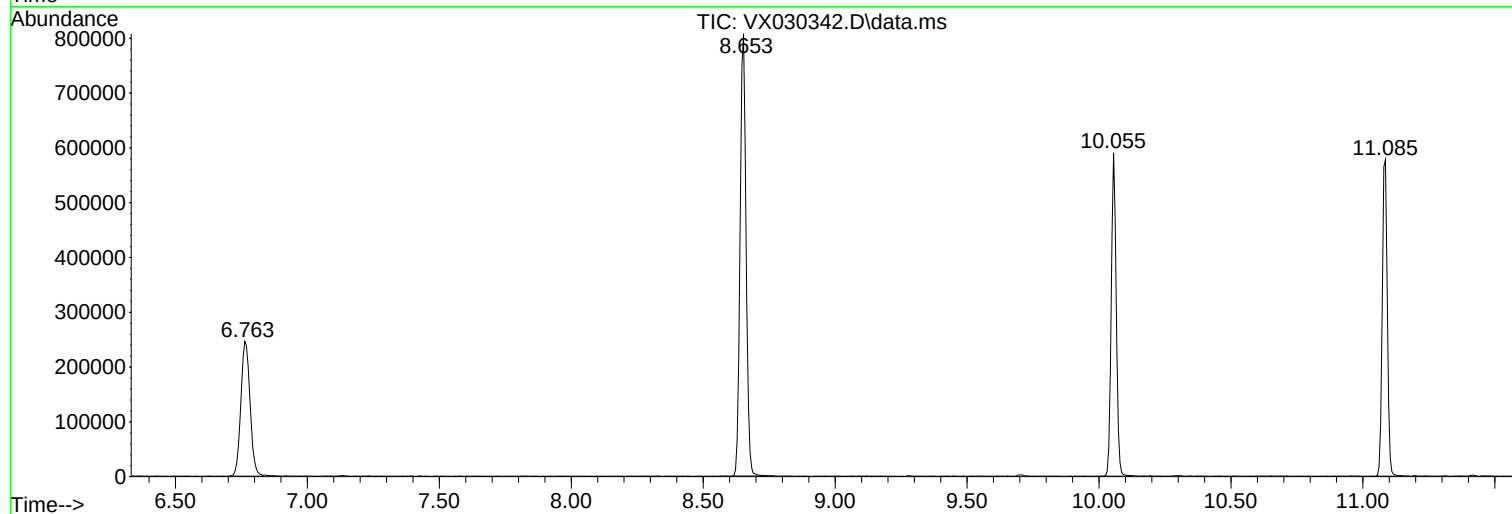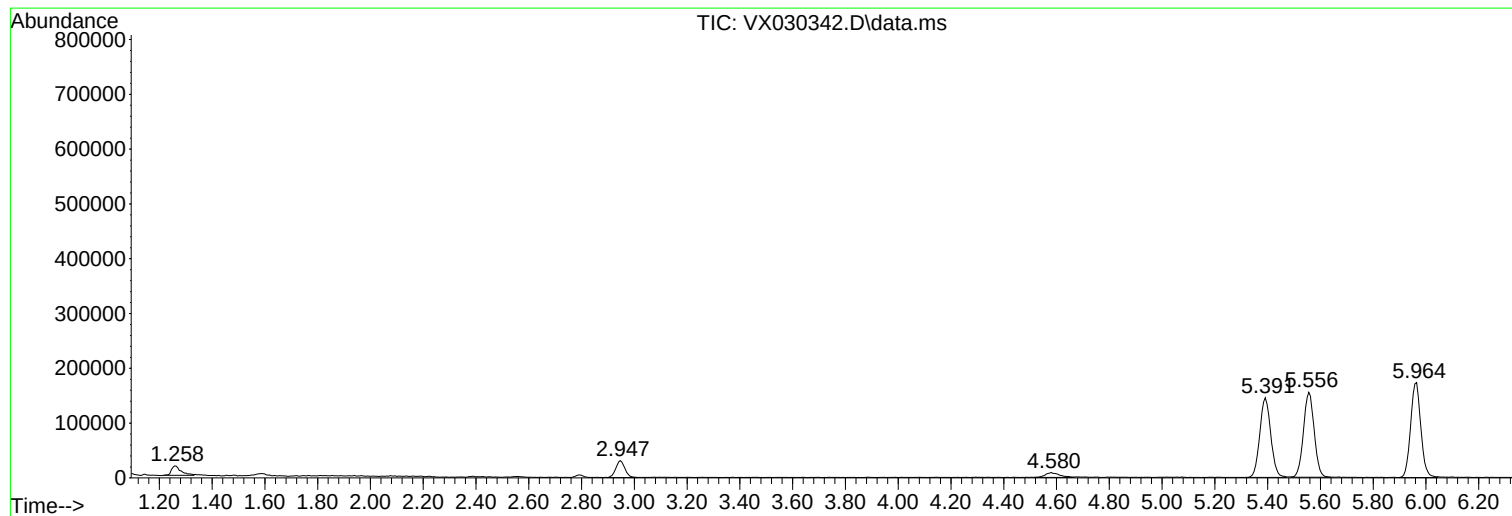

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
Data File : VX030342.D
Acq On : 02 Aug 2022 10:53
Operator : JC/MD
Sample : VX0802WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0802WBL01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Silane, (2-methoxyethyl)tri... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.947	8.43 ug/l	73774	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, (2-methoxyethyl)trimethyl-	132	C6H16OSi	018173-63-2	83
2			Methanol, TMS derivative	104	C4H12OSi	001825-61-2	83
3			Ethyl(dimethyl)methoxysilane	118	C5H14OSi	052686-75-6	74
4			10-Oxatetracyclo[5.5.2.0(1,5).0(...	352	C18H24O7	1000154-01-5	74
5			Silane, (3-chloropropyl)methoxyd...	166	C6H15ClOSi	018171-14-7	74

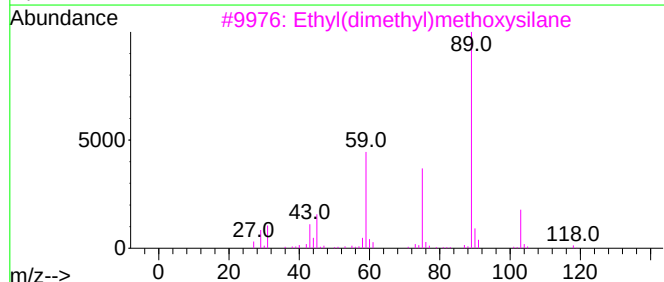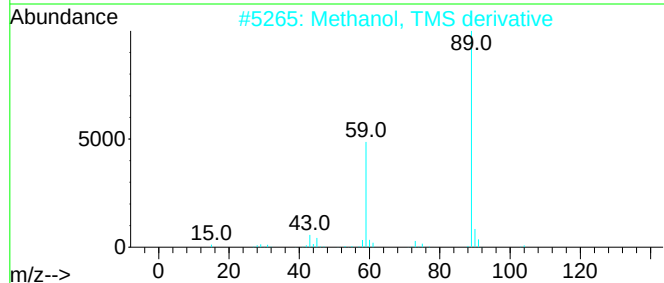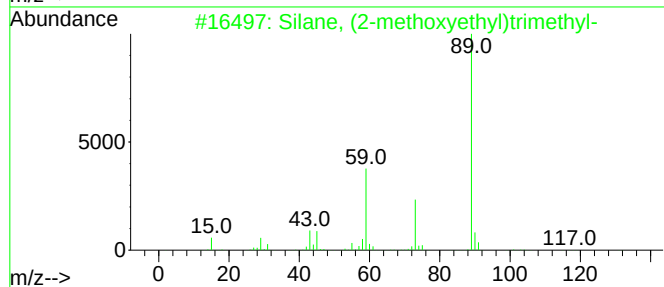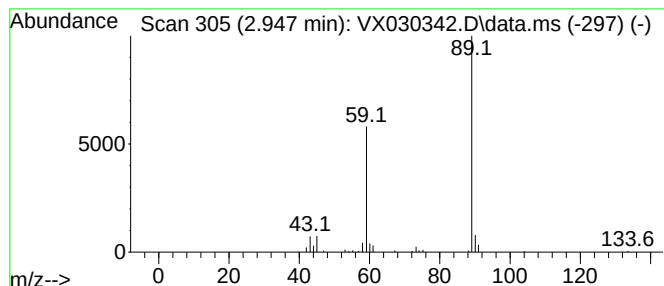

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
Data File : VX030342.D
Acq On : 02 Aug 2022 10:53
Operator : JC/MD
Sample : VX0802WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0802WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Silane, (2-meth...	2.947	8.4	ug/l	73774	1	5.556	437775	50.0