



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080222\
Data File : VX030339.D
Acq On : 02 Aug 2022 09:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Title : SW846 8260
Last Update : Mon Jul 25 16:49:17 2022

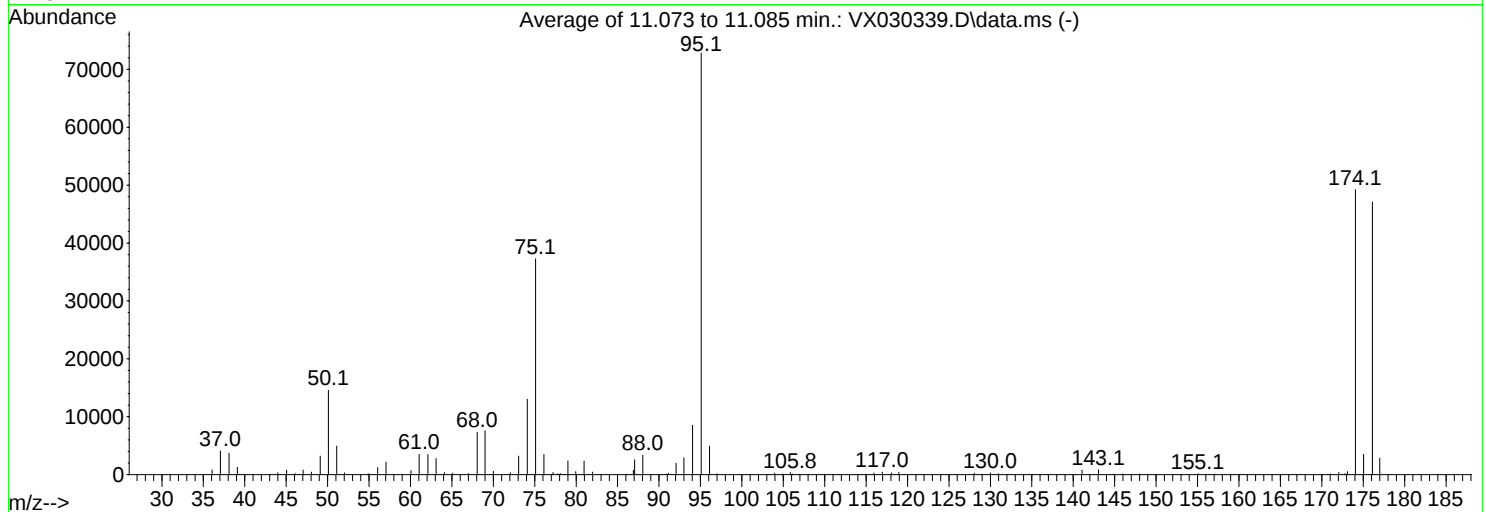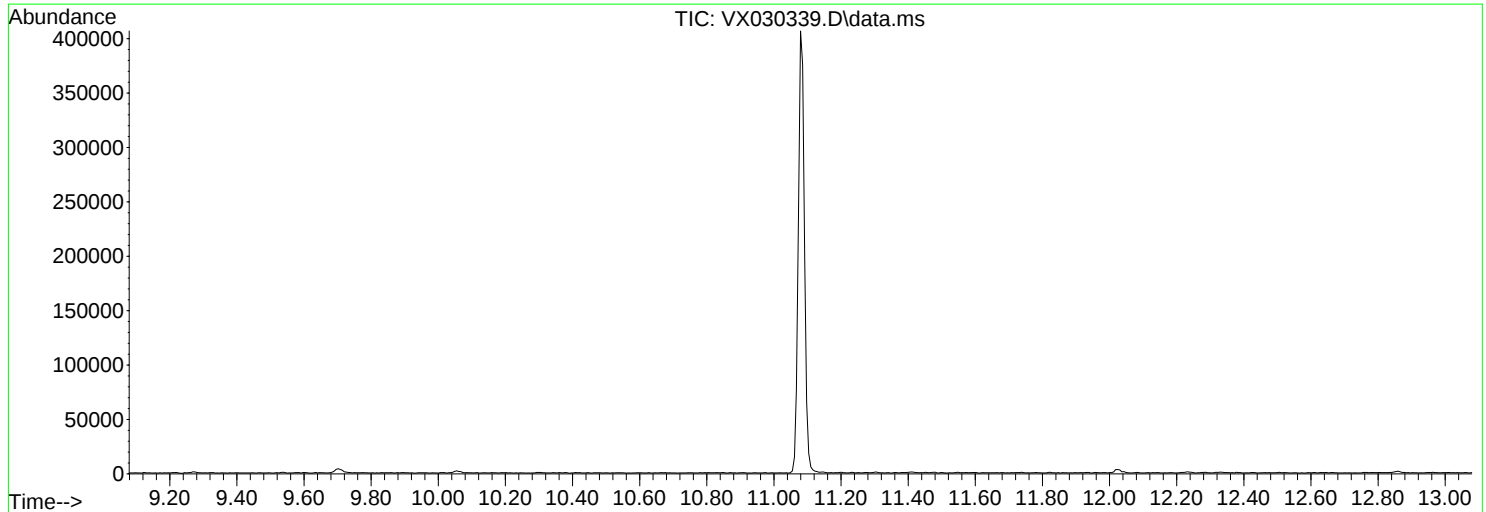

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	14577	PASS
75	95	30	60	51.2	37288	PASS
95	95	100	100	100.0	72853	PASS
96	95	5	9	6.8	4959	PASS
173	174	0.00	2	1.1	525	PASS
174	95	50	100	67.6	49229	PASS
175	174	5	9	7.1	3516	PASS
176	174	95	101	95.7	47091	PASS
177	176	5	9	6.1	2851	PASS