

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080223\
 Data File : VX036778.D
 Acq On : 02 Aug 2023 18:17
 Operator : JC/MD
 Sample : 03815-02 10X
 Misc : 5.12g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUILDING-A-2-(0-5)

Quant Time: Aug 03 07:30:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.549	168	123799	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	225663	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	208060	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	101505	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	84469	46.113	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	92.220%		
35) Dibromofluoromethane	5.385	113	71751	46.259	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.520%		
50) Toluene-d8	8.646	98	269083	48.920	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	97.840%		
62) 4-Bromofluorobenzene	11.079	95	104213	50.217	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	100.440%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.940	59	4781	11.025	ug/l #	80
13) Acrolein	2.245	56	61	0.246	ug/l #	1
16) Acetone	2.379	43	1345	1.769	ug/l #	86
17) Carbon Disulfide	2.507	76	4707	1.230	ug/l #	95
18) Methyl Acetate	2.708	43	2640	0.826	ug/l	99
20) Methylene Chloride	2.788	84	1030	0.609	ug/l #	83
25) 2-Butanone	4.586	43	989	0.802	ug/l #	51
36) 1,1-Dichloropropene	5.556	75	10290	4.451	ug/l #	50
38) Carbon Tetrachloride	5.549	117	13266	5.397	ug/l #	14
39) Methylcyclohexane	7.384	83	1575	0.548	ug/l #	89
40) Benzene	6.037	78	443915	65.997	ug/l	99
42) 1,2-Dichloroethane	6.031	62	4084	1.661	ug/l #	77
52) Toluene	8.720	92	232341	55.127	ug/l	98
53) t-1,3-Dichloropropene	8.720	75	2746	0.942	ug/l #	1
55) 1,1,2-Trichloroethane	9.012	97	4758	2.686	ug/l #	20
67) Ethyl Benzene	10.195	91	339943	40.575	ug/l	99
68) m/p-Xylenes	10.299	106	134495	43.025	ug/l	99
69) o-Xylene	10.640	106	61245	19.628	ug/l	100
70) Styrene	10.652	104	52247	10.149	ug/l	92
73) Isopropylbenzene	10.963	105	11857	1.411	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	53618	22.458	ug/l #	39
78) n-propylbenzene	11.305	91	6330	0.652	ug/l	94
79) 2-Chlorotoluene	11.628	91	3376	0.573	ug/l	87
80) 1,3,5-Trimethylbenzene	11.451	105	52199	7.428	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	53618	50.902	ug/l #	5
82) 4-Chlorotoluene	11.628	91	3653	0.545	ug/l	98
83) tert-Butylbenzene	11.750	119	18553	2.687	ug/l #	54
84) 1,2,4-Trimethylbenzene	11.750	105	154593	21.996	ug/l	96
85) sec-Butylbenzene	11.750	105	154593	17.955	ug/l #	57
86) p-Isopropyltoluene	11.969	119	5730	0.809	ug/l	97
89) n-Butylbenzene	12.317	91	3935	0.620	ug/l #	12
90) Hexachloroethane	12.548	117	3738	2.603	ug/l #	17
95) Naphthalene	13.780	128	8733885	1189.756	ug/l #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080223\
Data File : VX036778.D
Acq On : 02 Aug 2023 18:17
Operator : JC/MD
Sample : 03815-02 10X
Misc : 5.12g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Quant Time: Aug 03 07:30:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration

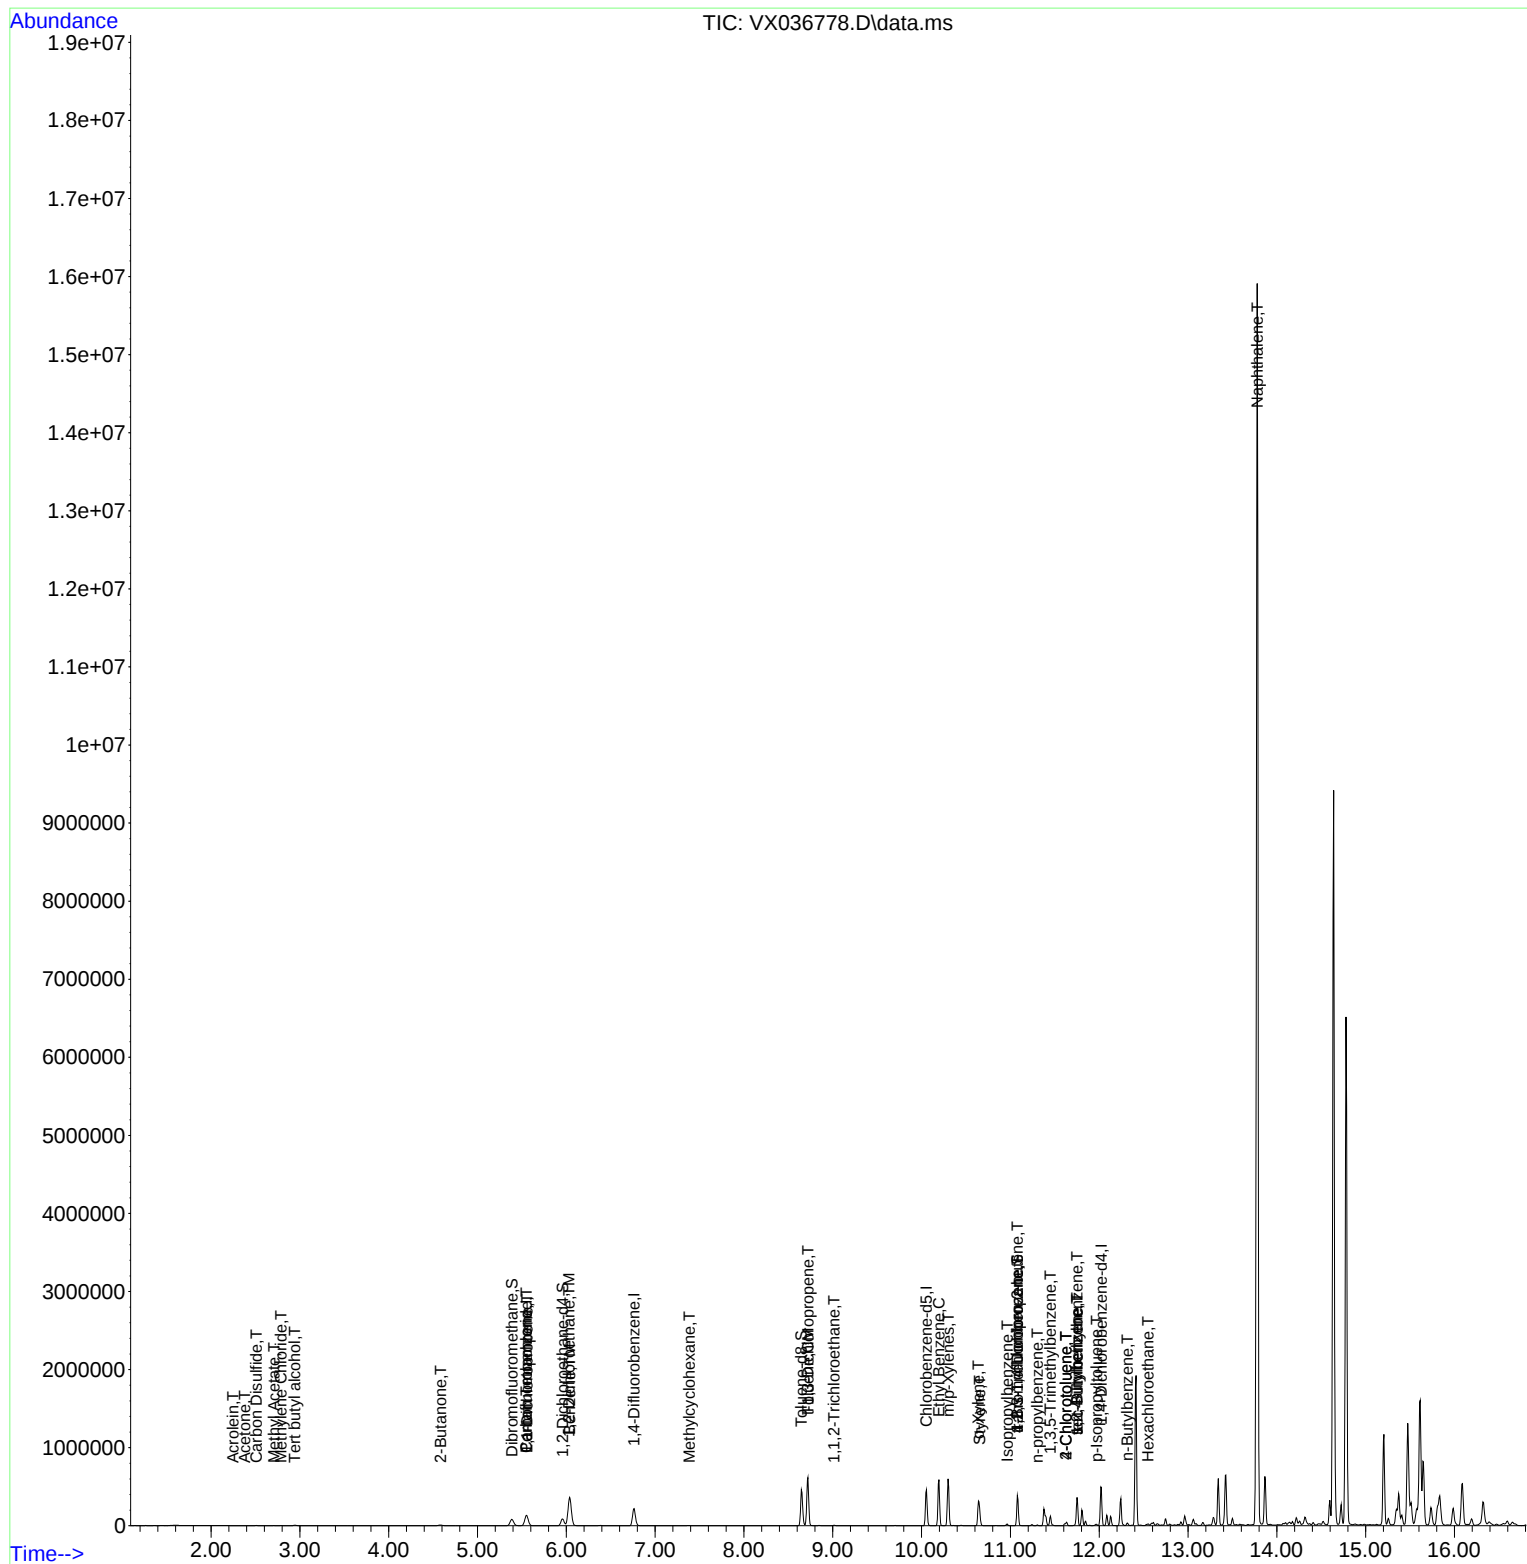



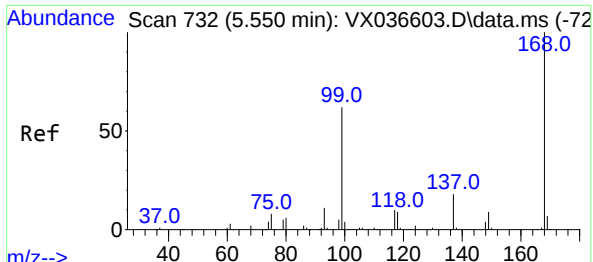


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.549 min Scan# 71
Delta R.T. -0.001 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)



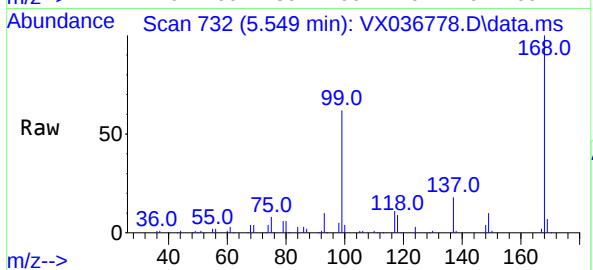



Tgt Ion:168 Resp: 123799
Ion Ratio Lower Upper
168 100
99 62.1 56.6 85.0

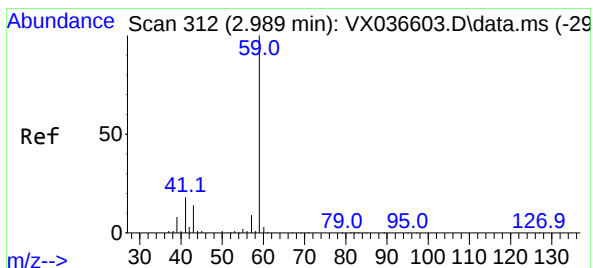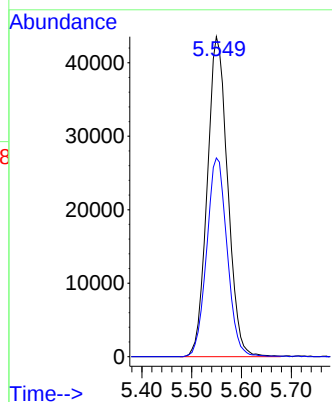

#11
Tert butyl alcohol
Concen: 11.025 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.049 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 59 Resp: 4781
Ion Ratio Lower Upper
59 100
57 0.4 6.0 9.0#


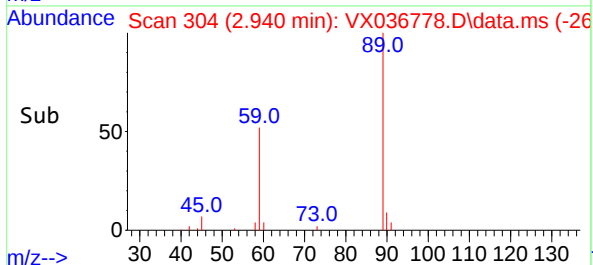

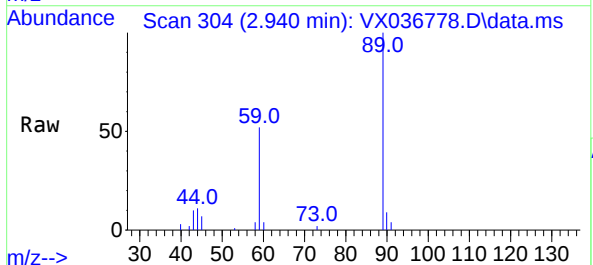




#13
Acrolein
Concen: 0.246 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 56 Resp: 61
Ion Ratio Lower Upper
56 100
55 157.4 57.1 85.7#



#16
Acetone
Concen: 1.769 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.012 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 43 Resp: 1345
Ion Ratio Lower Upper
43 100
58 34.8 21.9 32.9#


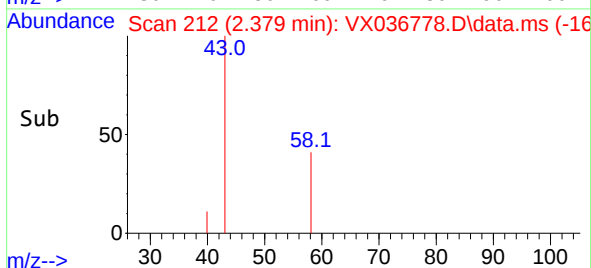
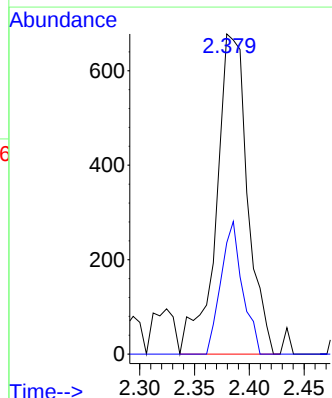





#17
Carbon Disulfide
Concen: 1.230 ug/l
RT: 2.507 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 76 Resp: 4707
Ion Ratio Lower Upper
76 100
78 10.7 7.0 10.6#



#18
Methyl Acetate
Concen: 0.826 ug/l
RT: 2.708 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17


Tgt Ion: 43 Resp: 2640
Ion Ratio Lower Upper
43 100
74 21.9 17.8 26.8

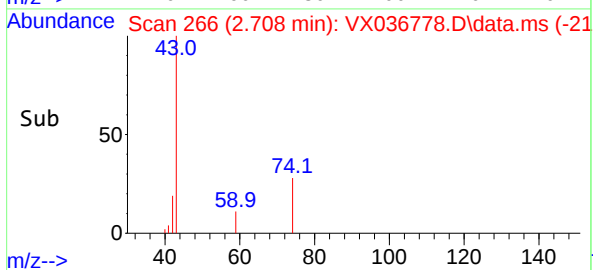






#20
Methylene Chloride
Concen: 0.609 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)

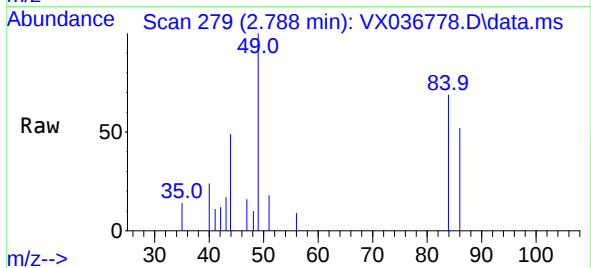

Tgt Ion: 84 Resp: 1030




Ion	Ratio	Lower	Upper
84	100		
49	145.1	103.6	155.4
51	26.5	33.8	50.6#
86	75.6	49.4	74.0#




#25
2-Butanone
Concen: 0.802 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.024 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 43 Resp: 989

Ion	Ratio	Lower	Upper
43	100		
72	0.0	19.4	29.2#


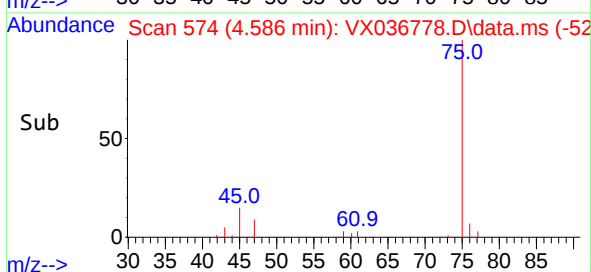






#33
1,2-Dichloroethane-d4
Concen: 46.113 ug/l
RT: 5.958 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 65 Resp: 84469
Ion Ratio Lower Upper
65 100
67 52.6 0.0 100.2

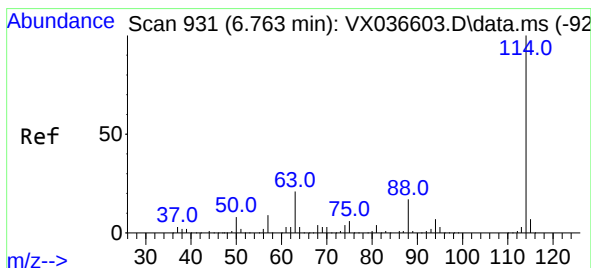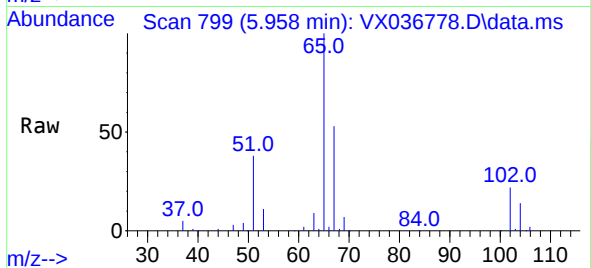

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 114 Resp: 225663
Ion Ratio Lower Upper
114 100
63 20.1 0.0 45.0
88 16.6 0.0 36.6

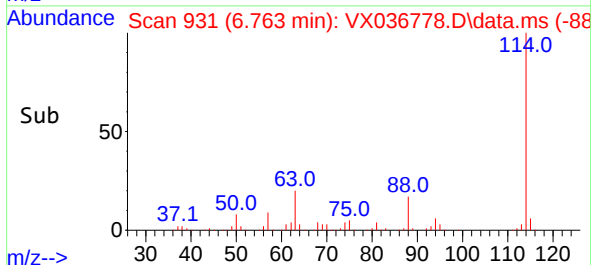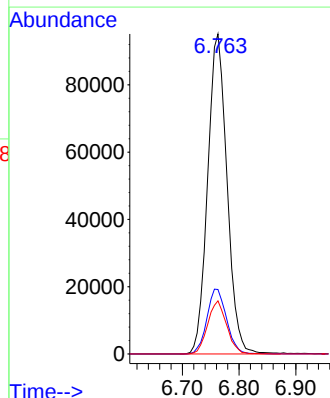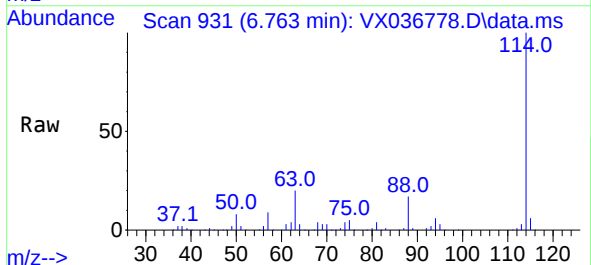







#35
Dibromofluoromethane
Concen: 46.259 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)

Tgt Ion:113 Resp: 71751




Ion	Ratio	Lower	Upper
113	100		
111	102.4	82.9	124.3
192	18.1	13.3	19.9

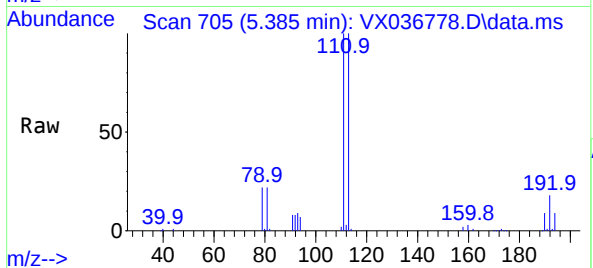


#36
1,1-Dichloropropene
Concen: 4.451 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 75 Resp: 10290


Ion	Ratio	Lower	Upper
75	100		
110	8.6	17.0	50.9#
77	0.0	24.7	37.1#

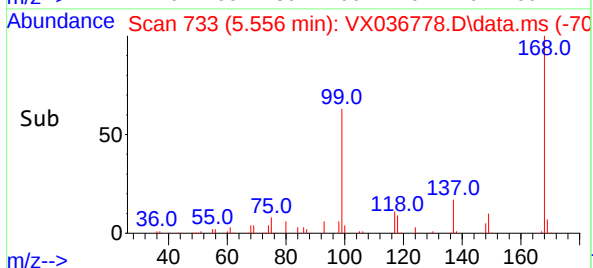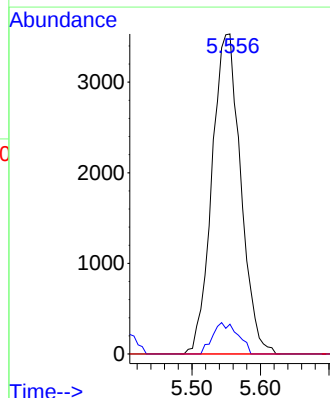



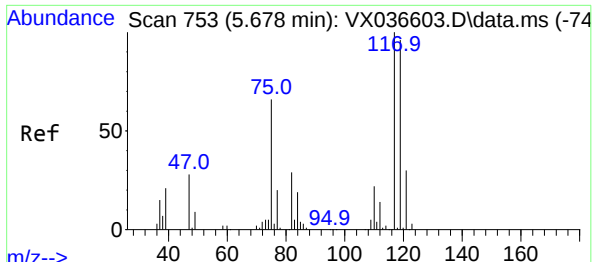


#38
Carbon Tetrachloride
Concen: 5.397 ug/l
RT: 5.549 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17


Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)

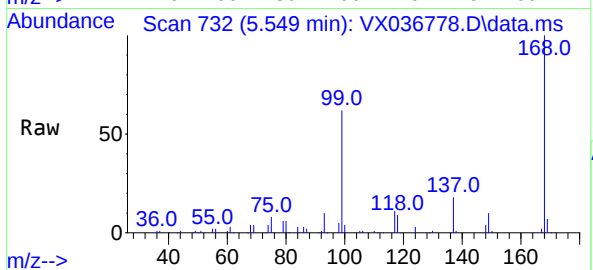



Tgt Ion:117 Resp: 13266
Ion Ratio Lower Upper
117 100
119 4.1 78.2 117.2#
121 0.0 24.4 36.6#

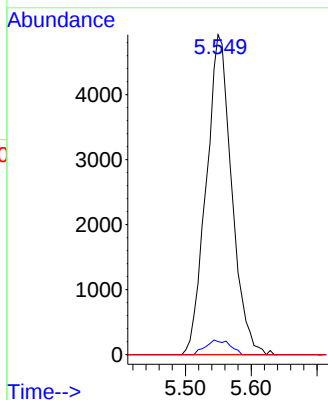


#39
Methylcyclohexane
Concen: 0.548 ug/l
RT: 7.384 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

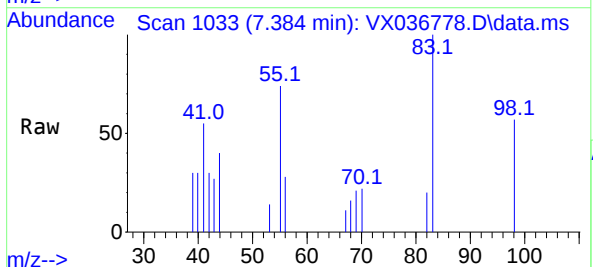

Tgt Ion: 83 Resp: 1575
Ion Ratio Lower Upper
83 100
55 73.9 64.6 97.0
98 57.1 36.7 55.1#



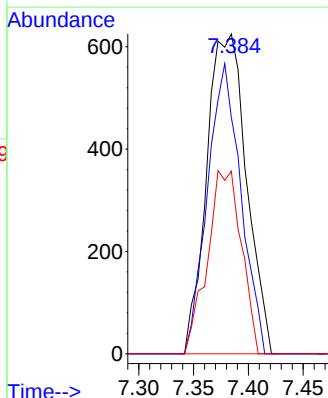
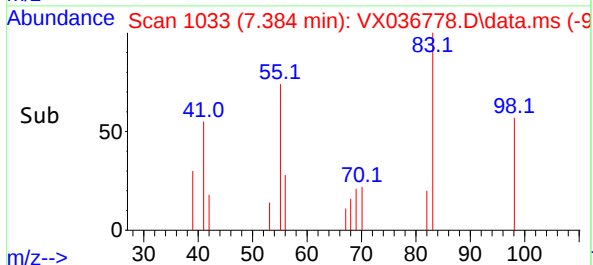




#40
Benzene
Concen: 65.997 ug/l
RT: 6.037 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 78 Resp: 443915
Ion Ratio Lower Upper
78 100
77 23.4 19.3 28.9

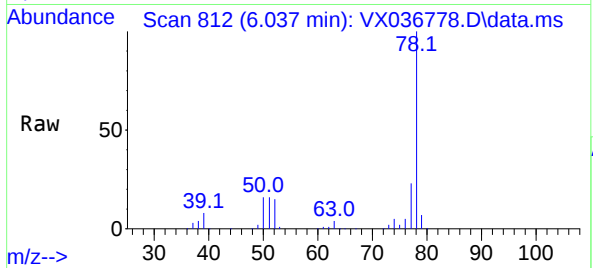

#42
1,2-Dichloroethane
Concen: 1.661 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.055 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 62 Resp: 4084
Ion Ratio Lower Upper
62 100
98 0.0 0.0 16.0


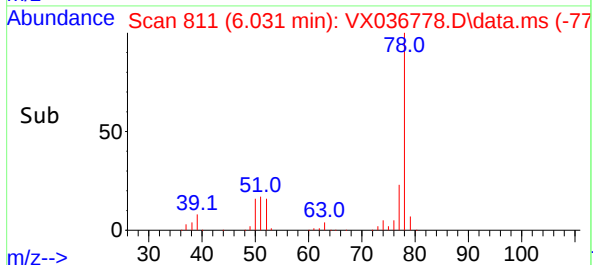
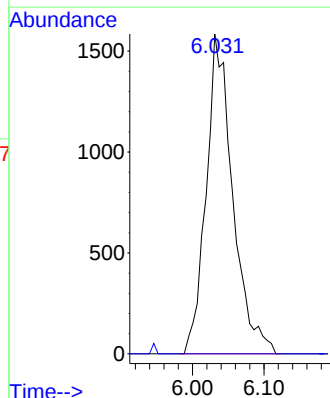
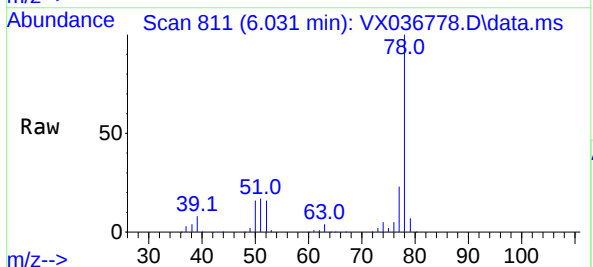




#50
Toluene-d8
Concen: 48.920 ug/l
RT: 8.646 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 98 Resp: 269083
Ion Ratio Lower Upper
98 100
100 66.5 53.1 79.7

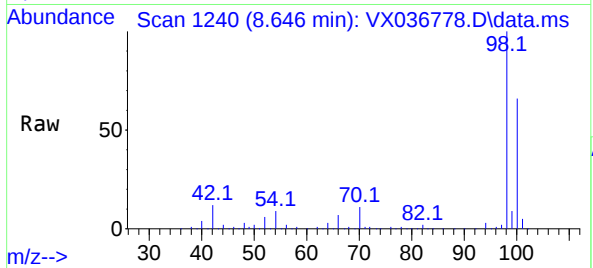

#52
Toluene
Concen: 55.127 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 92 Resp: 232341
Ion Ratio Lower Upper
92 100
91 170.0 134.2 201.2

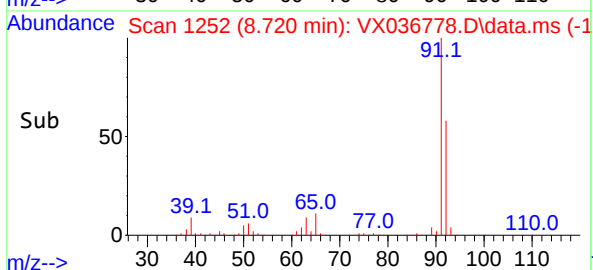



#53

t-1,3-Dichloropropene

Concen: 0.942 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.256 min

Lab File: VX036778.D

Acq: 02 Aug 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUILDING-A-2-(0-5)

Tgt Ion: 75 Resp: 2746

Ion Ratio Lower Upper

75 100

77 163.2 25.7 38.5#

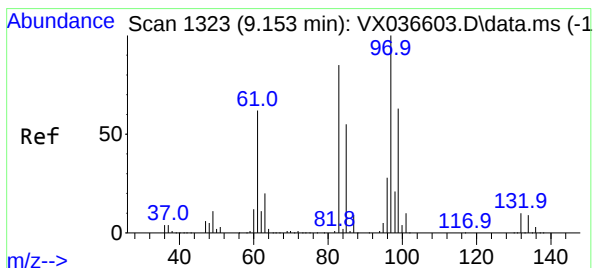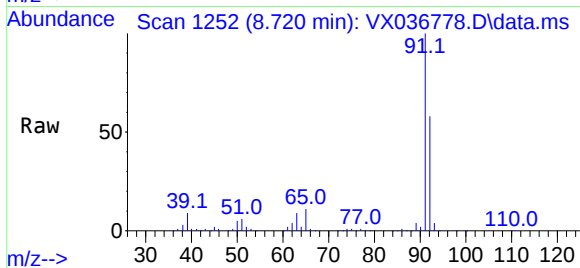

#55

1,1,2-Trichloroethane

Concen: 2.686 ug/l

RT: 9.012 min Scan# 1300

Delta R.T. -0.140 min

Lab File: VX036778.D

Acq: 02 Aug 2023 18:17

Tgt Ion: 97 Resp: 4758




Ion Ratio Lower Upper


97 100

83 0.0 65.8 98.8#

85 0.0 41.6 62.4#

99 7.1 47.8 71.8#


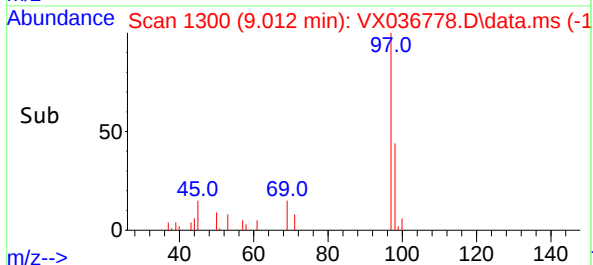
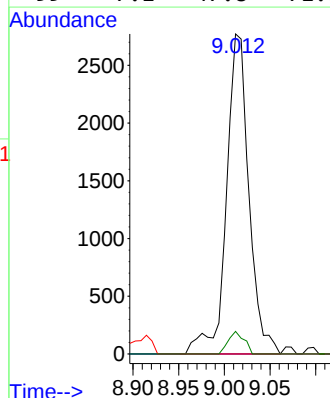
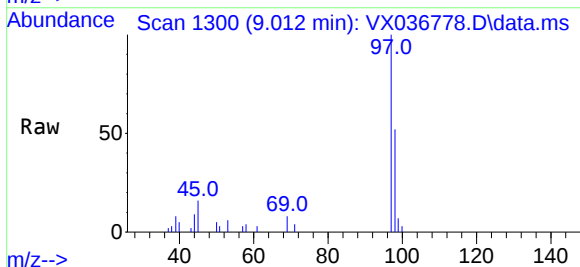




#62
4-Bromofluorobenzene
Concen: 50.217 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 95 Resp: 104213
Ion Ratio Lower Upper
95 100
174 72.8 0.0 135.6
176 71.7 0.0 131.0

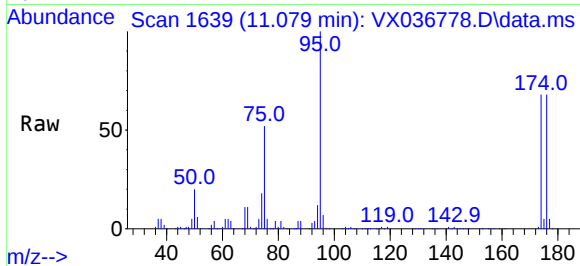

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 117 Resp: 208060
Ion Ratio Lower Upper
117 100
82 55.3 46.2 69.4
119 31.6 25.5 38.3


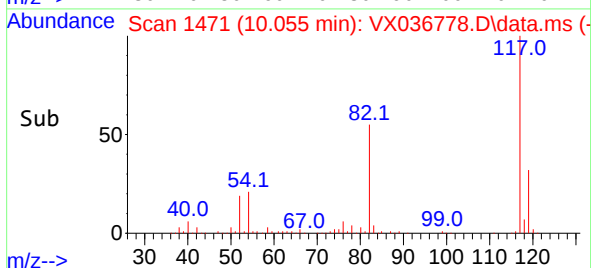
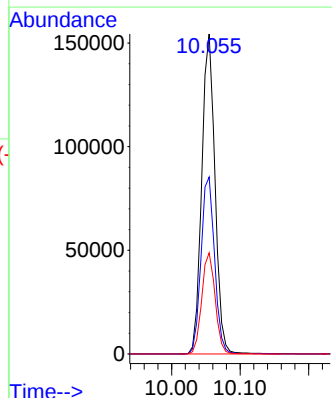
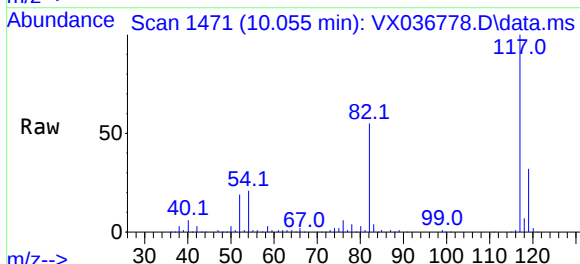




#67
Ethyl Benzene
Concen: 40.575 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 91 Resp: 339943
Ion Ratio Lower Upper
91 100
106 31.5 24.9 37.3

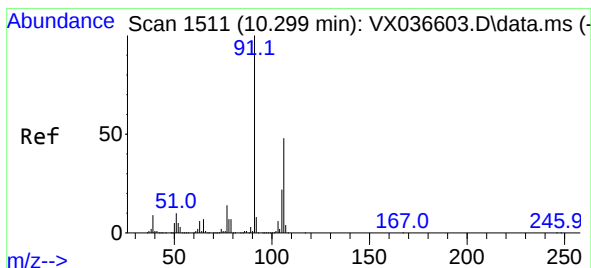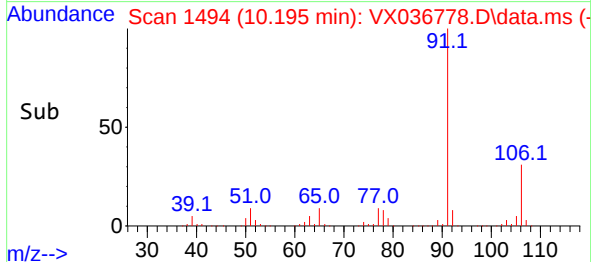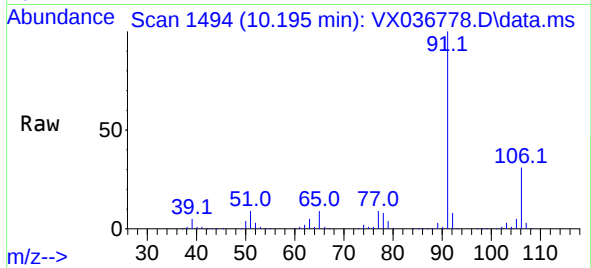

#68
m/p-Xylenes
Concen: 43.025 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 106 Resp: 134495
Ion Ratio Lower Upper
106 100
91 205.9 165.5 248.3


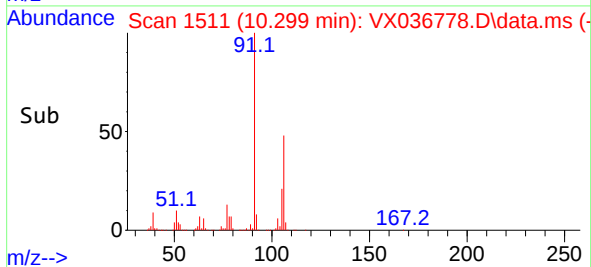

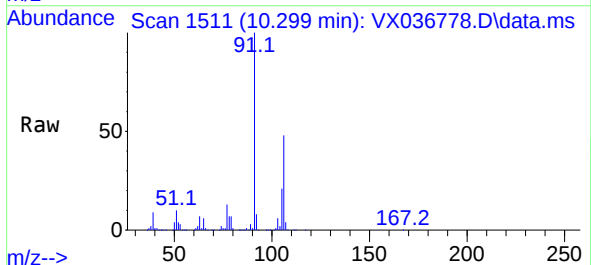




#69
o-Xylene
Concen: 19.628 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion:106 Resp: 61245
Ion Ratio Lower Upper
106 100
91 217.4 108.9 326.8

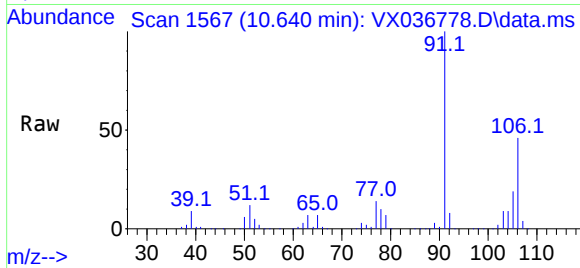

#70
Styrene
Concen: 10.149 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion:104 Resp: 52247
Ion Ratio Lower Upper
104 100
78 59.1 43.6 65.4
103 61.1 43.6 65.4


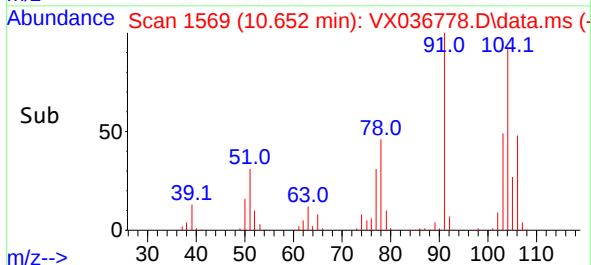
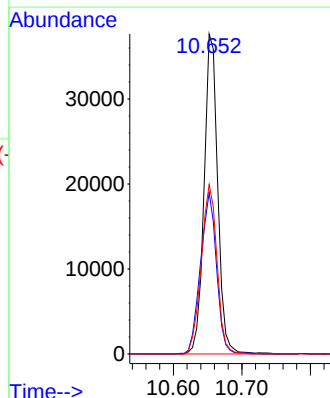
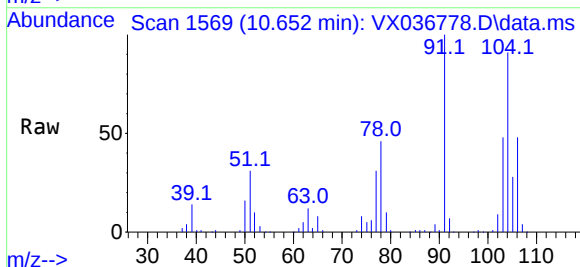




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion:152 Resp: 101505
Ion Ratio Lower Upper
152 100
115 62.4 43.3 129.9
150 157.0 0.0 345.0

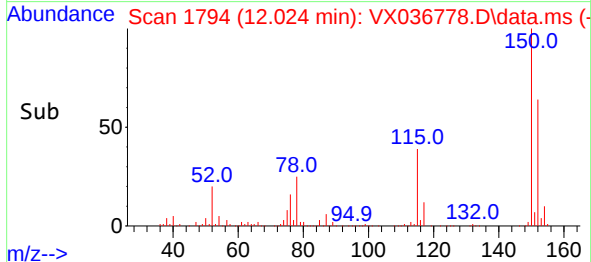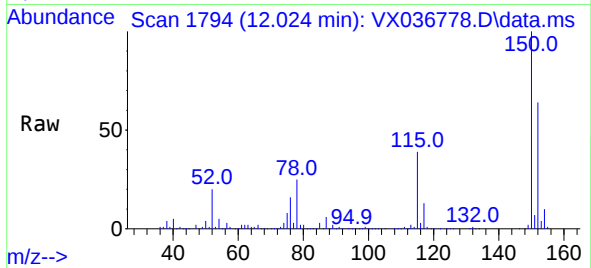

#73
Isopropylbenzene
Concen: 1.411 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion:105 Resp: 11857
Ion Ratio Lower Upper
105 100
120 25.1 12.9 38.6


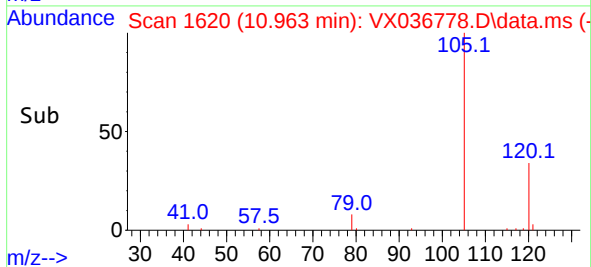

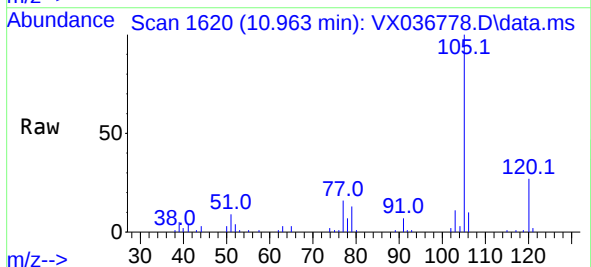




#76
1,2,3-Trichloropropane
Concen: 22.458 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 75 Resp: 53618
Ion Ratio Lower Upper
75 100
77 1.1 19.1 57.5#

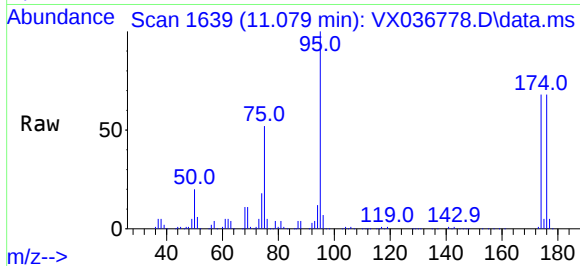

#78
n-propylbenzene
Concen: 0.652 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 91 Resp: 6330
Ion Ratio Lower Upper
91 100
120 25.7 11.5 34.4

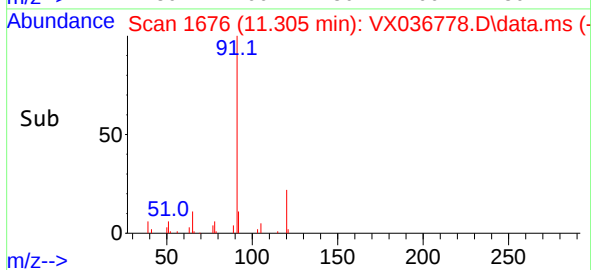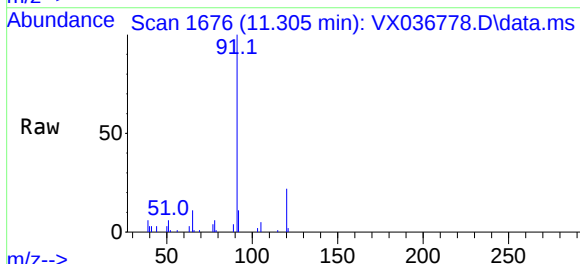



#79

2-Chlorotoluene

Concen: 0.573 ug/l

RT: 11.628 min Scan# 11

Delta R.T. 0.262 min

Lab File: VX036778.D

Acq: 02 Aug 2023 18:17

Instrument :

MSVOA_X

ClientSampleId :





BUILDING-A-2-(0-5)

Tgt Ion: 91 Resp: 3376

Ion Ratio Lower Upper

91 100

126 25.3 16.3 48.8

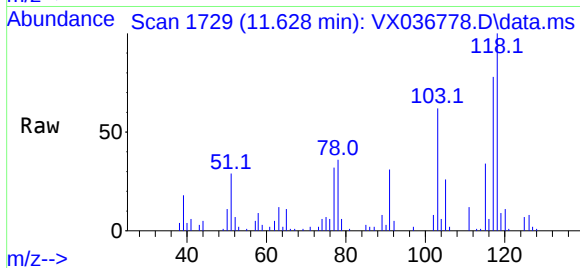

#80

1,3,5-Trimethylbenzene

Concen: 7.428 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX036778.D




Acq: 02 Aug 2023 18:17


Tgt Ion:105 Resp: 52199

Ion Ratio Lower Upper

105 100

120 49.3 24.1 72.3


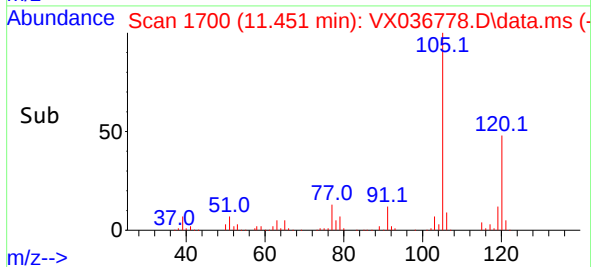

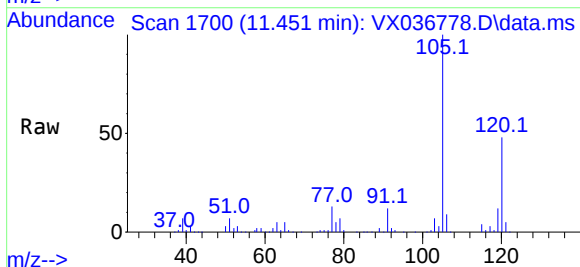




#81
trans-1,4-Dichloro-2-butene
Concen: 50.902 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 75 Resp: 53618
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

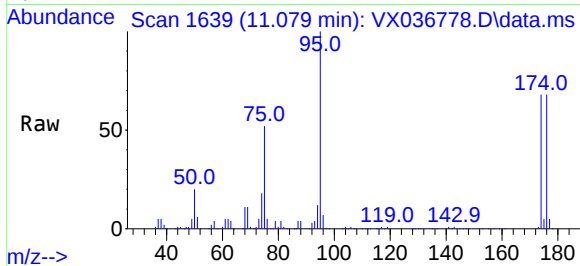

#82
4-Chlorotoluene
Concen: 0.545 ug/l
RT: 11.628 min Scan# 1729
Delta R.T. 0.177 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion: 91 Resp: 3653
Ion Ratio Lower Upper
91 100
126 27.6 14.2 42.6


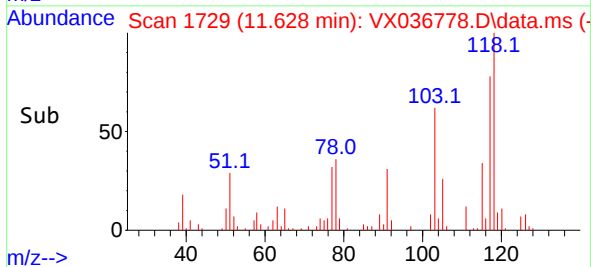

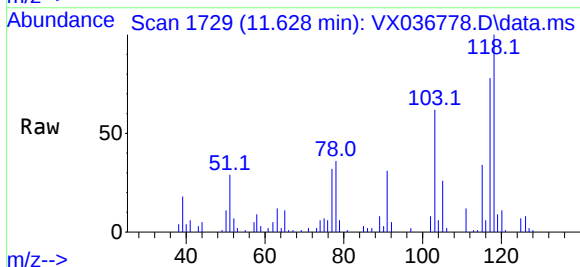




#83
tert-Butylbenzene
Concen: 2.687 ug/l
RT: 11.750 min Scan# 11
Delta R.T. 0.036 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion:119 Resp: 18553
Ion Ratio Lower Upper
119 100
91 97.4 31.2 93.6#
134 0.0 11.7 35.0#

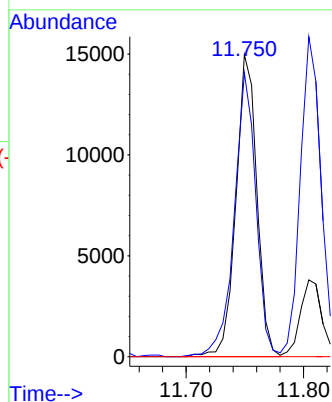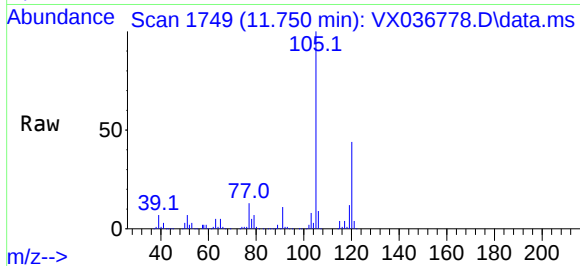

#84
1,2,4-Trimethylbenzene
Concen: 21.996 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion:105 Resp: 154593
Ion Ratio Lower Upper
105 100
120 45.1 21.2 63.6


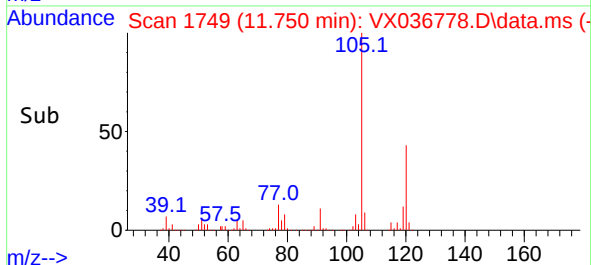

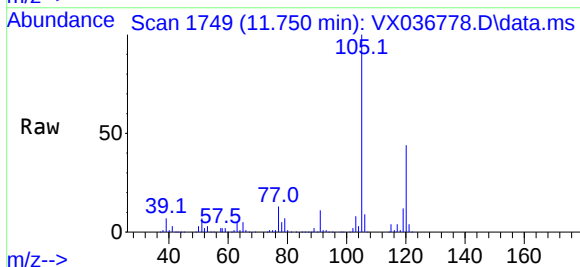




#85
sec-Butylbenzene
Concen: 17.955 ug/l
RT: 11.750 min Scan# 11
Delta R.T. -0.140 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion:105 Resp: 154593
Ion Ratio Lower Upper
105 100
134 0.0 9.8 29.4#



#86
p-Isopropyltoluene
Concen: 0.809 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.037 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Tgt Ion:119 Resp: 5730
Ion Ratio Lower Upper
119 100
134 27.5 12.8 38.3
91 25.5 13.1 39.3


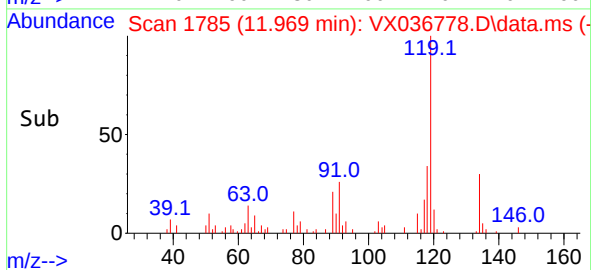






#89
n-Butylbenzene
Concen: 0.620 ug/l
RT: 12.317 min Scan# 119
Delta R.T. -0.012 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17




Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)


Tgt Ion: 91 Resp: 3935
Ion Ratio Lower Upper
91 100
92 27.5 27.4 82.0
134 124.7 12.6 37.8#

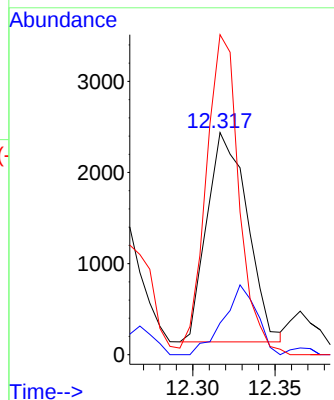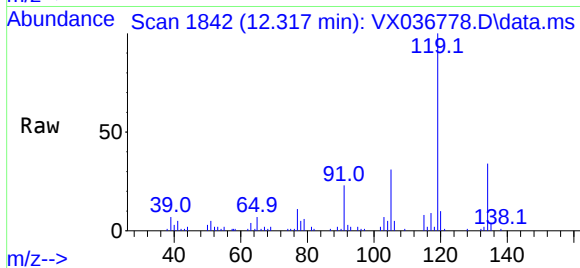

#90
Hexachloroethane
Concen: 2.603 ug/l
RT: 12.548 min Scan# 1880
Delta R.T. 0.012 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17


Tgt Ion: 117 Resp: 3738
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

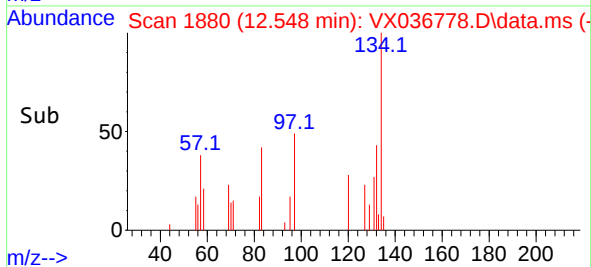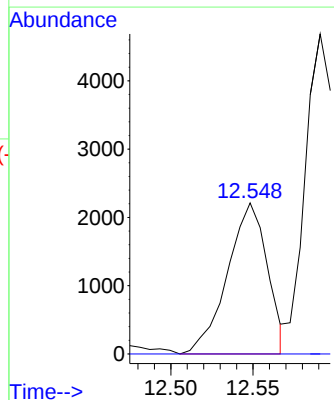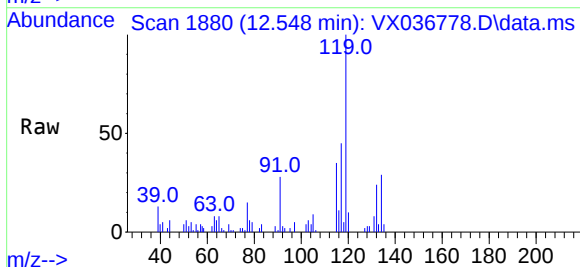



#95
Naphthalene
Concen: 1189.756 ug/l
RT: 13.780 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX036778.D
Acq: 02 Aug 2023 18:17

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-2-(0-5)

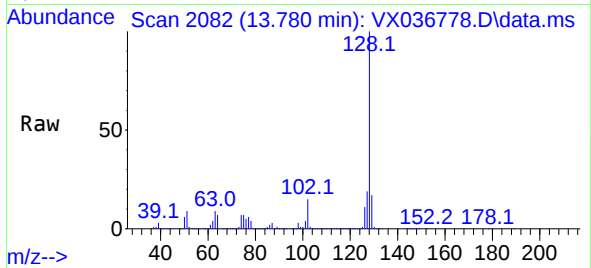

Tgt Ion:128 Resp: 8733885
Ion Ratio Lower Upper
128 100
127 16.9 10.3 15.5#
129 14.7 8.8 13.2#

