

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080223\
 Data File : VX036781.D
 Acq On : 02 Aug 2023 19:29
 Operator : JC/MD
 Sample : 03872-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50107

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.568	558	571	586	rBV2	10115	33142	4.55%	0.785%
2	5.385	695	705	721	rBV	83164	245437	33.67%	5.816%
3	5.550	721	732	751	rVB	136394	385498	52.89%	9.135%
4	5.958	789	799	816	rBV2	90339	242913	33.32%	5.756%
5	6.763	921	931	945	rBV	223907	531945	72.98%	12.605%
6	8.647	1233	1240	1250	rBV	459098	728922	100.00%	17.272%
7	8.964	1287	1292	1300	rBV3	4215	7476	1.03%	0.177%
8	10.055	1465	1471	1485	rBV	464821	646437	88.68%	15.318%
9	11.079	1634	1639	1651	rBV	396892	500099	68.61%	11.850%
10	12.024	1788	1794	1803	rBV	467777	615668	84.46%	14.589%
11	12.817	1907	1924	1925	rBV3	21283	63731	8.74%	1.510%
12	13.774	2075	2081	2090	rBV	22060	32276	4.43%	0.765%
13	14.134	2132	2140	2149	rVB5	2911	9274	1.27%	0.220%
14	14.634	2218	2222	2234	rVB	26714	36453	5.00%	0.864%
15	14.780	2239	2246	2252	rVB	18642	25614	3.51%	0.607%
16	15.207	2309	2316	2322	rBV	9340	13635	1.87%	0.323%
17	15.475	2354	2360	2370	rBV3	10717	20068	2.75%	0.476%
18	15.615	2372	2383	2386	rVV	14213	26540	3.64%	0.629%
19	15.646	2386	2388	2394	rVV3	7767	11385	1.56%	0.270%
20	15.835	2411	2419	2427	rVB5	4238	10851	1.49%	0.257%
21	16.091	2454	2461	2467	rBV3	12304	21342	2.93%	0.506%
22	16.322	2490	2499	2507	rBV5	4975	11519	1.58%	0.273%


Sum of corrected areas: 4220225

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080223\
Data File : VX036781.D
Acq On : 02 Aug 2023 19:29
Operator : JC/MD
Sample : 03872-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

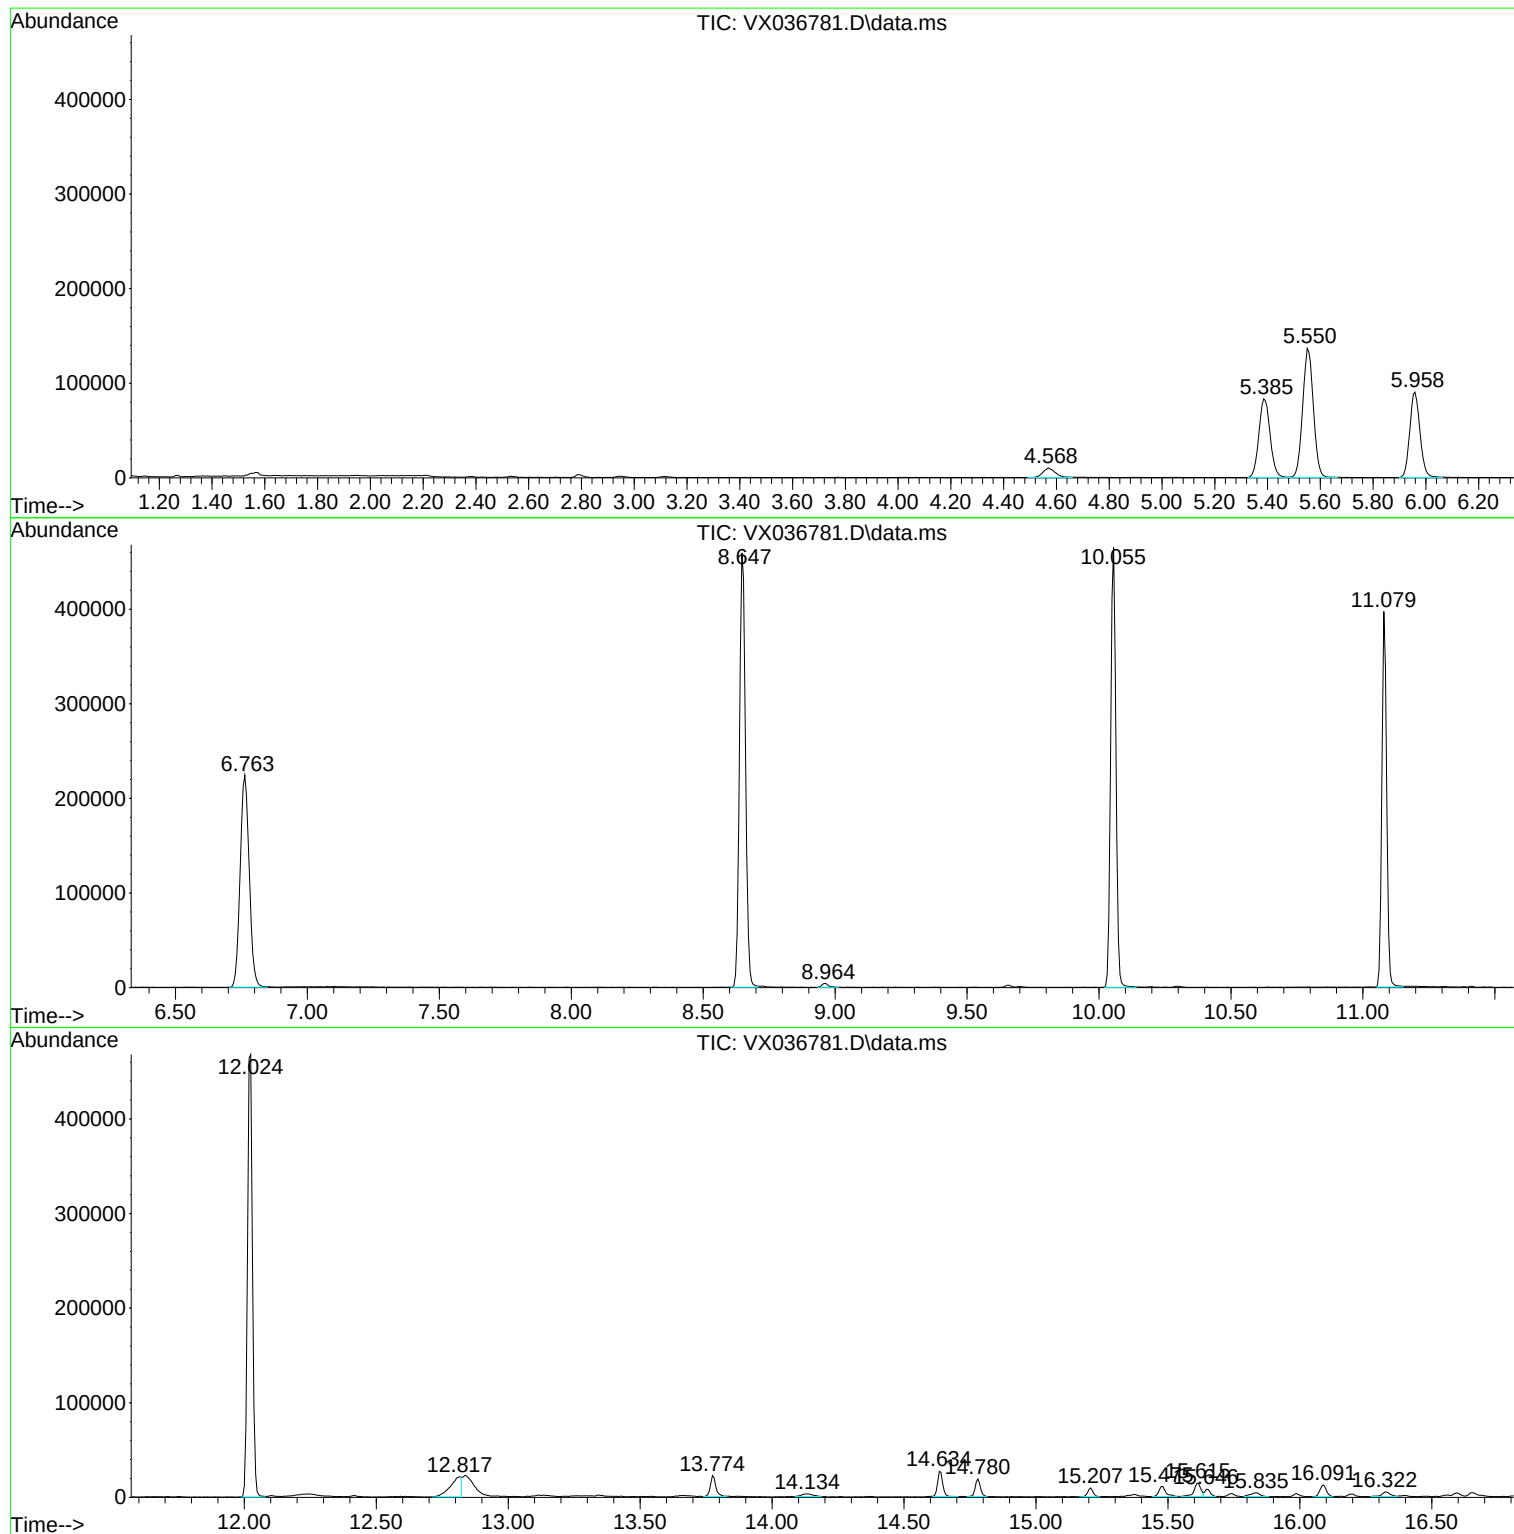

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080223\
Data File : VX036781.D
Acq On : 02 Aug 2023 19:29
Operator : JC/MD
Sample : 03872-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50107










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.817	5.18 ug/l	63731	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorene	166	C13H10	000086-73-7	97
2			1,3-Benzodioxole-5-carboxylic acid	166	C8H6O4	000094-53-1	59
3			1H-Phenylene	166	C13H10	000203-80-5	53
4			3-Trifluoromethylbenzhydryl chlo...	270	C14H10ClF3	067240-79-3	40
5			Ethionamide	166	C8H10N2S	000536-33-4	39

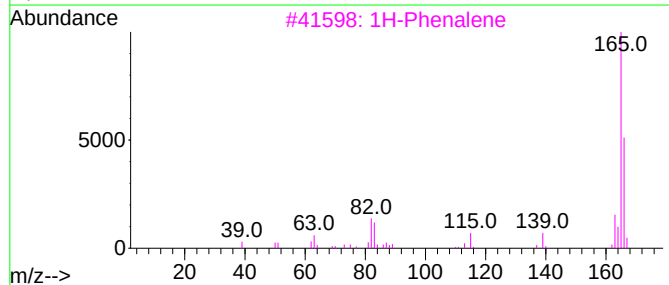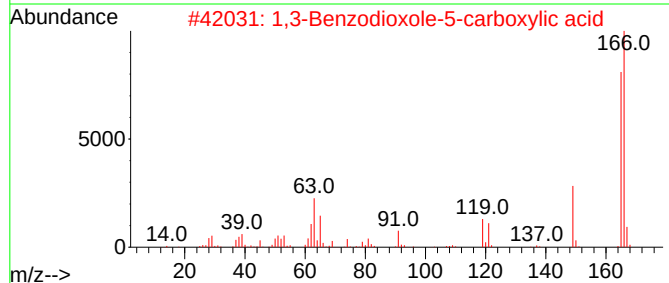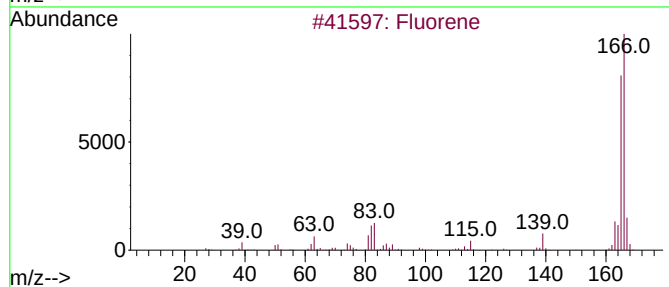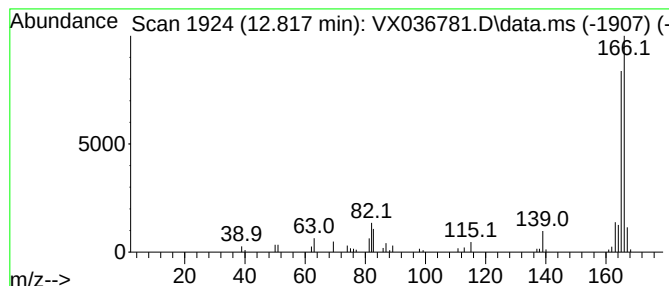

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080223\
Data File : VX036781.D
Acq On : 02 Aug 2023 19:29
Operator : JC/MD
Sample : 03872-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorene	12.817	5.2	ug/l	63731	4	12.024	615668	50.0