
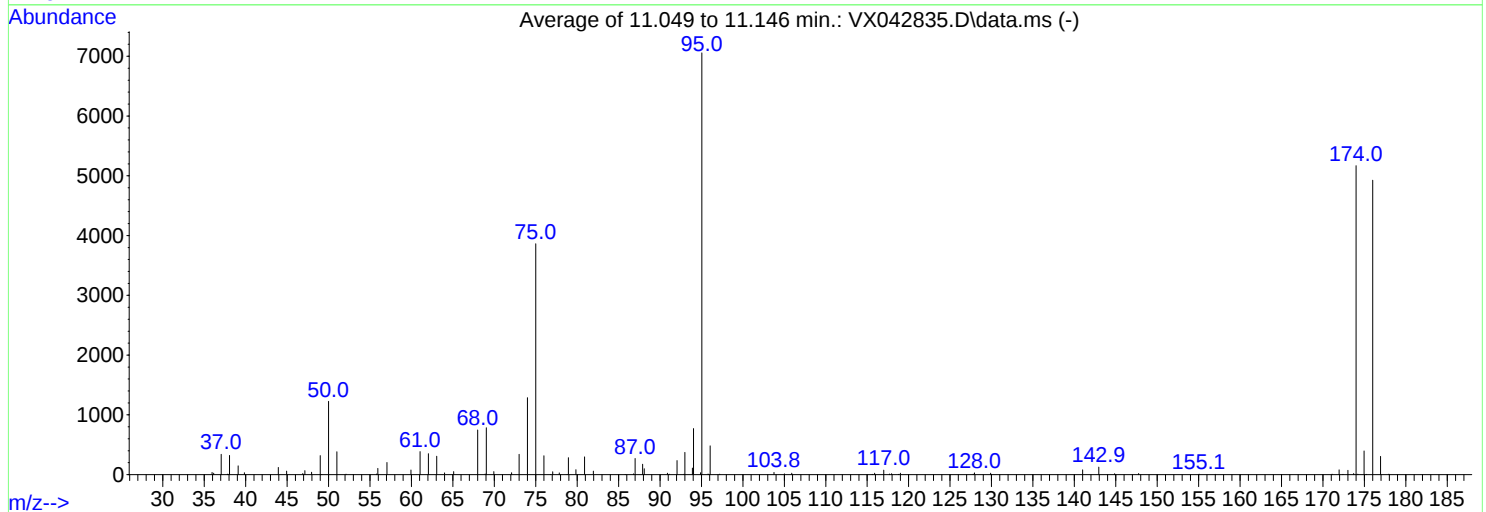


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080224\
Data File : VX042835.D
Acq On : 02 Aug 2024 11:21
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080224W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Aug 02 21:32:14 2024

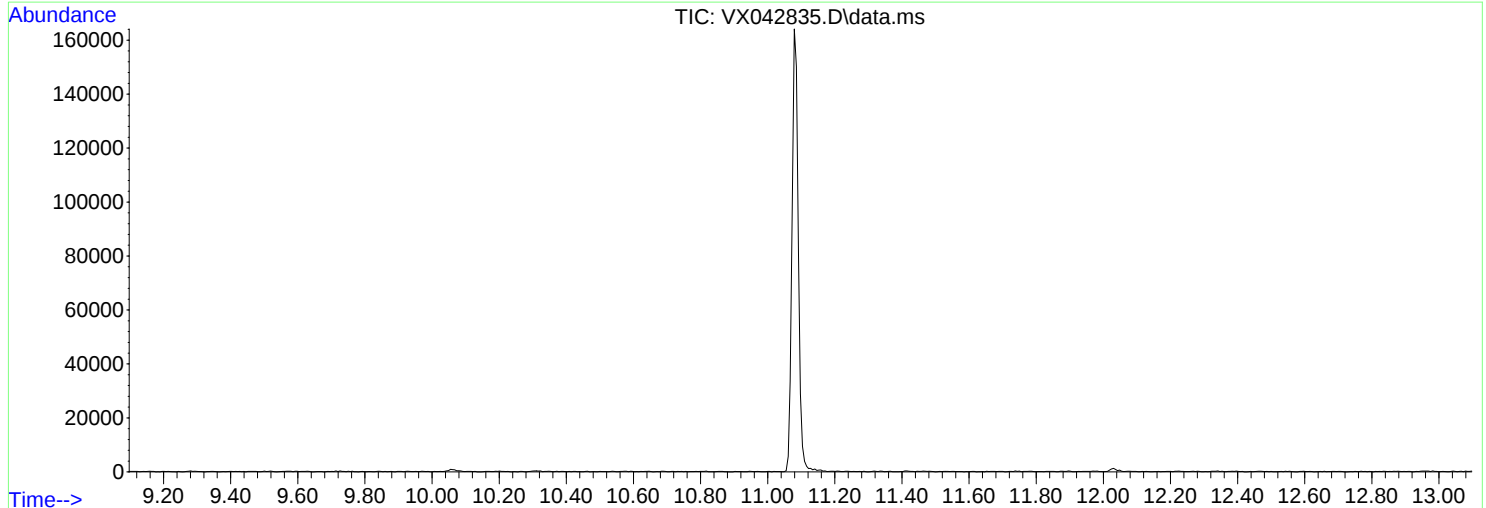

AutoFind: Averaged scan 1634 to 1650; Bkg corrected with scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	1226	PASS
75	95	30	60	54.8	3864	PASS
95	95	100	100	100.0	7057	PASS
96	95	5	9	6.8	483	PASS
173	174	0.00	2	1.4	73	PASS
174	95	50	100	73.2	5169	PASS
175	174	5	9	7.7	397	PASS
176	174	95	101	95.3	4925	PASS
177	176	5	9	6.2	306	PASS