


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080318\
 Data File : VX003830.D
 Acq On : 02 Aug 2018 18:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080318W.M
 Title : SW846 8260
 Last Update : Fri Aug 03 01:55:28 2018

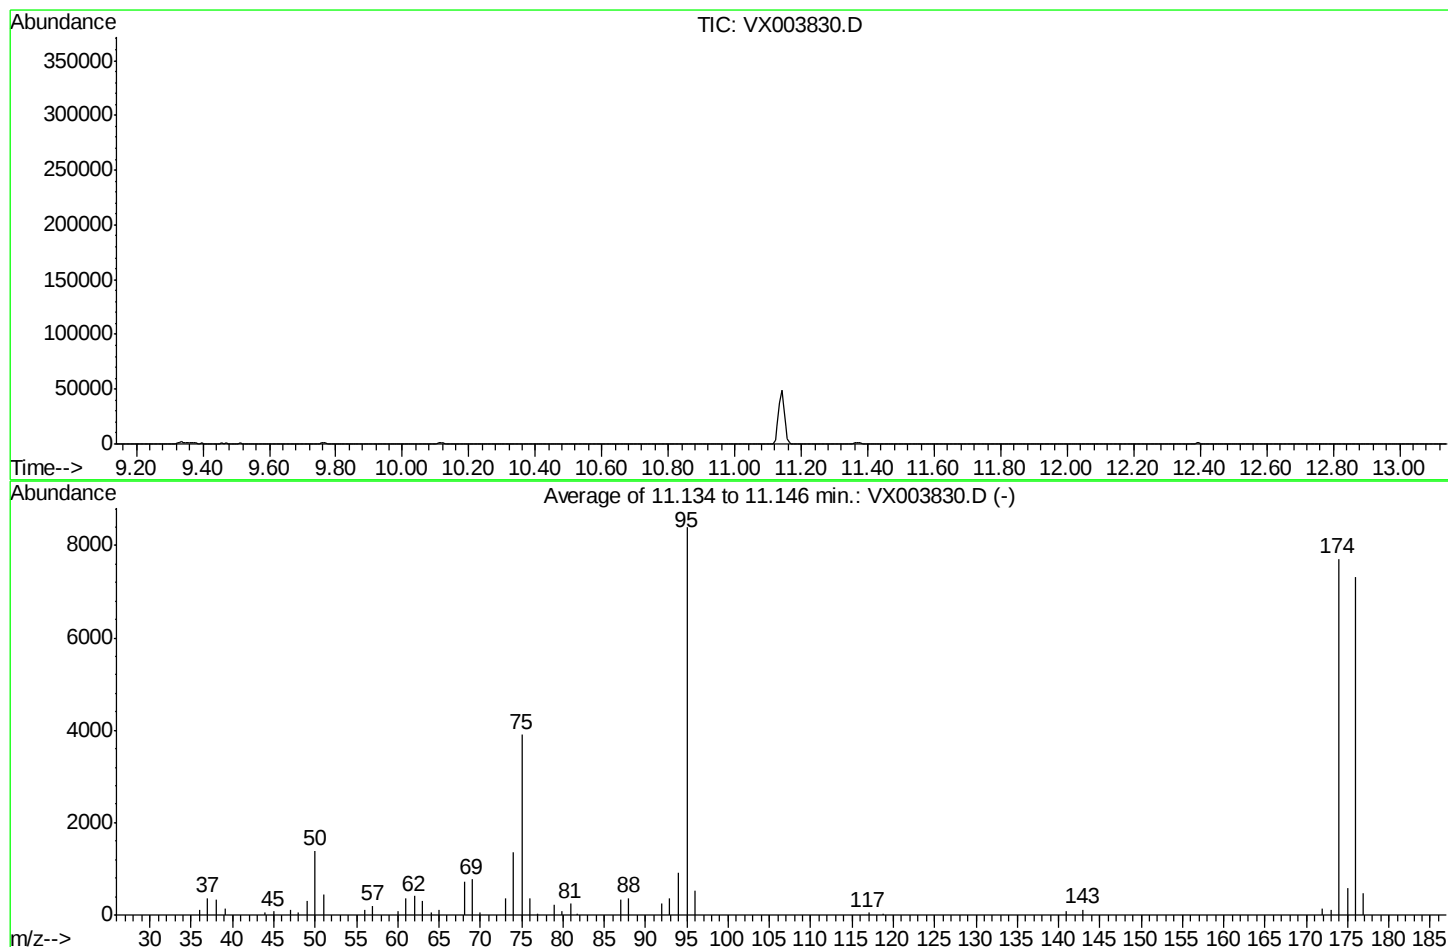

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	1388	PASS
75	95	30	60	46.5	3899	PASS
95	95	100	100	100.0	8393	PASS
96	95	5	9	6.3	531	PASS
173	174	0.00	2	1.3	100	PASS
174	95	50	100	91.9	7710	PASS
175	174	5	9	7.7	594	PASS
176	174	95	101	95.0	7323	PASS
177	176	5	9	6.4	472	PASS