

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080320\
 Data File : VX017749.D
 Acq On : 03 Aug 2020 16:32
 Operator : JC/SP
 Sample : L3526-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB179-GW-278-280

Quant Time: Aug 04 06:55:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	605762	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	897789	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	820785	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	405939	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.04	65	388629	49.94	ug/l	0.00
Spiked Amount			Recovery	=	99.88%	
35) Dibromofluoromethane	5.46	113	302744	50.42	ug/l	0.00
Spiked Amount			Recovery	=	100.84%	
50) Toluene-d8	8.70	98	1040417	48.03	ug/l	0.00
Spiked Amount			Recovery	=	96.06%	
62) 4-Bromofluorobenzene	11.12	95	399234	46.05	ug/l	0.00
Spiked Amount			Recovery	=	92.10%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.19	85	673	Below Cal	#	42
3) Chloromethane	1.32	50	2002	0.632	ug/l #	69
5) Bromomethane	1.62	94	322	Below Cal	#	3
6) Chloroethane	1.72	64	225	Below Cal	#	76
8) Diethyl Ether	2.22	74	427	Below Cal		72
11) Tert butyl alcohol	3.00	59	778	0.474	ug/l #	1
12) 1,1-Dichloroethene	2.36	96	5146	0.822	ug/l	87
13) Acrolein	2.27	56	751	4.738	ug/l #	81
16) Acetone	2.42	43	21458	6.265	ug/l #	81
19) Methyl tert-butyl Ether	3.17	73	25204	1.164	ug/l	96
20) Methylene Chloride	2.83	84	1253	Below Cal	#	61
24) 1,1-Dichloroethane	3.68	63	5188	0.431	ug/l #	81
25) 2-Butanone	4.65	43	5870	1.207	ug/l #	85
27) cis-1,2-Dichloroethene	4.57	96	60442	8.302	ug/l	88
31) Cyclohexane	5.64	56	13151	1.370	ug/l #	1
32) 1,1,1-Trichloroethane	5.46	97	6032	0.520	ug/l #	40
36) 1,1-Dichloropropene	5.64	75	45744	5.313	ug/l #	52
38) Carbon Tetrachloride	5.63	117	62522	5.979	ug/l #	17
44) Trichloroethene	7.19	130	386030	53.509	ug/l	94
49) 1,4-Dioxane	7.72	88	177	1.198	ug/l #	1
59) 2-Hexanone	9.48	43	1950	0.279	ug/l	75
60) Dibromochloromethane	9.32	129	29275	3.492	ug/l #	12
64) Tetrachloroethene	9.32	164	30331	4.117	ug/l	99
76) 1,2,3-Trichloropropane	11.12	75	198986	23.830	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.12	75	198986	60.045	ug/l #	12
92) 1,2-Dibromo-3-Chloropropan	12.99	75	392	2.728	ug/l #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080320\
Data File : VX017749.D
Acq On : 03 Aug 2020 16:32
Operator : JC/SP
Sample : L3526-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB179-GW-278-280

Quant Time: Aug 04 06:55:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 24 05:48:09 2020
Response via : Initial Calibration

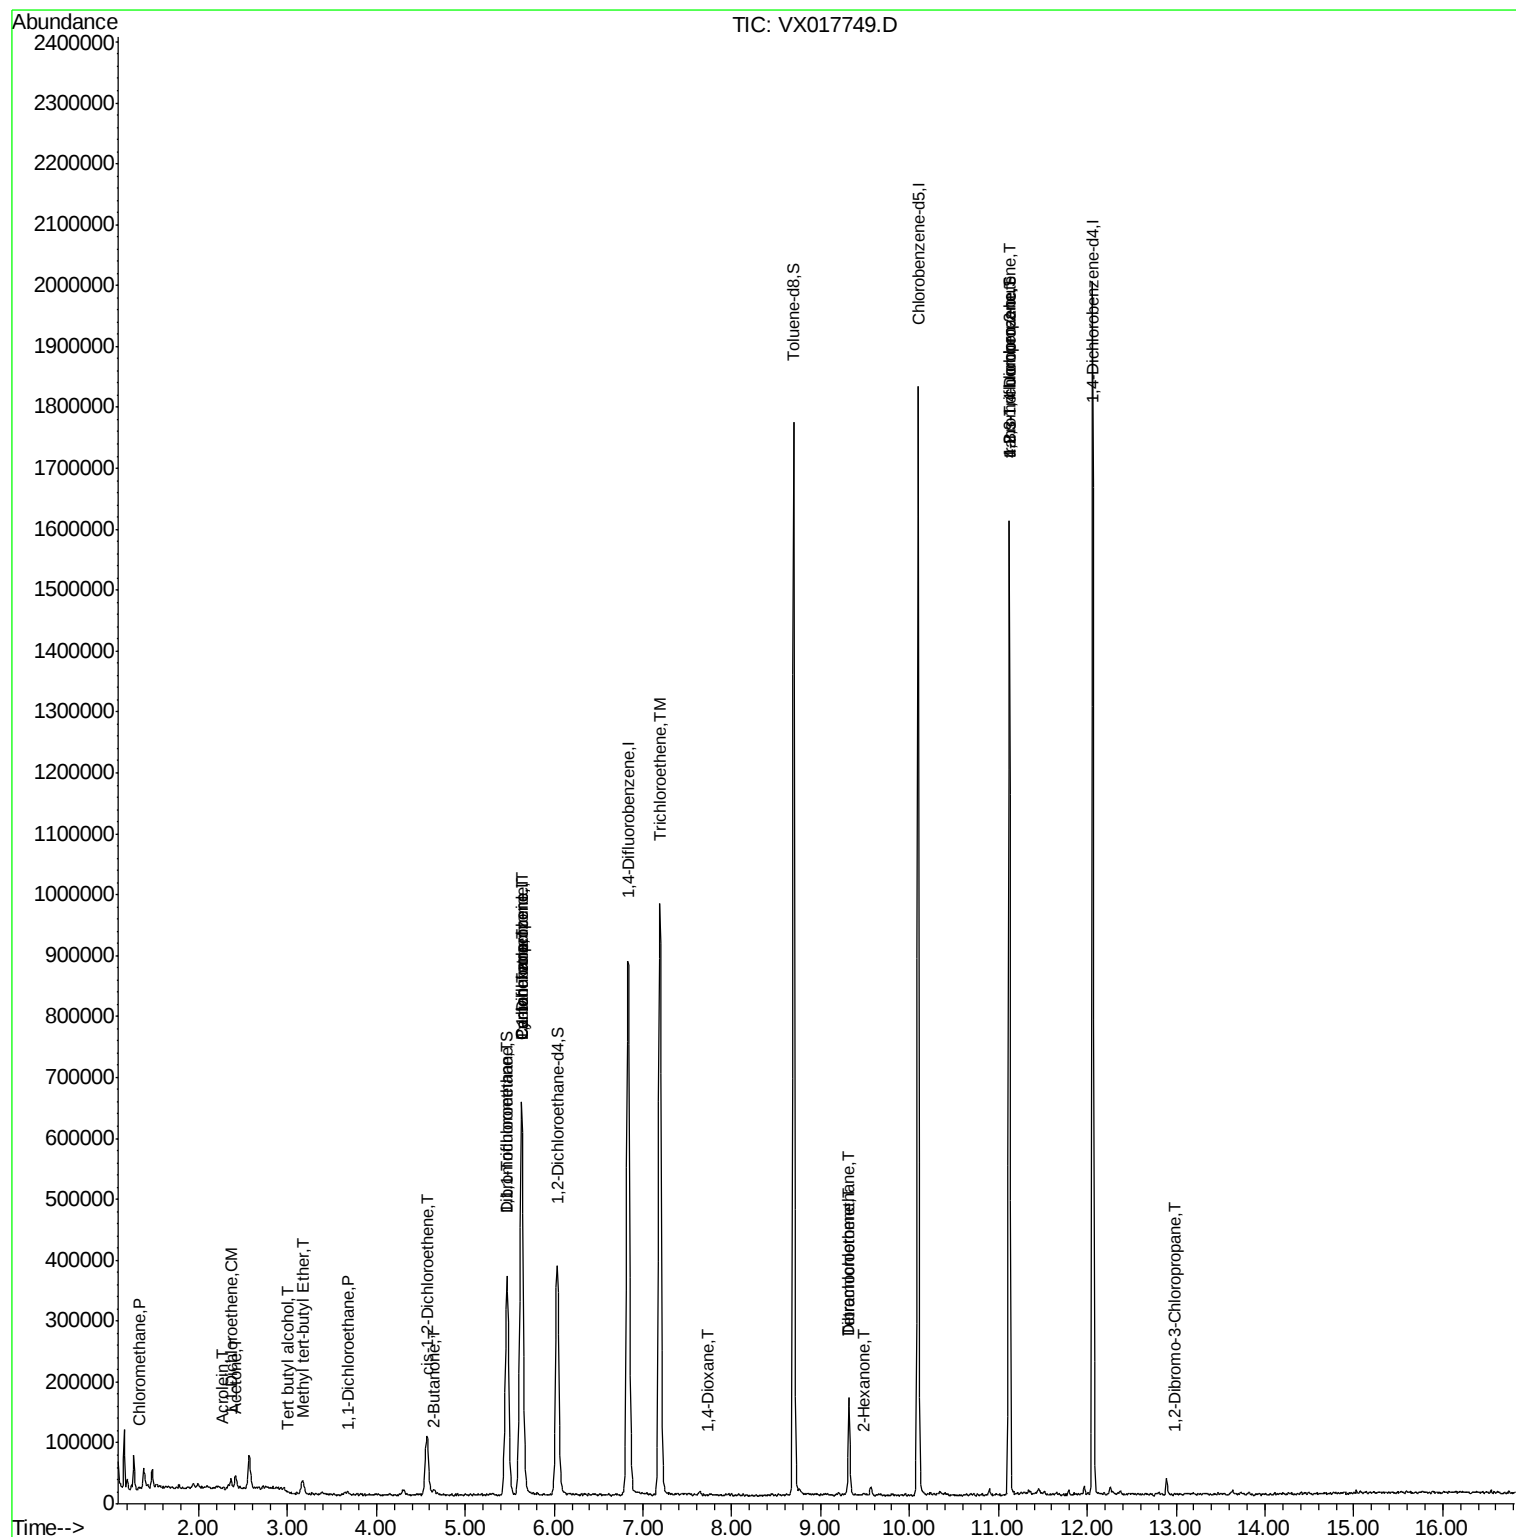



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.00 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB179-GW-278-280

Tot Ion:168 Resp: 605762

Ion Ratio Lower Upper

168 100

99 57.8 43.4 65.2

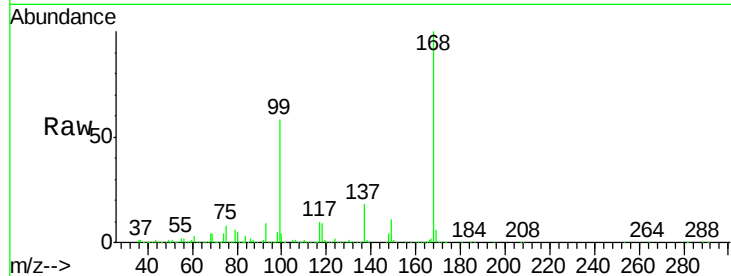

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

250000

200000



150000

100000

50000

0

Time-->

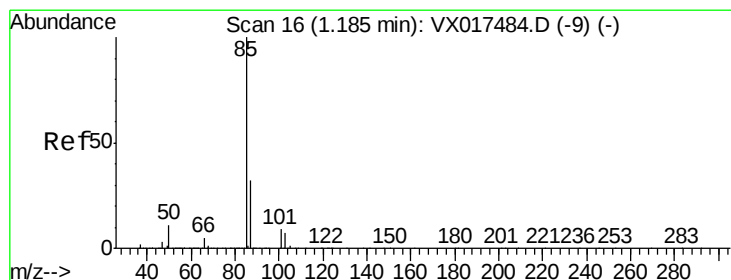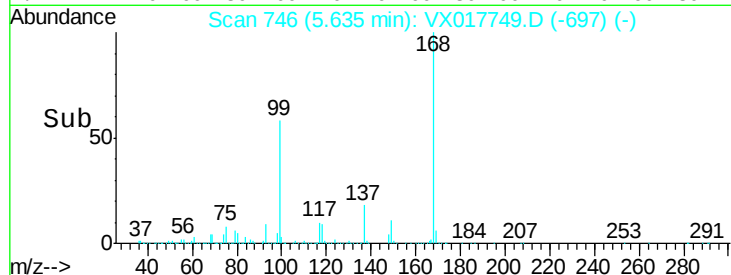

#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.19 min Scan# 17

Delta R.T. 0.01 min

Lab File: VX017749.D


Acq: 03 Aug 2020 16:32

Tgt Ion: 85 Resp: 673

Ion Ratio Lower Upper

85 100

87 0.0 16.1 48.3#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.19

600

500

400


300


200

100

0

Time-->



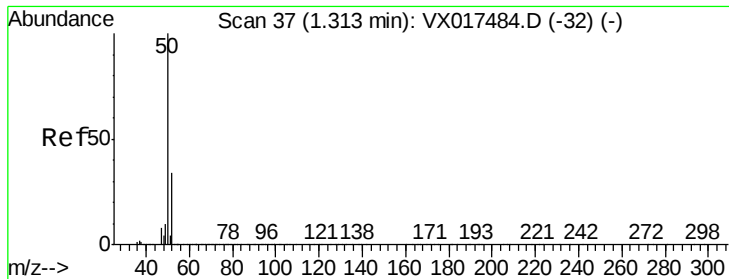

#3

Chloromethane

Concen: 0.632 ug/l

RT: 1.32 min Scan# 38

Delta R.T. 0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB179-GW-278-280

Tot Ion: 50 Resp: 2002

Ion Ratio Lower Upper

50 100

52 49.9 25.9 38.9#

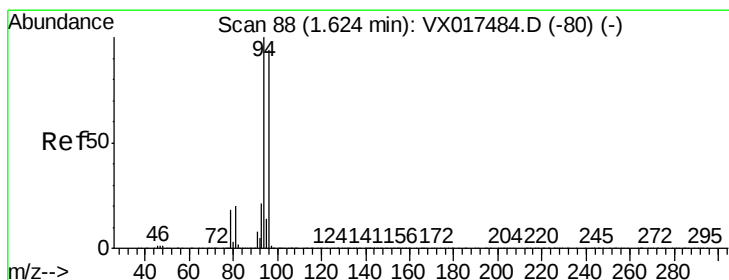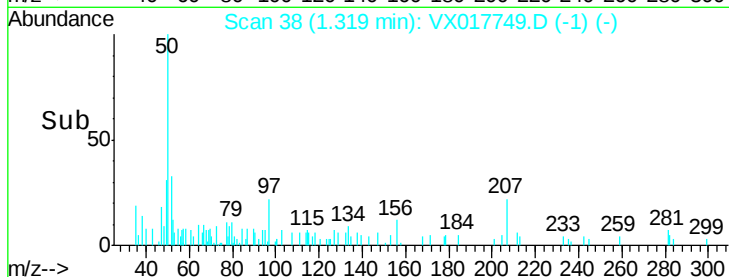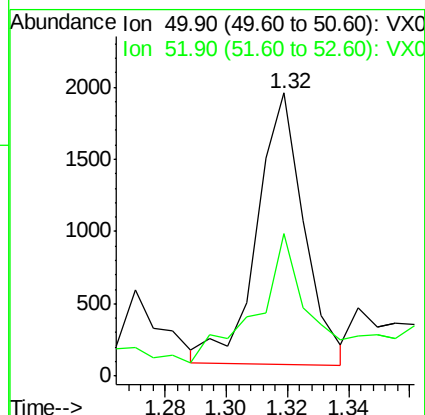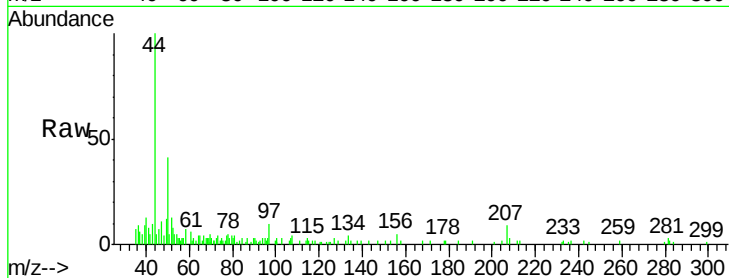

#5

Bromomethane

Concen: Below Cal

RT: 1.62 min Scan# 87

Delta R.T. -0.01 min

Lab File: VX017749.D




Acq: 03 Aug 2020 16:32


Tgt Ion: 94 Resp: 322

Ion Ratio Lower Upper

94 100

96 0.0 74.1 111.1#

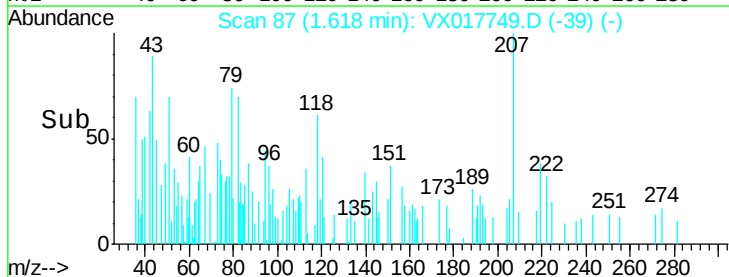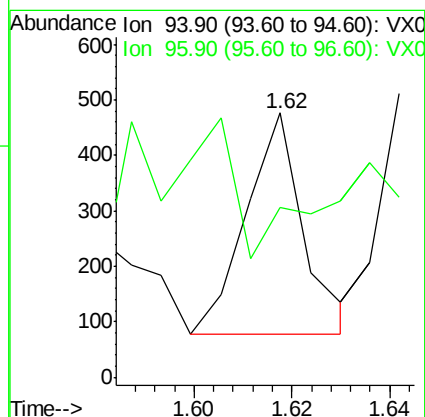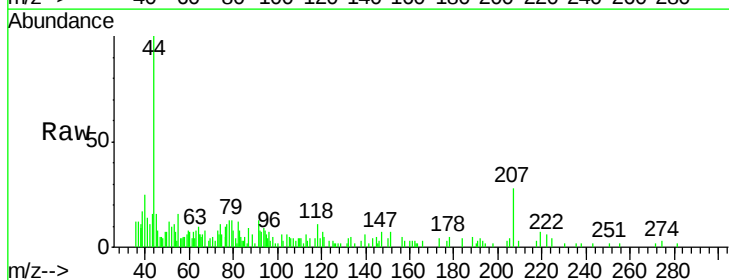



#6

Chloroethane

Concen: Below Cal

RT: 1.72 min Scan# 104

Delta R.T. 0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB179-GW-278-280

Tot Ion: 64 Resp: 225

Ion Ratio Lower Upper

64 100

66 17.9 24.9 37.3#

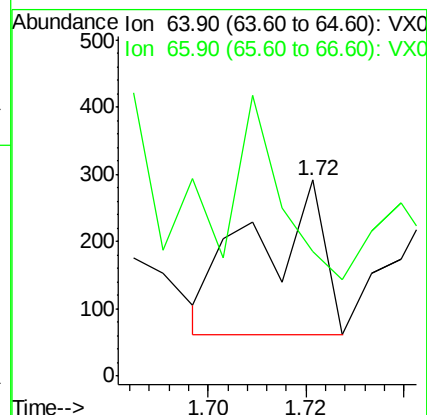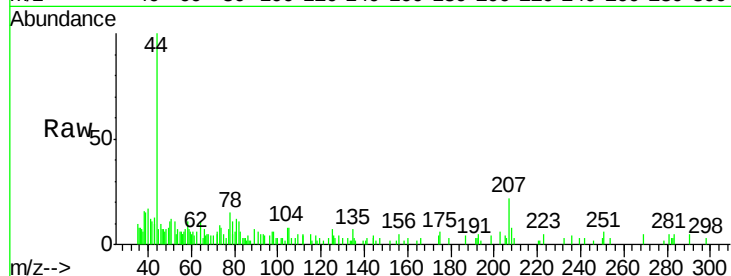

#8

Diethyl Ether

Concen: Below Cal

RT: 2.22 min Scan# 185

Delta R.T. 0.05 min

Lab File: VX017749.D




Acq: 03 Aug 2020 16:32


Tgt Ion: 74 Resp: 427

Ion Ratio Lower Upper

74 100

45 73.1 50.8 152.5

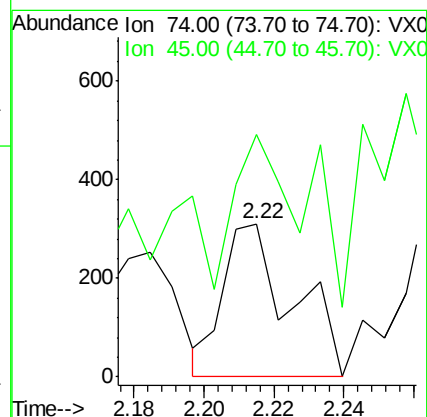







#11

Tert butyl alcohol
Concen: 0.474 ug/l
RT: 3.00 min Scan# 313
Delta R.T. -0.02 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB179-GW-278-280




Tot Ion: 59 Resp: 778
Ion Ratio Lower Upper
59 100
57 51.9 8.6 12.8#

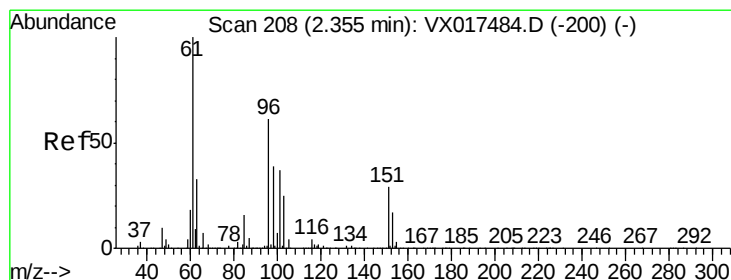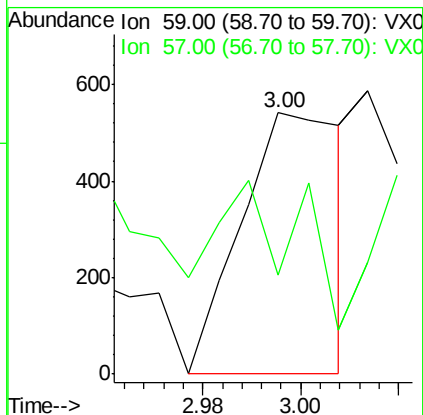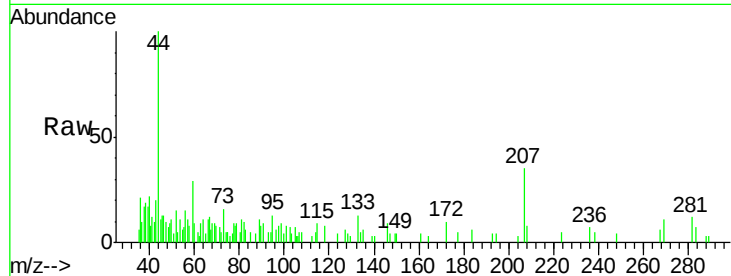


#12

1,1-Dichloroethene
Concen: 0.822 ug/l
RT: 2.36 min Scan# 209
Delta R.T. 0.01 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Tgt Ion: 96 Resp: 5146
Ion Ratio Lower Upper
96 100
61 150.3 134.0 201.0
98 52.9 51.0 76.4

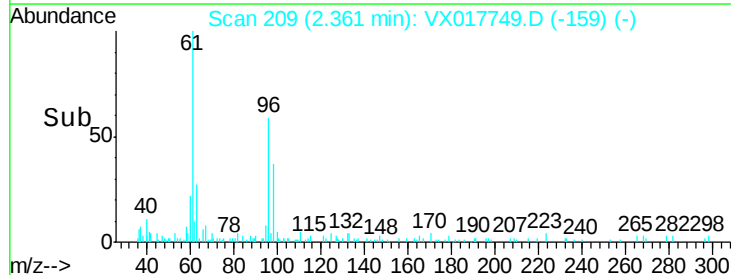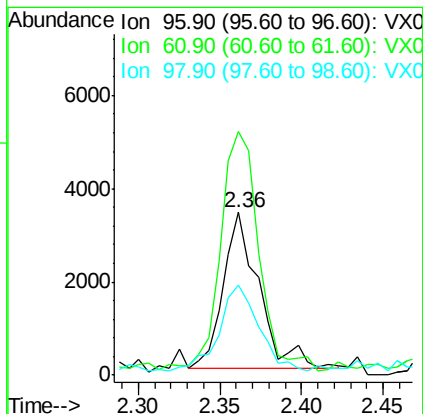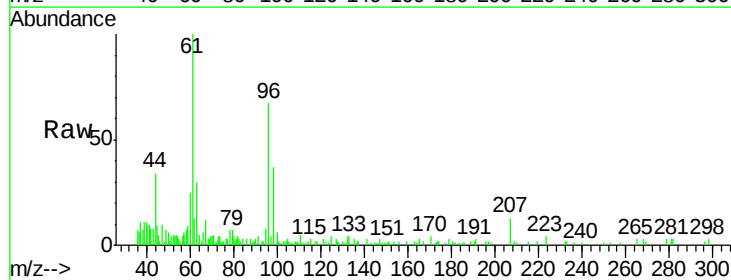



#13

Acrolein

Concen: 4.738 ug/l

RT: 2.27 min Scan# 194

Delta R.T. -0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB179-GW-278-280

Tot Ion: 56 Resp: 751

Ion Ratio Lower Upper

56 100

55 87.5 57.4 86.2#

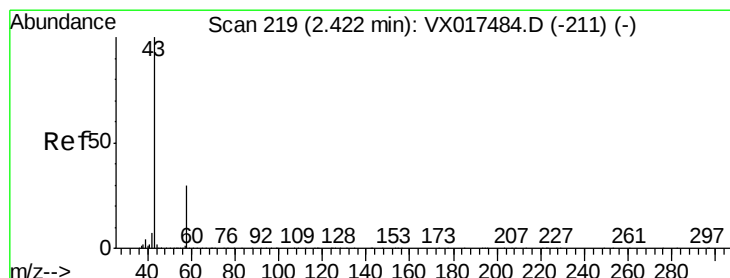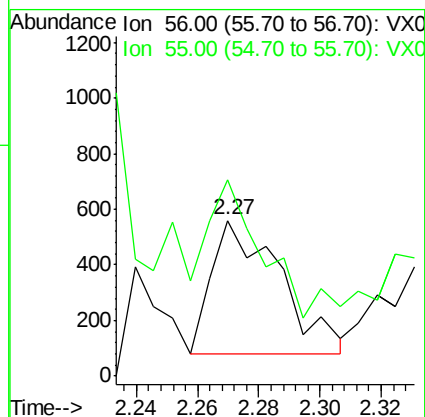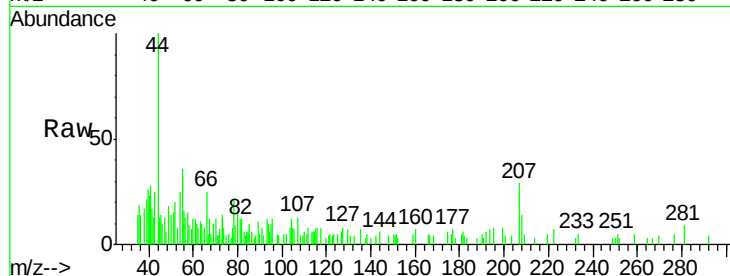

#16

Acetone

Concen: 6.265 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.01 min

Lab File: VX017749.D




Acq: 03 Aug 2020 16:32


Tgt Ion: 43 Resp: 21458

Ion Ratio Lower Upper

43 100

58 20.0 24.2 36.4#



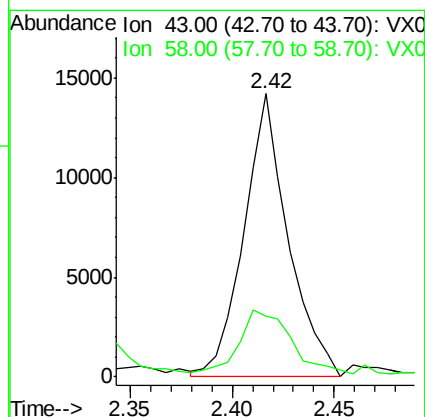
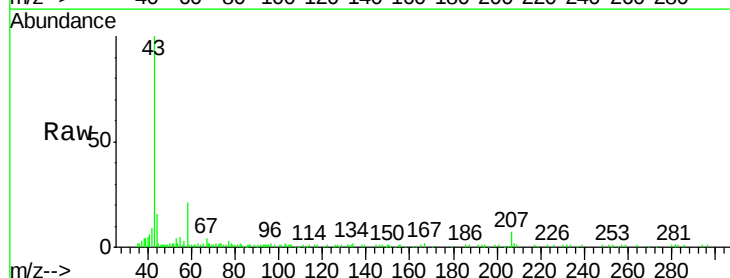




#19
Methvl tert-butvl Ether
Concen: 1.164 ug/l
RT: 3.17 min Scan# 342
Delta R.T. -0.00 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB179-GW-278-280


Tot Ion: 73 Resp: 25204
Ion Ratio Lower Upper
73 100
57 23.0 17.0 25.4

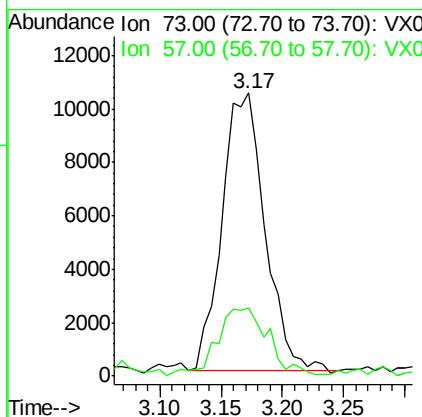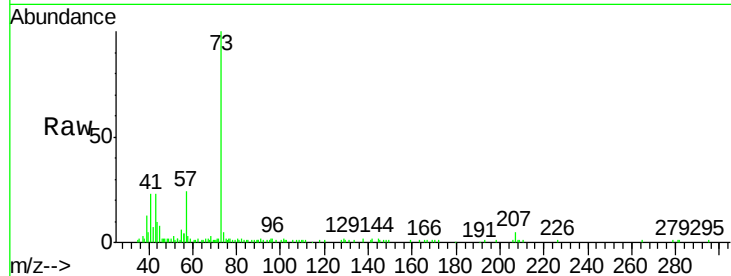

#20
Methylene Chloride
Concen: Below Cal
RT: 2.83 min Scan# 286
Delta R.T. -0.01 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Tgt Ion: 84 Resp: 1253
Ion Ratio Lower Upper
84 100
49 50.3 100.3 150.5#
51 40.7 30.5 45.7
86 59.3 51.1 76.7

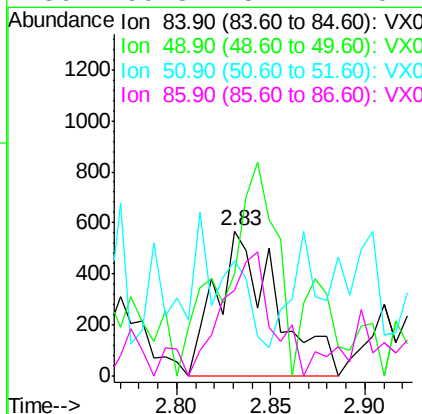



#24

1,1-Dichloroethane

Concen: 0.431 ug/l

RT: 3.68 min Scan# 425

Delta R.T. 0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB179-GW-278-280


Tot Ion: 63 Resp: 5188

Ion Ratio Lower Upper

63 100

98 11.6 3.4 10.1#




100 12.6 1.9 5.7#

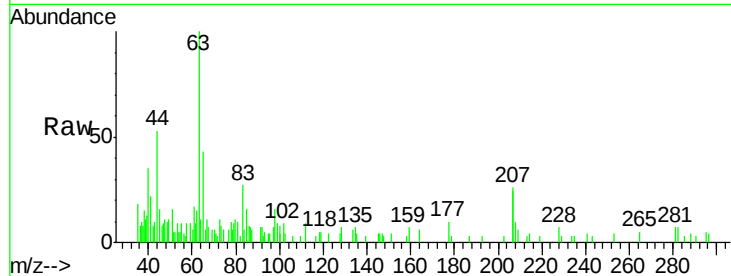

Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

Ion 99.90 (99.60 to 100.60): VX0

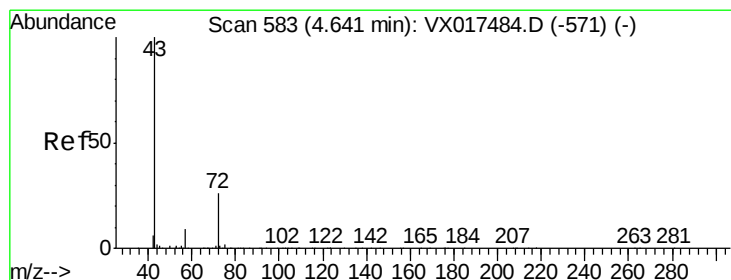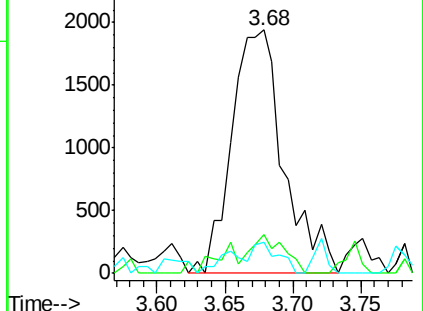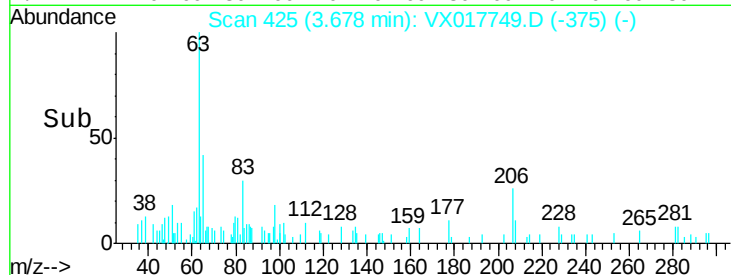

#25

2-Butanone

Concen: 1.207 ug/l

RT: 4.65 min Scan# 584

Delta R.T. 0.01 min

Lab File: VX017749.D


Acq: 03 Aug 2020 16:32

Tgt Ion: 43 Resp: 5870

Ion Ratio Lower Upper



43 100


72 31.0 19.0 28.4#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

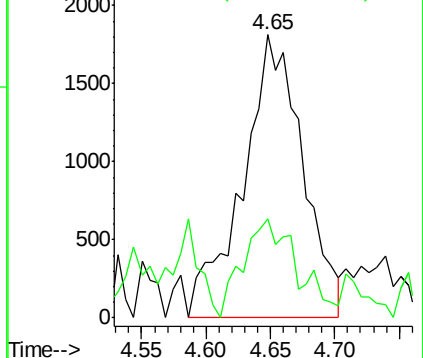







#27

cis-1,2-Dichloroethene
Concen: 8.302 ug/l
RT: 4.57 min Scan# 571
Delta R.T. -0.00 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB179-GW-278-280




Tot Ion: 96 Resp: 60442
Ion Ratio Lower Upper
96 100
61 128.9 0.0 301.2
98 65.9 0.0 130.0

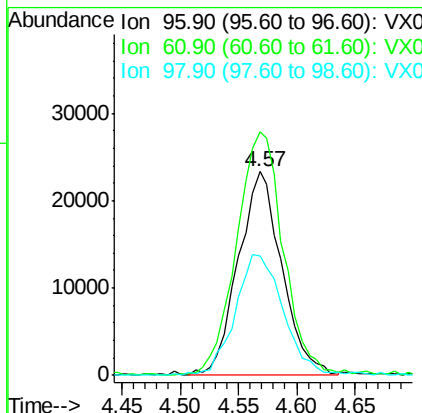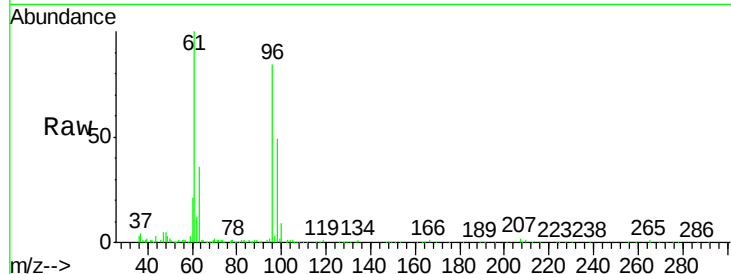


#31

Cyclohexane
Concen: 1.370 ug/l
RT: 5.64 min Scan# 746
Delta R.T. 0.08 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Tgt Ion: 56 Resp: 13151
Ion Ratio Lower Upper
56 100
69 190.2 24.2 36.4#
84 127.2 69.0 103.6#

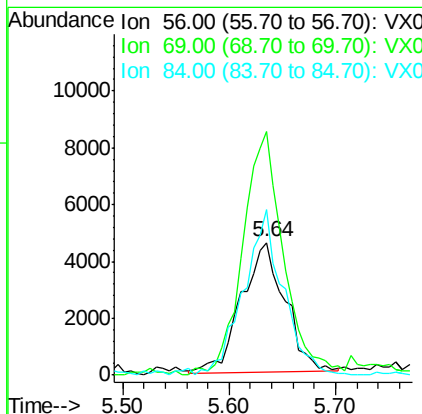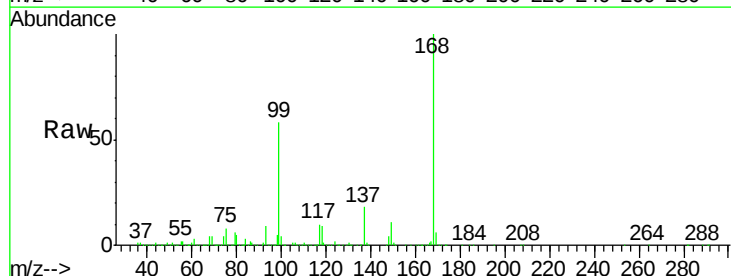



#32

1,1,1-Trichloroethane

Concen: 0.520 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB179-GW-278-280





Tot Ion: 97 Resp: 6032

Ion Ratio Lower Upper

97 100

99 0.0 51.9 77.9#

61 59.6 34.1 51.1#

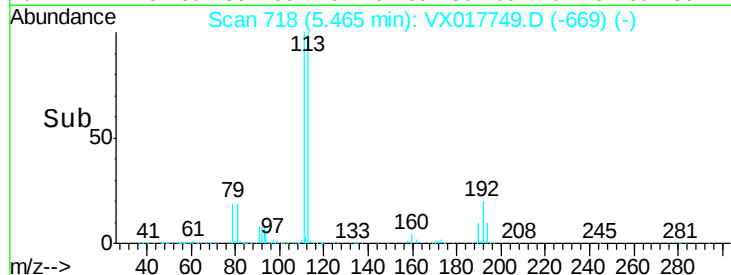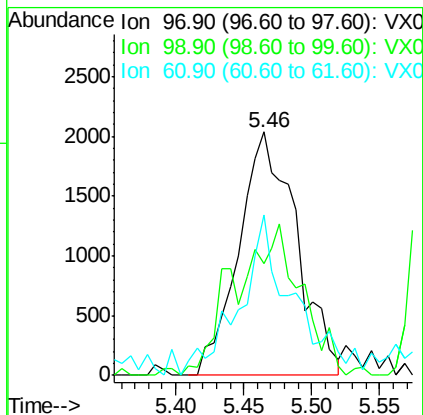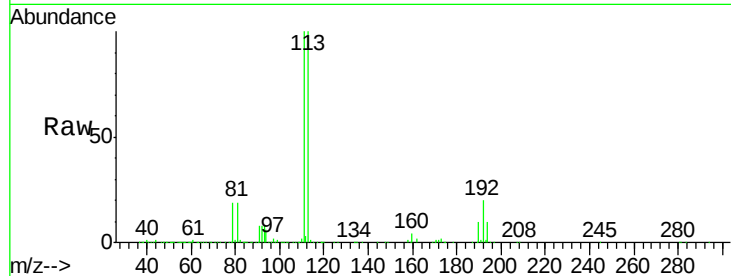

#33

1,2-Dichloroethane-d4

Concen: 49.944 ug/l

RT: 6.04 min Scan# 812

Delta R.T. 0.01 min

Lab File: VX017749.D




Acq: 03 Aug 2020 16:32


Tgt Ion: 65 Resp: 388629

Ion Ratio Lower Upper

65 100

67 50.4 0.0 102.8

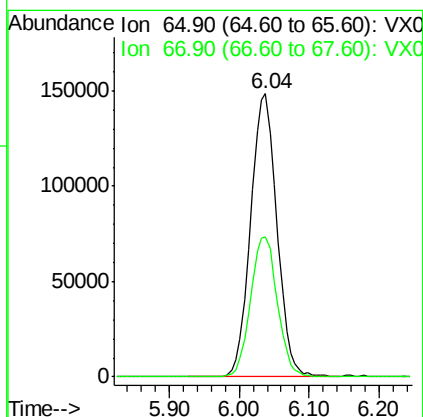



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB179-GW-278-280



Tot Ion:114 Resp: 897789

Ion Ratio Lower Upper

114 100

63 20.7 0.0 40.6

88 15.6 0.0 33.4

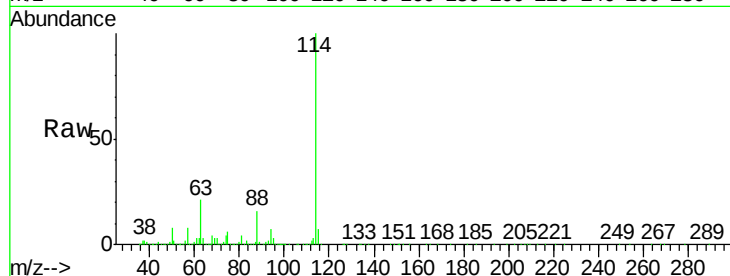

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.83

400000


300000

200000

100000

0

Time-->

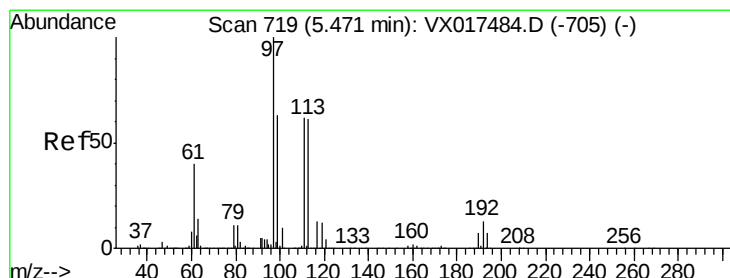

#35

Dibromofluoromethane

Concen: 50.420 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32



Tgt Ion:113 Resp: 302744

Ion Ratio Lower Upper

113 100

111 103.1 80.7 121.1

192 21.4 16.9 25.3

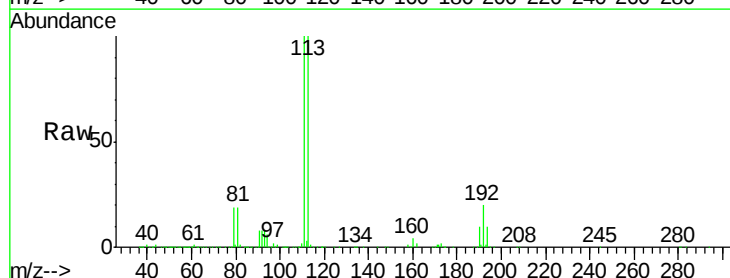

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

5.46


150000

100000

50000

0

Time-->



#36

1,1-Dichloropropene

Concen: 5.313 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.13 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB179-GW-278-280


Tot Ion: 75 Resp: 45744

Ion Ratio Lower Upper

75 100

110 11.5 18.1 54.3#




77 0.4 24.6 37.0#

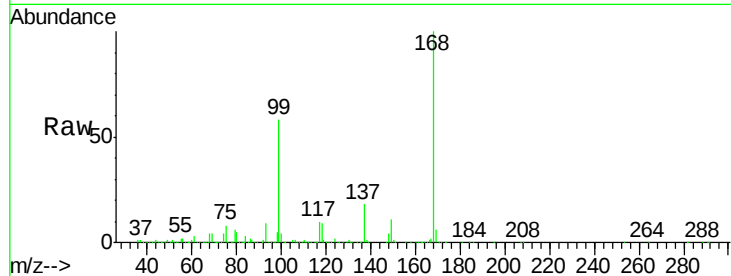

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

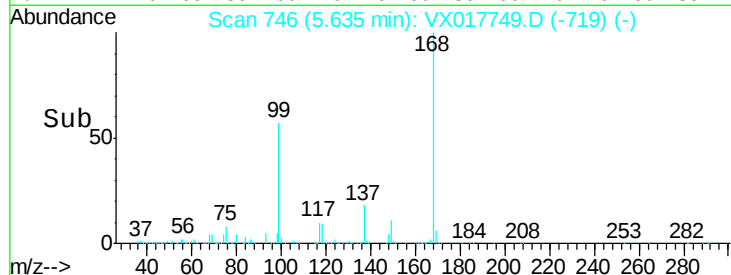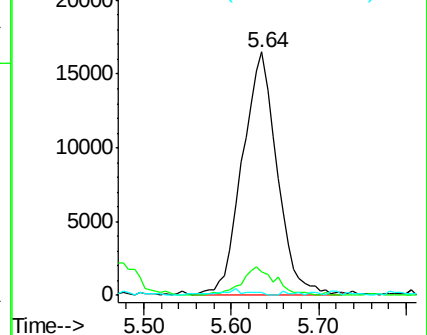

#38

Carbon Tetrachloride

Concen: 5.979 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32


Tgt Ion: 117 Resp: 62522

Ion Ratio Lower Upper

117 100

119 5.9 75.4 113.0#



121 0.0 24.3 36.5#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

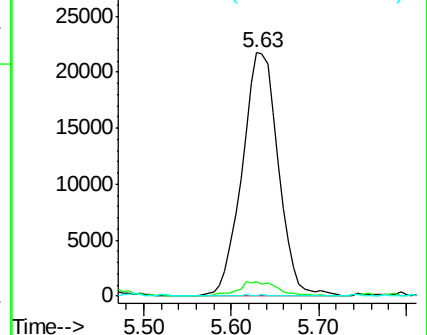



#44

Trichloroethene

Concen: 53.509 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. -0.00 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB179-GW-278-280

Tot Ion:130 Resp: 386030

Ion Ratio Lower Upper

130 100

95 100.2 0.0 189.0



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

7.19

200000



150000

100000

50000

0

Time-->



#49

1,4-Dioxane

Concen: 1.198 ug/l

RT: 7.72 min Scan# 1088

Delta R.T. 0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32


Tgt Ion: 88 Resp: 177

Ion Ratio Lower Upper

88 100

43 212.4 27.8 41.6#

58 0.0 58.3 87.5#



Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0


600


400

200

0

Time-->





#50

Toluene-d8

Concen: 48.032 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB179-GW-278-280

Tot Ion: 98 Resp: 1040417

Ion Ratio Lower Upper

98 100

100 65.0 52.3 78.5

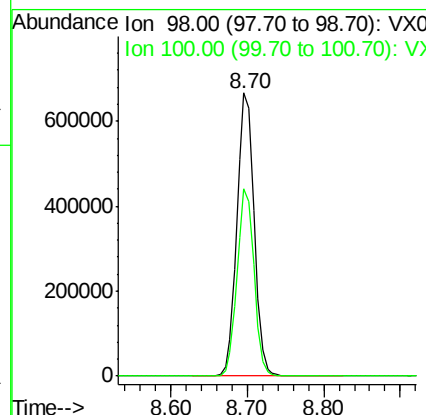

#59

2-Hexanone

Concen: 0.279 ug/l

RT: 9.48 min Scan# 1376

Delta R.T. -0.00 min

Lab File: VX017749.D




Acq: 03 Aug 2020 16:32


Tgt Ion: 43 Resp: 1950

Ion Ratio Lower Upper

43 100

58 35.6 26.6 79.8



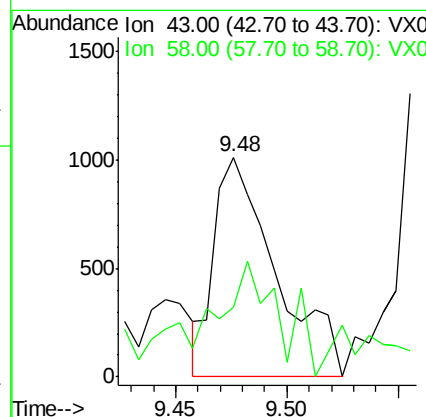





#60
Dibromochloromethane
Concen: 3.492 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.25 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB179-GW-278-280


Tot Ion:129 Resp: 29275
Ion Ratio Lower Upper
129 100
127 0.4 38.4 115.1#

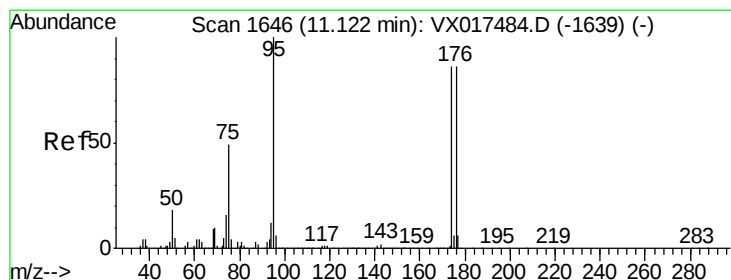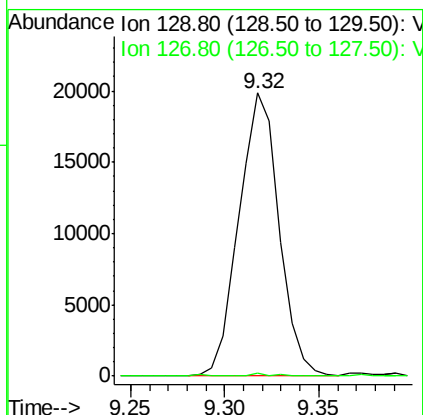

#62
4-Bromofluorobenzene
Concen: 46.054 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Tgt Ion: 95 Resp: 399234
Ion Ratio Lower Upper
95 100
174 82.4 0.0 169.0
176 77.9 0.0 161.0



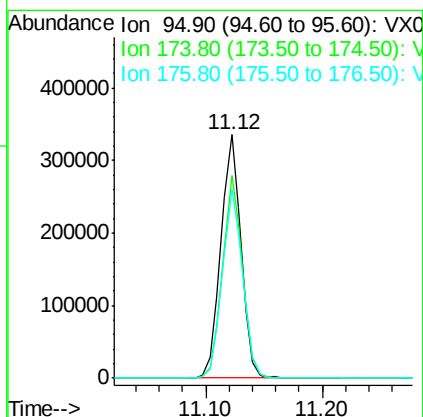
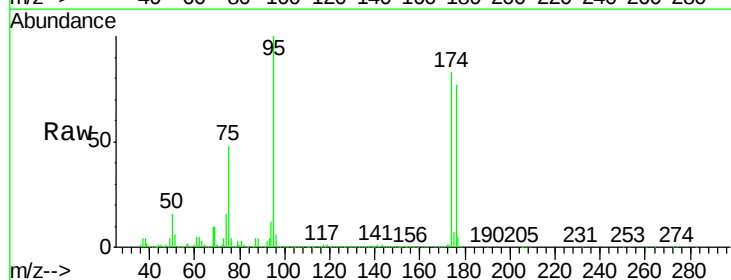


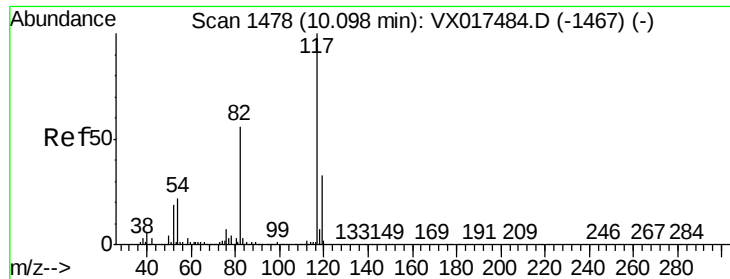

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB179-GW-278-280


Tot Ion	Ratio	Lower	Upper
117	100		
82	54.0	44.0	66.0
119	32.3	25.4	38.0

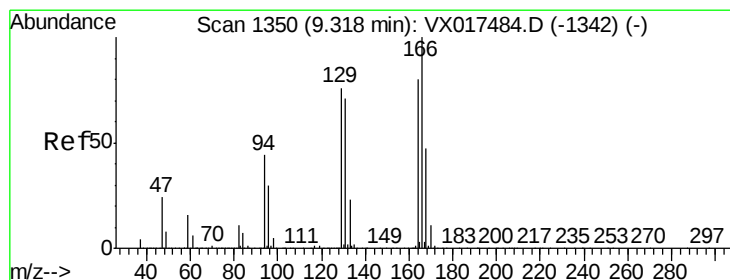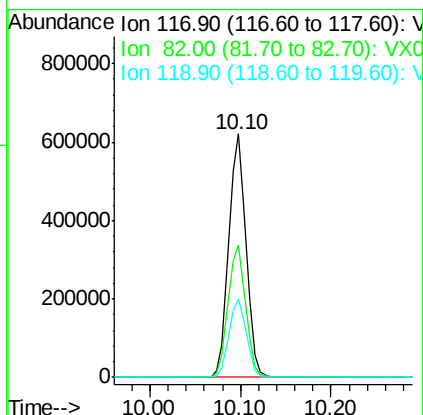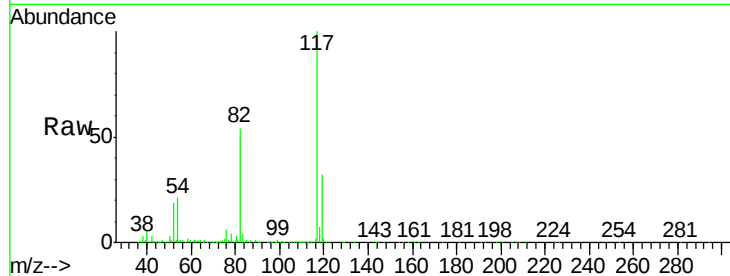

#64
Tetrachloroethene
Concen: 4.117 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX017749.D
Acq: 03 Aug 2020 16:32

Tgt Ion	Ratio	Lower	Upper
164	100		
166	125.1	100.6	150.8
129	95.5	75.0	112.6
131	95.1	75.2	112.8

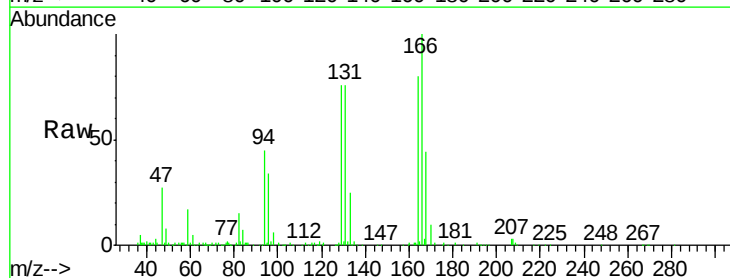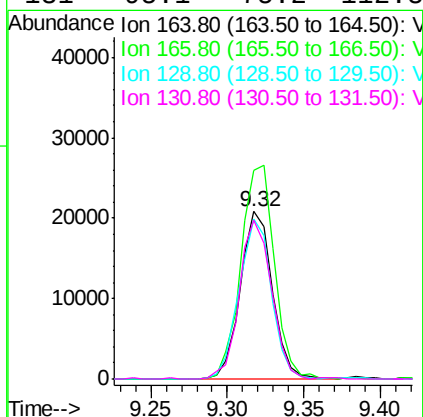



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB179-GW-278-280


Tot Ion:152 Resp: 405939

Ion Ratio Lower Upper

152 100

115 58.6 65.5 196.6#




150 156.0 0.0 412.6

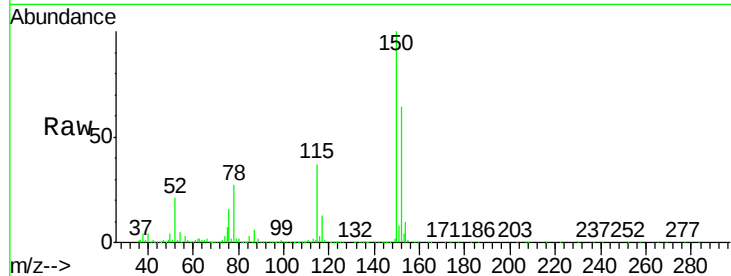

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

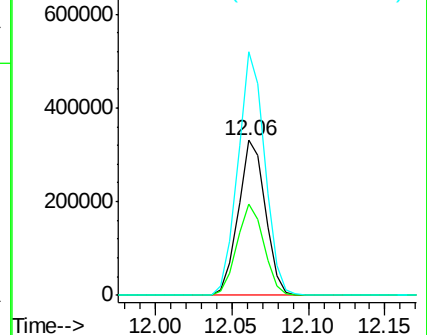

#76

1,2,3-Trichloropropane

Concen: 23.830 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017749.D


Acq: 03 Aug 2020 16:32

Tgt Ion: 75 Resp: 198986

Ion Ratio Lower Upper



75 100


77 1.5 21.8 65.3#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

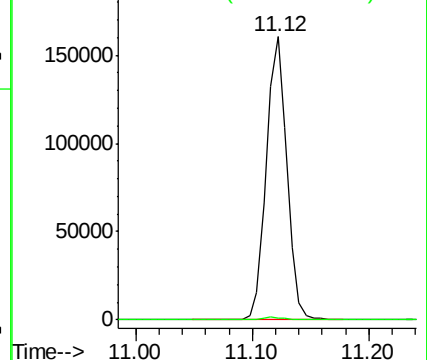



#81

trans-1,4-Dichloro-2-butene

Concen: 60.045 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB179-GW-278-280


Tot Ion: 75 Resp: 198986

Ion Ratio Lower Upper

75 100

53 0.4 75.9 113.9#




89 0.1 37.8 56.6#

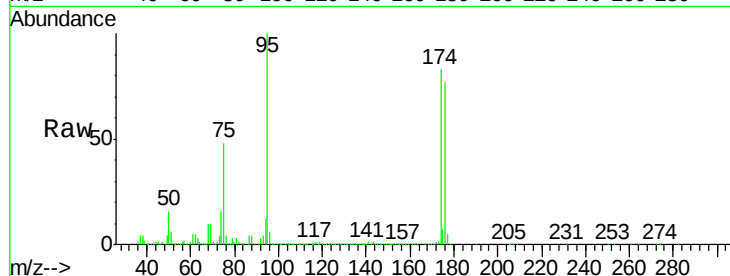

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

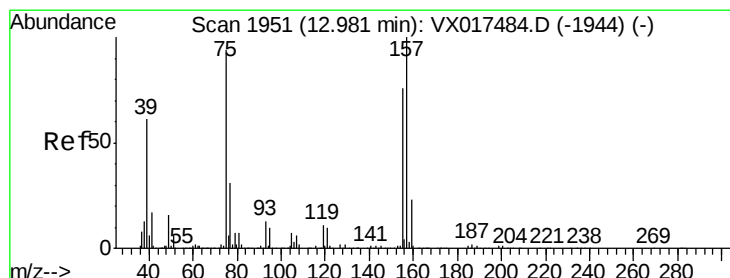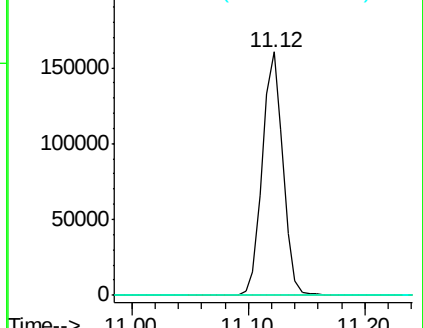

#92

1,2-Dibromo-3-Chloropropane

Concen: 2.728 ug/l

RT: 12.99 min Scan# 1953

Delta R.T. 0.01 min

Lab File: VX017749.D

Acq: 03 Aug 2020 16:32


Tgt Ion: 75 Resp: 392

Ion Ratio Lower Upper

75 100

155 0.0 42.3 126.8#

157 7.7 54.3 162.9#

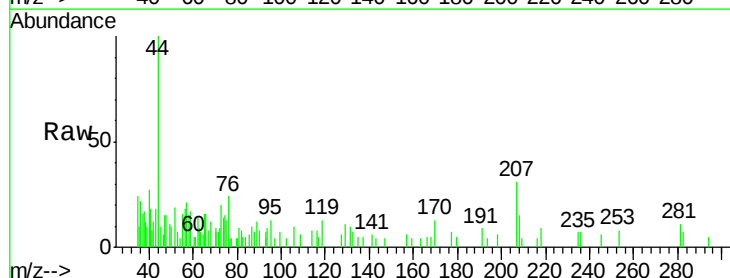

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

