

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080321\
 Data File : VX023523.D
 Acq On : 03 Aug 2021 11:59
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Manual Integrations
 APPROVED

MMDadoda
 8/6/2021 5:39:25 PM

Quant Time: Aug 04 04:54:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue Aug 03 12:05:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.916	128	38172	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.769	114	210586	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	183273	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.964	65	89247	30.232	ug/l	0.00
Spiked Amount 30.000	Range 91 - 110		Recovery = 100.767%			
60) 4-Bromofluorobenzene	11.085	95	80796	26.915	ug/l	0.00
Spiked Amount 30.000	Range 63 - 112		Recovery = 89.733%			
63) Toluene-d8	8.653	98	248819	30.166	ug/l	0.00
Spiked Amount 30.000	Range 91 - 112		Recovery = 100.567%			
Target Compounds						
					Qvalue	
16) Carbon Disulfide	2.514	76	8533	1.564	ug/l #	94
18) Methylene Chloride	2.794	84	2370	0.911	ug/l #	87
19) trans-1,2-Dichloroethene	3.099	96	1639	0.692	ug/l	96
29) 1,1-Dichloropropene	5.696	75	1667	0.508	ug/l	74
37) Trichloroethene	7.123	130	1274m	0.474	ug/l	
38) Methylcyclohexane	7.385	83	1671	0.401	ug/l	84
61) Tetrachloroethene	9.275	164	1314	0.534	ug/l #	79
64) Chlorobenzene	10.086	112	2250	0.344	ug/l	98
66) Ethyl Benzene	10.195	91	3348	0.293	ug/l	95
67) m/p-Xylenes	10.305	106	2652	0.599	ug/l	97
69) Styrene	10.659	104	1970	0.274	ug/l	91
70) Isopropylbenzene	10.963	105	3399	0.296	ug/l	100
74) n-propylbenzene	11.311	91	5334	0.402	ug/l	99
75) 2-Chlorotoluene	11.366	91	2703	0.341	ug/l	99
76) 1,3,5-Trimethylbenzene	11.457	105	3203	0.337	ug/l	93
78) 4-Chlorotoluene	11.457	91	4154	0.464	ug/l	100
79) tert-butylbenzene	11.719	119	3047	0.330	ug/l	95
80) 1,2,4-Trimethylbenzene	11.756	105	3179	0.337	ug/l	98
81) sec-Butylbenzene	11.896	105	4852	0.410	ug/l	98
82) p-Isopropyltoluene	12.012	119	4051	0.417	ug/l	97
83) 1,3-Dichlorobenzene	11.969	146	2719	0.538	ug/l	96
84) 1,4-Dichlorobenzene	12.042	146	3140	0.628	ug/l	97
85) n-Butylbenzene	12.335	91	4408	0.512	ug/l	94
87) 1,2-Dichlorobenzene	12.341	146	2051	0.420	ug/l	91
89) 1,2,4-Trichlorobenzene	13.591	180	2577	0.854	ug/l	93
90) Hexachlorobutadiene	13.725	225	1335	0.986	ug/l	98
91) Naphthalene	13.780	128	4938	0.476	ug/l	98
92) 1,2,3-Trichlorobenzene	13.963	180	2104	0.694	ug/l	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


MMDadoda
8/6/2021 5:39:25 PM

Abundance


TIC: VX023523.D\data.ms

Time-->



Compound	Retention Time (min)
Carbon Disulfide, M	~2.5
Methylene Chloride, M	~2.8
trans-1,2-Dichloroethene, M	~3.2
Bromochloromethane, l	~4.8
1,1-Dichloropropene	~5.8
1,2-Dichloroethane-d4, s	~6.0
1,4-Difluorobenzene, l	~6.8
Trichloroethene, M	~7.2
Methylcyclohexane	~7.5
Toluene-d8, S	~8.8
Tetrachloroethene, M	~9.2
Chlorobenzene, M	~10.2
Ethylbenzene, M	~10.3
m,p-Xylenes, M	~10.4
Styrene, M	~10.8
Isopropylbenzene	~11.2
2-Chlorobenzene	~11.5
1,2-Dichlorobenzene	~11.8
1,3-Dichlorobenzene	~12.0
1,4-Dichlorobenzene	~12.2
1,2,4-Trichlorobenzene	~12.5
1,2,3-Trichlorobenzene	~12.8
1,2,4-Trichlorobenzene	~13.5
1,2,3-Trichlorobenzene	~13.8

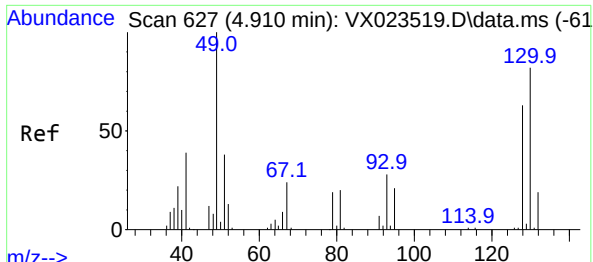

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.916 min Scan# 628
Delta R.T. 0.006 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

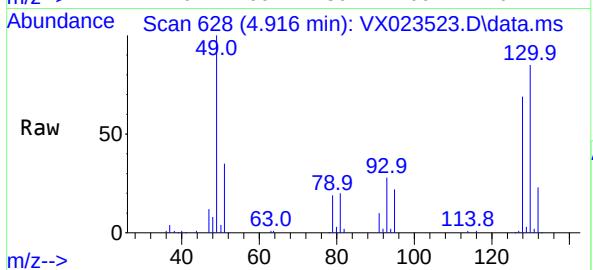


Tgt Ion:128 Resp: 38172
Ion Ratio Lower Upper
128 100
49 157.7 0.0 402.5
130 129.4 0.0 326.5

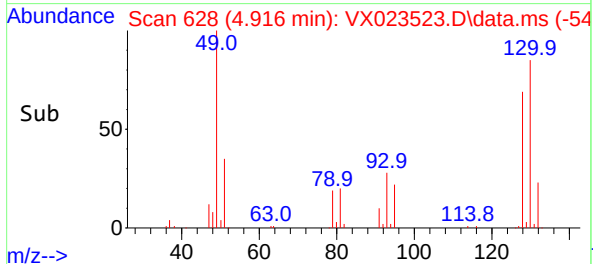


Instrument :
MSVOA_X
ClientSampled :
IBLK

Manual Integrations
APPROVED



MMDadoda
8/6/2021 5:39:25 PM

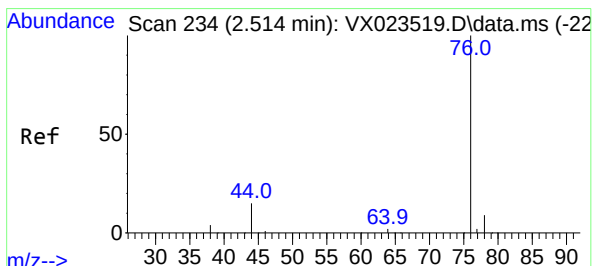


#16
Carbon Disulfide
Concen: 1.564 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

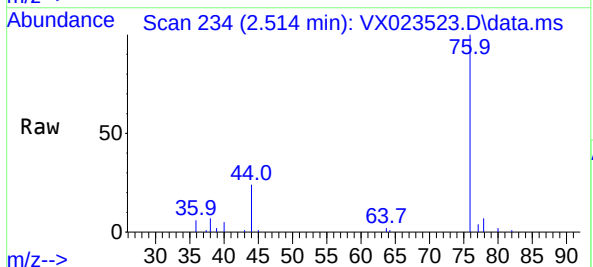


Tgt Ion: 76 Resp: 8533
Ion Ratio Lower Upper
76 100
78 6.8 7.3 10.9#

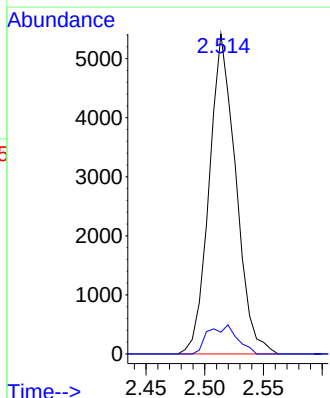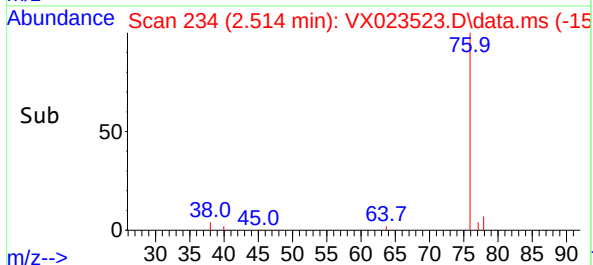




#18
Methylene Chloride
Concen: 0.911 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59




Tgt Ion:	84	Resp:	2370
Ion	Ratio	Lower	Upper
84	100		
49	113.0	104.3	156.5
51	46.0	30.3	45.5#
86	58.7	51.7	77.5

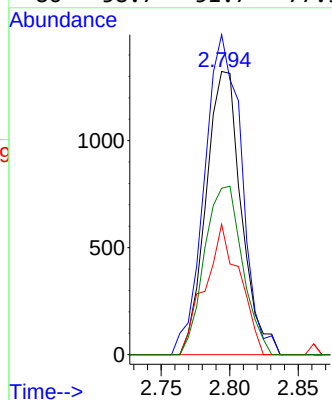


Instrument :
MSVOA_X
ClientSampled :
IBLK

Manual Integrations
APPROVED



MMDadoda
8/6/2021 5:39:25 PM




#19
trans-1,2-Dichloroethene
Concen: 0.692 ug/l
RT: 3.099 min Scan# 330
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

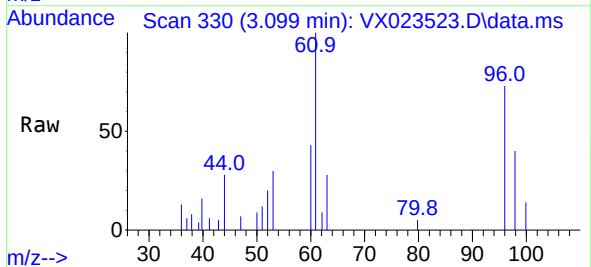

Tgt Ion:	96	Resp:	1639
Ion	Ratio	Lower	Upper
96	100		
61	136.7	109.2	163.8
98	54.1	50.8	76.2

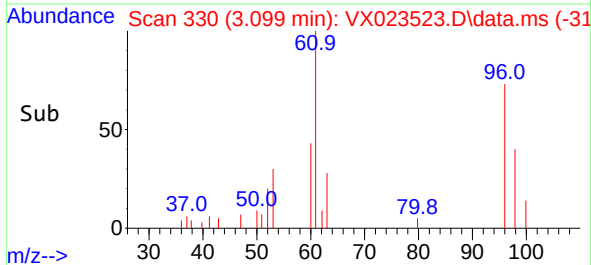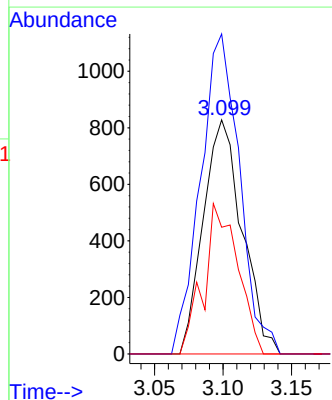

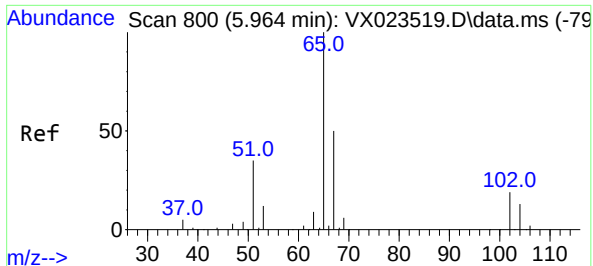





#27
1,2-Dichloroethane-d4
Concen: 30.232 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 65 Resp: 89247
Ion Ratio Lower Upper
65 100
67 50.8 42.4 63.6

Instrument :
MSVOA_X
ClientSampleId :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

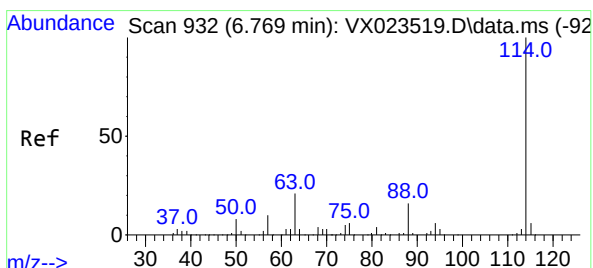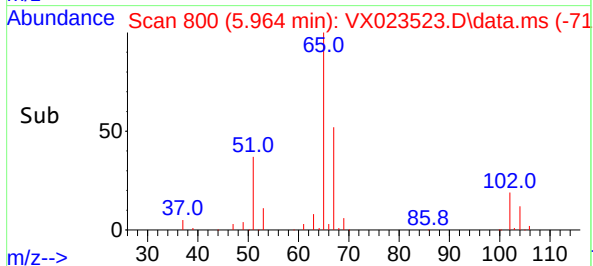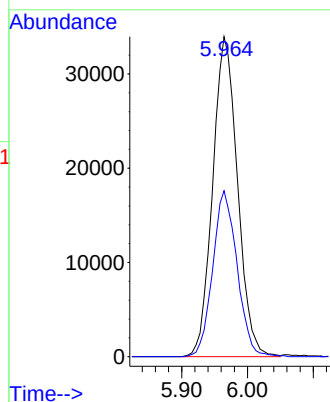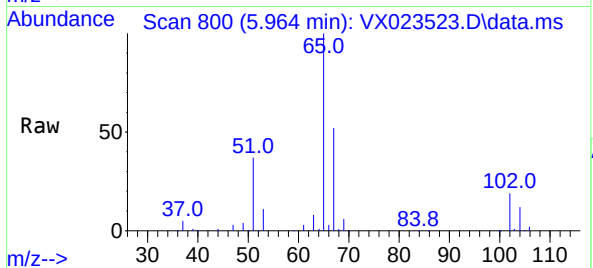

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 114 Resp: 210586
Ion Ratio Lower Upper
114 100
63 20.6 16.4 24.6
88 16.0 12.7 19.1

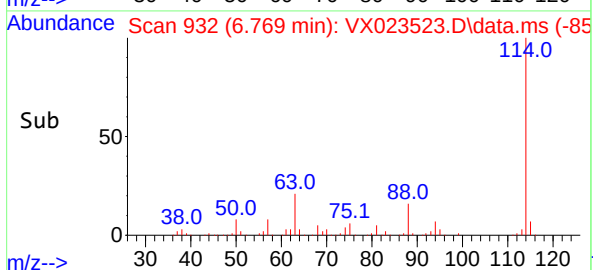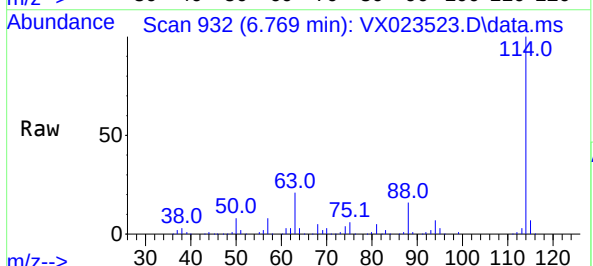

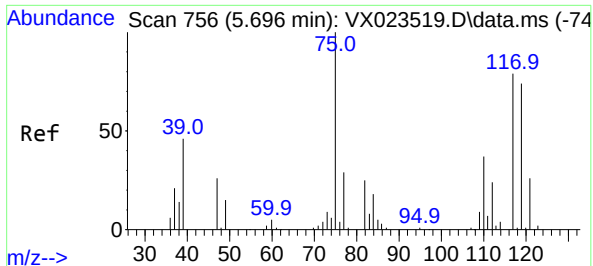





#29
1,1-Dichloropropene
Concen: 0.508 ug/l
RT: 5.696 min Scan# 756
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 75 Resp: 1667
Ion Ratio Lower Upper
75 100
110 30.6 0.0 72.0
77 5.4 0.0 61.8

Instrument :
MSVOA_X
ClientSampled :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

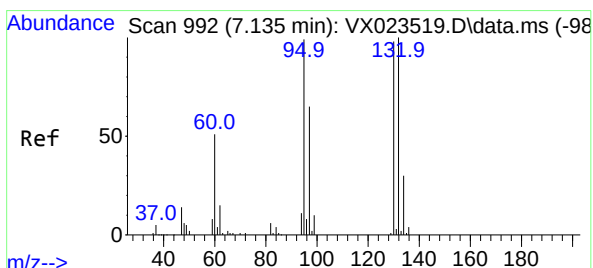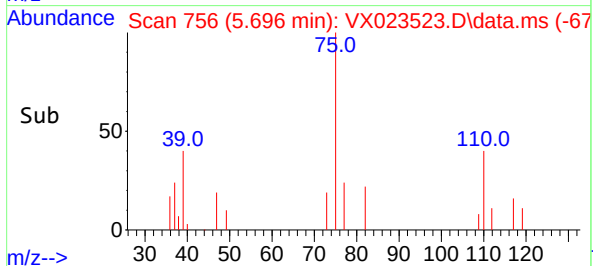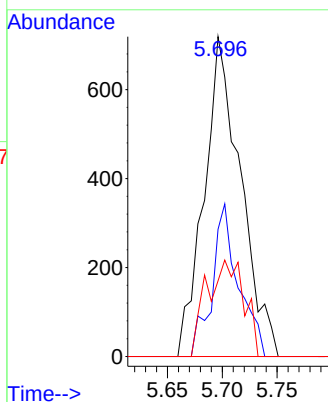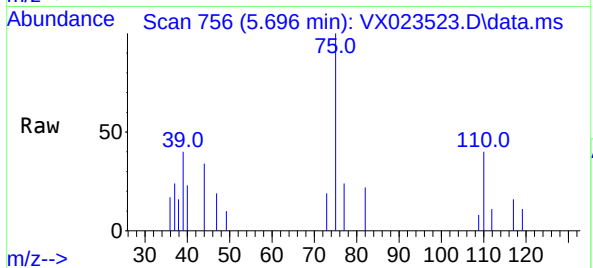


#37
Trichloroethene
Concen: 0.474 ug/l m
RT: 7.123 min Scan# 990
Delta R.T. -0.012 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 130 Resp: 1274
Ion Ratio Lower Upper
130 100
95 99.3 77.0 115.4

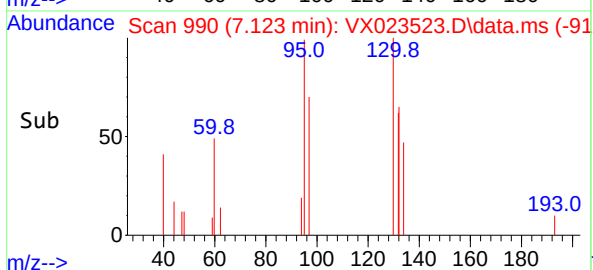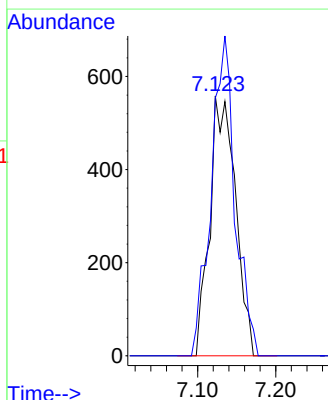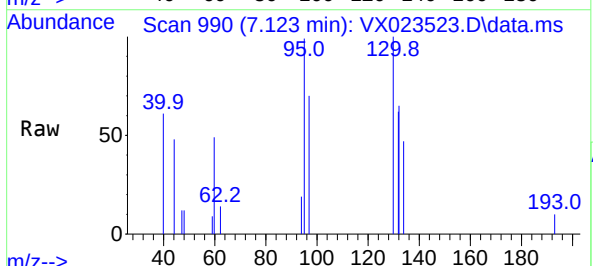



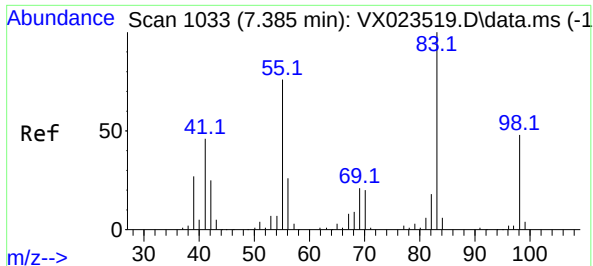


#38
Methylcyclohexane
Concen: 0.401 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

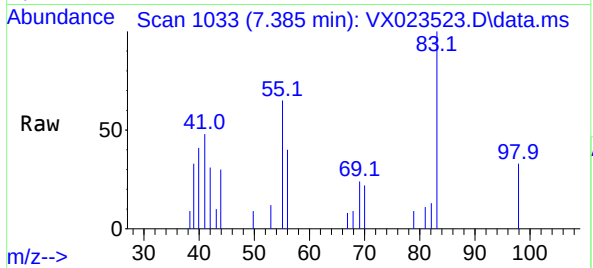


Tgt Ion: 83 Resp: 1671

Ion	Ratio	Lower	Upper
83	100		
55	69.4	37.8	113.4
98	27.7	23.4	70.3

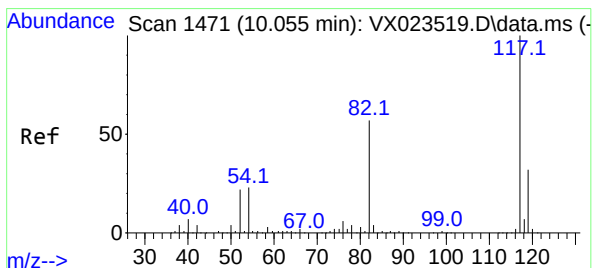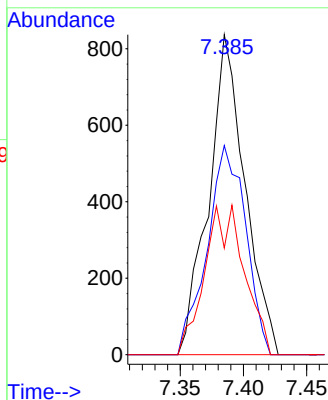
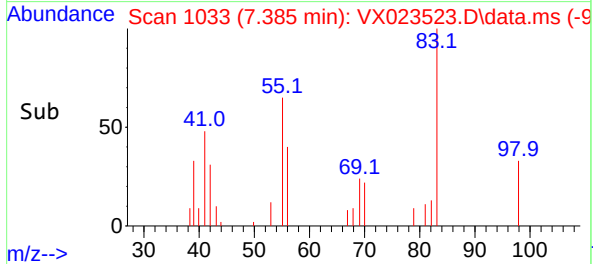


#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

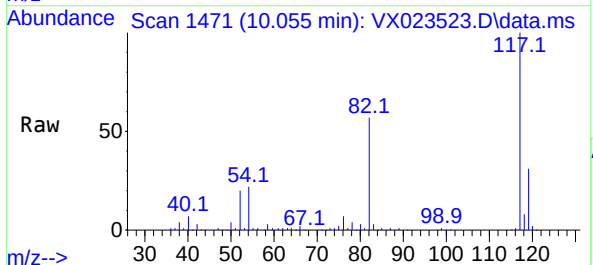

Tgt Ion: 117 Resp: 183273


Ion	Ratio	Lower	Upper
117	100		
82	55.5	45.0	67.4
119	31.5	26.2	39.2

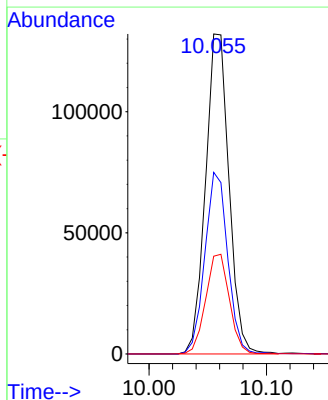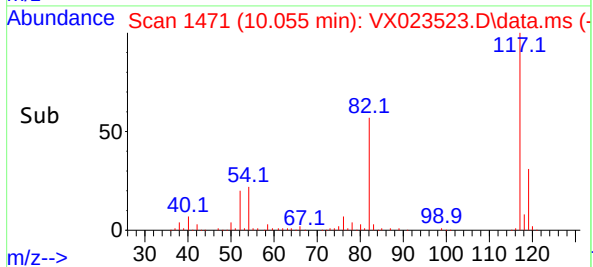


Instrument :
MSVOA_X
ClientSampled :
IBLK

Manual Integrations
APPROVED




MMDadoda
8/6/2021 5:39:25 PM




#60
4-Bromofluorobenzene
Concen: 26.915 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59





Tgt Ion: 95 Resp: 80796
Ion Ratio Lower Upper
95 100
174 82.9 63.5 95.3
176 79.0 63.0 94.4



#61
Tetrachloroethene
Concen: 0.534 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

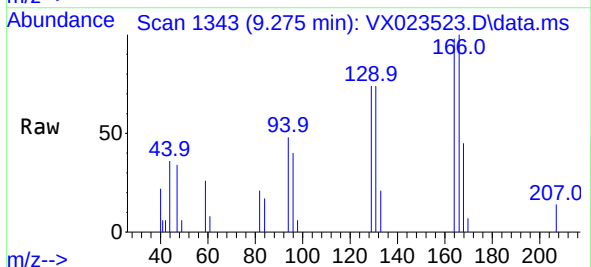


Tgt Ion: 164 Resp: 1314
Ion Ratio Lower Upper
164 100
166 102.0 98.6 147.8
129 75.3 79.7 119.5#
131 75.1 76.6 115.0#

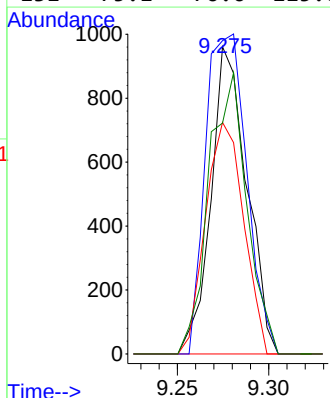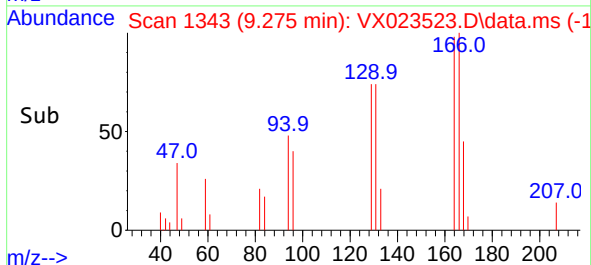

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Manual Integrations
APPROVED

MMDadoda
8/6/2021 5:39:25 PM

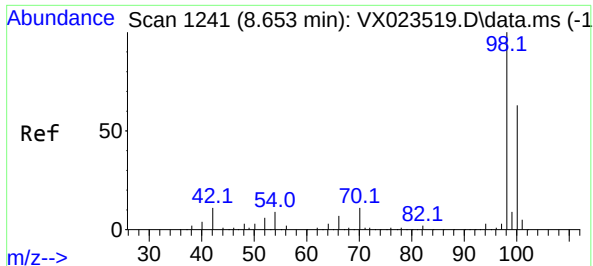





#63
Toluene-d8
Concen: 30.166 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 98 Resp: 248819
Ion Ratio Lower Upper
98 100
100 63.6 51.4 77.0

Instrument :
MSVOA_X
ClientSampled :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

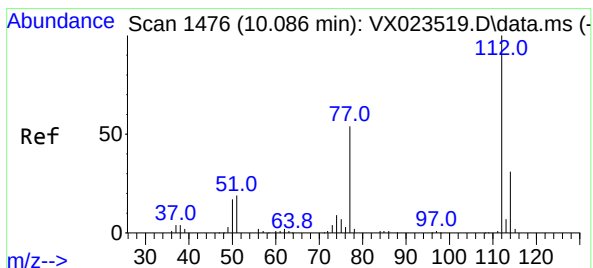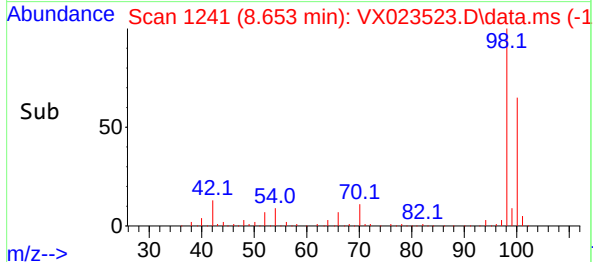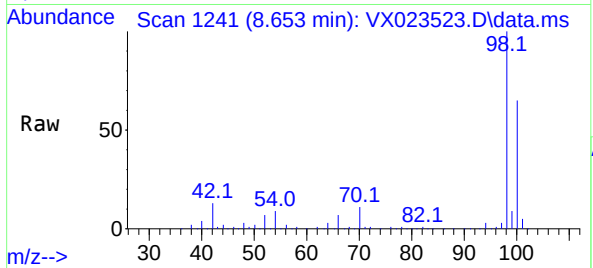

#64
Chlorobenzene
Concen: 0.344 ug/l
RT: 10.086 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 112 Resp: 2250
Ion Ratio Lower Upper
112 100
114 31.2 26.0 39.0

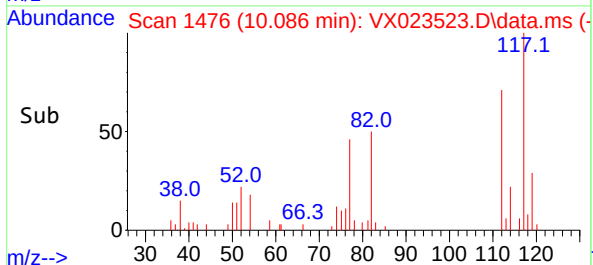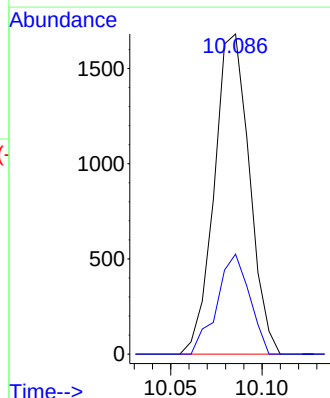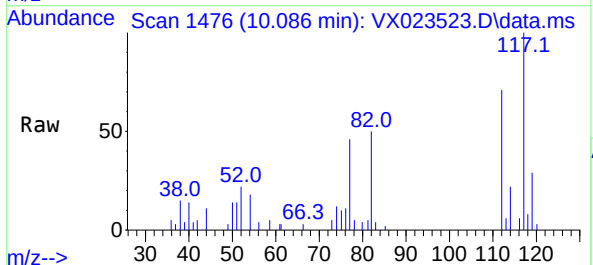







#66
Ethyl Benzene
Concen: 0.293 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Instrument :
MSVOA_X
ClientSampled :
IBLK

Tgt Ion: 91 Resp: 3348
Ion Ratio Lower Upper
91 100
106 33.7 24.7 37.1




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM



#67
m/p-Xylenes
Concen: 0.599 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 106 Resp: 2652
Ion Ratio Lower Upper
106 100
91 198.1 162.4 243.6

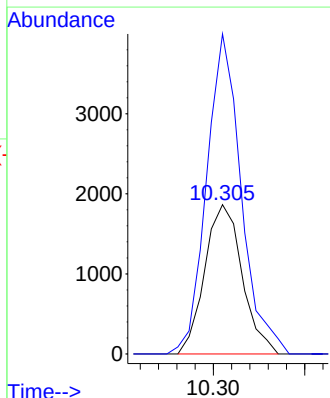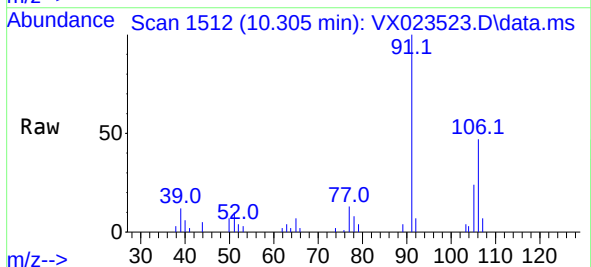







#69
Styrene
Concen: 0.274 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion:	104	Resp:	1970
Ion	Ratio	Lower	Upper
104	100		
78	42.9	41.4	62.0
103	59.2	44.2	66.4

Instrument :
MSVOA_X
ClientSampled :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

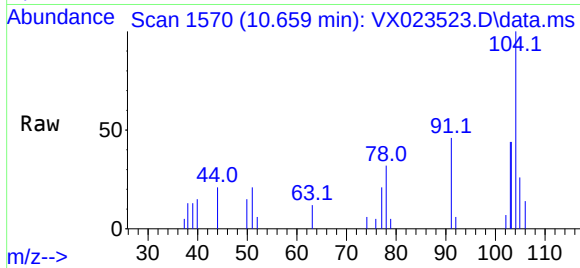

#70
Isopropylbenzene
Concen: 0.296 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion:	105	Resp:	3399
Ion	Ratio	Lower	Upper
105	100		
120	26.8	18.7	34.7

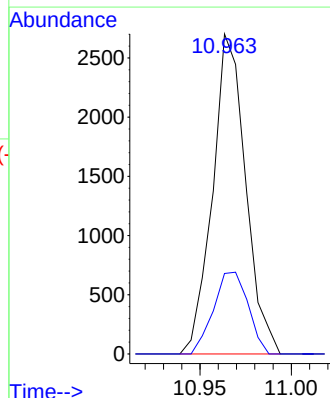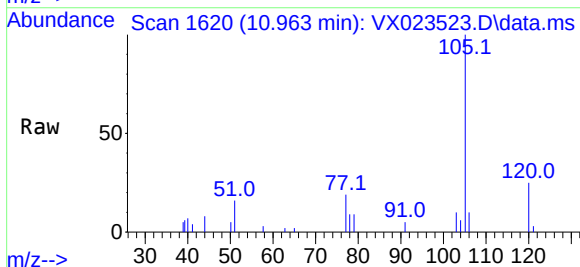







#74
n-propylbenzene
Concen: 0.402 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Instrument :
MSVOA_X
ClientSampled :
IBLK

Tgt Ion: 91 Resp: 5334
Ion Ratio Lower Upper
91 100
120 22.7 0.0 46.0




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

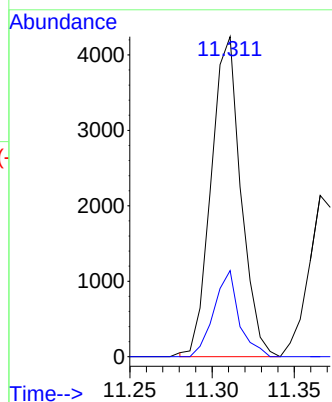

#75
2-Chlorotoluene
Concen: 0.341 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 91 Resp: 2703
Ion Ratio Lower Upper
91 100
126 33.7 0.0 69.0

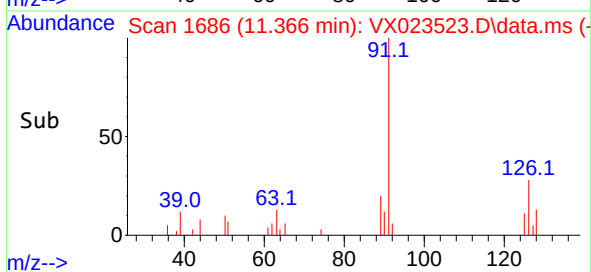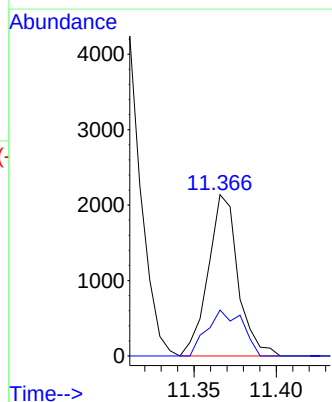







#76
1,3,5-Trimethylbenzene
Concen: 0.337 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion: 105 Resp: 3203
Ion Ratio Lower Upper
105 100
120 44.3 0.0 98.0

Instrument :
MSVOA_X
ClientSampled :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

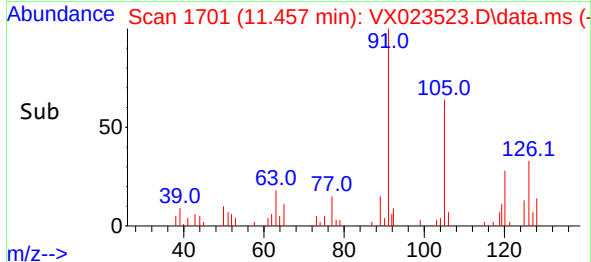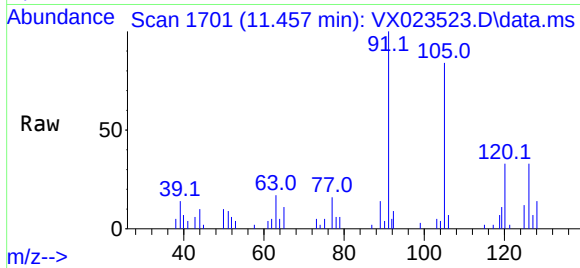

#78
4-Chlorotoluene
Concen: 0.464 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59


Tgt Ion: 91 Resp: 4154
Ion Ratio Lower Upper
91 100
126 30.0 0.0 59.6

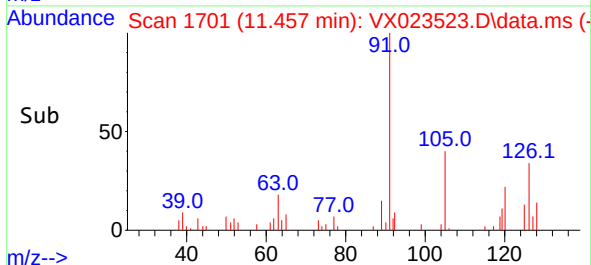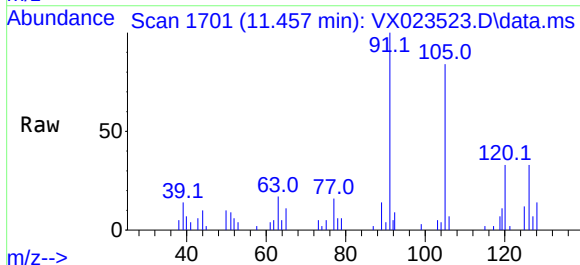



#79
tert-butylbenzene
Concen: 0.330 ug/l
RT: 11.719 min Scan# 1744
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59




Instrument :
MSVOA_X
ClientSampled :
IBLK

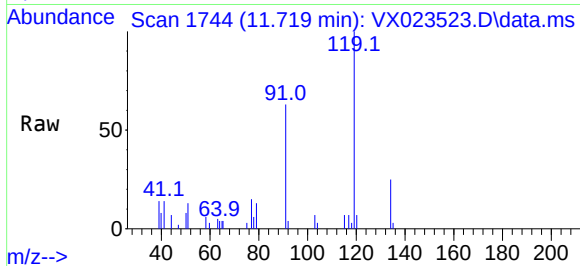


Tgt Ion:119 Resp: 3047
Ion Ratio Lower Upper
119 100
91 65.3 0.0 121.2
134 25.5 0.0 47.4

Manual Integrations
APPROVED



MMDadoda
8/6/2021 5:39:25 PM




#80
1,2,4-Trimethylbenzene
Concen: 0.337 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

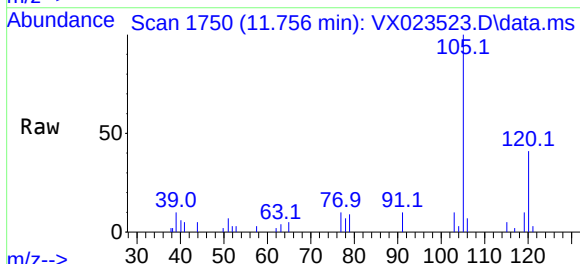

Tgt Ion:105 Resp: 3179
Ion Ratio Lower Upper
105 100
120 46.4 0.0 90.4









#81
 sec-Butylbenzene
 Concen: 0.410 ug/l
 RT: 11.896 min Scan# 1773
 Delta R.T. 0.000 min
 Lab File: VX023523.D
 Acq: 03 Aug 2021 11:59

Instrument :
 MSVOA_X
 ClientSampled :
 IBLK

Tgt Ion:105 Resp: 4852
 Ion Ratio Lower Upper
 105 100
 134 19.3 0.0 40.2




Manual Integrations
 APPROVED


MMDadoda
 8/6/2021 5:39:25 PM



#82
 p-Isopropyltoluene
 Concen: 0.417 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX023523.D
 Acq: 03 Aug 2021 11:59

Tgt Ion:119 Resp: 4051
 Ion Ratio Lower Upper
 119 100
 134 28.0 0.0 52.8
 91 25.7 0.0 48.6

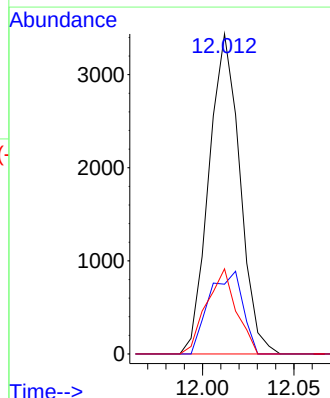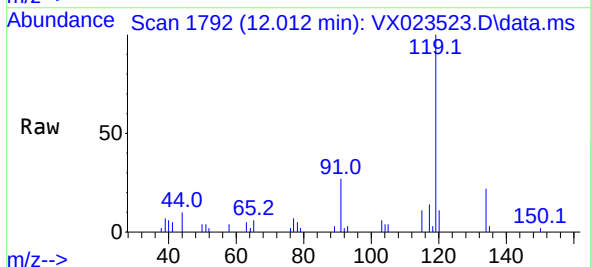







#83
1,3-Dichlorobenzene
Concen: 0.538 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion:146 Resp: 2719
Ion Ratio Lower Upper
146 100
111 42.8 20.1 60.2
148 67.0 31.9 95.5

Instrument :
MSVOA_X
ClientSampled :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

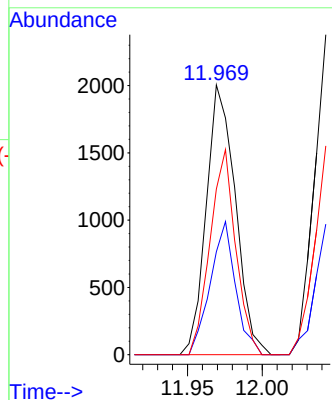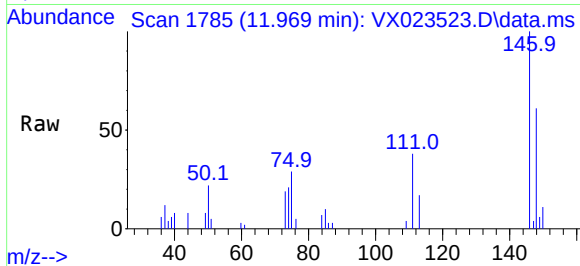

#84
1,4-Dichlorobenzene
Concen: 0.628 ug/l
RT: 12.042 min Scan# 1797
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion:146 Resp: 3140
Ion Ratio Lower Upper
146 100
111 37.3 18.9 56.9
148 65.6 31.4 94.2

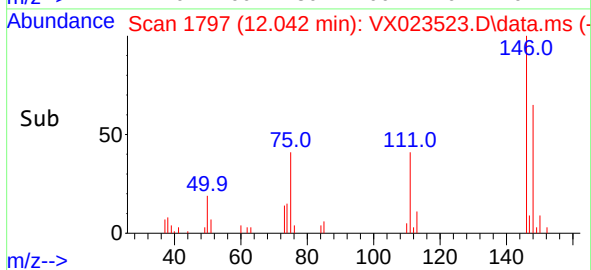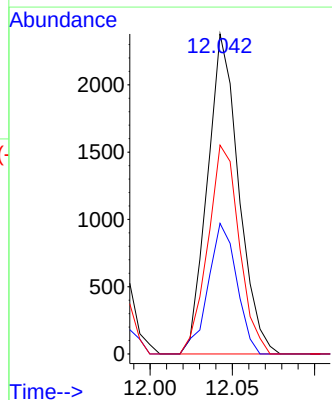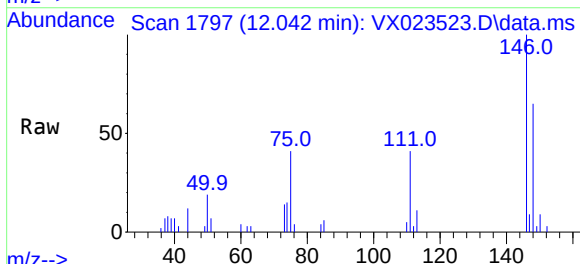







#85
n-Butylbenzene
Concen: 0.512 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

Tgt Ion:	91	Resp:	4408
Ion	Ratio	Lower	Upper
91	100		
92	58.7	0.0	105.4
134	27.0	0.0	52.4

Instrument :
MSVOA_X
ClientSampled :
IBLK




Manual Integrations
APPROVED


MMDadoda
8/6/2021 5:39:25 PM

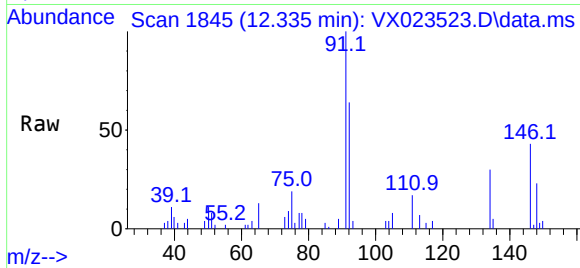

#87
1,2-Dichlorobenzene
Concen: 0.420 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.006 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59


Tgt Ion:	146	Resp:	2051
Ion	Ratio	Lower	Upper
146	100		
111	36.9	20.7	62.1
148	56.8	32.6	97.8

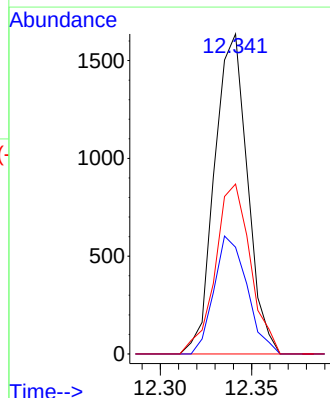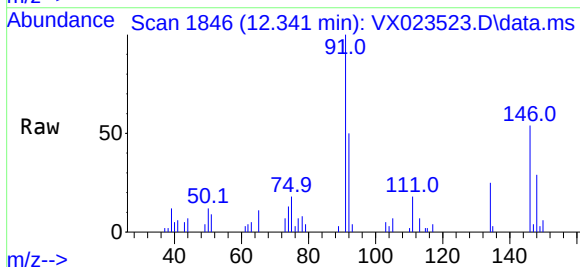



#89
1,2,4-Trichlorobenzene
Concen: 0.854 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59




Instrument :
MSVOA_X
ClientSampled :
IBLK




Tgt Ion:180 Resp: 2577
Ion Ratio Lower Upper
180 100
182 87.3 75.9 113.9
145 28.2 24.2 36.4

Manual Integrations
APPROVED



MMDadoda
8/6/2021 5:39:25 PM




#90
Hexachlorobutadiene
Concen: 0.986 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

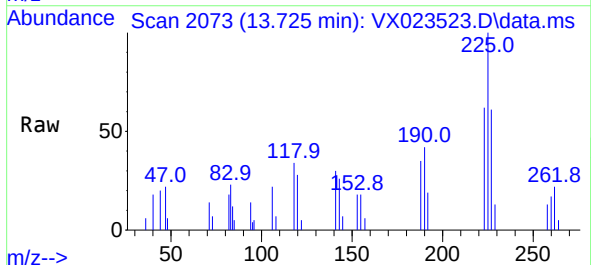


Tgt Ion:225 Resp: 1335
Ion Ratio Lower Upper
225 100
223 65.7 0.0 126.4
227 63.1 0.0 125.0

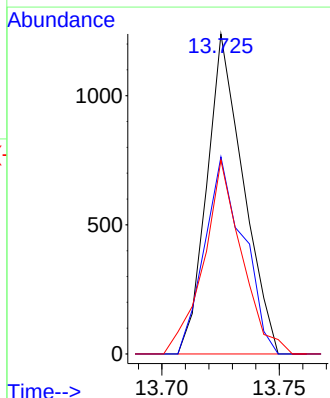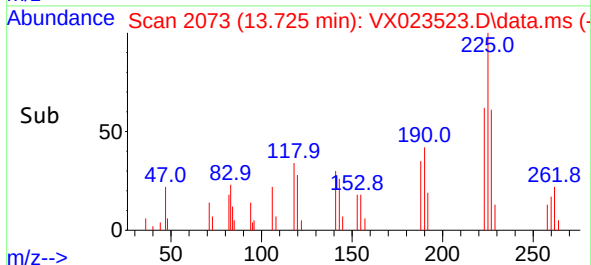

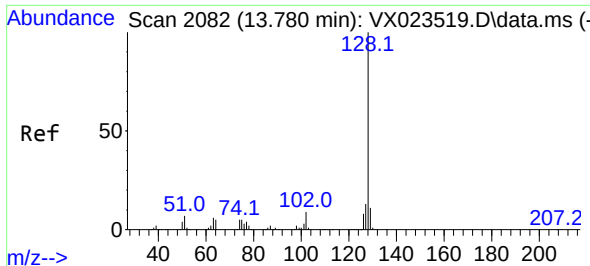

#91
Naphthalene
Concen: 0.476 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59




Instrument :
MSVOA_X
ClientSampled :
IBLK

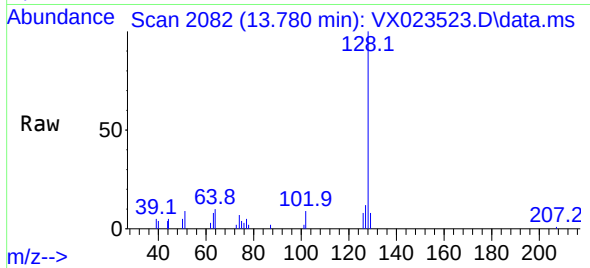


Tgt Ion:128 Resp: 4938
Ion Ratio Lower Upper
128 100
127 12.3 10.1 15.1
129 9.5 8.6 12.8

Manual Integrations
APPROVED

MMDadoda
8/6/2021 5:39:25 PM

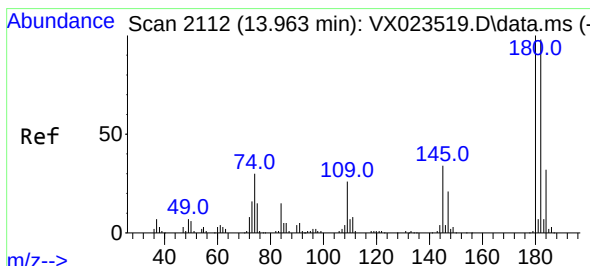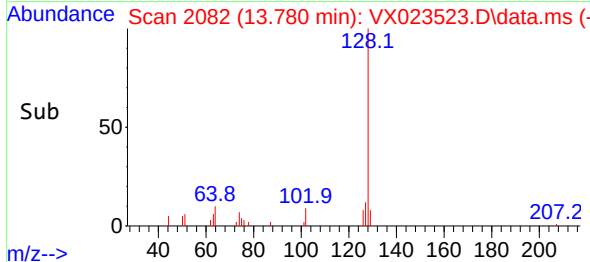

#92
1,2,3-Trichlorobenzene
Concen: 0.694 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX023523.D
Acq: 03 Aug 2021 11:59

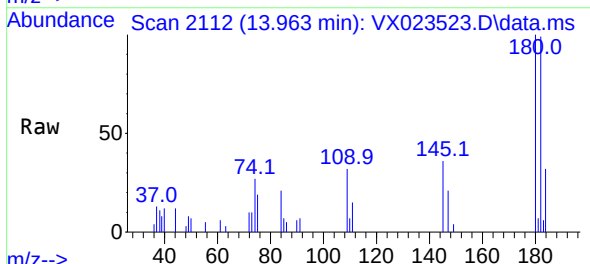

Tgt Ion:180 Resp: 2104
Ion Ratio Lower Upper
180 100
182 92.3 0.0 193.4
145 39.5 0.0 64.4

