

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080322\
 Data File : VX030363.D
 Acq On : 03 Aug 2022 12:14
 Operator : JC/MD
 Sample : VX0803WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0803WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	72	82	85	rBV4	6982	18170	2.17%	0.462%
2	2.947	297	305	313	rBV	12832	29648	3.55%	0.753%
3	4.580	565	573	584	rBV2	7050	25452	3.04%	0.646%
4	5.391	694	706	718	rBV	99360	289959	34.68%	7.365%
5	5.556	722	733	748	rVB	110545	316959	37.91%	8.051%
6	5.958	790	799	814	rBV	121506	318117	38.05%	8.080%
7	6.763	923	931	943	rBV	169160	409455	48.98%	10.400%
8	8.653	1234	1241	1251	rBV	548835	836007	100.00%	21.235%
9	10.055	1465	1471	1484	rBV	398993	539441	64.53%	13.702%
10	11.085	1634	1640	1654	rVB	410258	536415	64.16%	13.625%
11	12.024	1788	1794	1803	rBV	505058	617373	73.85%	15.681%




Sum of corrected areas: 3936996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080322\
Data File : VX030363.D
Acq On : 03 Aug 2022 12:14
Operator : JC/MD
Sample : VX0803WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0803WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

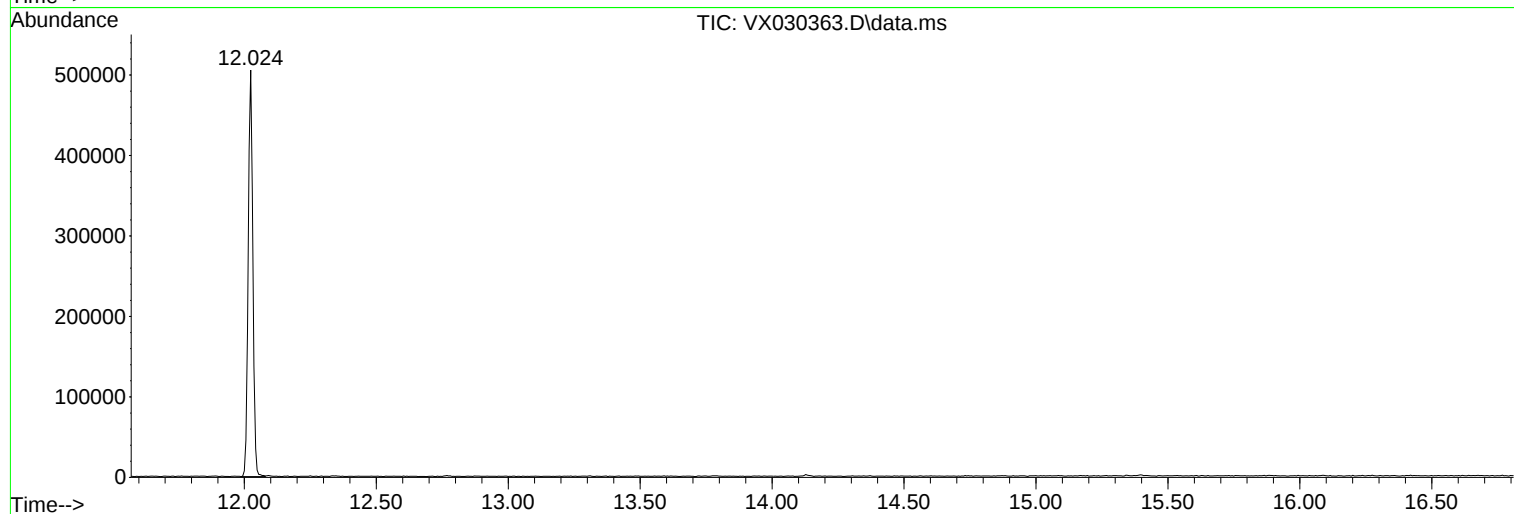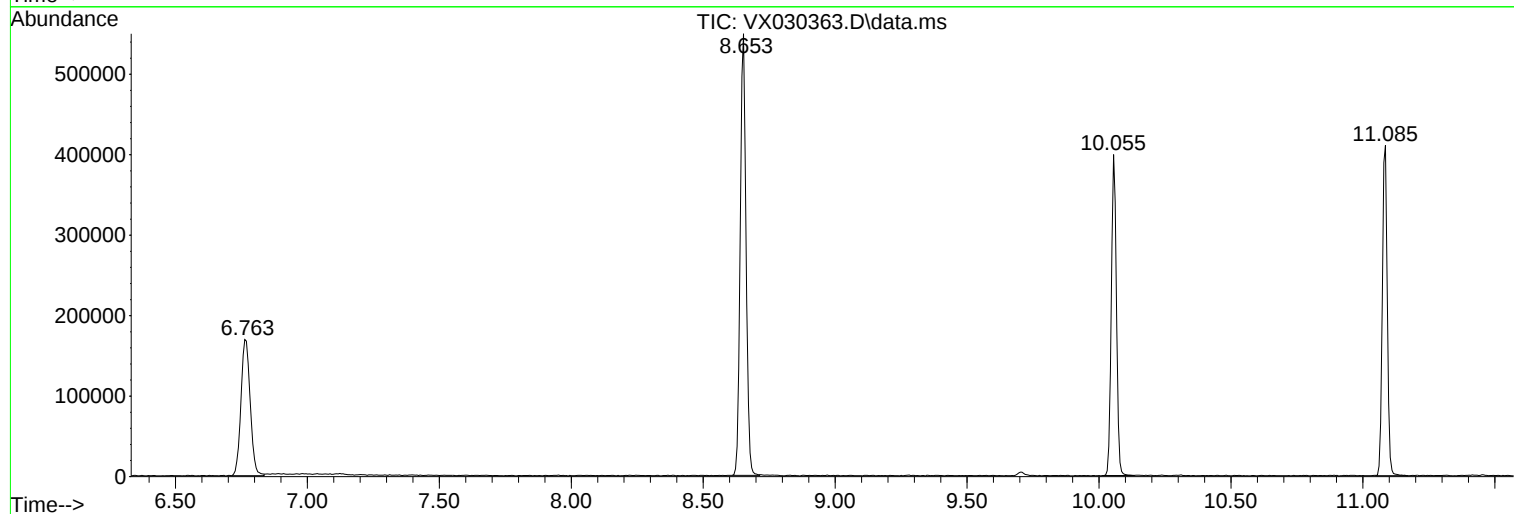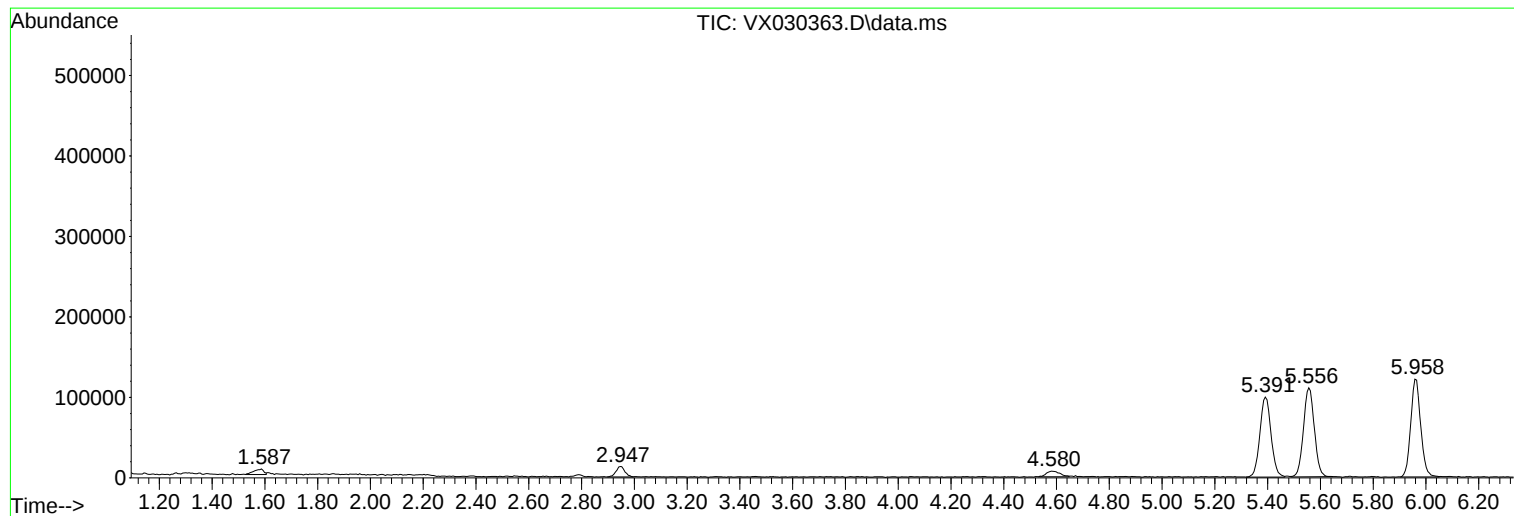

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080322\
Data File : VX030363.D
Acq On : 03 Aug 2022 12:14
Operator : JC/MD
Sample : VX0803WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0803WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080322\
Data File : VX030363.D
Acq On : 03 Aug 2022 12:14
Operator : JC/MD
Sample : VX0803WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0803WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc