

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080323\
 Data File : VX036794.D
 Acq On : 03 Aug 2023 12:55
 Operator : JC/MD
 Sample : 03882-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRE-1763

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036794.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	70	82	87	rBV7	4711	16883	1.98%	0.360%
2	2.788	274	279	286	rBV	4643	9092	1.07%	0.194%
3	5.385	692	705	720	rBV2	96820	286854	33.60%	6.122%
4	5.550	721	732	745	rVV	159507	450058	52.72%	9.605%
5	5.958	786	799	817	rBV	104127	278965	32.68%	5.954%
6	6.763	921	931	944	rBV	263708	626715	73.42%	13.375%
7	8.647	1233	1240	1261	rBV	547461	853651	100.00%	18.218%
8	10.055	1465	1471	1484	rBV	550561	759488	88.97%	16.209%
9	11.079	1634	1639	1652	rBV	458498	578828	67.81%	12.353%
10	12.018	1788	1793	1803	rBV	531493	696498	81.59%	14.865%
11	14.036	2118	2124	2128	rBV	12500	14317	1.68%	0.306%
12	14.176	2143	2147	2151	rVB3	9834	12119	1.42%	0.259%
13	14.262	2157	2161	2167	rBV	9196	11702	1.37%	0.250%
14	14.609	2215	2218	2224	rVB2	7887	9284	1.09%	0.198%
15	14.755	2238	2242	2246	rBV	28011	31975	3.75%	0.682%
16	14.987	2277	2280	2286	rVB3	9308	12050	1.41%	0.257%
17	15.103	2293	2299	2302	rBV4	7677	12605	1.48%	0.269%
18	15.207	2314	2316	2320	rVB	8294	9514	1.11%	0.203%
19	15.487	2358	2362	2368	rBV	11375	15036	1.76%	0.321%




Sum of corrected areas: 4685634

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080323\
Data File : VX036794.D
Acq On : 03 Aug 2023 12:55
Operator : JC/MD
Sample : 03882-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1763

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

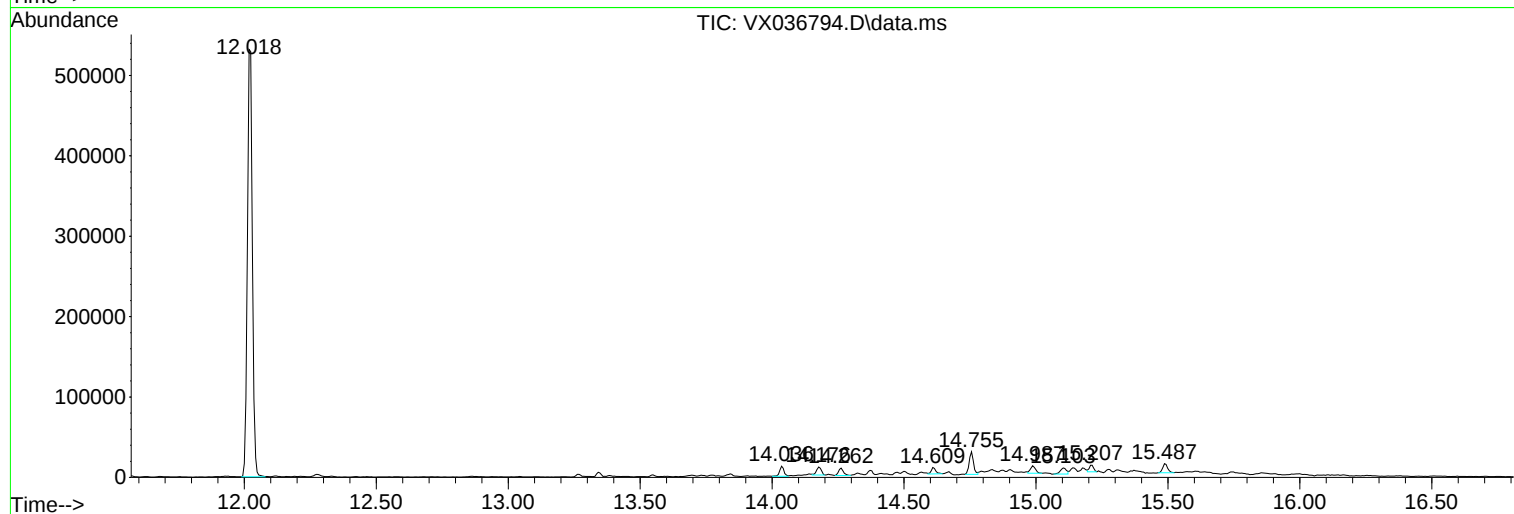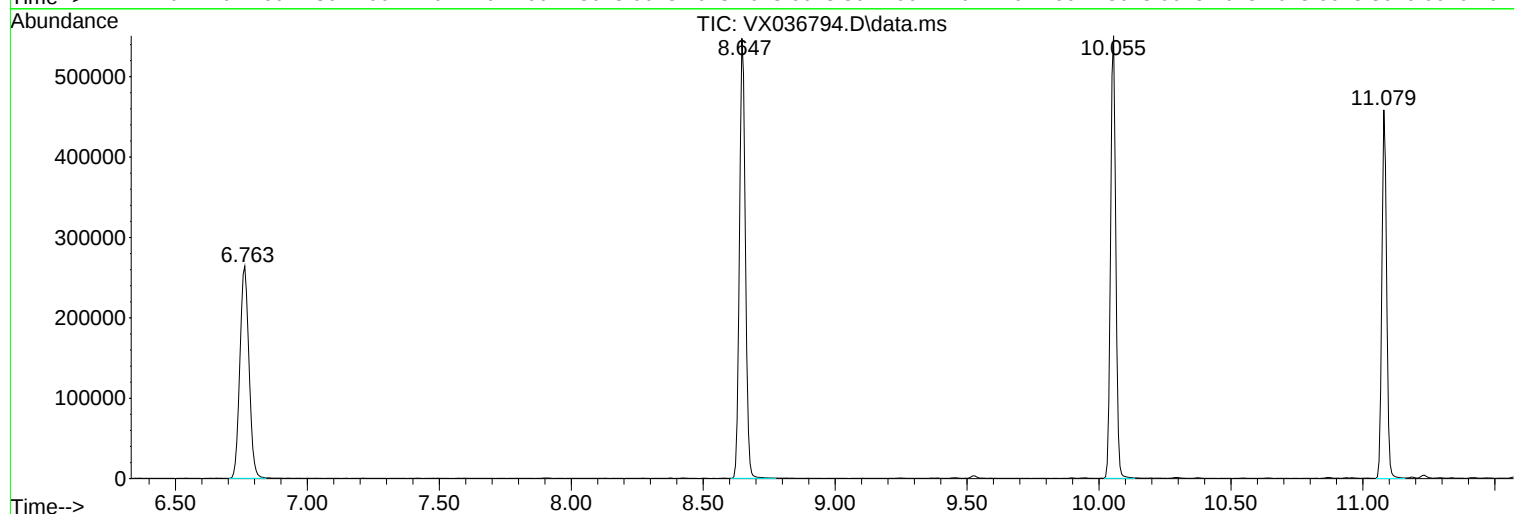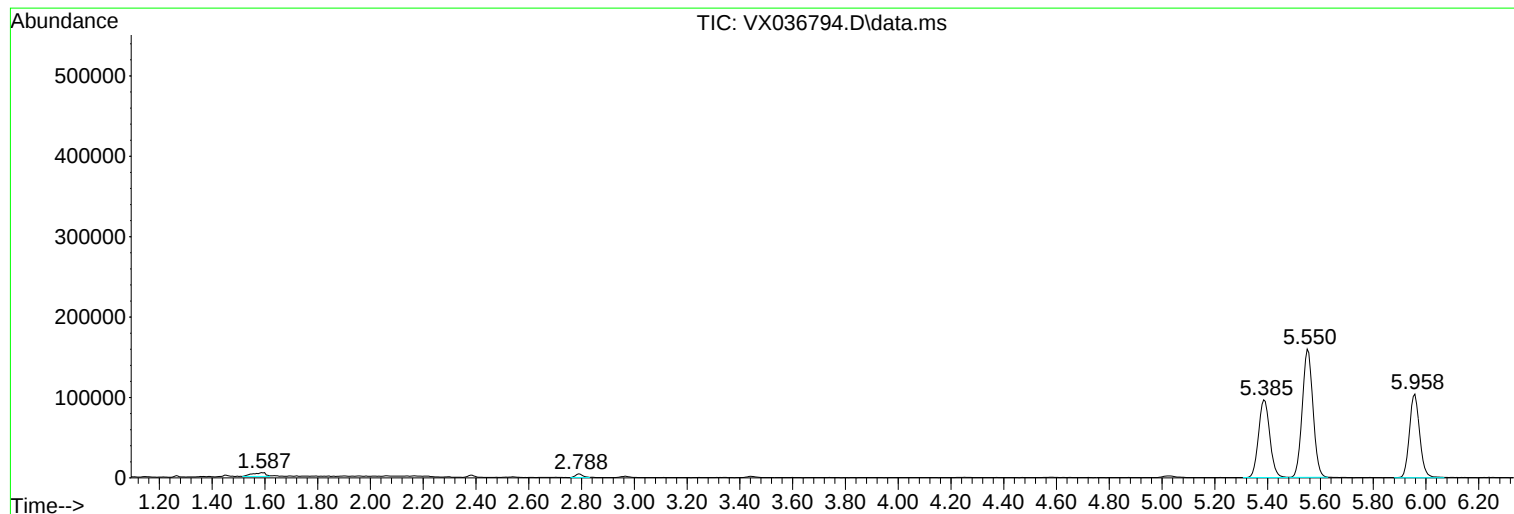

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080323\
Data File : VX036794.D
Acq On : 03 Aug 2023 12:55
Operator : JC/MD
Sample : 03882-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1763

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080323\
Data File : VX036794.D
Acq On : 03 Aug 2023 12:55
Operator : JC/MD
Sample : 03882-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1763

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------