


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080420\
 Data File : VX017757.D
 Acq On : 04 Aug 2020 08:44
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Title : SW846 8260
 Last Update : Fri Jul 24 05:48:09 2020

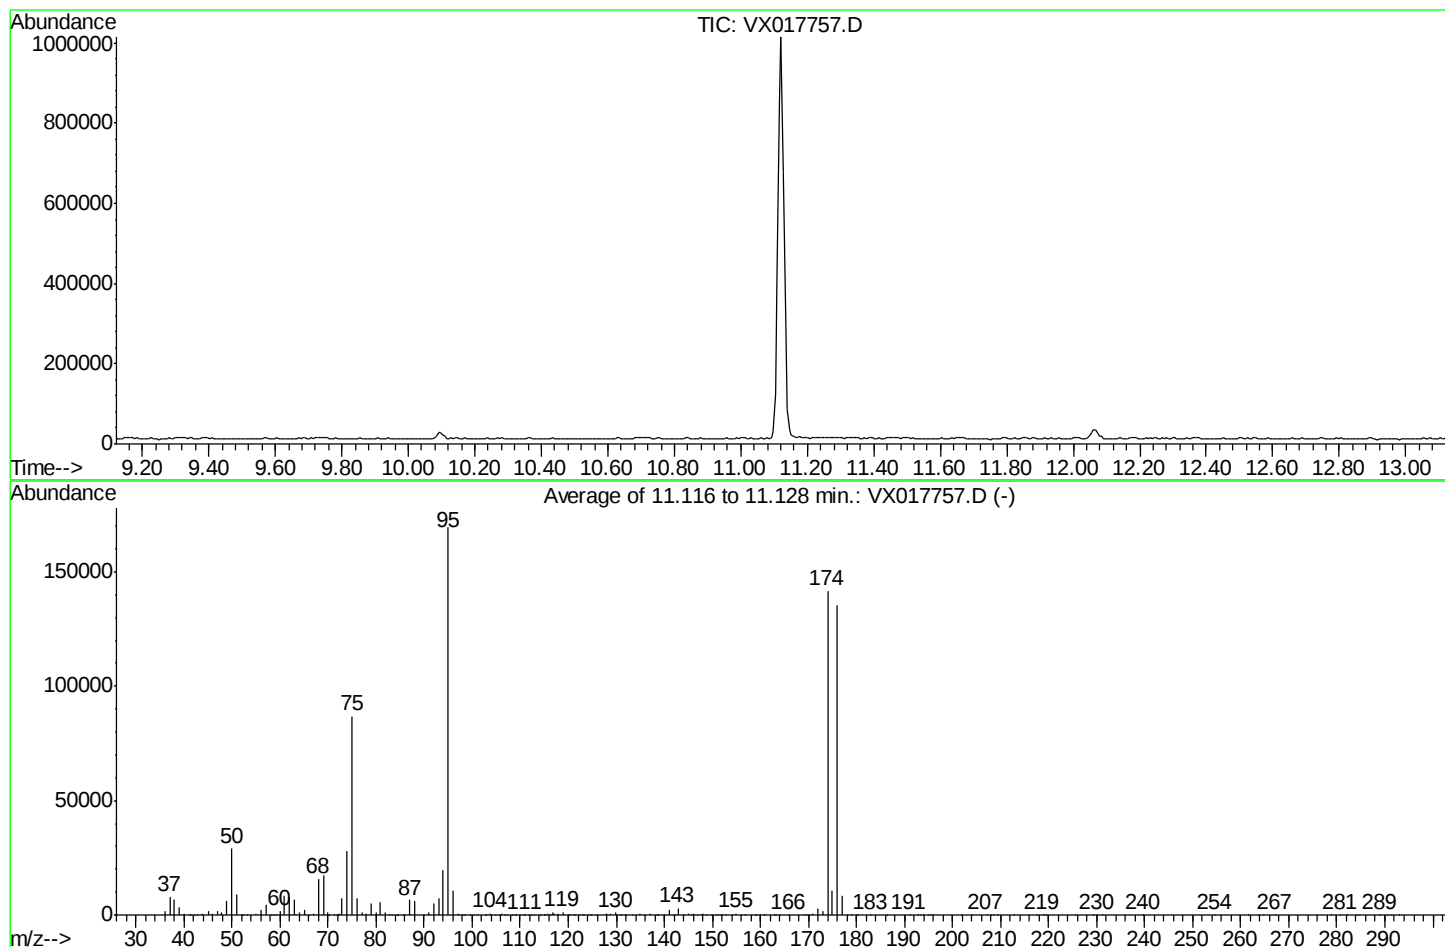

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	29052	PASS
75	95	30	60	51.2	86803	PASS
95	95	100	100	100.0	169498	PASS
96	95	5	9	6.1	10402	PASS
173	174	0.00	2	1.2	1769	PASS
174	95	50	100	83.6	141669	PASS
175	174	5	9	7.6	10805	PASS
176	174	95	101	95.6	135378	PASS
177	176	5	9	6.4	8629	PASS