

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080421\
 Data File : VX023542.D
 Acq On : 04 Aug 2021 14:45
 Operator : JC/MD
 Sample : M3281-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP03

Integration Parameters: RTEINT3.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX023542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	72	79	82	rBV5	5974	10274	1.08%	0.077%
2	2.386	206	213	223	rBV	10591	18086	1.91%	0.136%
3	2.550	230	240	249	rVB2	9058	18306	1.93%	0.138%
4	2.965	298	308	317	rVB4	4548	13805	1.45%	0.104%
5	3.123	325	334	344	rVB	35376	81330	8.57%	0.613%
6	4.587	565	574	583	rBV2	3715	11572	1.22%	0.087%
7	4.910	615	627	643	rBV2	86114	255496	26.92%	1.925%
8	5.964	790	800	810	rBV2	88287	233840	24.64%	1.762%
9	6.050	810	814	822	rVB4	4521	9760	1.03%	0.074%
10	6.769	919	932	946	rBV	195949	468897	49.41%	3.532%
11	7.385	1026	1033	1042	rVB3	12400	27986	2.95%	0.211%
12	8.604	1225	1233	1235	rBV3	9505	16145	1.70%	0.122%
13	8.653	1235	1241	1249	rVV	417721	649972	68.49%	4.897%
14	8.720	1249	1252	1257	rVB	7321	10626	1.12%	0.080%
15	8.982	1289	1295	1301	rBV4	9425	16067	1.69%	0.121%
16	9.519	1376	1383	1387	rBV6	7101	16102	1.70%	0.121%
17	9.567	1387	1391	1396	rVB	16569	23419	2.47%	0.176%
18	9.622	1396	1400	1404	rBV2	8777	13132	1.38%	0.099%
19	9.830	1429	1434	1439	rBV6	5762	11268	1.19%	0.085%
20	10.055	1466	1471	1477	rBV	413730	548558	57.81%	4.133%
21	10.128	1480	1483	1488	rVB2	7892	10342	1.09%	0.078%
22	10.195	1488	1494	1499	rVB	8812	14185	1.49%	0.107%
23	10.305	1503	1512	1518	rBV2	26623	58353	6.15%	0.440%
24	10.592	1551	1559	1565	rBV5	15453	36714	3.87%	0.277%
25	10.646	1565	1568	1576	rVB2	13913	23460	2.47%	0.177%
26	10.781	1581	1590	1595	rVB4	23497	40477	4.27%	0.305%
27	10.860	1596	1603	1607	rBV3	23771	38509	4.06%	0.290%
28	10.963	1615	1620	1624	rBV	26298	33604	3.54%	0.253%
29	11.085	1635	1640	1645	rBV	330970	421045	44.37%	3.172%
30	11.128	1645	1647	1651	rVB2	12068	13120	1.38%	0.099%
31	11.220	1655	1662	1671	rVB4	16109	29911	3.15%	0.225%
32	11.305	1671	1676	1680	rBV	28993	38702	4.08%	0.292%
33	11.384	1685	1689	1694	rVV4	18882	38930	4.10%	0.293%
34	11.451	1694	1700	1703	rVV3	16841	38799	4.09%	0.292%
35	11.482	1703	1705	1709	rVV3	9508	12232	1.29%	0.092%
36	11.616	1722	1727	1734	rVB3	27453	46062	4.85%	0.347%
37	11.719	1740	1744	1746	rBV	10301	12010	1.27%	0.090%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080421\
 Data File : VX023542.D
 Acq On : 04 Aug 2021 14:45
 Operator : JC/MD
 Sample : M3281-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP03

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

38	11.756	1746	1750	1760	rVB	54350	85681	9.03%	0.645%
39	11.866	1760	1768	1770	rBV	27305	48983	5.16%	0.369%
40	11.890	1770	1772	1777	rVV	43540	55949	5.90%	0.421%
41	11.945	1777	1781	1784	rVV	15659	23116	2.44%	0.174%
42	12.091	1800	1805	1809	rBV	32906	44715	4.71%	0.337%
43	12.183	1815	1820	1823	rBV	16390	20716	2.18%	0.156%
44	12.244	1823	1830	1837	rVB2	212527	307901	32.45%	2.320%
45	12.317	1837	1842	1849	rVB3	67986	122692	12.93%	0.924%
46	12.408	1850	1857	1863	rBV2	43077	69918	7.37%	0.527%
47	12.469	1863	1867	1873	rVB5	17073	27562	2.90%	0.208%
48	12.536	1873	1878	1879	rBV4	13970	18329	1.93%	0.138%
49	12.616	1886	1891	1894	rBV	274631	314473	33.14%	2.369%
50	12.646	1894	1896	1901	rVB2	57362	68856	7.26%	0.519%
51	12.701	1901	1905	1913	rVB3	188897	325727	34.32%	2.454%
52	12.762	1913	1915	1917	rBV3	11763	13858	1.46%	0.104%
53	12.841	1921	1928	1933	rVB4	67748	140282	14.78%	1.057%
54	12.927	1933	1942	1946	rBV	274937	388496	40.94%	2.927%
55	12.969	1946	1949	1951	rBV2	22358	32122	3.39%	0.242%
56	13.030	1955	1959	1965	rVB3	72044	108402	11.42%	0.817%
57	13.097	1965	1970	1974	rBV2	60630	96655	10.19%	0.728%
58	13.140	1974	1977	1979	rBV2	65137	71523	7.54%	0.539%
59	13.170	1979	1982	1985	rVB	122961	125095	13.18%	0.942%
60	13.262	1992	1997	1998	rBV2	51948	69236	7.30%	0.522%
61	13.292	1998	2002	2009	rVB2	655075	948950	100.00%	7.149%
62	13.372	2012	2015	2018	rVB	64151	63558	6.70%	0.479%
63	13.426	2018	2024	2032	rVB5	74454	151028	15.92%	1.138%
64	13.506	2033	2037	2040	rBV	78366	109895	11.58%	0.828%
65	13.548	2040	2044	2047	rBV	149960	188985	19.92%	1.424%
66	13.585	2047	2050	2054	rVB2	232513	281477	29.66%	2.121%
67	13.646	2054	2060	2061	rBV2	105945	164782	17.36%	1.241%
68	13.664	2061	2063	2072	rVB2	242962	392611	41.37%	2.958%
69	13.756	2072	2078	2079	rBV2	74667	107730	11.35%	0.812%
70	13.780	2079	2082	2084	rBV	62551	76541	8.07%	0.577%
71	13.853	2090	2094	2099	rVB2	173490	231507	24.40%	1.744%
72	13.926	2099	2106	2111	rBV2	241885	380543	40.10%	2.867%
73	13.975	2111	2114	2117	rVV	115744	149328	15.74%	1.125%
74	14.006	2117	2119	2123	rVB3	34298	38497	4.06%	0.290%
75	14.079	2126	2131	2134	rBV	242343	305493	32.19%	2.301%
76	14.103	2134	2135	2139	rVV2	29204	31566	3.33%	0.238%
77	14.164	2142	2145	2149	rVV2	31870	42771	4.51%	0.322%
78	14.231	2149	2156	2163	rVV3	386131	839850	88.50%	6.327%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080421\
 Data File : VX023542.D
 Acq On : 04 Aug 2021 14:45
 Operator : JC/MD
 Sample : M3281-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TWP03

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

79	14.292	2163	2166	2167	rVV3	23815	27761	2.93%	0.209%
80	14.323	2167	2171	2175	rVV	175711	231962	24.44%	1.747%
81	14.377	2175	2180	2184	rVV2	296955	393954	41.51%	2.968%
82	14.420	2184	2187	2192	rVB	67547	90312	9.52%	0.680%
83	14.481	2192	2197	2202	rBV2	331689	473447	49.89%	3.567%
84	14.524	2202	2204	2207	rVB3	27638	29229	3.08%	0.220%
85	14.615	2210	2219	2220	rBV3	200223	258331	27.22%	1.946%
86	14.640	2220	2223	2226	rVV	302681	411562	43.37%	3.101%
87	14.676	2226	2229	2233	rVB	136616	170848	18.00%	1.287%
88	14.731	2233	2238	2241	rBV2	75106	98736	10.40%	0.744%
89	14.786	2242	2247	2250	rBV2	264694	387001	40.78%	2.915%
90	14.816	2250	2252	2255	rVV2	82286	104693	11.03%	0.789%
91	14.853	2255	2258	2261	rVB3	53752	67122	7.07%	0.506%
92	14.908	2262	2267	2273	rBV3	42542	82585	8.70%	0.622%




Sum of corrected areas: 13274038

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080421\
Data File : VX023542.D
Acq On : 04 Aug 2021 14:45
Operator : JC/MD
Sample : M3281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

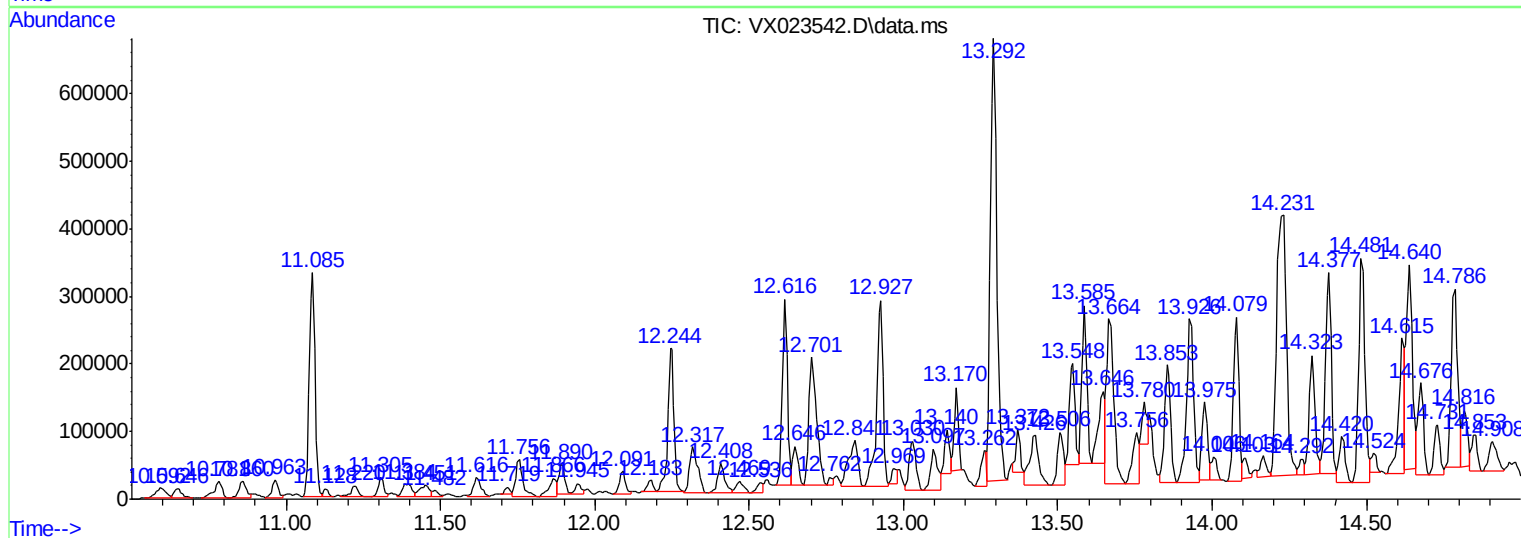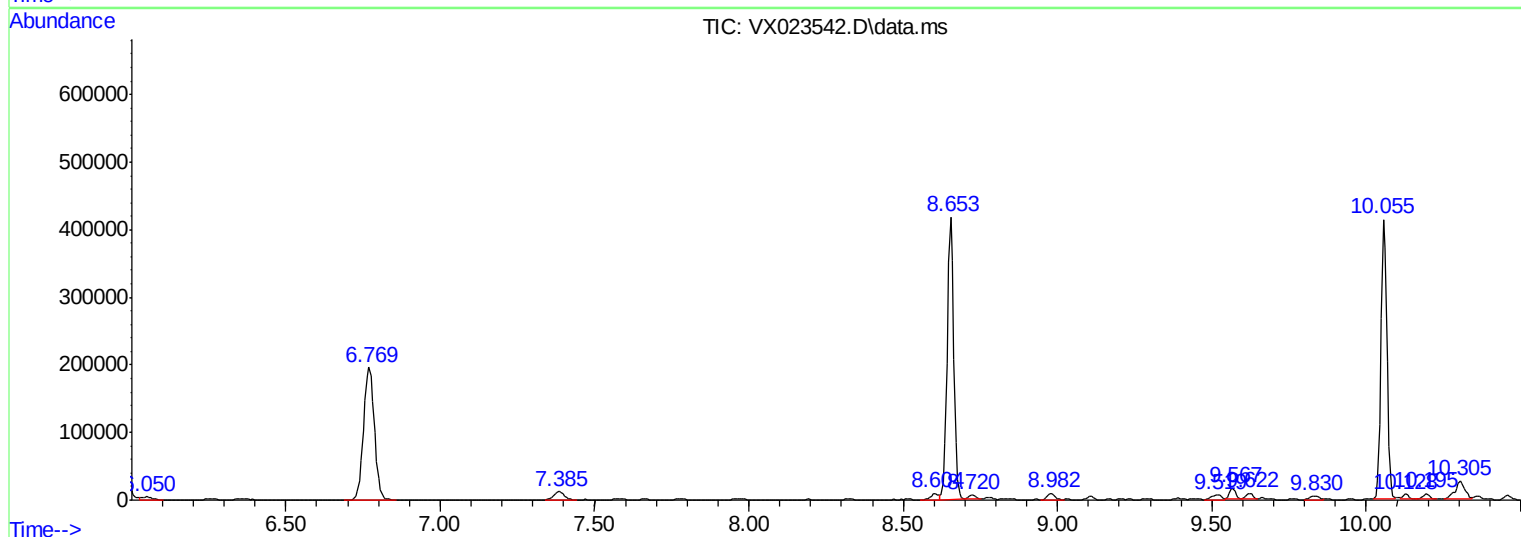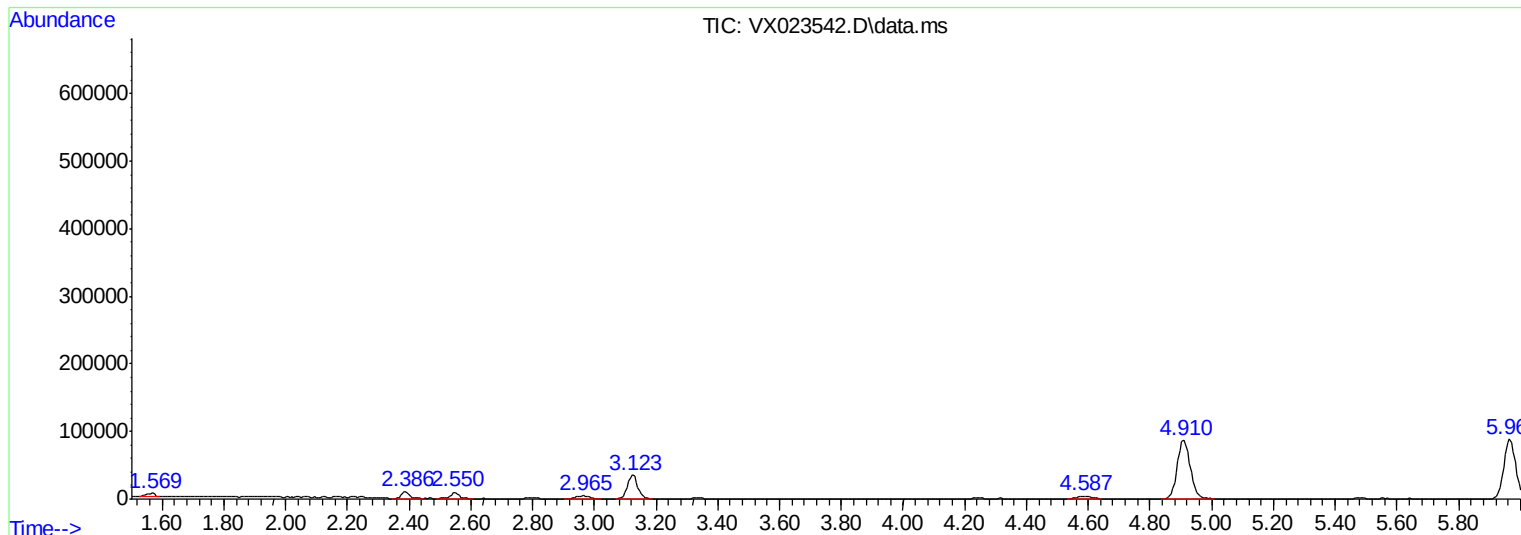

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080421\
Data File : VX023542.D
Acq On : 04 Aug 2021 14:45
Operator : JC/MD
Sample : M3281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080421\
Data File : VX023542.D
Acq On : 04 Aug 2021 14:45
Operator : JC/MD
Sample : M3281-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TWP03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc
