

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030392.D
 Acq On : 04 Aug 2022 15:30
 Operator : JC/MD
 Sample : N4008-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZF0

Quant Time: Aug 05 05:26:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Aug 05 05:25:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	310840	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	277869	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	125094	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	95394	47.789	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	95.580%		
7) Chloroethane-d5	1.666	69	75863	53.911	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	107.820%		
11) 1,1-Dichloroethene-d2	2.307	63	153519	40.657	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.320%		
21) 2-Butanone-d5	4.465	46	183656	99.298	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.300%		
24) Chloroform-d	5.062	84	189764	46.181	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.360%		
26) 1,2-Dichloroethane-d4	5.958	65	130844	46.895	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.800%		
32) Benzene-d6	5.977	84	381430	47.922	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.840%		
36) 1,2-Dichloropropane-d6	7.312	67	122410	47.402	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.800%		
41) Toluene-d8	8.653	98	349022	46.520	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.040%		
43) trans-1,3-Dichloroprop...	8.952	79	57446	44.716	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.440%		
47) 2-Hexanone-d5	9.385	63	125530	95.366	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.370%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	155402	45.808	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.620%		
66) 1,2-Dichlorobenzene-d4	12.323	152	117379	48.377	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.760%		
Target Compounds					Qvalue	
13) Acetone	2.392	43	5233	3.860	ug/L	89
44) trans-1,3-Dichloropropene	8.958	75	3070	0.888	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030392.D
Acq On : 04 Aug 2022 15:30
Operator : JC/MD
Sample : N4008-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF0

Quant Time: Aug 05 05:26:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Aug 05 05:25:14 2022
Response via : Initial Calibration

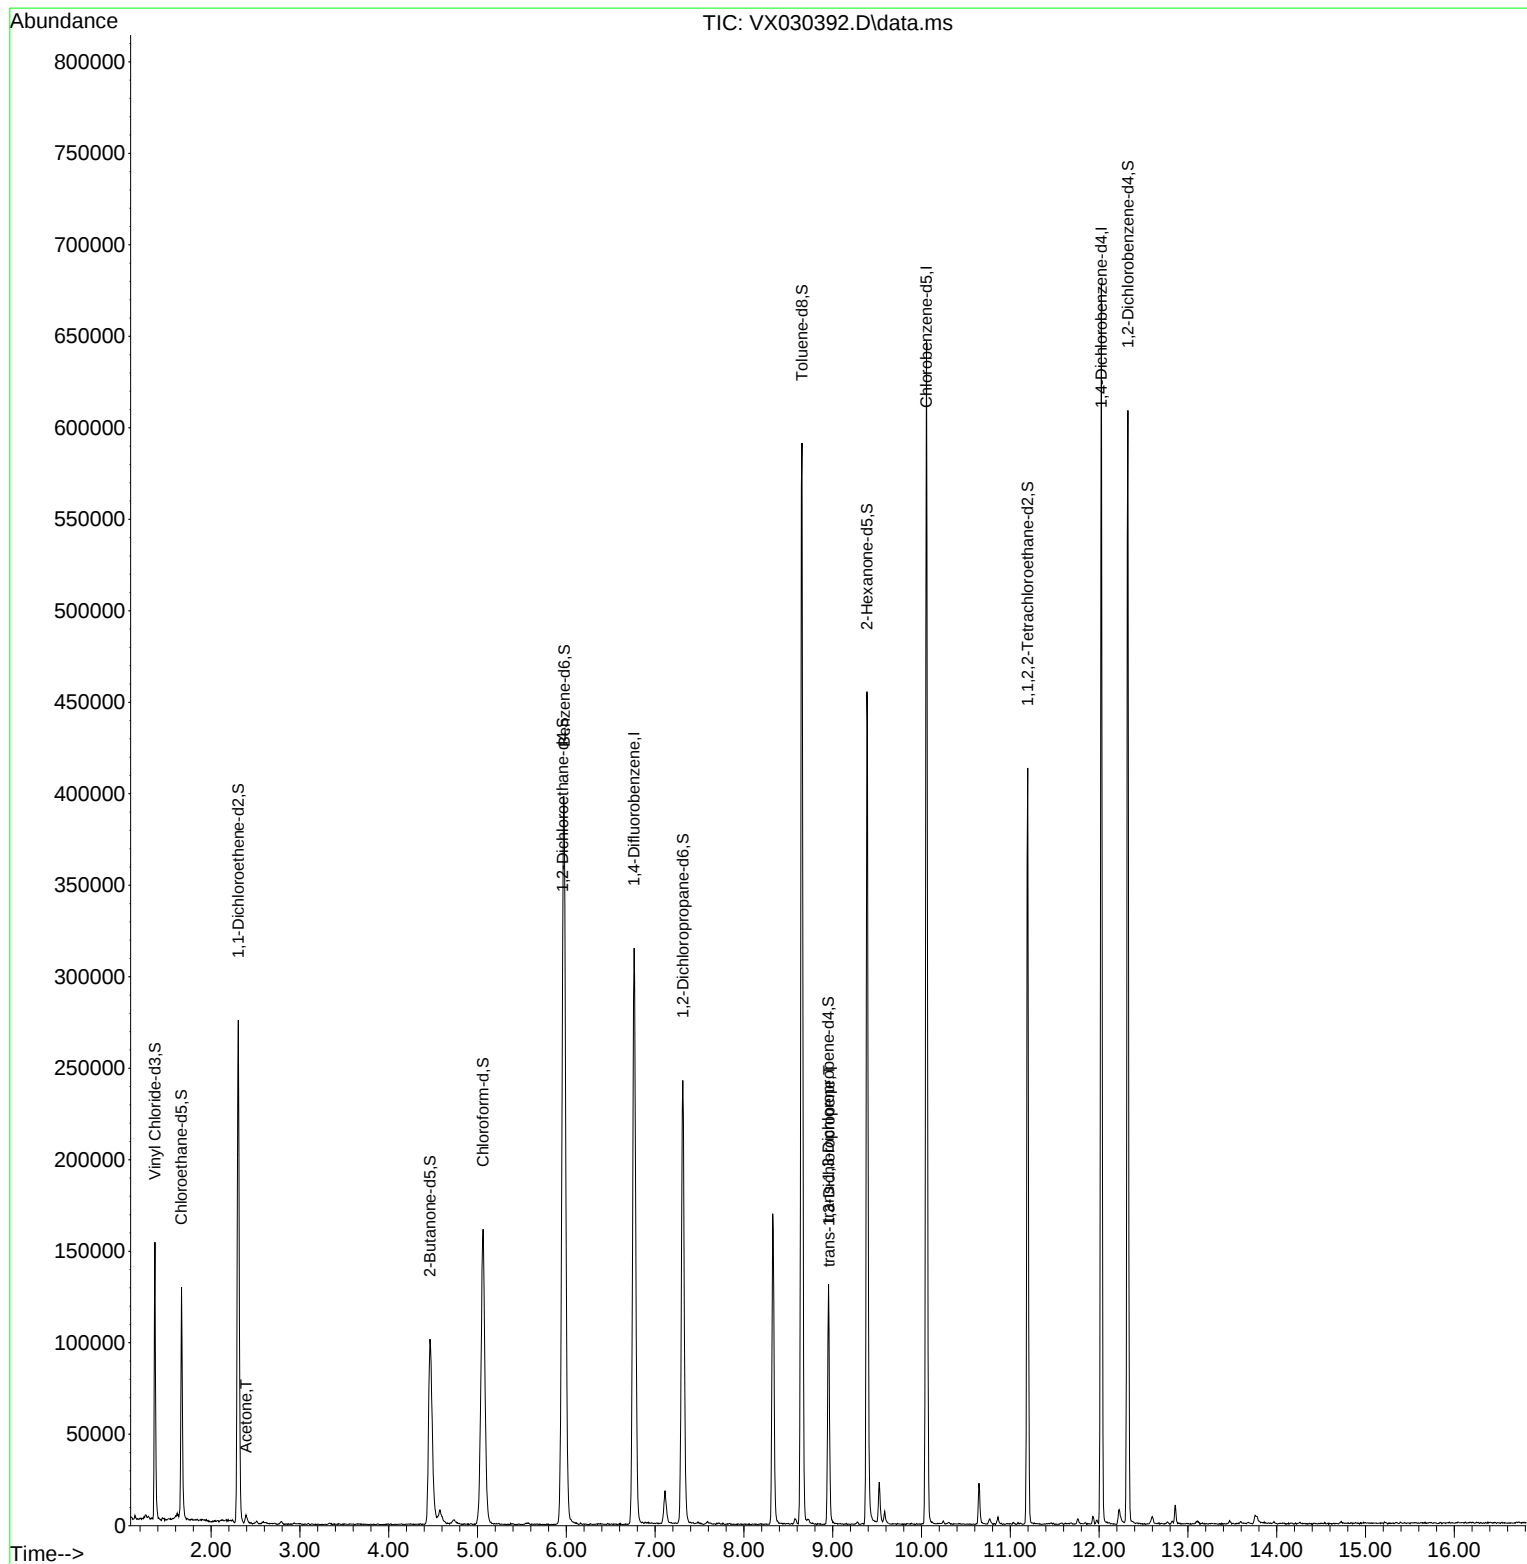

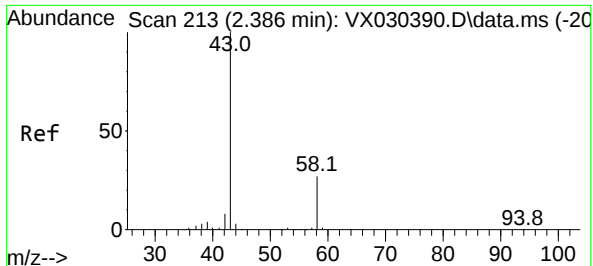

#13

Acetone

Concen: 3.860 ug/L

RT: 2.392 min Scan# 213

Delta R.T. 0.006 min

Lab File: VX030392.D

Acq: 04 Aug 2022 15:30

Instrument :

MSVOA_X

ClientSampleId :





C0ZF0

Tgt Ion: 43 Resp: 5233

Ion Ratio Lower Upper

43 100

58 34.5 0.0 57.8

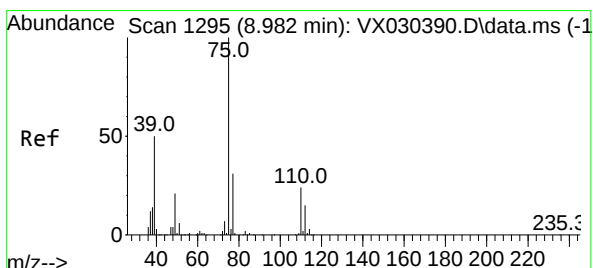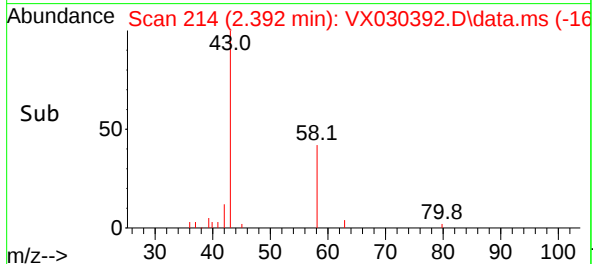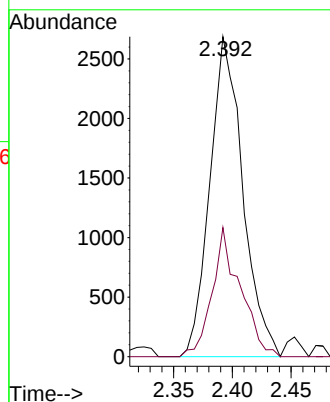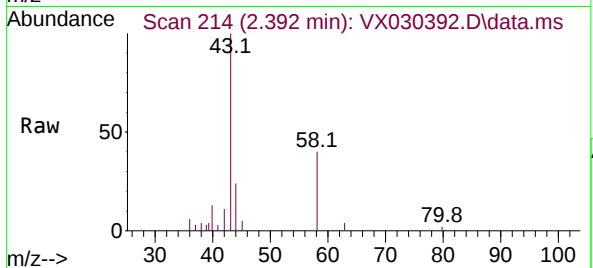

#44

trans-1,3-Dichloropropene

Concen: 0.888 ug/L

RT: 8.958 min Scan# 1291

Delta R.T. -0.024 min

Lab File: VX030392.D

Acq: 04 Aug 2022 15:30

Tgt Ion: 75 Resp: 3070

Ion Ratio Lower Upper

75 100

77 35.8 22.5 41.7

