

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX080422\  
 Data File : VX030392.D  
 Acq On : 04 Aug 2022 15:30  
 Operator : JC/MD  
 Sample : N4008-06  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 COZF0

Quant Time: Aug 05 05:26:17 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML080422WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Aug 05 05:25:14 2022  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|--------|----------|
| -----                         |                |      |            |          |        |          |
| Internal Standards            |                |      |            |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.763          | 114  | 310840     | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 10.055         | 117  | 277869     | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 125094     | 50.000   | ug/L   | 0.00     |
|                               |                |      |            |          |        |          |
| System Monitoring Compounds   |                |      |            |          |        |          |
| 4) Vinyl Chloride-d3          | 1.368          | 65   | 95394      | 47.789   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 135 |      | Recovery = | 95.580%  |        |          |
| 7) Chloroethane-d5            | 1.666          | 69   | 75863      | 53.911   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 130 |      | Recovery = | 107.820% |        |          |
| 11) 1,1-Dichloroethene-d2     | 2.307          | 63   | 153519     | 40.657   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 81.320%  |        |          |
| 21) 2-Butanone-d5             | 4.465          | 46   | 183656     | 99.298   | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 40 - 130 |      | Recovery = | 99.300%  |        |          |
| 24) Chloroform-d              | 5.062          | 84   | 189764     | 46.181   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 92.360%  |        |          |
| 26) 1,2-Dichloroethane-d4     | 5.958          | 65   | 130844     | 46.895   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 93.800%  |        |          |
| 32) Benzene-d6                | 5.977          | 84   | 381430     | 47.922   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 95.840%  |        |          |
| 36) 1,2-Dichloropropane-d6    | 7.312          | 67   | 122410     | 47.402   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 120 |      | Recovery = | 94.800%  |        |          |
| 41) Toluene-d8                | 8.653          | 98   | 349022     | 46.520   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 93.040%  |        |          |
| 43) trans-1,3-Dichloroprop... | 8.952          | 79   | 57446      | 44.716   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 89.440%  |        |          |
| 47) 2-Hexanone-d5             | 9.385          | 63   | 125530     | 95.366   | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 45 - 130 |      | Recovery = | 95.370%  |        |          |
| 56) 1,1,2,2-Tetrachloroeth... | 11.195         | 84   | 155402     | 45.808   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 120 |      | Recovery = | 91.620%  |        |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.323         | 152  | 117379     | 48.377   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 96.760%  |        |          |
|                               |                |      |            |          |        |          |
| Target Compounds              |                |      |            |          | Qvalue |          |
| 13) Acetone                   | 2.392          | 43   | 5233       | 3.860    | ug/L   | 89       |
| -----                         |                |      |            |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX080422\  
Data File : VX030392.D  
Acq On : 04 Aug 2022 15:30  
Operator : JC/MD  
Sample : N4008-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
C0ZF0

Quant Time: Aug 05 05:26:17 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML080422WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Aug 05 05:25:14 2022  
Response via : Initial Calibration

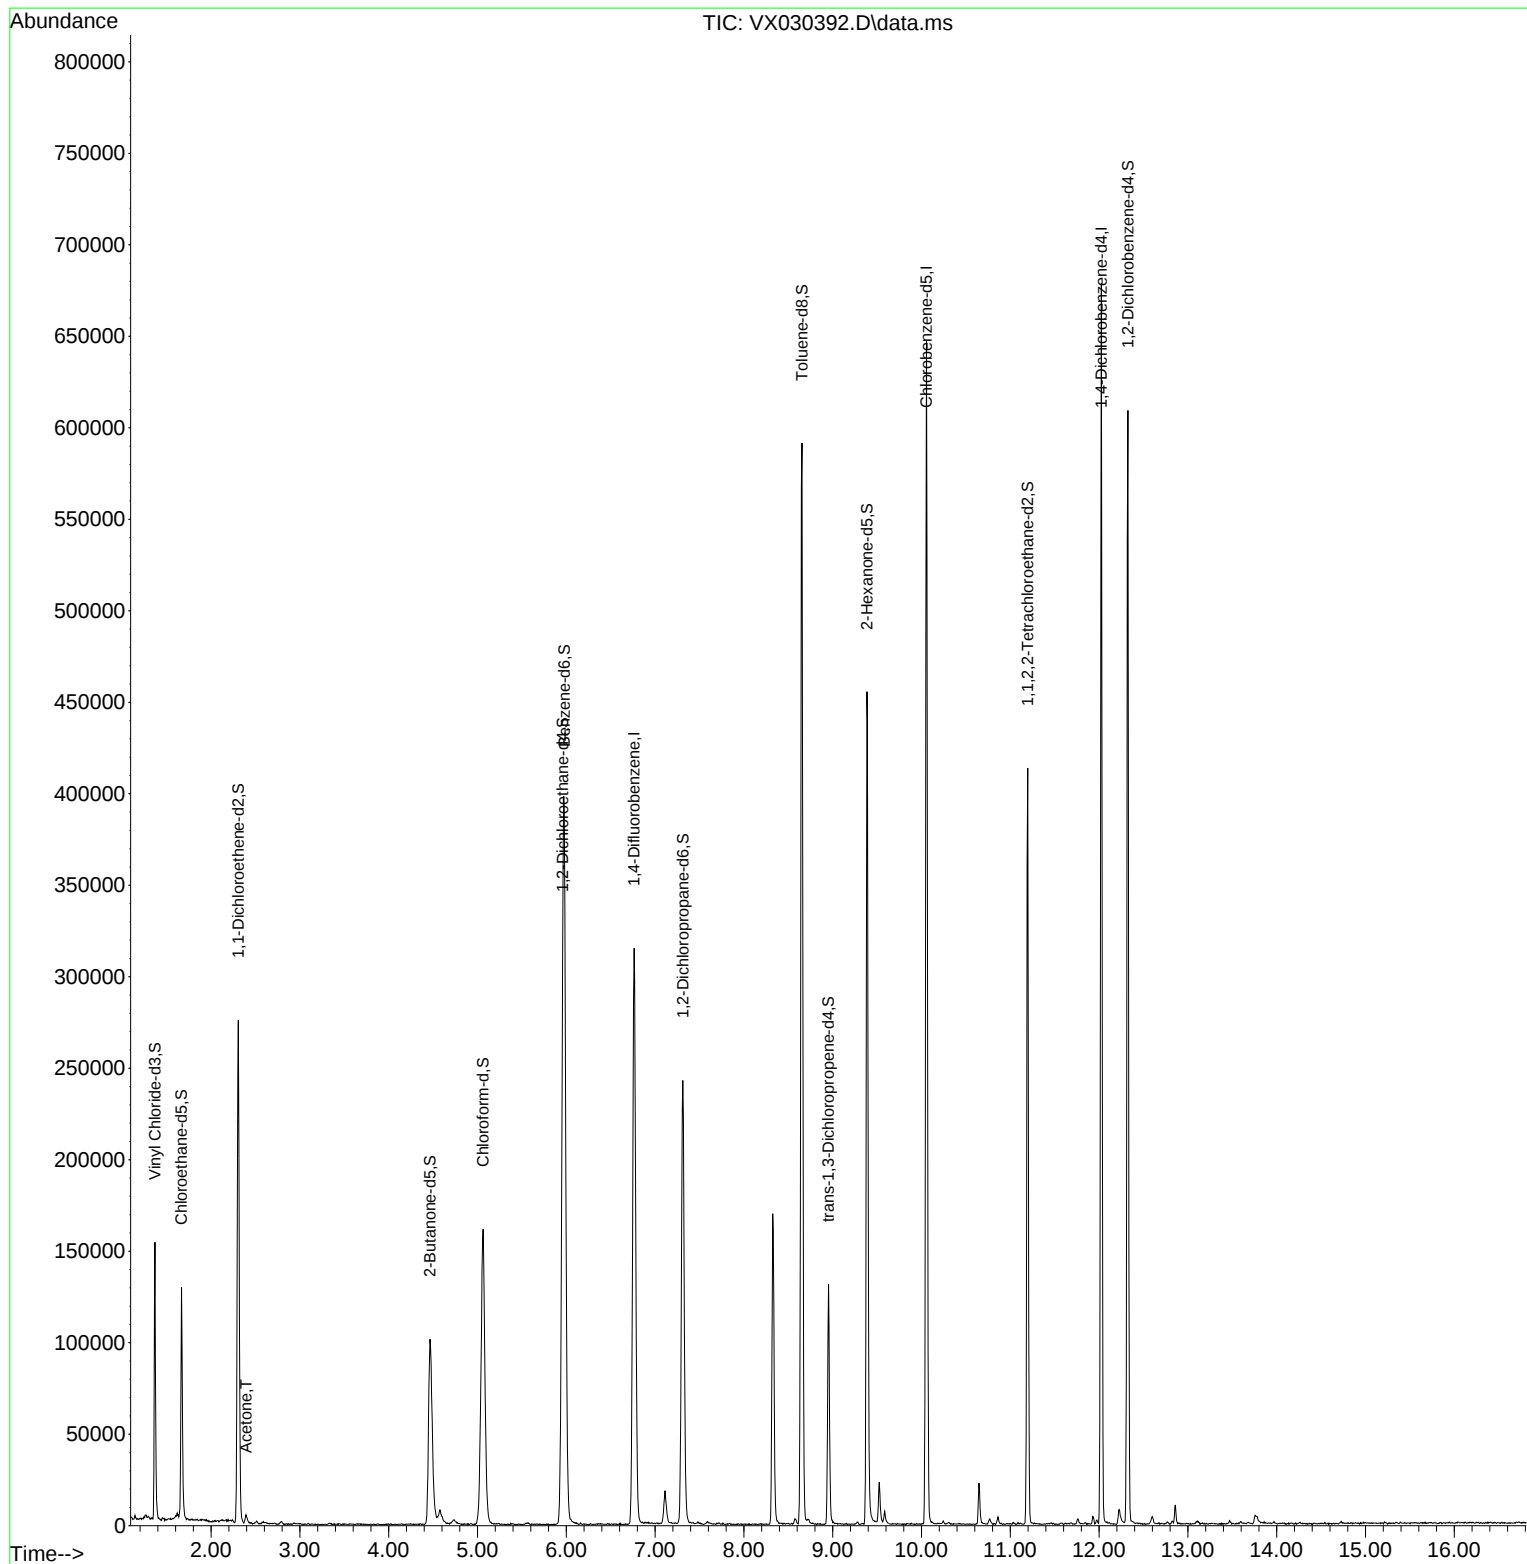

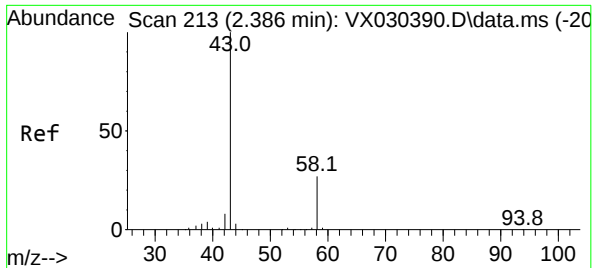

#13  
 Acetone  
 Concen: 3.860 ug/L  
 RT: 2.392 min Scan# 21  
 Delta R.T. 0.006 min  
 Lab File: VX030392.D  
 Acq: 04 Aug 2022 15:30

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 C0ZF0

Tgt Ion: 43 Resp: 5233  
 Ion Ratio Lower Upper  
 43 100  
 58 34.5 0.0 57.8

