

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030391.D
 Acq On : 04 Aug 2022 14:58
 Operator : JC/MD
 Sample : VX0804WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	150624	157376	13.33%	1.735%
2	1.666	91	95	105	rVB	115068	144927	12.27%	1.597%
3	2.307	194	200	211	rVB	250399	383837	32.50%	4.231%
4	2.435	220	221	223	rVB	1250	732	0.06%	0.008%
5	2.514	229	234	238	rVB3	2043	3171	0.27%	0.035%
6	2.709	264	266	268	rVB2	722	369	0.03%	0.004%
7	2.733	268	270	273	rVB2	581	699	0.06%	0.008%
8	2.788	273	279	286	rBV6	2449	4883	0.41%	0.054%
9	2.855	288	290	291	rBV	504	375	0.03%	0.004%
10	2.947	300	305	313	rVB5	2394	6413	0.54%	0.071%
11	3.056	320	323	325	rBV	499	527	0.04%	0.006%
12	3.087	325	328	330	rBV4	977	1142	0.10%	0.013%
13	3.337	367	369	372	rBV2	622	681	0.06%	0.008%
14	3.556	402	405	407	rBV2	565	457	0.04%	0.005%
15	4.008	478	479	483	rVB	429	407	0.03%	0.004%
16	4.215	512	513	518	rBV2	312	344	0.03%	0.004%
17	4.349	533	535	537	rBV	374	335	0.03%	0.004%
18	4.465	545	554	569	rBV	106063	303640	25.71%	3.347%
19	4.904	625	626	628	rVB	787	477	0.04%	0.005%
20	4.934	628	631	634	rBV2	466	676	0.06%	0.007%
21	5.062	640	652	668	rBV	159464	478438	40.51%	5.273%
22	5.391	700	706	714	rBV4	1195	3345	0.28%	0.037%
23	5.562	727	734	740	rVV5	2136	5449	0.46%	0.060%
24	5.690	754	755	758	rVB2	635	474	0.04%	0.005%
25	5.977	788	802	818	rBV2	405691	1180911	100.00%	13.016%
26	6.312	855	857	858	rBV	661	336	0.03%	0.004%
27	6.336	858	861	864	rBV	431	735	0.06%	0.008%
28	6.361	864	865	868	rVB2	445	419	0.04%	0.005%
29	6.434	875	877	880	rBV2	598	331	0.03%	0.004%
30	6.458	880	881	887	rVB2	869	850	0.07%	0.009%
31	6.513	888	890	896	rBV2	336	569	0.05%	0.006%
32	6.769	922	932	950	rBV	322807	750653	63.57%	8.274%
33	7.044	975	977	978	rBV2	412	347	0.03%	0.004%
34	7.117	981	989	999	rVB4	13000	31914	2.70%	0.352%
35	7.190	999	1001	1002	rBV2	528	493	0.04%	0.005%
36	7.312	1010	1021	1035	rBV	237164	539095	45.65%	5.942%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030391.D
 Acq On : 04 Aug 2022 14:58
 Operator : JC/MD
 Sample : VX0804WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.556	1060	1061	1065	rBV2	686	711	0.06%	0.008%
38	7.586	1065	1066	1068	rBV2	430	340	0.03%	0.004%
39	7.751	1091	1093	1096	rBV2	316	429	0.04%	0.005%
40	7.940	1121	1124	1127	rBV3	533	670	0.06%	0.007%
41	8.104	1148	1151	1152	rBV2	486	355	0.03%	0.004%
42	8.141	1155	1157	1160	rVB2	337	344	0.03%	0.004%
43	8.330	1181	1188	1200	rBV	184457	287823	24.37%	3.172%
44	8.519	1218	1219	1221	rVB	866	385	0.03%	0.004%
45	8.653	1234	1241	1250	rBV	607825	932938	79.00%	10.283%
46	8.915	1281	1284	1285	rBV2	838	804	0.07%	0.009%
47	8.952	1285	1290	1300	rBV	127426	187642	15.89%	2.068%
48	9.202	1330	1331	1334	rVB	556	339	0.03%	0.004%
49	9.232	1334	1336	1338	rBV2	412	334	0.03%	0.004%
50	9.275	1340	1343	1349	rVB3	2218	3370	0.29%	0.037%
51	9.336	1352	1353	1356	rBV3	477	514	0.04%	0.006%
52	9.385	1356	1361	1376	rBV	459908	677610	57.38%	7.468%
53	9.543	1386	1387	1388	rBV	704	370	0.03%	0.004%
54	9.604	1396	1397	1399	rBV	514	523	0.04%	0.006%
55	9.653	1404	1405	1410	rVB2	421	424	0.04%	0.005%
56	9.702	1410	1413	1418	rBV3	2585	3553	0.30%	0.039%
57	9.799	1428	1429	1432	rBV3	420	412	0.03%	0.005%
58	9.909	1444	1447	1452	rBV3	476	800	0.07%	0.009%
59	10.055	1466	1471	1480	rVV	620044	822801	69.68%	9.069%
60	10.202	1492	1495	1498	rVB3	1070	1337	0.11%	0.015%
61	10.311	1508	1513	1517	rBV5	1489	2559	0.22%	0.028%
62	10.458	1535	1537	1541	rVB2	530	456	0.04%	0.005%
63	10.653	1564	1569	1574	rVB4	1281	2359	0.20%	0.026%
64	10.744	1581	1584	1587	rBV2	423	618	0.05%	0.007%
65	10.811	1593	1595	1601	rVB2	401	638	0.05%	0.007%
66	10.970	1618	1621	1624	rVB2	807	786	0.07%	0.009%
67	11.092	1639	1641	1642	rBV	656	613	0.05%	0.007%
68	11.195	1652	1658	1666	rBV	418377	534039	45.22%	5.886%
69	11.457	1698	1701	1704	rBV2	1213	1478	0.13%	0.016%
70	11.640	1727	1731	1732	rBV2	425	438	0.04%	0.005%
71	11.701	1739	1741	1742	rBV	557	544	0.05%	0.006%
72	11.720	1742	1744	1745	rVB	755	465	0.04%	0.005%
73	11.817	1757	1760	1761	rBV	475	340	0.03%	0.004%
74	11.835	1761	1763	1768	rVB2	751	806	0.07%	0.009%
75	11.976	1783	1786	1789	rBV3	1909	1975	0.17%	0.022%
76	12.024	1789	1794	1802	rVV	635988	765333	64.81%	8.435%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030391.D
 Acq On : 04 Aug 2022 14:58
 Operator : JC/MD
 Sample : VX0804WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.226	1826	1827	1832	rVB3	765	736	0.06%	0.008%
78	12.268	1832	1834	1836	rVB	364	331	0.03%	0.004%
79	12.323	1837	1843	1851	rVV	632797	810222	68.61%	8.930%
80	12.585	1884	1886	1887	rBV	464	419	0.04%	0.005%
81	12.914	1938	1940	1941	rBV	498	379	0.03%	0.004%
82	12.933	1941	1943	1944	rVV	818	687	0.06%	0.008%
83	12.982	1948	1951	1953	rVV2	636	772	0.07%	0.009%
84	13.018	1953	1957	1960	rVV3	658	797	0.07%	0.009%
85	13.110	1970	1972	1979	rVB2	1935	2793	0.24%	0.031%
86	13.238	1991	1993	1997	rVB2	435	549	0.05%	0.006%
87	13.305	2003	2004	2006	rBV	409	357	0.03%	0.004%
88	13.390	2016	2018	2020	rVB2	367	389	0.03%	0.004%
89	13.420	2020	2023	2024	rBV2	679	713	0.06%	0.008%
90	13.475	2030	2032	2035	rVB	431	349	0.03%	0.004%
91	13.591	2049	2051	2055	rVB3	1709	1968	0.17%	0.022%
92	13.628	2055	2057	2058	rBV	391	348	0.03%	0.004%
93	13.744	2072	2076	2078	rBV2	495	737	0.06%	0.008%
94	13.780	2079	2082	2086	rVV	1596	2152	0.18%	0.024%
95	14.158	2142	2144	2146	rBV	417	397	0.03%	0.004%
96	15.231	2318	2320	2321	rBV	580	526	0.04%	0.006%
97	15.329	2334	2336	2337	rBV2	790	641	0.05%	0.007%
98	15.493	2359	2363	2366	rBV3	853	1219	0.10%	0.013%
99	16.060	2455	2456	2458	rBV	708	623	0.05%	0.007%
100	16.170	2472	2474	2476	rBV3	909	730	0.06%	0.008%




Sum of corrected areas: 9072936

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030391.D
Acq On : 04 Aug 2022 14:58
Operator : JC/MD
Sample : VX0804WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK668

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

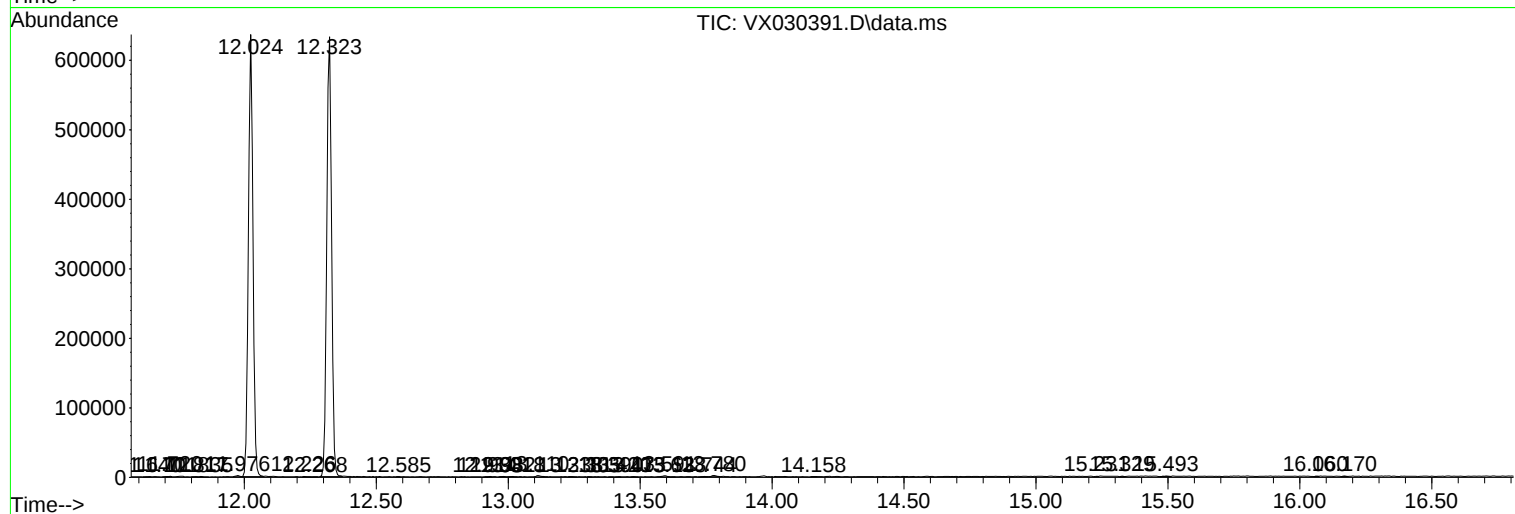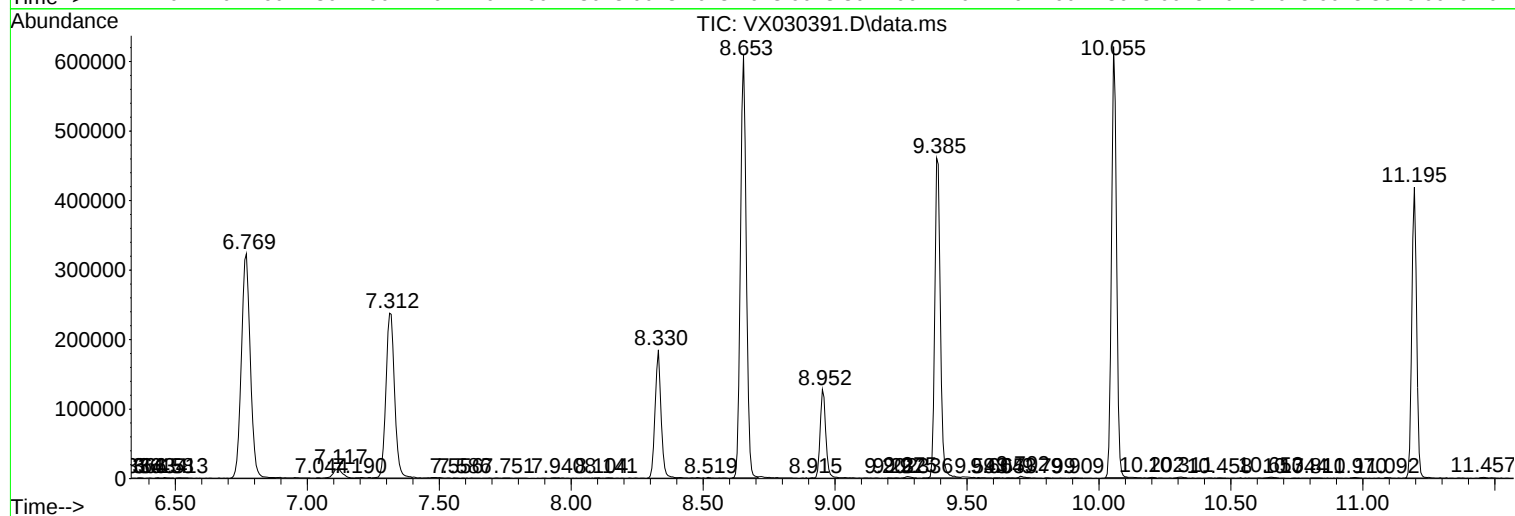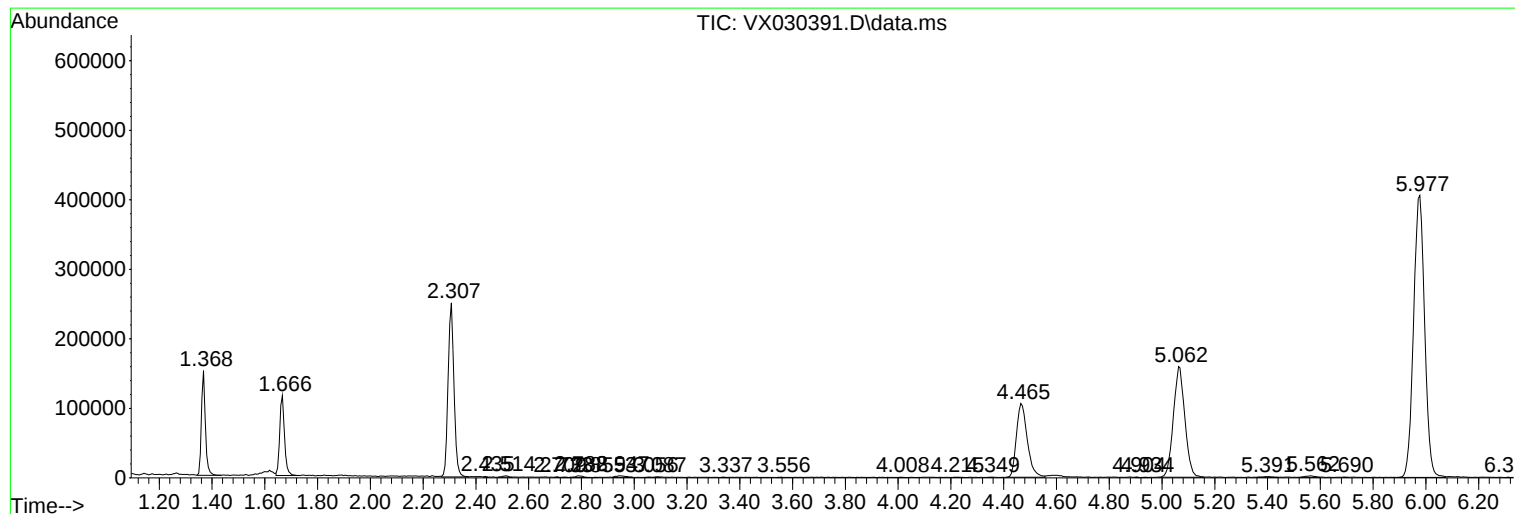

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030391.D
Acq On : 04 Aug 2022 14:58
Operator : JC/MD
Sample : VX0804WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK668

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030391.D
Acq On : 04 Aug 2022 14:58
Operator : JC/MD
Sample : VX0804WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK668

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc