

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030392.D
 Acq On : 04 Aug 2022 15:30
 Operator : JC/MD
 Sample : N4008-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COZF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	152056	159955	13.70%	1.726%
2	1.666	91	95	104	rVB	126940	154516	13.23%	1.667%
3	2.307	194	200	210	rVB	274904	419874	35.96%	4.531%
4	2.392	210	214	222	rVB	4610	7739	0.66%	0.084%
5	2.788	275	279	284	rVB4	1557	2743	0.23%	0.030%
6	2.867	291	292	294	rBV	618	445	0.04%	0.005%
7	2.941	300	304	306	rVV2	570	742	0.06%	0.008%
8	3.093	327	329	332	rVB3	744	781	0.07%	0.008%
9	3.136	332	336	340	rBV2	496	868	0.07%	0.009%
10	3.288	357	361	363	rBV2	273	415	0.04%	0.004%
11	3.331	365	368	371	rVV3	697	959	0.08%	0.010%
12	3.648	415	420	421	rBV3	513	792	0.07%	0.009%
13	3.800	440	445	448	rBV2	355	597	0.05%	0.006%
14	4.020	479	481	483	rBV2	476	440	0.04%	0.005%
15	4.245	516	518	523	rVB2	513	586	0.05%	0.006%
16	4.361	535	537	539	rVB2	456	408	0.03%	0.004%
17	4.465	544	554	566	rBV	101258	295673	25.32%	3.191%
18	4.696	590	592	593	rBV2	739	608	0.05%	0.007%
19	4.739	593	599	607	rVB5	2235	5840	0.50%	0.063%
20	4.849	616	617	620	rBV2	448	400	0.03%	0.004%
21	4.922	626	629	633	rVB2	479	720	0.06%	0.008%
22	5.062	637	652	665	rBV	161366	496842	42.55%	5.362%
23	5.343	695	698	701	rBV3	533	645	0.06%	0.007%
24	5.373	701	703	704	rBV	867	510	0.04%	0.006%
25	5.550	729	732	733	rBV2	703	784	0.07%	0.008%
26	5.971	786	801	822	rBV2	398116	1167653	100.00%	12.601%
27	6.160	830	832	835	rVB3	943	775	0.07%	0.008%
28	6.269	847	850	855	rBV2	630	916	0.08%	0.010%
29	6.355	863	864	867	rBV2	449	515	0.04%	0.006%
30	6.464	880	882	884	rBV2	620	607	0.05%	0.007%
31	6.763	922	931	945	rBV	314487	743226	63.65%	8.021%
32	6.885	949	951	955	rBV2	710	879	0.08%	0.009%
33	7.111	981	988	998	rBV3	17928	35914	3.08%	0.388%
34	7.312	1011	1021	1034	rBV	242013	529631	45.36%	5.716%
35	7.482	1047	1049	1051	rVB3	853	575	0.05%	0.006%
36	7.696	1082	1084	1086	rBV2	883	821	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030392.D
 Acq On : 04 Aug 2022 15:30
 Operator : JC/MD
 Sample : N4008-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COZF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.720	1086	1088	1091	rVV	913	948	0.08%	0.010%
38	7.934	1122	1123	1126	rBV2	404	397	0.03%	0.004%
39	8.098	1148	1150	1152	rBV	359	388	0.03%	0.004%
40	8.135	1155	1156	1159	rVB	535	390	0.03%	0.004%
41	8.324	1180	1187	1198	rBV	169647	285301	24.43%	3.079%
42	8.482	1211	1213	1215	rBV2	332	432	0.04%	0.005%
43	8.537	1220	1222	1224	rVB2	537	397	0.03%	0.004%
44	8.574	1224	1228	1234	rBV6	3059	5280	0.45%	0.057%
45	8.653	1234	1241	1250	rBV	590716	939864	80.49%	10.143%
46	8.775	1259	1261	1264	rVB3	760	631	0.05%	0.007%
47	8.805	1264	1266	1269	rVB	555	431	0.04%	0.005%
48	8.952	1284	1290	1298	rVV	130930	186327	15.96%	2.011%
49	9.153	1321	1323	1325	rVB	776	554	0.05%	0.006%
50	9.281	1341	1344	1348	rVB2	1364	1631	0.14%	0.018%
51	9.342	1348	1354	1355	rBV3	517	820	0.07%	0.009%
52	9.385	1355	1361	1375	rVV	455039	657740	56.33%	7.098%
53	9.525	1379	1384	1390	rVV2	23050	34745	2.98%	0.375%
54	9.586	1390	1394	1404	rVV	6873	10890	0.93%	0.118%
55	9.781	1425	1426	1429	rVB2	494	371	0.03%	0.004%
56	9.945	1451	1453	1454	rBV	591	445	0.04%	0.005%
57	10.006	1461	1463	1465	rBV	437	437	0.04%	0.005%
58	10.055	1465	1471	1480	rVV	646212	868479	74.38%	9.372%
59	10.244	1499	1502	1506	rVB2	1725	1938	0.17%	0.021%
60	10.647	1564	1568	1577	rVV	22446	29629	2.54%	0.320%
61	10.768	1584	1588	1594	rVB4	3134	5486	0.47%	0.059%
62	10.823	1594	1597	1598	rVB	569	582	0.05%	0.006%
63	10.860	1598	1603	1608	rBV3	4110	6043	0.52%	0.065%
64	10.994	1624	1625	1629	rVB3	435	370	0.03%	0.004%
65	11.037	1629	1632	1635	rVB2	982	1223	0.10%	0.013%
66	11.085	1638	1640	1642	rVV2	881	533	0.05%	0.006%
67	11.110	1642	1644	1649	rVB2	705	840	0.07%	0.009%
68	11.195	1652	1658	1666	rVV	413140	521720	44.68%	5.630%
69	11.488	1704	1706	1708	rVB2	799	616	0.05%	0.007%
70	11.579	1716	1721	1724	rVB4	763	1407	0.12%	0.015%
71	11.616	1724	1727	1729	rBV2	750	831	0.07%	0.009%
72	11.756	1747	1750	1755	rVB3	2620	3750	0.32%	0.040%
73	11.927	1775	1778	1782	rVB3	4130	5124	0.44%	0.055%
74	11.976	1782	1786	1789	rBV3	2164	2961	0.25%	0.032%
75	12.024	1789	1794	1803	rBV	677693	810900	69.45%	8.751%
76	12.226	1822	1827	1836	rBV2	8104	17629	1.51%	0.190%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030392.D
 Acq On : 04 Aug 2022 15:30
 Operator : JC/MD
 Sample : N4008-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0ZF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1851	rVV	607703	770151	65.96%	8.311%
78	12.543	1876	1879	1880	rBV2	442	497	0.04%	0.005%
79	12.597	1882	1888	1897	rVV5	4064	8041	0.69%	0.087%
80	12.744	1910	1912	1913	rBV	493	397	0.03%	0.004%
81	12.768	1913	1916	1920	rVB4	1301	1795	0.15%	0.019%
82	12.823	1922	1925	1927	rVV3	1540	1928	0.17%	0.021%
83	12.860	1927	1931	1935	rVB2	9978	12301	1.05%	0.133%
84	13.103	1968	1971	1976	rVB5	1938	3532	0.30%	0.038%
85	13.164	1976	1981	1984	rBV2	881	1300	0.11%	0.014%
86	13.244	1992	1994	1996	rBV3	334	380	0.03%	0.004%
87	13.353	2009	2012	2015	rVB2	433	374	0.03%	0.004%
88	13.469	2028	2031	2035	rVB4	1912	2584	0.22%	0.028%
89	13.591	2048	2051	2054	rBV3	1236	1688	0.14%	0.018%
90	13.756	2073	2078	2081	rBV4	4730	8719	0.75%	0.094%
91	14.115	2135	2137	2139	rBV	594	616	0.05%	0.007%
92	14.262	2154	2161	2163	rBV3	1076	1775	0.15%	0.019%
93	14.414	2184	2186	2187	rBV	717	594	0.05%	0.006%
94	14.725	2232	2237	2239	rBV5	1349	1756	0.15%	0.019%
95	14.865	2258	2260	2262	rBV2	545	583	0.05%	0.006%
96	14.945	2271	2273	2274	rBV	858	604	0.05%	0.007%
97	15.213	2315	2317	2318	rBV2	1164	878	0.08%	0.009%
98	15.268	2323	2326	2327	rBV2	685	786	0.07%	0.008%
99	15.390	2344	2346	2350	rBV3	761	744	0.06%	0.008%
100	16.292	2492	2494	2498	rVB3	615	630	0.05%	0.007%




Sum of corrected areas: 9266527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030392.D
Acq On : 04 Aug 2022 15:30
Operator : JC/MD
Sample : N4008-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

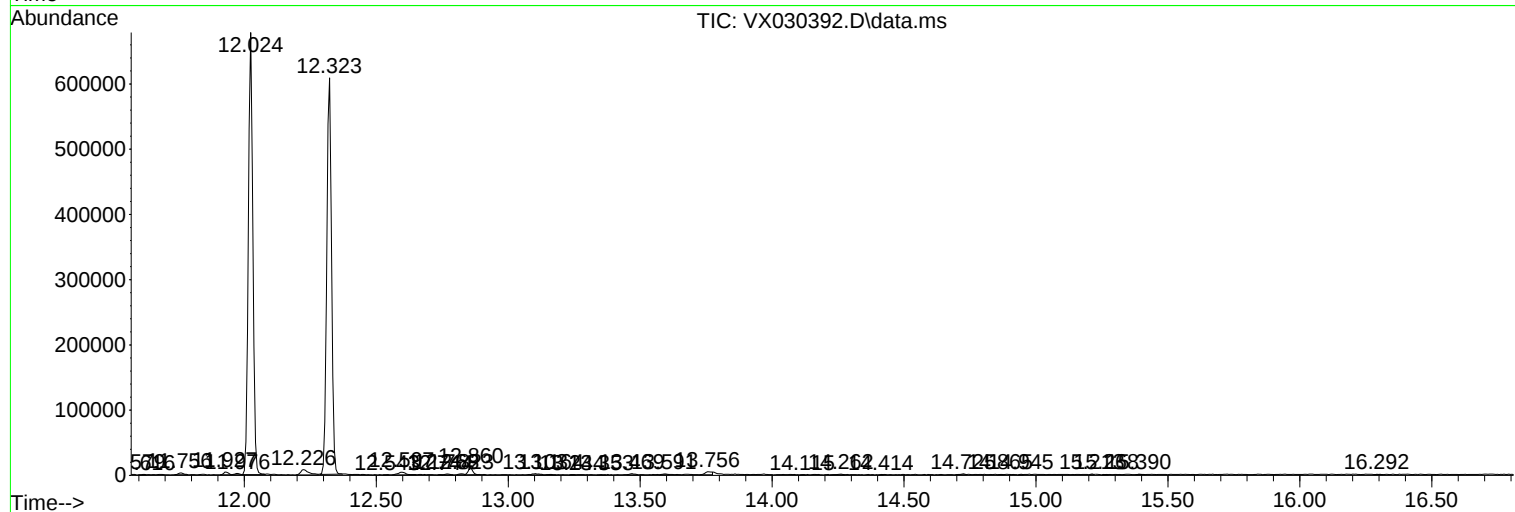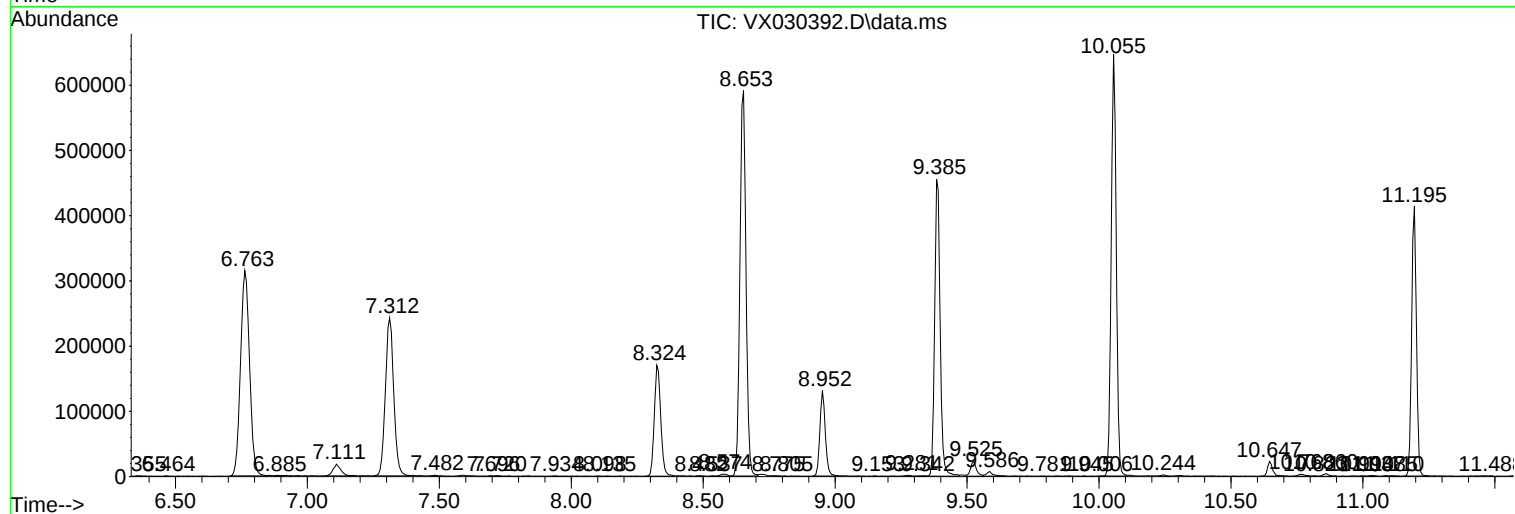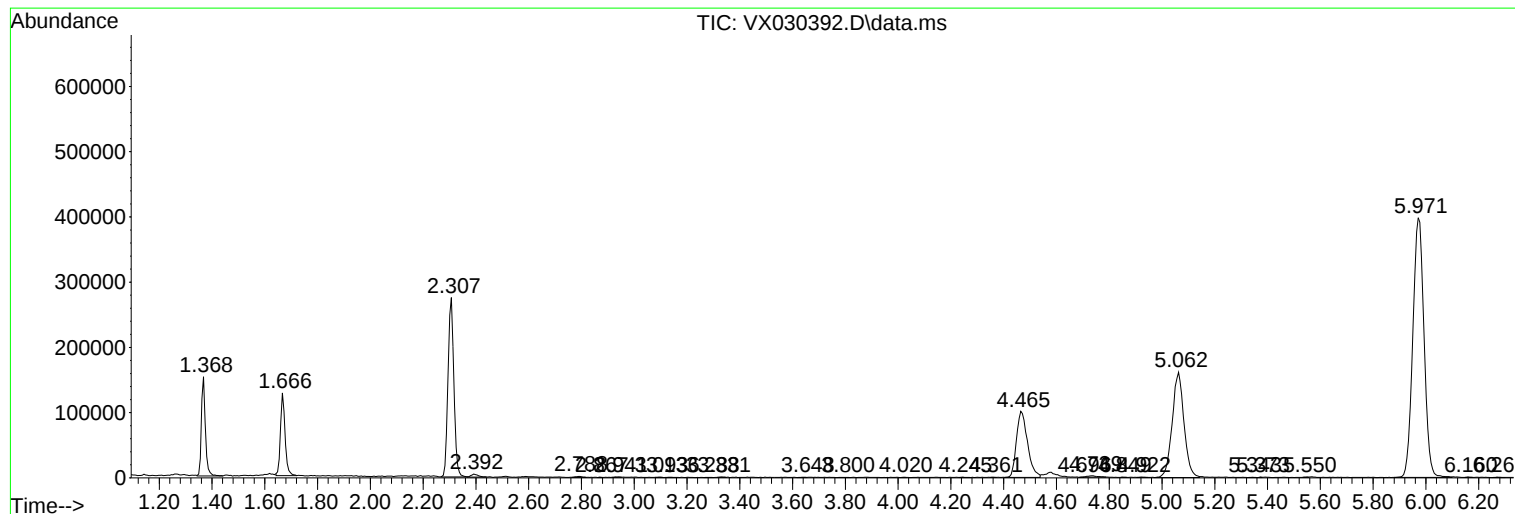

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030392.D
Acq On : 04 Aug 2022 15:30
Operator : JC/MD
Sample : N4008-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030392.D
Acq On : 04 Aug 2022 15:30
Operator : JC/MD
Sample : N4008-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0ZF0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc