

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030393.D
 Acq On : 04 Aug 2022 15:53
 Operator : JC/MD
 Sample : N4003-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	178013	186893	14.32%	1.866%
2	1.666	91	95	107	rVB	131079	156810	12.02%	1.566%
3	2.306	194	200	210	rBV	310056	462132	35.41%	4.614%
4	2.514	232	234	239	rVB2	1366	1297	0.10%	0.013%
5	2.660	256	258	260	rVB2	469	420	0.03%	0.004%
6	2.691	260	263	264	rVB	452	373	0.03%	0.004%
7	2.782	276	278	280	rBV3	958	1127	0.09%	0.011%
8	2.873	291	293	295	rVB2	429	299	0.02%	0.003%
9	2.959	305	307	310	rVB	475	426	0.03%	0.004%
10	3.062	323	324	325	rBV	484	284	0.02%	0.003%
11	3.105	325	331	333	rVB3	1460	2816	0.22%	0.028%
12	3.172	340	342	345	rBV2	549	567	0.04%	0.006%
13	3.306	362	364	366	rBV2	539	338	0.03%	0.003%
14	3.428	383	384	387	rBV	349	353	0.03%	0.004%
15	3.465	387	390	393	rVB2	542	772	0.06%	0.008%
16	3.501	393	396	397	rBV2	397	451	0.03%	0.005%
17	3.532	399	401	402	rBV2	318	288	0.02%	0.003%
18	3.715	430	431	433	rBV	348	242	0.02%	0.002%
19	3.745	433	436	437	rBV2	417	467	0.04%	0.005%
20	3.965	468	472	473	rBV	469	530	0.04%	0.005%
21	3.983	473	475	478	rBV	315	366	0.03%	0.004%
22	4.178	504	507	509	rVB2	379	461	0.04%	0.005%
23	4.477	545	556	573	rVV2	138412	507630	38.90%	5.068%
24	4.836	613	615	618	rBV2	354	406	0.03%	0.004%
25	4.971	636	637	638	rVV	612	263	0.02%	0.003%
26	4.989	638	640	641	rVV2	605	427	0.03%	0.004%
27	5.062	641	652	669	rVB	167181	521321	39.95%	5.205%
28	5.336	696	697	699	rBV2	337	295	0.02%	0.003%
29	5.550	727	732	733	rBV	860	1061	0.08%	0.011%
30	5.763	766	767	770	rBV2	336	299	0.02%	0.003%
31	5.812	773	775	777	rBV2	298	317	0.02%	0.003%
32	5.873	783	785	787	rBV2	317	260	0.02%	0.003%
33	5.977	789	802	821	rBV2	440810	1305065	100.00%	13.030%
34	6.354	861	864	866	rBV2	564	490	0.04%	0.005%
35	6.373	866	867	870	rBV2	430	479	0.04%	0.005%
36	6.763	920	931	947	rBV	301521	728323	55.81%	7.272%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030393.D
 Acq On : 04 Aug 2022 15:53
 Operator : JC/MD
 Sample : N4003-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.123	982	990	1001	rBV4	21529	53834	4.13%	0.538%
38	7.312	1012	1021	1033	rBV	268199	586768	44.96%	5.859%
39	7.452	1042	1044	1045	rBV2	664	415	0.03%	0.004%
40	7.482	1045	1049	1052	rBV2	959	1360	0.10%	0.014%
41	7.543	1057	1059	1062	rBV2	483	275	0.02%	0.003%
42	7.586	1062	1066	1073	rVB3	347	786	0.06%	0.008%
43	7.690	1082	1083	1085	rBV	553	368	0.03%	0.004%
44	7.775	1094	1097	1101	rBV3	428	623	0.05%	0.006%
45	7.873	1111	1113	1114	rBV	356	239	0.02%	0.002%
46	8.001	1132	1134	1135	rBV	527	305	0.02%	0.003%
47	8.141	1155	1157	1159	rVB	445	309	0.02%	0.003%
48	8.238	1172	1173	1177	rVB2	430	501	0.04%	0.005%
49	8.275	1177	1179	1180	rBV	526	246	0.02%	0.002%
50	8.330	1180	1188	1201	rBV	194631	318584	24.41%	3.181%
51	8.531	1220	1221	1222	rBV	441	258	0.02%	0.003%
52	8.653	1234	1241	1251	rBV	662426	1043250	79.94%	10.416%
53	8.756	1257	1258	1263	rVB2	1034	1024	0.08%	0.010%
54	8.878	1276	1278	1279	rBV2	615	347	0.03%	0.003%
55	8.952	1284	1290	1299	rBV	141474	206919	15.86%	2.066%
56	9.275	1337	1343	1351	rVB	48414	72205	5.53%	0.721%
57	9.384	1356	1361	1378	rVV	524471	741915	56.85%	7.408%
58	9.805	1425	1430	1431	rBV3	537	856	0.07%	0.009%
59	9.848	1435	1437	1439	rBV2	400	291	0.02%	0.003%
60	10.055	1465	1471	1485	rVV	622575	820068	62.84%	8.188%
61	10.305	1510	1512	1516	rVB3	1183	1363	0.10%	0.014%
62	10.360	1518	1521	1524	rBV2	673	1061	0.08%	0.011%
63	10.439	1530	1534	1537	rBV	651	1053	0.08%	0.011%
64	10.482	1539	1541	1542	rVV	396	300	0.02%	0.003%
65	10.524	1547	1548	1550	rVB	606	276	0.02%	0.003%
66	10.592	1556	1559	1560	rBV2	335	277	0.02%	0.003%
67	10.622	1560	1564	1566	rBV2	371	473	0.04%	0.005%
68	10.829	1596	1598	1602	rVB2	514	638	0.05%	0.006%
69	10.860	1602	1603	1605	rBV2	455	380	0.03%	0.004%
70	10.963	1617	1620	1624	rVB2	873	902	0.07%	0.009%
71	11.085	1638	1640	1641	rBV2	413	310	0.02%	0.003%
72	11.195	1652	1658	1669	rBV	468195	604326	46.31%	6.034%
73	11.543	1713	1715	1719	rBV3	501	632	0.05%	0.006%
74	11.677	1733	1737	1740	rVB2	425	543	0.04%	0.005%
75	11.707	1740	1742	1744	rBV2	649	712	0.05%	0.007%
76	11.756	1748	1750	1752	rBV3	723	694	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030393.D
 Acq On : 04 Aug 2022 15:53
 Operator : JC/MD
 Sample : N4003-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.902	1771	1774	1776	rVB2	585	714	0.05%	0.007%
78	11.927	1776	1778	1779	rBV	668	690	0.05%	0.007%
79	11.969	1783	1785	1789	rVV3	1196	1474	0.11%	0.015%
80	12.024	1789	1794	1808	rVV	636539	769318	58.95%	7.681%
81	12.183	1819	1820	1823	rVB2	583	501	0.04%	0.005%
82	12.323	1837	1843	1852	rBV	689852	881904	67.58%	8.805%
83	12.463	1864	1866	1867	rBV2	687	451	0.03%	0.005%
84	12.768	1915	1916	1919	rVB3	603	427	0.03%	0.004%
85	12.798	1919	1921	1923	rBV2	370	403	0.03%	0.004%
86	12.835	1925	1927	1929	rVV	378	285	0.02%	0.003%
87	12.908	1938	1939	1942	rBV2	541	553	0.04%	0.006%
88	12.987	1951	1952	1955	rBV	440	447	0.03%	0.004%
89	13.280	1998	2000	2001	rBV	460	307	0.02%	0.003%
90	13.585	2046	2050	2051	rBV	911	946	0.07%	0.009%
91	13.707	2068	2070	2074	rBV2	658	821	0.06%	0.008%
92	13.774	2078	2081	2086	rVV4	1342	2178	0.17%	0.022%
93	13.823	2087	2089	2090	rVB	648	373	0.03%	0.004%
94	14.012	2118	2120	2123	rVB2	642	673	0.05%	0.007%
95	14.134	2136	2140	2141	rVB2	694	730	0.06%	0.007%
96	14.152	2141	2143	2146	rBV2	629	619	0.05%	0.006%
97	14.304	2166	2168	2169	rBV	510	361	0.03%	0.004%
98	14.359	2174	2177	2179	rBV2	564	586	0.04%	0.006%
99	14.768	2242	2244	2246	rBV3	501	304	0.02%	0.003%
100	15.292	2328	2330	2331	rBV	625	482	0.04%	0.005%




Sum of corrected areas: 10015581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030393.D
Acq On : 04 Aug 2022 15:53
Operator : JC/MD
Sample : N4003-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

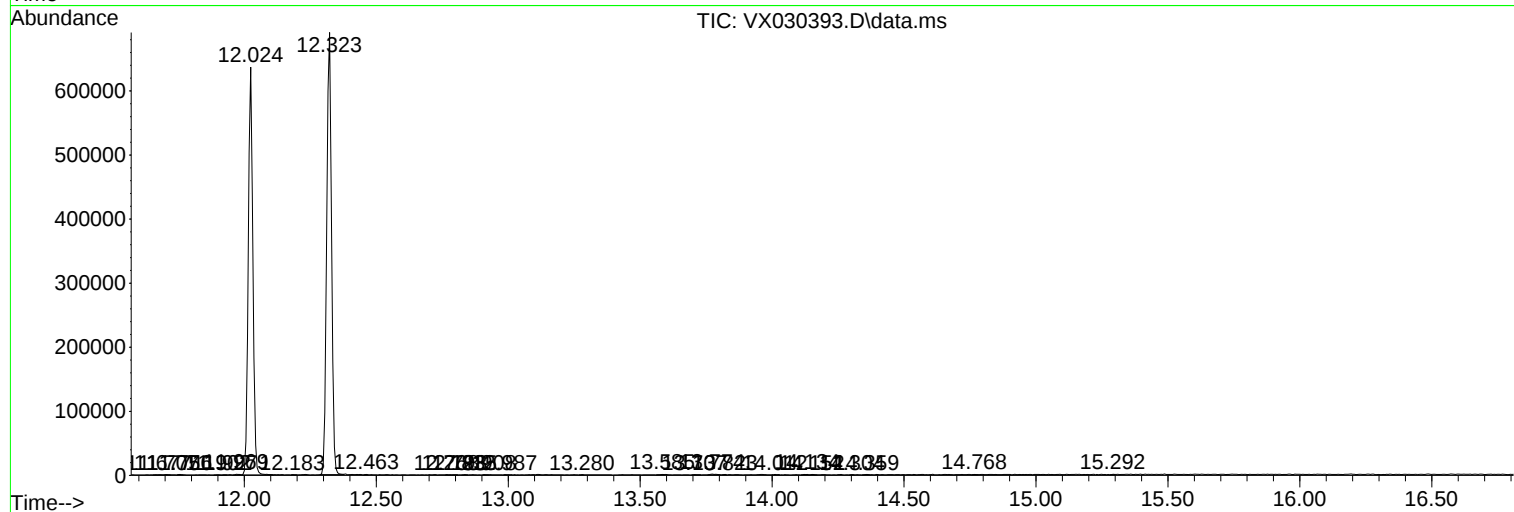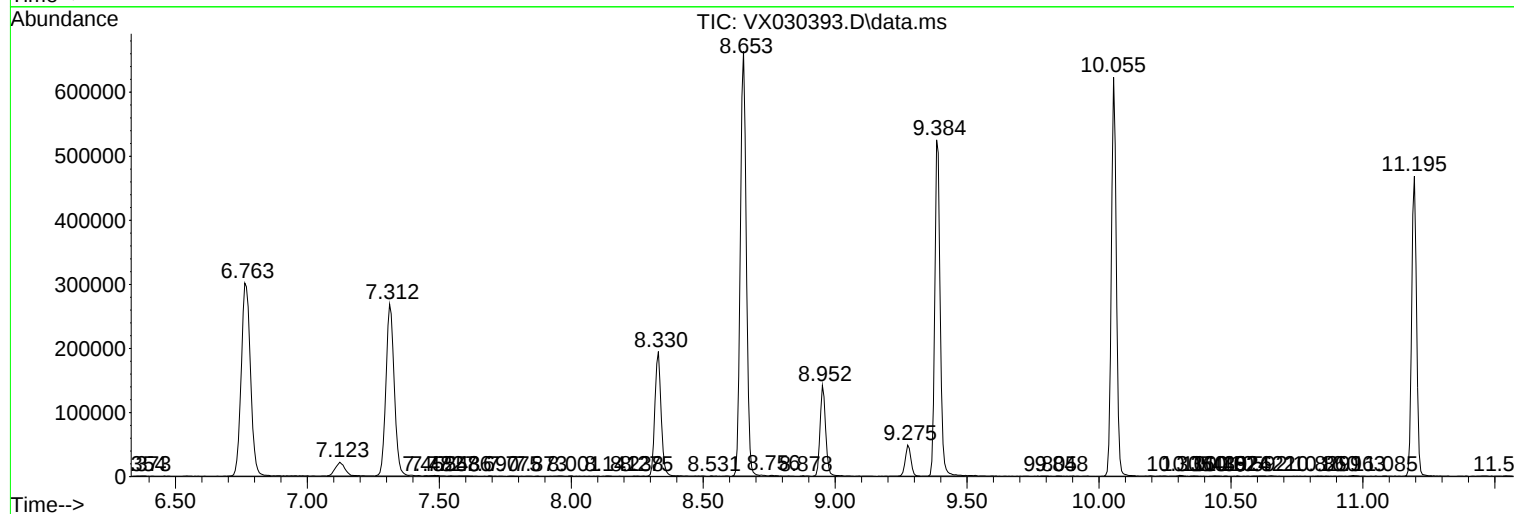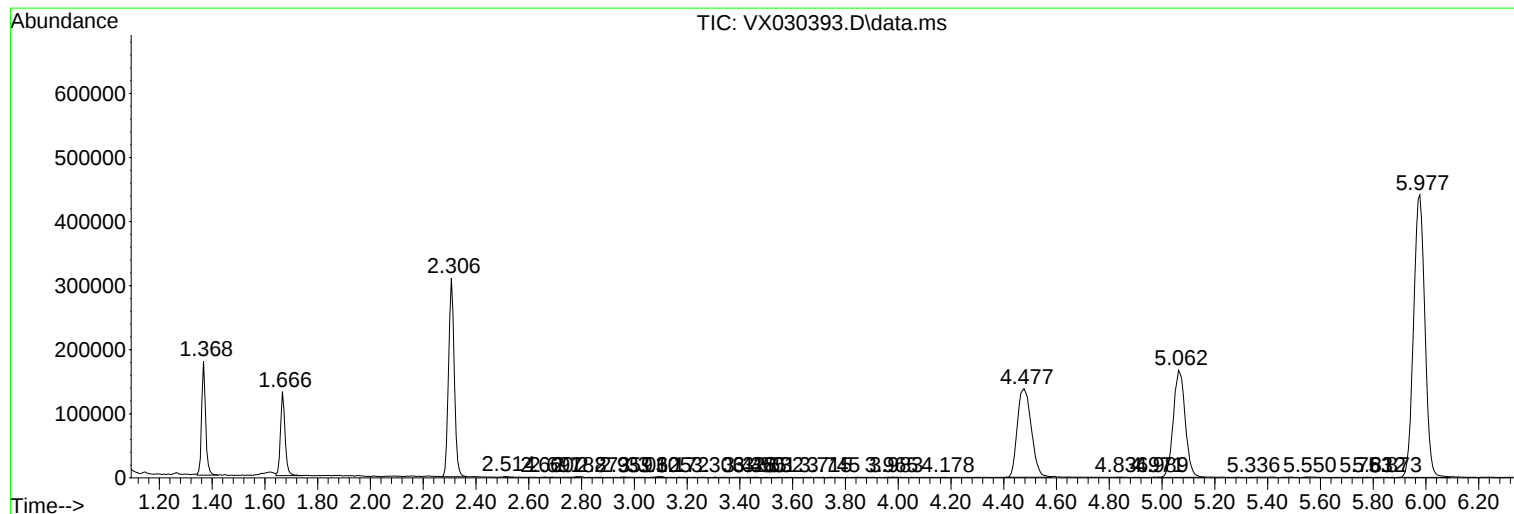

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030393.D
Acq On : 04 Aug 2022 15:53
Operator : JC/MD
Sample : N4003-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030393.D
Acq On : 04 Aug 2022 15:53
Operator : JC/MD
Sample : N4003-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc