

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030394.D
 Acq On : 04 Aug 2022 16:17
 Operator : JC/MD
 Sample : N4003-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	174636	184318	10.39%	1.696%
2	1.666	91	95	104	rVB	125629	154562	8.71%	1.422%
3	2.306	194	200	211	rVB	289201	453895	25.58%	4.176%
4	2.514	231	234	239	rVB3	1033	1492	0.08%	0.014%
5	2.660	255	258	260	rVB2	390	471	0.03%	0.004%
6	2.715	264	267	270	rVV3	607	859	0.05%	0.008%
7	2.739	270	271	274	rVB2	699	380	0.02%	0.003%
8	2.794	274	280	285	rBV3	1633	2724	0.15%	0.025%
9	2.855	289	290	293	rVV2	489	463	0.03%	0.004%
10	3.026	314	318	320	rBV2	424	558	0.03%	0.005%
11	3.093	323	329	335	rVV3	5482	10336	0.58%	0.095%
12	3.227	347	351	352	rBV2	394	538	0.03%	0.005%
13	3.251	352	355	357	rVB2	460	459	0.03%	0.004%
14	3.276	357	359	361	rBV	454	472	0.03%	0.004%
15	3.446	383	387	388	rBV2	349	461	0.03%	0.004%
16	3.574	404	408	410	rBV2	625	695	0.04%	0.006%
17	3.959	467	471	473	rVV3	508	607	0.03%	0.006%
18	4.495	545	559	582	rBV2	581927	1774245	100.00%	16.324%
19	4.885	621	623	626	rBV	565	695	0.04%	0.006%
20	4.946	631	633	636	rBV	471	642	0.04%	0.006%
21	5.068	640	653	671	rVV	160011	505943	28.52%	4.655%
22	5.263	682	685	687	rBV3	599	680	0.04%	0.006%
23	5.288	687	689	694	rVV2	338	398	0.02%	0.004%
24	5.391	703	706	711	rVV4	552	872	0.05%	0.008%
25	5.538	728	730	731	rBV	786	535	0.03%	0.005%
26	5.556	731	733	734	rBV	736	597	0.03%	0.005%
27	5.976	790	802	817	rVV2	438613	1266696	71.39%	11.654%
28	6.336	859	861	862	rBV	426	365	0.02%	0.003%
29	6.367	864	866	868	rVV	898	650	0.04%	0.006%
30	6.415	872	874	876	rBV2	452	576	0.03%	0.005%
31	6.598	902	904	907	rBV2	310	420	0.02%	0.004%
32	6.659	910	914	915	rBV	408	536	0.03%	0.005%
33	6.769	921	932	947	rBV	280409	687554	38.75%	6.326%
34	7.007	969	971	976	rBV4	442	711	0.04%	0.007%
35	7.117	982	989	997	rBV5	10796	27199	1.53%	0.250%
36	7.214	1001	1005	1008	rBV4	666	982	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030394.D
 Acq On : 04 Aug 2022 16:17
 Operator : JC/MD
 Sample : N4003-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1013	1021	1038	rBV	259601	575731	32.45%	5.297%
38	7.543	1057	1059	1060	rBV	556	374	0.02%	0.003%
39	7.586	1063	1066	1068	rVB2	536	528	0.03%	0.005%
40	7.702	1082	1085	1086	rBV2	378	380	0.02%	0.003%
41	8.104	1148	1151	1152	rVB2	493	380	0.02%	0.003%
42	8.116	1152	1153	1158	rBV2	471	583	0.03%	0.005%
43	8.153	1158	1159	1162	rVB2	467	362	0.02%	0.003%
44	8.208	1165	1168	1170	rBV2	385	391	0.02%	0.004%
45	8.330	1181	1188	1199	rVV	185798	304492	17.16%	2.802%
46	8.567	1224	1227	1228	rBV2	454	485	0.03%	0.004%
47	8.653	1234	1241	1251	rBV	650645	1011865	57.03%	9.310%
48	8.897	1279	1281	1284	rVB2	434	384	0.02%	0.004%
49	8.952	1284	1290	1300	rBV	135345	200622	11.31%	1.846%
50	9.122	1314	1318	1322	rVB3	598	1163	0.07%	0.011%
51	9.171	1322	1326	1327	rBV	504	645	0.04%	0.006%
52	9.281	1341	1344	1349	rVB3	1059	1057	0.06%	0.010%
53	9.384	1356	1361	1379	rBV	472245	690142	38.90%	6.350%
54	9.701	1411	1413	1415	rVB2	603	527	0.03%	0.005%
55	9.775	1423	1425	1428	rVB2	527	363	0.02%	0.003%
56	9.957	1453	1455	1459	rVV	388	365	0.02%	0.003%
57	10.055	1465	1471	1479	rBV	590469	784855	44.24%	7.221%
58	10.287	1507	1509	1510	rBV	513	428	0.02%	0.004%
59	10.305	1510	1512	1516	rVV3	807	1025	0.06%	0.009%
60	10.342	1516	1518	1520	rVV2	441	418	0.02%	0.004%
61	10.366	1520	1522	1527	rVB2	556	654	0.04%	0.006%
62	10.415	1527	1530	1531	rBV	530	410	0.02%	0.004%
63	10.634	1563	1566	1567	rBV2	546	518	0.03%	0.005%
64	10.787	1589	1591	1592	rVB	551	383	0.02%	0.004%
65	10.860	1600	1603	1604	rBV2	772	520	0.03%	0.005%
66	10.969	1619	1621	1624	rVB3	716	748	0.04%	0.007%
67	11.037	1630	1632	1635	rBV2	433	449	0.03%	0.004%
68	11.195	1652	1658	1668	rBV	449955	572689	32.28%	5.269%
69	11.390	1688	1690	1694	rVV2	342	448	0.03%	0.004%
70	11.713	1741	1743	1746	rBV2	819	853	0.05%	0.008%
71	11.762	1748	1751	1752	rVB	643	605	0.03%	0.006%
72	11.975	1782	1786	1788	rBV	669	753	0.04%	0.007%
73	12.024	1789	1794	1801	rBV	585183	725082	40.87%	6.671%
74	12.274	1833	1835	1837	rBV2	655	625	0.04%	0.006%
75	12.323	1837	1843	1854	rVV	706121	885235	49.89%	8.145%
76	12.701	1904	1905	1908	rBV2	392	467	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030394.D
 Acq On : 04 Aug 2022 16:17
 Operator : JC/MD
 Sample : N4003-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.061	1961	1964	1966	rBV	508	562	0.03%	0.005%
78	13.109	1970	1972	1977	rVB	978	1159	0.07%	0.011%
79	13.176	1980	1983	1984	rBV	400	432	0.02%	0.004%
80	13.554	2043	2045	2048	rBV	454	446	0.03%	0.004%
81	13.597	2048	2052	2054	rVV2	688	968	0.05%	0.009%
82	13.652	2058	2061	2064	rBV3	494	690	0.04%	0.006%
83	13.682	2064	2066	2068	rBV	509	500	0.03%	0.005%
84	13.707	2068	2070	2073	rVB2	766	844	0.05%	0.008%
85	13.737	2073	2075	2077	rBV2	490	510	0.03%	0.005%
86	13.957	2109	2111	2114	rBV3	643	747	0.04%	0.007%
87	14.054	2126	2127	2130	rBV	662	689	0.04%	0.006%
88	14.152	2141	2143	2146	rVB2	682	424	0.02%	0.004%
89	14.268	2158	2162	2166	rVB2	656	961	0.05%	0.009%
90	14.414	2184	2186	2187	rBV2	753	425	0.02%	0.004%
91	14.609	2215	2218	2219	rBV2	423	441	0.02%	0.004%
92	14.664	2225	2227	2228	rVB	843	490	0.03%	0.005%
93	14.694	2228	2232	2233	rBV2	660	755	0.04%	0.007%
94	14.944	2271	2273	2278	rVB2	829	1212	0.07%	0.011%
95	14.987	2278	2280	2282	rBV2	560	466	0.03%	0.004%
96	15.475	2359	2360	2361	rBV	987	511	0.03%	0.005%
97	15.804	2410	2414	2418	rBV4	958	1684	0.09%	0.015%
98	16.084	2459	2460	2462	rVV2	765	488	0.03%	0.004%
99	16.212	2479	2481	2484	rVB2	1017	1014	0.06%	0.009%
100	16.560	2536	2538	2541	rBV3	701	725	0.04%	0.007%


Sum of corrected areas: 10868733

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030394.D
Acq On : 04 Aug 2022 16:17
Operator : JC/MD
Sample : N4003-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

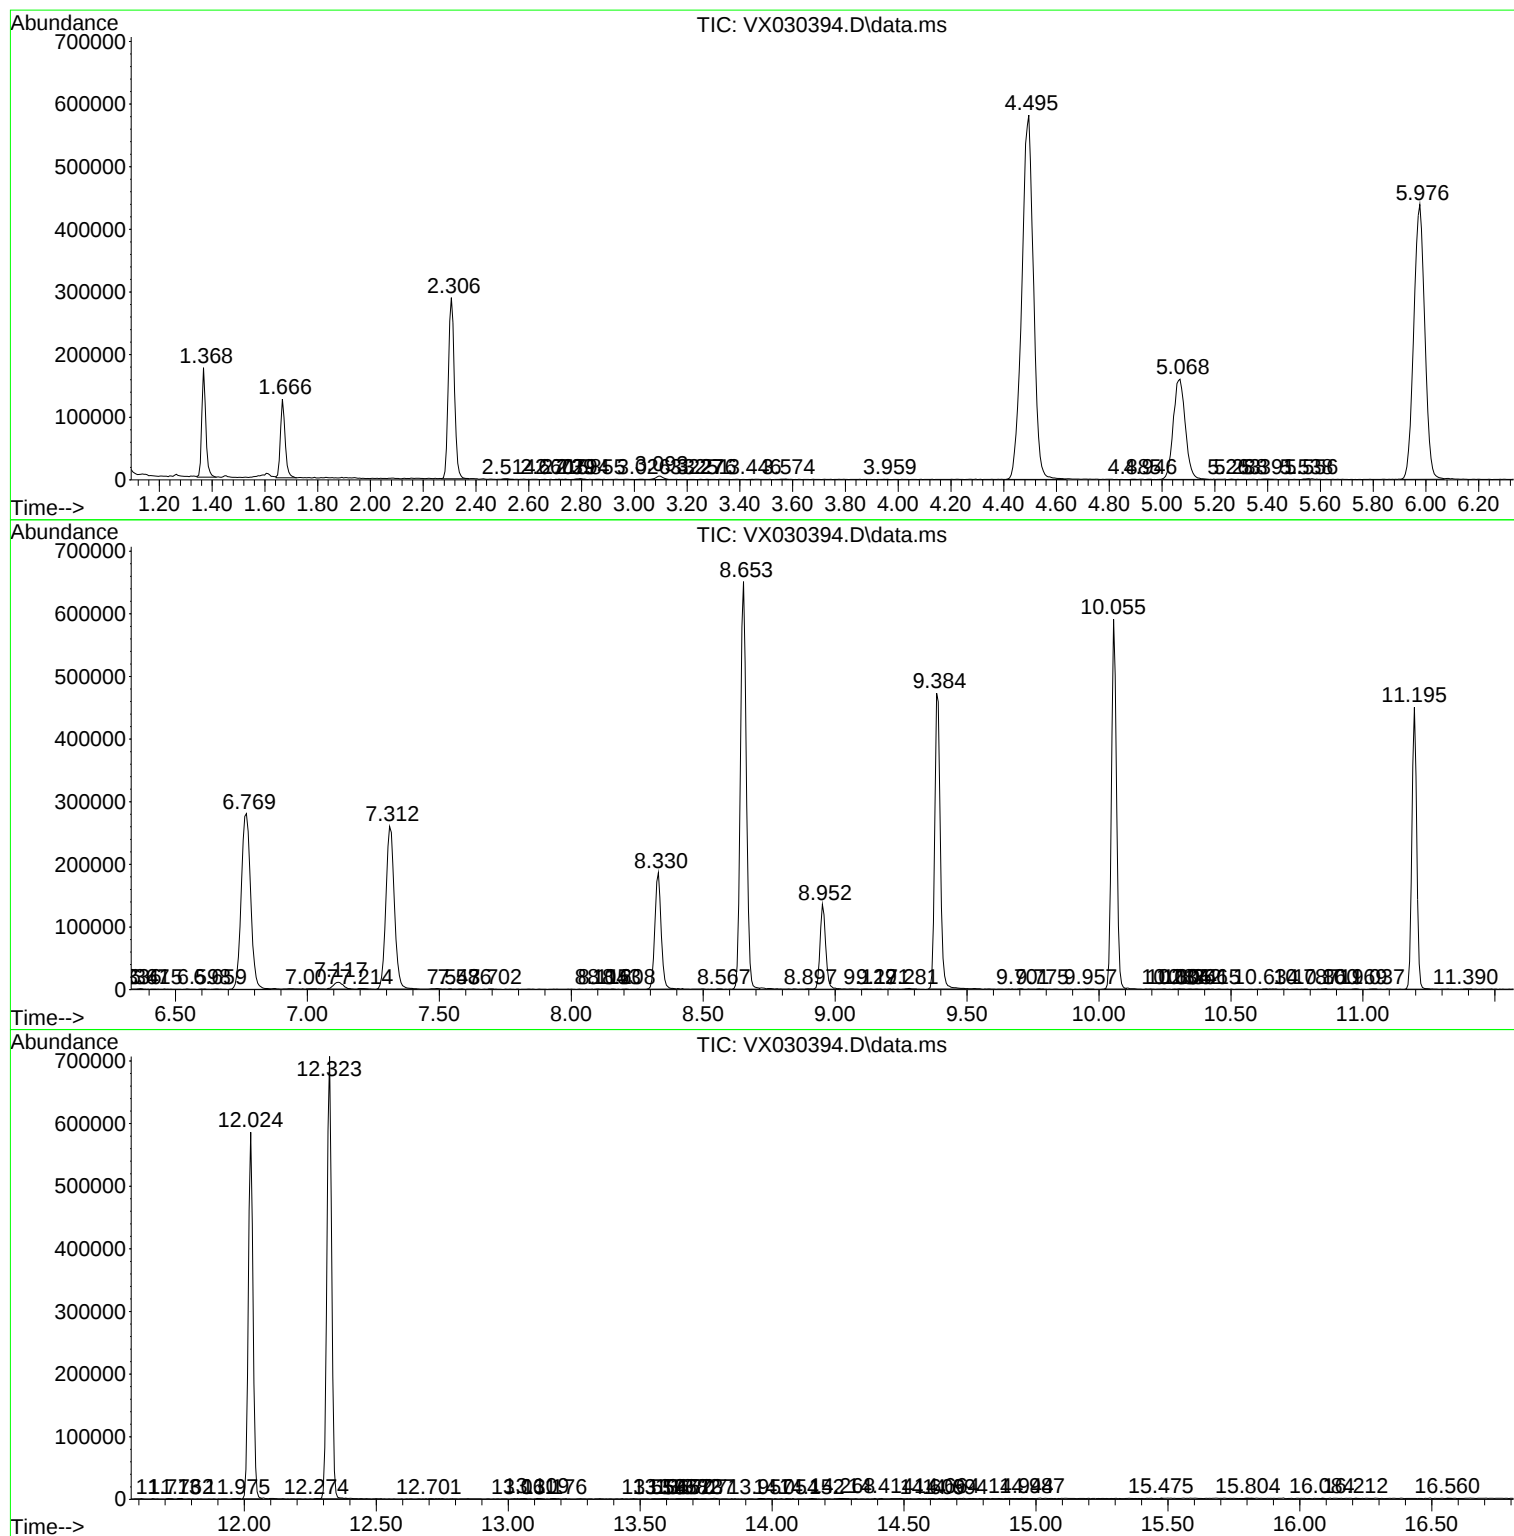

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030394.D
Acq On : 04 Aug 2022 16:17
Operator : JC/MD
Sample : N4003-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030394.D
Acq On : 04 Aug 2022 16:17
Operator : JC/MD
Sample : N4003-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc