

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030395.D
 Acq On : 04 Aug 2022 16:40
 Operator : JC/MD
 Sample : N4003-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	42	47	57	rVB2	675736	783522	13.90%	4.882%
2	1.666	91	95	102	rVB	132327	155845	2.77%	0.971%
3	2.307	194	200	210	rBV	314402	472562	8.39%	2.944%
4	2.496	229	231	233	rBV2	762	768	0.01%	0.005%
5	2.977	309	310	313	rVV2	399	381	0.01%	0.002%
6	3.014	313	316	318	rVV3	316	401	0.01%	0.002%
7	3.093	322	329	339	rVB	77618	151645	2.69%	0.945%
8	3.282	357	360	365	rVV2	470	773	0.01%	0.005%
9	3.355	370	372	374	rBV2	364	371	0.01%	0.002%
10	3.672	421	424	426	rBV2	409	347	0.01%	0.002%
11	3.703	426	429	430	rVB	495	396	0.01%	0.002%
12	3.764	436	439	444	rBV2	358	748	0.01%	0.005%
13	3.812	444	447	450	rVB	426	572	0.01%	0.004%
14	3.965	469	472	473	rBV2	436	380	0.01%	0.002%
15	4.068	486	489	494	rBV2	463	795	0.01%	0.005%
16	4.306	519	528	539	rBV7	2586	8330	0.15%	0.052%
17	4.489	545	558	581	rBV2	2015502	5634893	100.00%	35.107%
18	4.739	597	599	602	rBV3	616	519	0.01%	0.003%
19	4.861	617	619	621	rVB2	731	347	0.01%	0.002%
20	4.885	621	623	627	rVB3	737	843	0.01%	0.005%
21	4.922	627	629	631	rBV2	547	442	0.01%	0.003%
22	4.940	631	632	636	rBV2	637	499	0.01%	0.003%
23	5.062	639	652	668	rBV2	176408	538544	9.56%	3.355%
24	5.257	683	684	687	rBV2	489	523	0.01%	0.003%
25	5.300	690	691	694	rVB	647	359	0.01%	0.002%
26	5.556	731	733	736	rVB2	1133	947	0.02%	0.006%
27	5.696	753	756	759	rVB3	579	666	0.01%	0.004%
28	5.733	759	762	764	rBV	344	368	0.01%	0.002%
29	5.775	766	769	770	rVB2	400	372	0.01%	0.002%
30	5.800	770	773	776	rBV	543	522	0.01%	0.003%
31	5.836	776	779	780	rBV2	631	495	0.01%	0.003%
32	5.977	789	802	822	rBV2	445878	1334019	23.67%	8.311%
33	6.214	840	841	846	rBV3	292	368	0.01%	0.002%
34	6.263	846	849	856	rVB4	1105	2298	0.04%	0.014%
35	6.361	858	865	867	rBV4	1460	2686	0.05%	0.017%
36	6.470	879	883	884	rBV3	575	671	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030395.D
 Acq On : 04 Aug 2022 16:40
 Operator : JC/MD
 Sample : N4003-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.537	892	894	896	rBV2	738	874	0.02%	0.005%
38	6.647	910	912	915	rBV2	552	624	0.01%	0.004%
39	6.763	922	931	946	rBV	303907	723842	12.85%	4.510%
40	7.056	977	979	980	rBV2	534	429	0.01%	0.003%
41	7.129	982	991	1002	rVV4	68771	164213	2.91%	1.023%
42	7.312	1012	1021	1030	rBV	277305	599185	10.63%	3.733%
43	7.647	1073	1076	1078	rBV2	384	533	0.01%	0.003%
44	7.757	1090	1094	1098	rBV2	313	440	0.01%	0.003%
45	7.830	1104	1106	1108	rBV	644	413	0.01%	0.003%
46	7.946	1123	1125	1126	rBV	674	434	0.01%	0.003%
47	8.165	1159	1161	1164	rBV	469	418	0.01%	0.003%
48	8.330	1181	1188	1200	rBV	191740	318860	5.66%	1.987%
49	8.415	1200	1202	1204	rBV3	647	505	0.01%	0.003%
50	8.494	1213	1215	1217	rBV	499	386	0.01%	0.002%
51	8.555	1220	1225	1226	rBV	432	470	0.01%	0.003%
52	8.653	1234	1241	1252	rBV	684884	1058550	18.79%	6.595%
53	8.915	1282	1284	1285	rBV	569	419	0.01%	0.003%
54	8.952	1285	1290	1301	rVV	142046	209160	3.71%	1.303%
55	9.147	1320	1322	1324	rBV	401	372	0.01%	0.002%
56	9.171	1324	1326	1329	rVV3	362	401	0.01%	0.002%
57	9.275	1338	1343	1351	rVB	32010	48410	0.86%	0.302%
58	9.385	1356	1361	1374	rBV	505790	732190	12.99%	4.562%
59	9.933	1449	1451	1455	rVB2	417	529	0.01%	0.003%
60	9.988	1457	1460	1461	rBV2	518	574	0.01%	0.004%
61	10.055	1464	1471	1481	rBV	611702	816126	14.48%	5.085%
62	10.201	1492	1495	1498	rVB3	860	1048	0.02%	0.007%
63	10.269	1505	1506	1508	rBV	645	396	0.01%	0.002%
64	10.311	1509	1513	1515	rVB3	884	1258	0.02%	0.008%
65	10.506	1542	1545	1547	rVB3	597	425	0.01%	0.003%
66	10.640	1566	1567	1570	rBV2	503	436	0.01%	0.003%
67	10.707	1576	1578	1582	rVB2	453	536	0.01%	0.003%
68	10.744	1582	1584	1587	rBV2	546	639	0.01%	0.004%
69	10.976	1620	1622	1624	rBV3	538	448	0.01%	0.003%
70	11.085	1638	1640	1645	rVV3	641	807	0.01%	0.005%
71	11.195	1652	1658	1667	rBV	483600	602849	10.70%	3.756%
72	11.299	1673	1675	1678	rVB3	584	490	0.01%	0.003%
73	11.329	1678	1680	1682	rBV2	400	361	0.01%	0.002%
74	11.445	1696	1699	1701	rVB	546	475	0.01%	0.003%
75	11.470	1701	1703	1705	rBV2	456	578	0.01%	0.004%
76	11.530	1711	1713	1714	rBV2	464	392	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030395.D
 Acq On : 04 Aug 2022 16:40
 Operator : JC/MD
 Sample : N4003-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.567	1717	1719	1721	rVB2	555	442	0.01%	0.003%
78	11.585	1721	1722	1723	rBV	593	341	0.01%	0.002%
79	11.640	1729	1731	1732	rBV2	412	401	0.01%	0.002%
80	11.713	1741	1743	1745	rBV3	445	410	0.01%	0.003%
81	11.811	1757	1759	1763	rVB2	473	502	0.01%	0.003%
82	11.854	1763	1766	1769	rVB2	390	537	0.01%	0.003%
83	11.957	1780	1783	1784	rBV	385	407	0.01%	0.003%
84	12.024	1788	1794	1803	rBV	617482	748807	13.29%	4.665%
85	12.232	1822	1828	1829	rBV3	741	1102	0.02%	0.007%
86	12.323	1837	1843	1852	rBV	694513	899871	15.97%	5.606%
87	12.543	1877	1879	1882	rBV2	440	530	0.01%	0.003%
88	12.616	1888	1891	1898	rBV3	563	1378	0.02%	0.009%
89	12.719	1906	1908	1911	rBV2	396	425	0.01%	0.003%
90	12.853	1928	1930	1934	rVB3	1136	1122	0.02%	0.007%
91	12.981	1948	1951	1952	rBV2	373	421	0.01%	0.003%
92	13.109	1971	1972	1976	rVB2	741	631	0.01%	0.004%
93	13.292	2001	2002	2007	rVV2	587	359	0.01%	0.002%
94	13.597	2048	2052	2053	rBV	504	590	0.01%	0.004%
95	13.780	2079	2082	2085	rBV3	856	1132	0.02%	0.007%
96	14.091	2128	2133	2136	rBV	681	1010	0.02%	0.006%
97	15.060	2290	2292	2293	rBV	607	524	0.01%	0.003%
98	15.518	2365	2367	2369	rBV2	806	807	0.01%	0.005%
99	15.597	2378	2380	2384	rBV2	733	572	0.01%	0.004%
100	16.286	2492	2493	2496	rBV2	649	464	0.01%	0.003%




Sum of corrected areas: 16050497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030395.D
Acq On : 04 Aug 2022 16:40
Operator : JC/MD
Sample : N4003-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

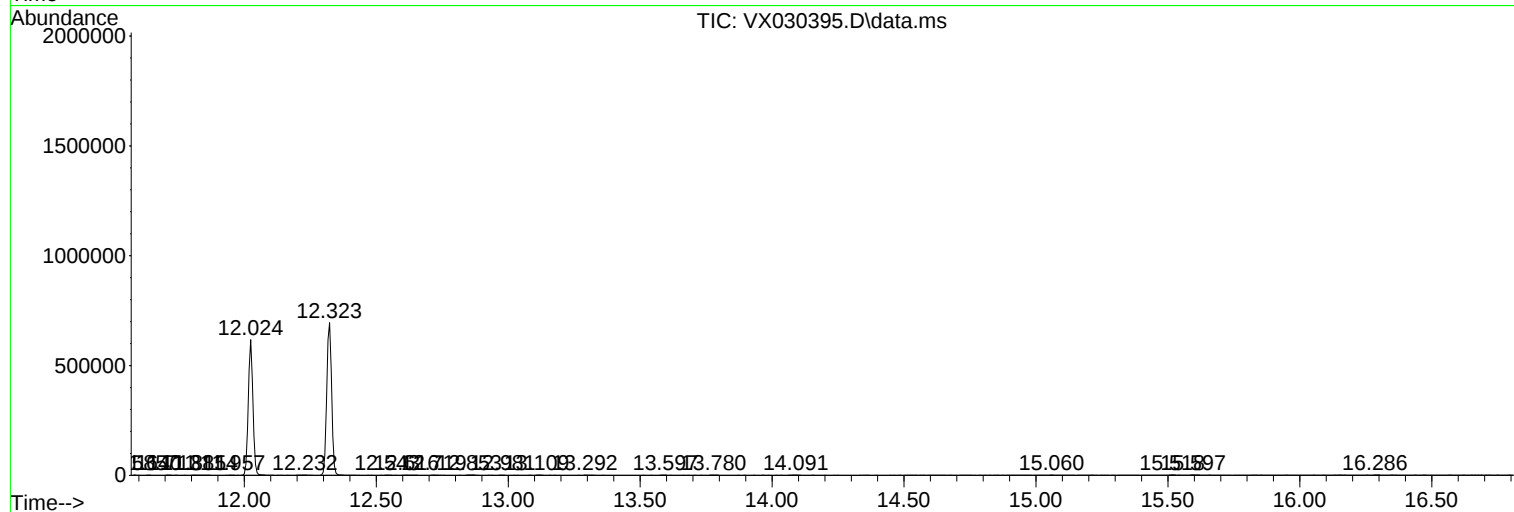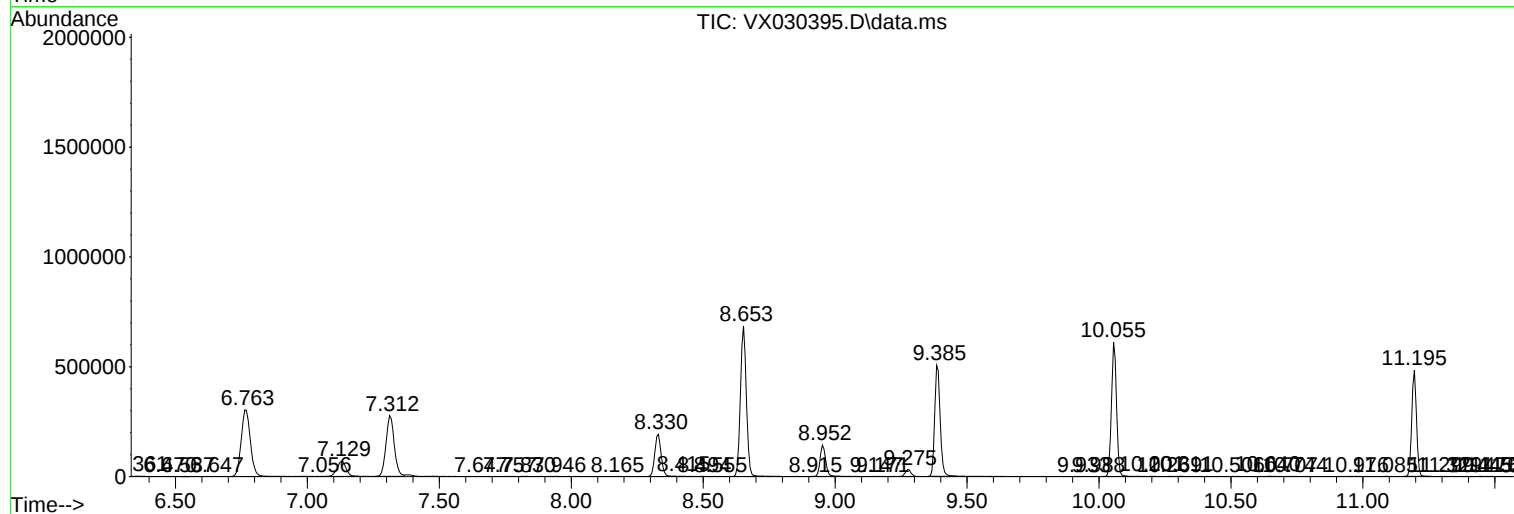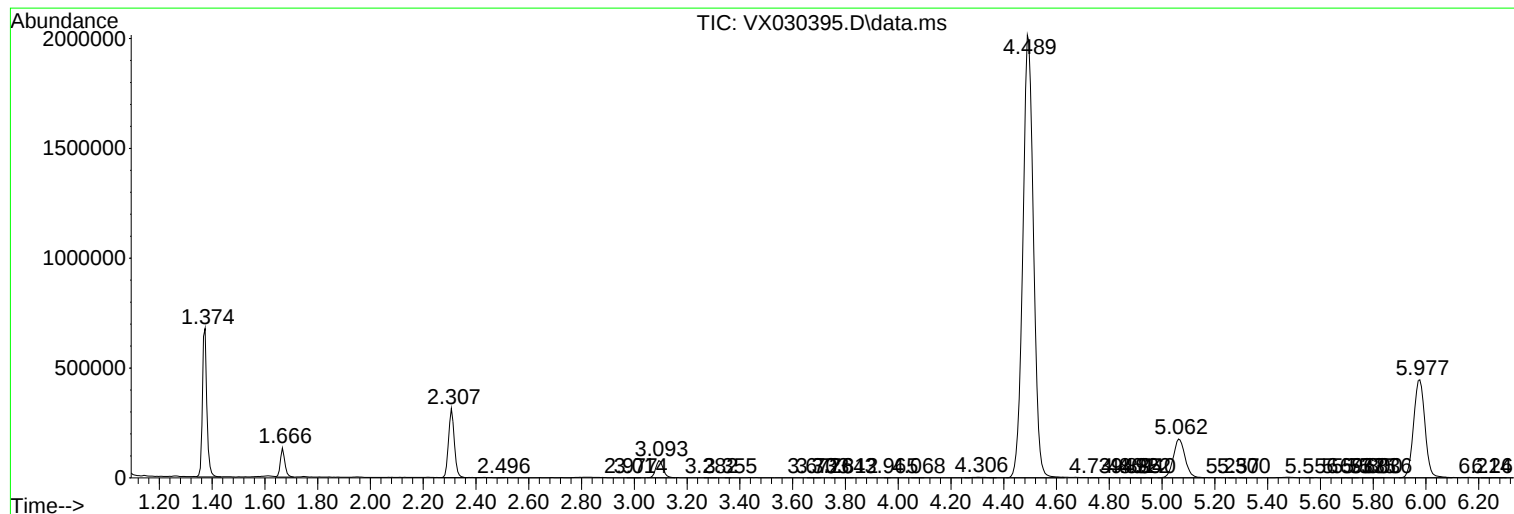

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030395.D
Acq On : 04 Aug 2022 16:40
Operator : JC/MD
Sample : N4003-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030395.D
Acq On : 04 Aug 2022 16:40
Operator : JC/MD
Sample : N4003-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc