

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030396.D
 Acq On : 04 Aug 2022 17:04
 Operator : JC/MD
 Sample : N4003-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	57	rVB2	572081	637038	4.46%	2.024%
2	1.666	91	95	103	rVV	119894	151237	1.06%	0.480%
3	1.746	105	108	115	rVB2	10383	14036	0.10%	0.045%
4	2.307	194	200	210	rVB	279158	435570	3.05%	1.384%
5	2.514	232	234	238	rVB2	1459	1506	0.01%	0.005%
6	2.563	240	242	244	rBV	427	354	0.00%	0.001%
7	2.654	255	257	259	rVB2	407	348	0.00%	0.001%
8	2.685	259	262	263	rBV2	470	371	0.00%	0.001%
9	2.782	271	278	283	rBV6	1741	4080	0.03%	0.013%
10	2.947	303	305	309	rVB3	307	401	0.00%	0.001%
11	2.977	309	310	313	rBV3	654	648	0.00%	0.002%
12	3.093	319	329	340	rBV	185974	363198	2.54%	1.154%
13	3.337	367	369	371	rVV2	470	552	0.00%	0.002%
14	3.380	374	376	379	rBV2	392	512	0.00%	0.002%
15	3.434	382	385	386	rBV	578	399	0.00%	0.001%
16	3.459	386	389	391	rBV3	555	672	0.00%	0.002%
17	3.489	391	394	397	rVB2	247	340	0.00%	0.001%
18	3.739	433	435	438	rVB	559	494	0.00%	0.002%
19	3.770	438	440	444	rBV2	515	541	0.00%	0.002%
20	3.910	461	463	466	rVB2	409	389	0.00%	0.001%
21	4.184	506	508	512	rBV2	323	413	0.00%	0.001%
22	4.312	518	529	535	rBV4	3265	9409	0.07%	0.030%
23	4.495	545	559	581	rBV	5165122	14277190	100.00%	45.356%
24	5.068	642	653	669	rVB	158490	494845	3.47%	1.572%
25	5.385	701	705	707	rBV	834	1330	0.01%	0.004%
26	5.483	716	721	727	rVB4	3312	7362	0.05%	0.023%
27	5.678	749	753	755	rBV3	269	336	0.00%	0.001%
28	5.775	765	769	772	rBV2	506	553	0.00%	0.002%
29	5.806	772	774	777	rBV2	443	528	0.00%	0.002%
30	5.885	785	787	789	rVB2	540	402	0.00%	0.001%
31	5.977	789	802	821	rBV2	420883	1236232	8.66%	3.927%
32	6.178	832	835	837	rVB2	640	727	0.01%	0.002%
33	6.202	837	839	842	rBV2	447	443	0.00%	0.001%
34	6.245	845	846	850	rBV2	359	470	0.00%	0.001%
35	6.355	861	864	867	rBV3	668	675	0.00%	0.002%
36	6.428	874	876	881	rVB3	465	525	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030396.D
 Acq On : 04 Aug 2022 17:04
 Operator : JC/MD
 Sample : N4003-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.470	881	883	885	rVB2	523	430	0.00%	0.001%
38	6.556	896	897	900	rBV2	530	456	0.00%	0.001%
39	6.769	922	932	945	rBV	289097	696823	4.88%	2.214%
40	7.129	981	991	1012	rBV	3121117	6702812	46.95%	21.294%
41	7.312	1013	1021	1037	rVB	251809	554628	3.88%	1.762%
42	7.592	1065	1067	1068	rBV2	454	440	0.00%	0.001%
43	7.708	1084	1086	1088	rBV	404	364	0.00%	0.001%
44	7.757	1088	1094	1095	rBV2	543	812	0.01%	0.003%
45	7.860	1109	1111	1113	rBV	595	589	0.00%	0.002%
46	7.934	1118	1123	1126	rBV4	519	869	0.01%	0.003%
47	8.330	1181	1188	1200	rBV	180216	297982	2.09%	0.947%
48	8.434	1203	1205	1206	rBV2	527	444	0.00%	0.001%
49	8.653	1234	1241	1255	rBV	642362	984000	6.89%	3.126%
50	8.952	1285	1290	1301	rBV	128460	193725	1.36%	0.615%
51	9.092	1311	1313	1315	rBV	725	736	0.01%	0.002%
52	9.159	1318	1324	1327	rVB2	462	840	0.01%	0.003%
53	9.275	1337	1343	1355	rBV	528361	742349	5.20%	2.358%
54	9.385	1356	1361	1374	rBV	473446	683412	4.79%	2.171%
55	9.744	1418	1420	1422	rBV	357	402	0.00%	0.001%
56	10.055	1465	1471	1480	rBV	621994	820263	5.75%	2.606%
57	10.238	1498	1501	1507	rBV	753	1267	0.01%	0.004%
58	10.281	1507	1508	1510	rBV	392	344	0.00%	0.001%
59	10.311	1511	1513	1514	rVB2	687	406	0.00%	0.001%
60	10.360	1519	1521	1524	rBV	518	439	0.00%	0.001%
61	10.409	1526	1529	1531	rBV2	432	409	0.00%	0.001%
62	10.616	1560	1563	1566	rBV2	433	645	0.00%	0.002%
63	10.653	1566	1569	1574	rVB	845	1169	0.01%	0.004%
64	10.768	1587	1588	1591	rVB2	476	375	0.00%	0.001%
65	10.793	1591	1592	1593	rBV	593	329	0.00%	0.001%
66	10.829	1596	1598	1603	rVB2	347	413	0.00%	0.001%
67	10.884	1603	1607	1610	rBV3	501	632	0.00%	0.002%
68	10.921	1610	1613	1614	rBV2	707	556	0.00%	0.002%
69	10.957	1614	1619	1620	rBV2	358	532	0.00%	0.002%
70	11.043	1628	1633	1637	rBV5	548	992	0.01%	0.003%
71	11.092	1639	1641	1642	rBV2	506	430	0.00%	0.001%
72	11.195	1652	1658	1669	rBV	441044	572043	4.01%	1.817%
73	11.445	1698	1699	1702	rVB2	550	620	0.00%	0.002%
74	11.610	1723	1726	1729	rBV2	422	569	0.00%	0.002%
75	11.695	1739	1740	1742	rBV	469	339	0.00%	0.001%
76	11.750	1747	1749	1752	rBV2	610	595	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030396.D
 Acq On : 04 Aug 2022 17:04
 Operator : JC/MD
 Sample : N4003-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.915	1774	1776	1778	rVB	463	356	0.00%	0.001%
78	11.951	1778	1782	1784	rBV	460	660	0.00%	0.002%
79	12.024	1789	1794	1804	rVB	617870	755190	5.29%	2.399%
80	12.323	1837	1843	1850	rBV	647501	798495	5.59%	2.537%
81	12.445	1862	1863	1866	rBV	350	381	0.00%	0.001%
82	12.469	1866	1867	1872	rVV3	682	642	0.00%	0.002%
83	12.506	1872	1873	1876	rVV2	455	377	0.00%	0.001%
84	12.604	1887	1889	1891	rBV2	460	475	0.00%	0.002%
85	12.908	1937	1939	1943	rBV2	468	440	0.00%	0.001%
86	13.238	1990	1993	1995	rBV2	294	384	0.00%	0.001%
87	13.353	2006	2012	2014	rBV3	458	936	0.01%	0.003%
88	13.451	2022	2028	2029	rBV3	337	655	0.00%	0.002%
89	13.506	2034	2037	2039	rVV2	407	507	0.00%	0.002%
90	13.530	2039	2041	2043	rVB2	543	320	0.00%	0.001%
91	13.707	2068	2070	2073	rVB	765	564	0.00%	0.002%
92	13.731	2073	2074	2076	rBV2	444	348	0.00%	0.001%
93	13.780	2079	2082	2087	rBV3	932	1592	0.01%	0.005%
94	13.817	2087	2088	2089	rBV	719	374	0.00%	0.001%
95	13.969	2109	2113	2117	rBV3	665	1128	0.01%	0.004%
96	14.414	2181	2186	2189	rBV3	667	1388	0.01%	0.004%
97	14.865	2256	2260	2263	rBV2	615	1118	0.01%	0.004%
98	15.036	2287	2288	2291	rBV2	543	550	0.00%	0.002%
99	15.627	2383	2385	2388	rBV2	696	805	0.01%	0.003%
100	15.829	2417	2418	2419	rBV	757	501	0.00%	0.002%




Sum of corrected areas: 31477792

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030396.D
Acq On : 04 Aug 2022 17:04
Operator : JC/MD
Sample : N4003-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

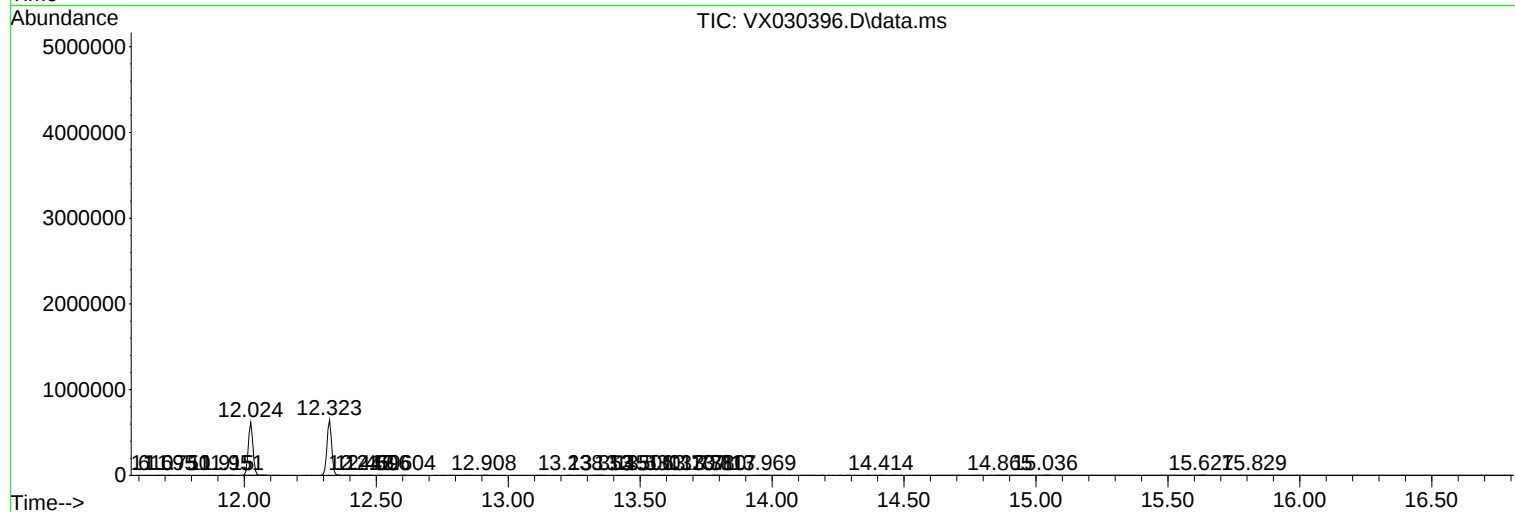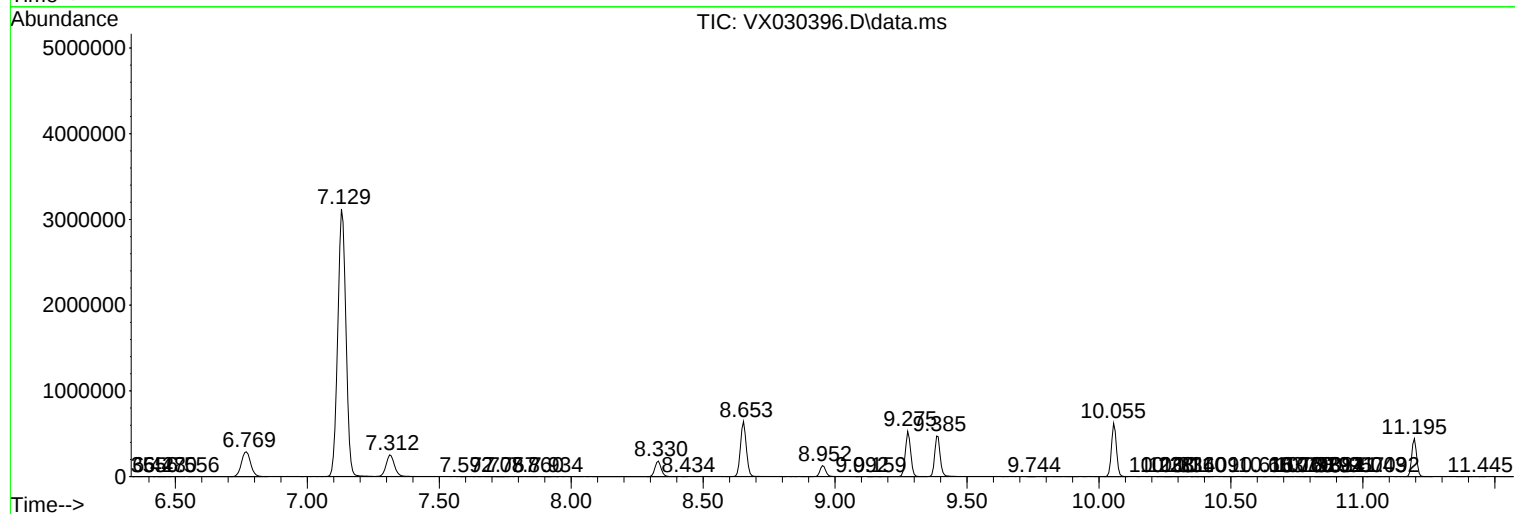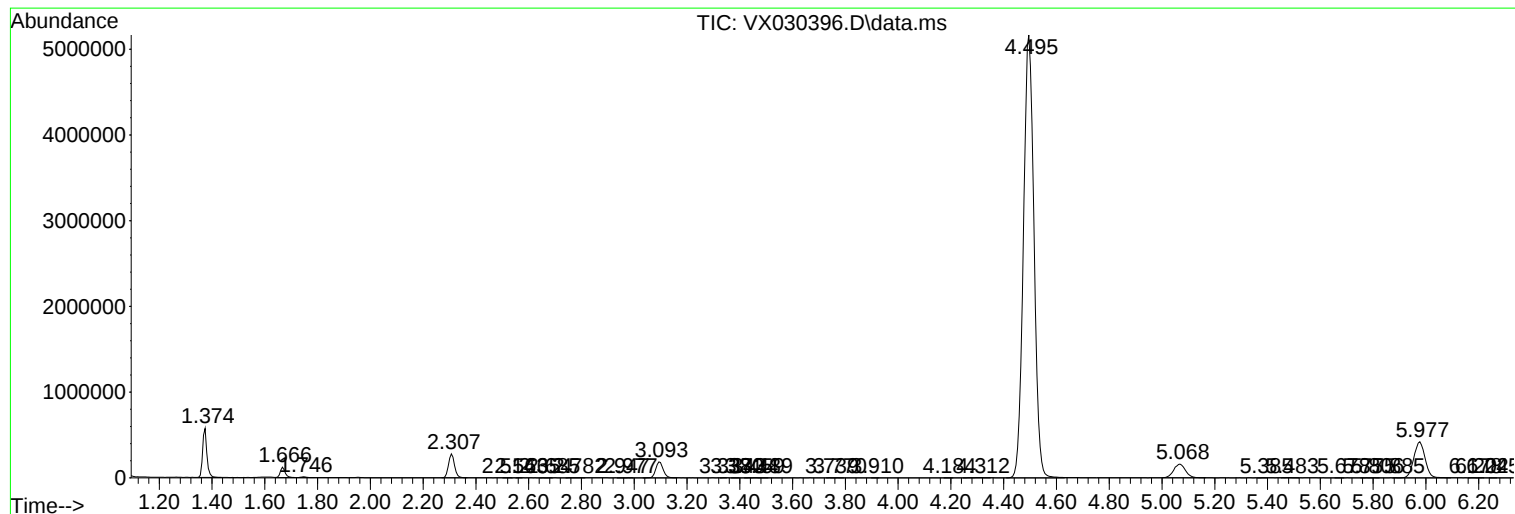

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030396.D
Acq On : 04 Aug 2022 17:04
Operator : JC/MD
Sample : N4003-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030396.D
Acq On : 04 Aug 2022 17:04
Operator : JC/MD
Sample : N4003-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc