

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030397.D
 Acq On : 04 Aug 2022 17:27
 Operator : JC/MD
 Sample : N4003-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	57	rVB2	556366	631348	4.30%	2.013%
2	1.666	91	95	104	rVB	125879	156204	1.06%	0.498%
3	1.746	105	108	113	rVB2	9181	10917	0.07%	0.035%
4	2.306	194	200	211	rVB	299853	463710	3.16%	1.479%
5	2.514	231	234	239	rVB5	898	1436	0.01%	0.005%
6	2.721	266	268	271	rBV2	386	520	0.00%	0.002%
7	2.788	274	279	282	rBV5	1239	2032	0.01%	0.006%
8	2.928	300	302	305	rBV2	463	461	0.00%	0.001%
9	2.965	307	308	310	rVV	400	355	0.00%	0.001%
10	2.989	310	312	314	rVV3	569	538	0.00%	0.002%
11	3.020	316	317	321	rVV2	581	512	0.00%	0.002%
12	3.093	321	329	343	rVV	191126	370335	2.52%	1.181%
13	3.197	343	346	352	rVB3	662	949	0.01%	0.003%
14	3.367	372	374	379	rVB2	567	742	0.01%	0.002%
15	3.404	379	380	382	rBV	469	339	0.00%	0.001%
16	3.440	382	386	387	rVV2	471	463	0.00%	0.001%
17	3.550	401	404	406	rVB3	515	554	0.00%	0.002%
18	3.574	406	408	415	rVB2	414	830	0.01%	0.003%
19	3.733	433	434	437	rBV2	393	418	0.00%	0.001%
20	3.849	450	453	456	rBV2	479	603	0.00%	0.002%
21	3.873	456	457	460	rBV	410	326	0.00%	0.001%
22	4.312	522	529	535	rVV5	2788	7071	0.05%	0.023%
23	4.495	546	559	579	rBV	5486938	14680861	100.00%	46.820%
24	4.922	628	629	631	rBV2	541	430	0.00%	0.001%
25	5.062	640	652	669	rBV	168243	518601	3.53%	1.654%
26	5.349	697	699	700	rVB2	658	329	0.00%	0.001%
27	5.391	702	706	710	rBV3	651	1147	0.01%	0.004%
28	5.477	717	720	723	rBV3	1747	2192	0.01%	0.007%
29	5.550	731	732	734	rBV	676	594	0.00%	0.002%
30	5.976	789	802	820	rBV3	445186	1284056	8.75%	4.095%
31	6.184	834	836	839	rBV2	403	448	0.00%	0.001%
32	6.373	865	867	868	rBV2	430	347	0.00%	0.001%
33	6.428	875	876	879	rBV2	496	396	0.00%	0.001%
34	6.464	879	882	884	rBV3	449	522	0.00%	0.002%
35	6.519	890	891	892	rBV	597	329	0.00%	0.001%
36	6.537	892	894	896	rVV	610	619	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030397.D
 Acq On : 04 Aug 2022 17:27
 Operator : JC/MD
 Sample : N4003-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	6.598	901	904	909	rVB	446	753	0.01%	0.002%
38	6.769	922	932	946	rVV	296312	700977	4.77%	2.236%
39	7.129	980	991	1012	rBV	2729184	6057137	41.26%	19.317%
40	7.312	1013	1021	1036	rVB	266161	585161	3.99%	1.866%
41	7.659	1076	1078	1081	rBV3	411	453	0.00%	0.001%
42	7.702	1084	1085	1087	rBV	418	335	0.00%	0.001%
43	7.732	1087	1090	1095	rVB4	679	1008	0.01%	0.003%
44	7.775	1095	1097	1098	rBV	624	406	0.00%	0.001%
45	7.799	1098	1101	1103	rBV2	333	463	0.00%	0.001%
46	7.946	1123	1125	1129	rBV3	894	1114	0.01%	0.004%
47	8.147	1152	1158	1160	rBV2	460	869	0.01%	0.003%
48	8.232	1170	1172	1175	rBV3	350	545	0.00%	0.002%
49	8.330	1181	1188	1198	rBV	185195	306029	2.08%	0.976%
50	8.446	1206	1207	1210	rVB2	631	414	0.00%	0.001%
51	8.482	1212	1213	1215	rBV2	810	663	0.00%	0.002%
52	8.653	1234	1241	1249	rVV	652464	1022057	6.96%	3.260%
53	8.952	1285	1290	1303	rVB	133510	201050	1.37%	0.641%
54	9.275	1337	1343	1355	rVB	378669	558882	3.81%	1.782%
55	9.384	1356	1361	1373	rBV	502882	714540	4.87%	2.279%
56	9.708	1412	1414	1416	rVB2	752	446	0.00%	0.001%
57	9.793	1425	1428	1429	rBV2	629	634	0.00%	0.002%
58	9.842	1434	1436	1441	rVB2	534	542	0.00%	0.002%
59	9.884	1441	1443	1445	rBV2	336	441	0.00%	0.001%
60	9.988	1458	1460	1462	rBV2	359	389	0.00%	0.001%
61	10.055	1465	1471	1484	rVV	602095	808795	5.51%	2.579%
62	10.262	1504	1505	1508	rVB2	496	389	0.00%	0.001%
63	10.311	1511	1513	1516	rBV2	840	914	0.01%	0.003%
64	10.555	1549	1553	1555	rBV	559	516	0.00%	0.002%
65	10.573	1555	1556	1558	rVB	477	315	0.00%	0.001%
66	10.652	1565	1569	1571	rVB3	942	937	0.01%	0.003%
67	10.732	1578	1582	1583	rVB2	383	365	0.00%	0.001%
68	10.823	1595	1597	1600	rVB	541	444	0.00%	0.001%
69	10.890	1606	1608	1611	rBV	405	397	0.00%	0.001%
70	11.195	1652	1658	1670	rBV	479158	594515	4.05%	1.896%
71	11.518	1709	1711	1714	rBV2	314	324	0.00%	0.001%
72	11.579	1716	1721	1724	rBV2	608	1137	0.01%	0.004%
73	11.610	1724	1726	1728	rVV2	432	377	0.00%	0.001%
74	11.634	1728	1730	1733	rVB2	446	476	0.00%	0.002%
75	11.707	1739	1742	1743	rBV2	623	509	0.00%	0.002%
76	11.835	1761	1763	1765	rBV	408	343	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030397.D
 Acq On : 04 Aug 2022 17:27
 Operator : JC/MD
 Sample : N4003-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1802	rBV	631196	769630	5.24%	2.455%
78	12.110	1807	1808	1810	rVB	1165	694	0.00%	0.002%
79	12.323	1837	1843	1850	rBV	697726	867468	5.91%	2.767%
80	12.573	1882	1884	1886	rBV	645	589	0.00%	0.002%
81	12.701	1903	1905	1909	rBV2	499	648	0.00%	0.002%
82	12.811	1922	1923	1925	rBV	502	343	0.00%	0.001%
83	12.853	1927	1930	1932	rVB3	631	741	0.01%	0.002%
84	12.945	1943	1945	1948	rBV2	464	398	0.00%	0.001%
85	12.975	1948	1950	1954	rVB2	487	527	0.00%	0.002%
86	13.012	1954	1956	1959	rVB2	401	457	0.00%	0.001%
87	13.036	1959	1960	1964	rBV3	553	630	0.00%	0.002%
88	13.567	2045	2047	2049	rBV2	481	482	0.00%	0.002%
89	13.591	2049	2051	2053	rVV3	620	610	0.00%	0.002%
90	13.640	2057	2059	2062	rBV2	317	315	0.00%	0.001%
91	13.835	2089	2091	2093	rBV	613	567	0.00%	0.002%
92	14.054	2125	2127	2129	rBV	443	395	0.00%	0.001%
93	14.109	2134	2136	2138	rBV2	479	467	0.00%	0.001%
94	14.170	2144	2146	2148	rVB	576	334	0.00%	0.001%
95	14.195	2148	2150	2152	rBV	509	541	0.00%	0.002%
96	14.335	2171	2173	2175	rBV	413	481	0.00%	0.002%
97	14.371	2177	2179	2181	rBV	530	340	0.00%	0.001%
98	14.530	2203	2205	2207	rBV2	597	537	0.00%	0.002%
99	14.908	2265	2267	2268	rBV2	698	455	0.00%	0.001%
100	15.280	2326	2328	2331	rVB2	960	581	0.00%	0.002%


Sum of corrected areas: 31355825

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030397.D
Acq On : 04 Aug 2022 17:27
Operator : JC/MD
Sample : N4003-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

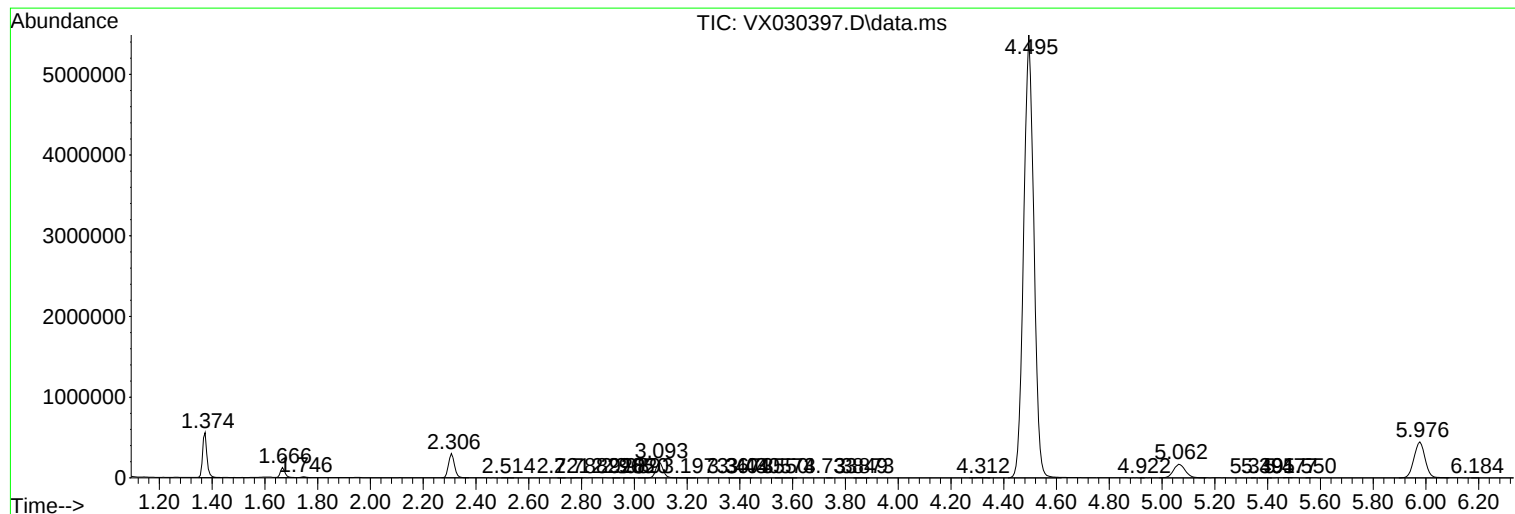

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030397.D
Acq On : 04 Aug 2022 17:27
Operator : JC/MD
Sample : N4003-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030397.D
Acq On : 04 Aug 2022 17:27
Operator : JC/MD
Sample : N4003-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------