

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030399.D
 Acq On : 04 Aug 2022 18:14
 Operator : JC/MD
 Sample : N4003-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	42	47	55	rVB2	437523	528090	8.26%	3.320%
2	1.666	91	95	105	rVB	124932	152176	2.38%	0.957%
3	2.307	194	200	210	rBV	288004	449303	7.03%	2.825%
4	2.422	217	219	222	rBV3	558	594	0.01%	0.004%
5	2.581	243	245	250	rBV2	588	616	0.01%	0.004%
6	2.624	250	252	254	rBV2	579	372	0.01%	0.002%
7	2.788	275	279	280	rBV4	811	1140	0.02%	0.007%
8	2.959	305	307	308	rBV2	434	386	0.01%	0.002%
9	3.093	322	329	341	rVB	53471	106248	1.66%	0.668%
10	3.191	344	345	349	rBV2	393	343	0.01%	0.002%
11	3.319	364	366	368	rBV	477	533	0.01%	0.003%
12	3.343	368	370	372	rVB	578	420	0.01%	0.003%
13	3.373	372	375	377	rBV	308	447	0.01%	0.003%
14	3.544	400	403	404	rBV2	419	392	0.01%	0.002%
15	3.709	428	430	436	rVB2	450	549	0.01%	0.003%
16	3.782	436	442	443	rBV	428	691	0.01%	0.004%
17	3.806	445	446	448	rBV2	594	419	0.01%	0.003%
18	4.184	506	508	510	rBV2	522	444	0.01%	0.003%
19	4.245	515	518	520	rBV	682	561	0.01%	0.004%
20	4.495	546	559	578	rVV	2322628	6395751	100.00%	40.209%
21	4.757	600	602	606	rBV4	732	941	0.01%	0.006%
22	5.062	641	652	668	rBV	168030	506648	7.92%	3.185%
23	5.263	683	685	687	rBV2	536	338	0.01%	0.002%
24	5.373	699	703	704	rBV2	544	667	0.01%	0.004%
25	5.562	727	734	736	rBV4	965	2099	0.03%	0.013%
26	5.794	770	772	778	rVB2	286	420	0.01%	0.003%
27	5.861	780	783	787	rBV3	464	607	0.01%	0.004%
28	5.977	787	802	821	rBV2	434670	1263220	19.75%	7.942%
29	6.355	862	864	865	rBV	527	341	0.01%	0.002%
30	6.434	873	877	881	rBV5	462	683	0.01%	0.004%
31	6.605	903	905	908	rVB	556	504	0.01%	0.003%
32	6.635	908	910	912	rBV2	403	370	0.01%	0.002%
33	6.763	921	931	951	rBV	293133	698100	10.92%	4.389%
34	7.043	976	977	980	rBV3	593	580	0.01%	0.004%
35	7.123	982	990	999	rVV5	18779	51291	0.80%	0.322%
36	7.190	999	1001	1002	rBV2	526	349	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030399.D
 Acq On : 04 Aug 2022 18:14
 Operator : JC/MD
 Sample : N4003-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1013	1021	1038	rBV	259094	573251	8.96%	3.604%
38	7.610	1069	1070	1073	rBV2	480	474	0.01%	0.003%
39	7.873	1109	1113	1114	rBV	235	357	0.01%	0.002%
40	7.934	1122	1123	1125	rBV	458	404	0.01%	0.003%
41	8.330	1179	1188	1201	rBV	182071	298673	4.67%	1.878%
42	8.421	1201	1203	1205	rBV2	568	531	0.01%	0.003%
43	8.543	1221	1223	1226	rVB2	597	617	0.01%	0.004%
44	8.653	1233	1241	1251	rBV	646410	1005918	15.73%	6.324%
45	8.836	1270	1271	1274	rBV2	550	535	0.01%	0.003%
46	8.952	1285	1290	1302	rVV	134350	195690	3.06%	1.230%
47	9.281	1340	1344	1348	rBV4	2615	4108	0.06%	0.026%
48	9.385	1356	1361	1375	rBV	482523	695933	10.88%	4.375%
49	9.799	1425	1429	1432	rVB2	690	943	0.01%	0.006%
50	9.933	1447	1451	1454	rBV2	538	861	0.01%	0.005%
51	10.055	1465	1471	1486	rBV	584358	792185	12.39%	4.980%
52	10.195	1492	1494	1497	rVB2	903	872	0.01%	0.005%
53	10.244	1498	1502	1505	rBV2	541	518	0.01%	0.003%
54	10.305	1509	1512	1518	rBV	803	950	0.01%	0.006%
55	10.348	1518	1519	1521	rVB	651	389	0.01%	0.002%
56	10.445	1533	1535	1536	rBV	369	370	0.01%	0.002%
57	10.598	1558	1560	1562	rBV2	524	539	0.01%	0.003%
58	10.634	1562	1566	1568	rVV2	350	521	0.01%	0.003%
59	10.707	1576	1578	1580	rVV2	406	347	0.01%	0.002%
60	10.750	1583	1585	1587	rBV2	344	370	0.01%	0.002%
61	10.890	1606	1608	1611	rBV2	349	540	0.01%	0.003%
62	11.006	1624	1627	1630	rBV	554	769	0.01%	0.005%
63	11.073	1634	1638	1640	rBV2	324	465	0.01%	0.003%
64	11.195	1652	1658	1668	rVV	450363	570279	8.92%	3.585%
65	11.293	1672	1674	1676	rVV2	474	419	0.01%	0.003%
66	11.341	1679	1682	1685	rVB3	376	535	0.01%	0.003%
67	11.451	1693	1700	1703	rBV2	482	1246	0.02%	0.008%
68	11.482	1703	1705	1708	rVV2	362	511	0.01%	0.003%
69	11.561	1715	1718	1720	rBV2	395	491	0.01%	0.003%
70	11.622	1724	1728	1729	rBV	360	365	0.01%	0.002%
71	11.750	1747	1749	1752	rVV3	312	394	0.01%	0.002%
72	11.878	1768	1770	1773	rBV	365	423	0.01%	0.003%
73	12.024	1789	1794	1802	rBV	599781	730793	11.43%	4.594%
74	12.225	1822	1827	1830	rBV4	625	998	0.02%	0.006%
75	12.250	1830	1831	1834	rVB	773	466	0.01%	0.003%
76	12.323	1837	1843	1849	rBV	681530	841748	13.16%	5.292%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030399.D
 Acq On : 04 Aug 2022 18:14
 Operator : JC/MD
 Sample : N4003-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.664	1896	1899	1903	rVB	461	550	0.01%	0.003%
78	12.701	1903	1905	1907	rBV2	460	491	0.01%	0.003%
79	12.738	1910	1911	1915	rBV2	465	605	0.01%	0.004%
80	12.792	1919	1920	1923	rBV2	421	370	0.01%	0.002%
81	12.920	1940	1941	1944	rBV	435	418	0.01%	0.003%
82	13.048	1959	1962	1963	rVV3	478	490	0.01%	0.003%
83	13.091	1967	1969	1972	rBV	789	676	0.01%	0.004%
84	13.378	2014	2016	2018	rBV	569	601	0.01%	0.004%
85	13.408	2018	2021	2023	rBV3	415	511	0.01%	0.003%
86	13.640	2058	2059	2061	rBV	601	355	0.01%	0.002%
87	13.780	2079	2082	2087	rVV3	826	1257	0.02%	0.008%
88	13.932	2105	2107	2109	rBV2	455	387	0.01%	0.002%
89	14.061	2125	2128	2129	rBV2	394	437	0.01%	0.003%
90	14.274	2161	2163	2164	rBV	436	338	0.01%	0.002%
91	14.359	2175	2177	2180	rBV2	389	442	0.01%	0.003%
92	14.481	2195	2197	2198	rBV2	549	454	0.01%	0.003%
93	14.548	2207	2208	2210	rBV2	532	441	0.01%	0.003%
94	14.670	2226	2228	2233	rBV3	655	810	0.01%	0.005%
95	14.768	2241	2244	2245	rBV	658	637	0.01%	0.004%
96	14.829	2252	2254	2257	rVB	698	578	0.01%	0.004%
97	15.152	2305	2307	2310	rBV3	603	855	0.01%	0.005%
98	15.207	2314	2316	2318	rVV2	802	510	0.01%	0.003%
99	15.914	2430	2432	2435	rBV2	761	1005	0.02%	0.006%
100	16.231	2482	2484	2486	rBV	744	468	0.01%	0.003%




Sum of corrected areas: 15906117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030399.D
Acq On : 04 Aug 2022 18:14
Operator : JC/MD
Sample : N4003-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

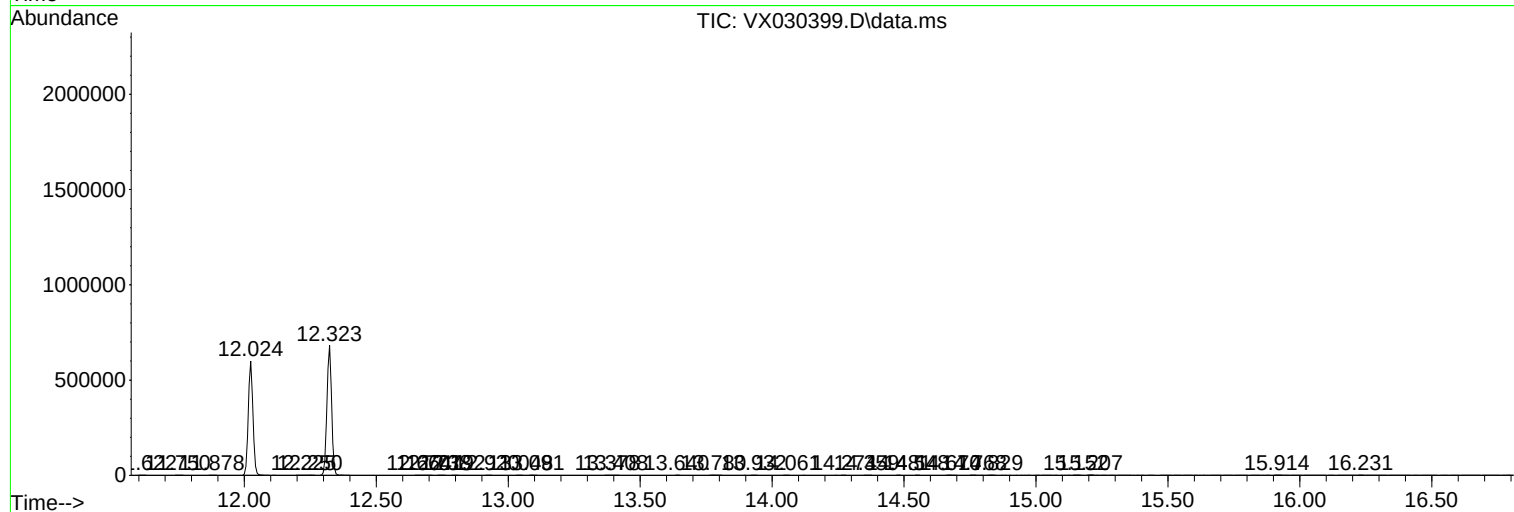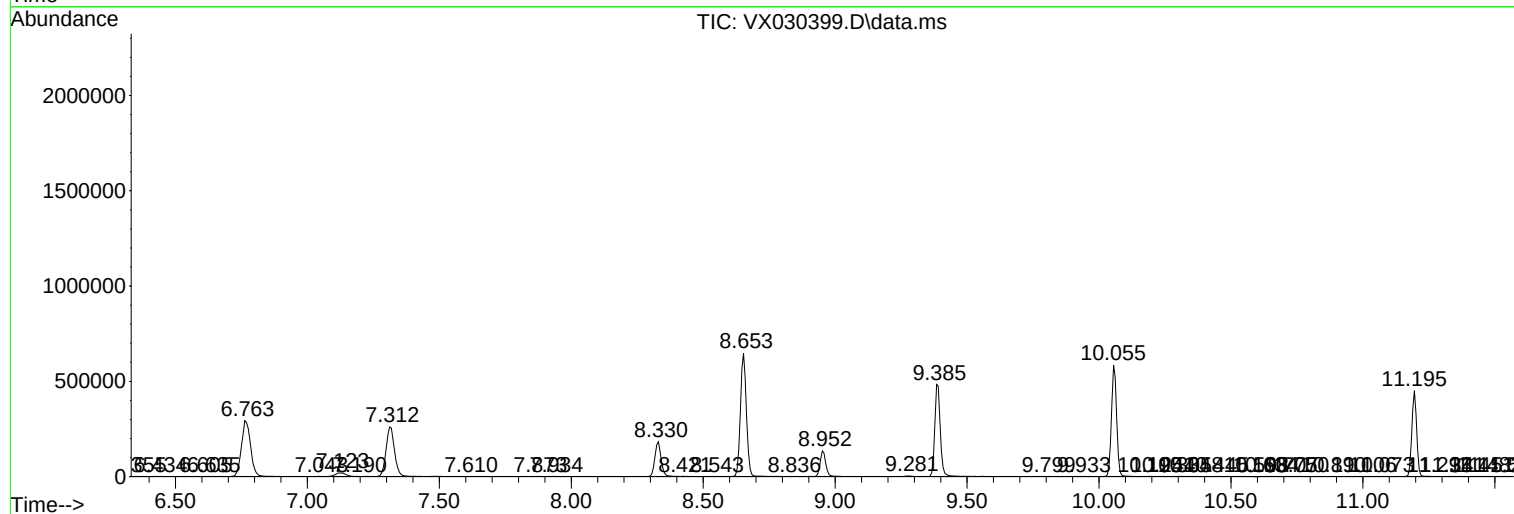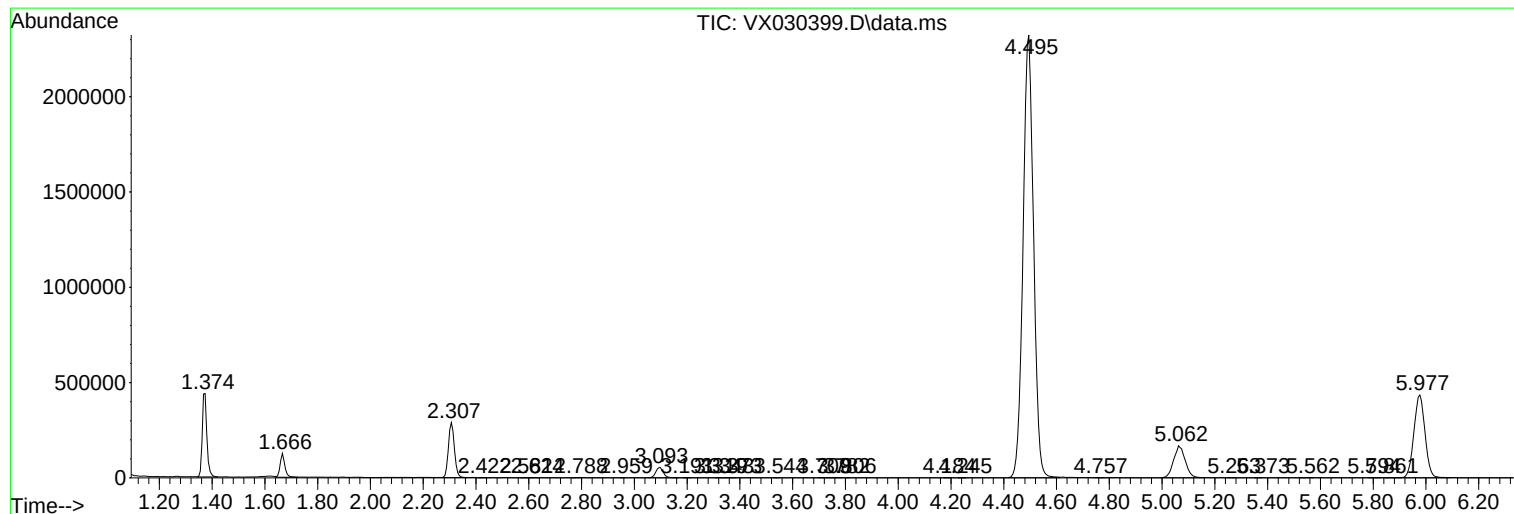

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030399.D
Acq On : 04 Aug 2022 18:14
Operator : JC/MD
Sample : N4003-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030399.D
Acq On : 04 Aug 2022 18:14
Operator : JC/MD
Sample : N4003-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc