

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030400.D
 Acq On : 04 Aug 2022 18:37
 Operator : JC/MD
 Sample : N4003-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030400.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	42	47	58	rVB2	465831	539559	8.41%	3.391%
2	1.666	91	95	105	rVB	122980	153412	2.39%	0.964%
3	2.306	194	200	213	rVB	282098	436540	6.81%	2.743%
4	2.434	218	221	224	rVB	938	1226	0.02%	0.008%
5	2.489	228	230	231	rBV	499	392	0.01%	0.002%
6	2.770	275	276	277	rBV	525	340	0.01%	0.002%
7	2.794	277	280	282	rVV3	822	975	0.02%	0.006%
8	2.965	306	308	311	rBV	375	413	0.01%	0.003%
9	3.093	321	329	339	rBV	55171	106547	1.66%	0.670%
10	3.166	339	341	343	rVV	393	381	0.01%	0.002%
11	3.264	354	357	359	rBV2	487	627	0.01%	0.004%
12	3.355	370	372	375	rVB	467	381	0.01%	0.002%
13	3.575	406	408	410	rBV2	337	406	0.01%	0.003%
14	3.629	413	417	418	rBV2	284	360	0.01%	0.002%
15	3.678	423	425	427	rVV2	392	331	0.01%	0.002%
16	3.806	444	446	447	rVB2	425	306	0.00%	0.002%
17	3.989	474	476	478	rBV	367	294	0.00%	0.002%
18	4.141	498	501	502	rBV2	348	341	0.01%	0.002%
19	4.495	544	559	579	rBV	2346339	6413503	100.00%	40.305%
20	4.867	619	620	623	rBV	371	311	0.00%	0.002%
21	5.062	638	652	669	rBV	158368	496224	7.74%	3.118%
22	5.519	725	727	729	rBV2	562	484	0.01%	0.003%
23	5.751	762	765	766	rVB2	408	380	0.01%	0.002%
24	5.873	783	785	787	rBV	330	305	0.00%	0.002%
25	5.977	790	802	817	rVV2	432820	1250397	19.50%	7.858%
26	6.190	836	837	840	rVB3	428	375	0.01%	0.002%
27	6.239	840	845	849	rBV4	623	880	0.01%	0.006%
28	6.342	861	862	864	rBV2	662	632	0.01%	0.004%
29	6.483	883	885	887	rVB3	668	427	0.01%	0.003%
30	6.513	887	890	892	rBV	314	334	0.01%	0.002%
31	6.537	892	894	896	rBV	521	554	0.01%	0.003%
32	6.769	922	932	947	rBV	290586	703357	10.97%	4.420%
33	7.001	968	970	972	rBV	537	570	0.01%	0.004%
34	7.031	972	975	979	rVV2	697	652	0.01%	0.004%
35	7.129	981	991	1002	rBV5	16373	47505	0.74%	0.299%
36	7.312	1012	1021	1033	rBV	257203	566796	8.84%	3.562%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030400.D
 Acq On : 04 Aug 2022 18:37
 Operator : JC/MD
 Sample : N4003-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.495	1045	1051	1055	rBV6	1426	2249	0.04%	0.014%
38	7.580	1063	1065	1069	rVB2	692	752	0.01%	0.005%
39	7.738	1088	1091	1093	rBV2	391	421	0.01%	0.003%
40	7.891	1112	1116	1117	rBV2	594	681	0.01%	0.004%
41	7.970	1127	1129	1134	rVB3	653	591	0.01%	0.004%
42	8.043	1139	1141	1143	rBV2	352	362	0.01%	0.002%
43	8.110	1150	1152	1154	rBV2	444	454	0.01%	0.003%
44	8.147	1154	1158	1159	rVB2	619	553	0.01%	0.003%
45	8.159	1159	1160	1166	rVB2	500	630	0.01%	0.004%
46	8.220	1166	1170	1172	rBV2	491	779	0.01%	0.005%
47	8.330	1181	1188	1199	rBV	175666	294568	4.59%	1.851%
48	8.513	1216	1218	1222	rVB2	482	453	0.01%	0.003%
49	8.555	1222	1225	1226	rBV2	510	445	0.01%	0.003%
50	8.653	1234	1241	1254	rBV	640708	989903	15.43%	6.221%
51	8.952	1285	1290	1301	rBV	130067	193341	3.01%	1.215%
52	9.134	1318	1320	1321	rVB	686	440	0.01%	0.003%
53	9.147	1321	1322	1325	rBV2	309	371	0.01%	0.002%
54	9.275	1339	1343	1351	rVB5	2173	3578	0.06%	0.022%
55	9.391	1356	1362	1373	rBV	479201	700934	10.93%	4.405%
56	9.793	1425	1428	1432	rBV2	504	590	0.01%	0.004%
57	9.860	1437	1439	1444	rVB2	449	370	0.01%	0.002%
58	9.903	1444	1446	1448	rBV	420	377	0.01%	0.002%
59	9.951	1451	1454	1456	rBV2	319	439	0.01%	0.003%
60	10.055	1465	1471	1481	rBV	598565	802825	12.52%	5.045%
61	10.372	1521	1523	1526	rVB2	494	533	0.01%	0.003%
62	10.403	1526	1528	1529	rBV	522	377	0.01%	0.002%
63	10.433	1532	1533	1536	rVB2	622	401	0.01%	0.003%
64	10.524	1546	1548	1551	rVB2	468	335	0.01%	0.002%
65	10.561	1551	1554	1556	rBV2	609	578	0.01%	0.004%
66	10.628	1563	1565	1566	rBV	475	408	0.01%	0.003%
67	10.787	1589	1591	1592	rVB	538	305	0.00%	0.002%
68	10.817	1592	1596	1598	rBV3	501	693	0.01%	0.004%
69	10.860	1601	1603	1606	rVB2	472	469	0.01%	0.003%
70	11.043	1632	1633	1635	rBV	507	321	0.01%	0.002%
71	11.195	1652	1658	1666	rVV	460678	576980	9.00%	3.626%
72	11.396	1689	1691	1694	rBV3	565	495	0.01%	0.003%
73	11.482	1703	1705	1708	rBV3	516	383	0.01%	0.002%
74	11.634	1728	1730	1732	rBV	435	291	0.00%	0.002%
75	12.024	1789	1794	1803	rBV	622508	757724	11.81%	4.762%
76	12.177	1817	1819	1822	rVB2	433	355	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030400.D
 Acq On : 04 Aug 2022 18:37
 Operator : JC/MD
 Sample : N4003-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.250	1826	1831	1833	rBV2	435	681	0.01%	0.004%
78	12.323	1837	1843	1852	rBV	660933	835717	13.03%	5.252%
79	12.719	1906	1908	1910	rBV	432	378	0.01%	0.002%
80	12.768	1914	1916	1919	rVB	618	431	0.01%	0.003%
81	12.811	1919	1923	1924	rBV3	315	348	0.01%	0.002%
82	13.006	1953	1955	1959	rVB	567	604	0.01%	0.004%
83	13.061	1961	1964	1965	rVB2	803	714	0.01%	0.004%
84	13.103	1969	1971	1974	rVV2	728	805	0.01%	0.005%
85	13.152	1977	1979	1981	rVV2	466	452	0.01%	0.003%
86	13.183	1983	1984	1987	rVV	502	365	0.01%	0.002%
87	13.426	2020	2024	2026	rBV	518	573	0.01%	0.004%
88	13.591	2049	2051	2052	rBV2	505	412	0.01%	0.003%
89	13.646	2058	2060	2063	rVB	585	476	0.01%	0.003%
90	13.780	2079	2082	2085	rBV3	729	1094	0.02%	0.007%
91	13.939	2104	2108	2109	rBV2	496	608	0.01%	0.004%
92	14.073	2129	2130	2134	rBV	551	554	0.01%	0.003%
93	14.365	2176	2178	2180	rBV3	511	483	0.01%	0.003%
94	14.579	2210	2213	2215	rBV2	488	741	0.01%	0.005%
95	14.670	2226	2228	2229	rBV2	692	602	0.01%	0.004%
96	14.816	2251	2252	2255	rBV3	724	694	0.01%	0.004%
97	14.963	2273	2276	2277	rBV	831	742	0.01%	0.005%
98	15.018	2283	2285	2286	rVB2	691	317	0.00%	0.002%
99	15.932	2433	2435	2438	rBV3	701	717	0.01%	0.005%
100	16.420	2513	2515	2518	rBV2	693	543	0.01%	0.003%




Sum of corrected areas: 15912322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030400.D
Acq On : 04 Aug 2022 18:37
Operator : JC/MD
Sample : N4003-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

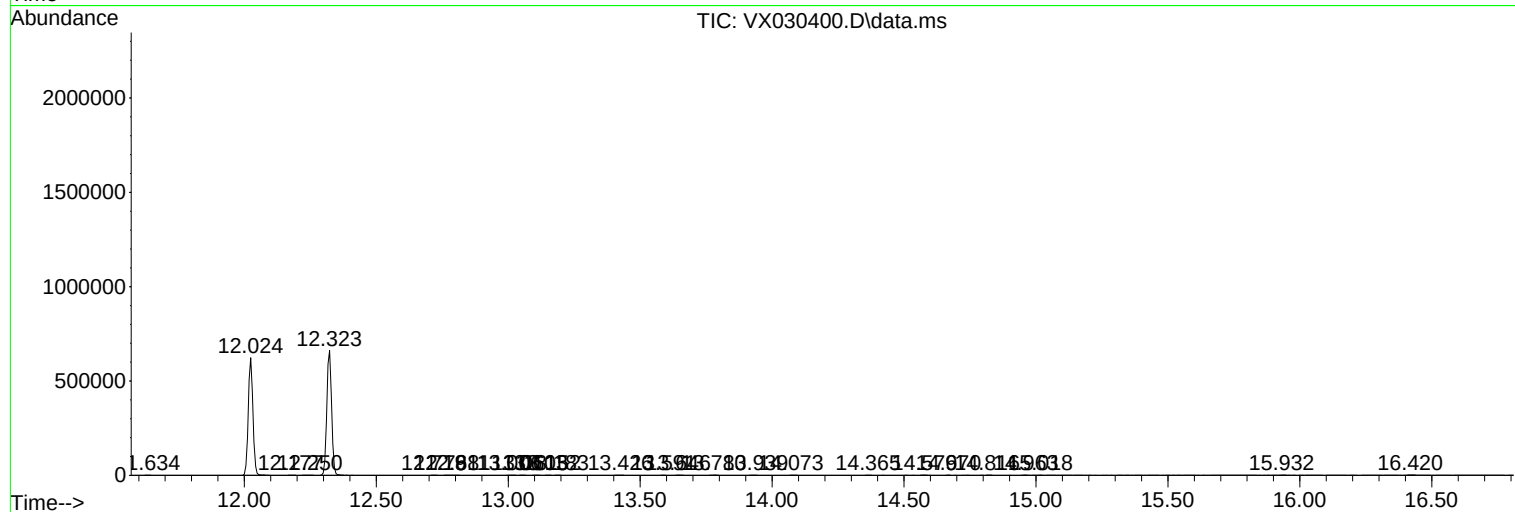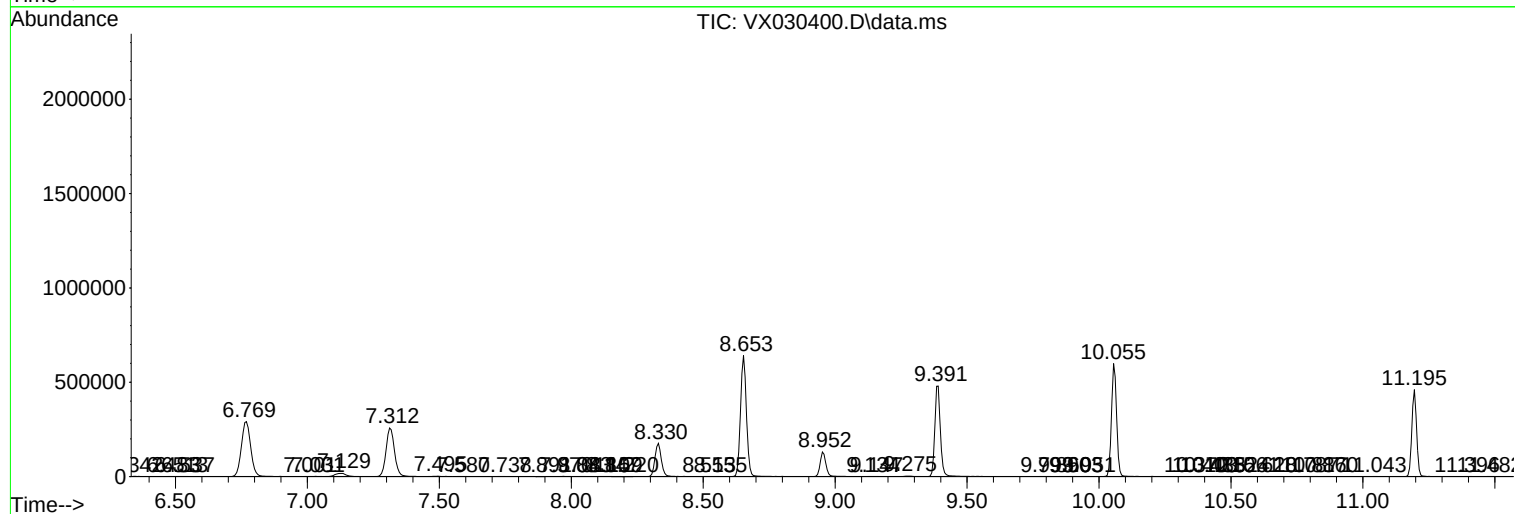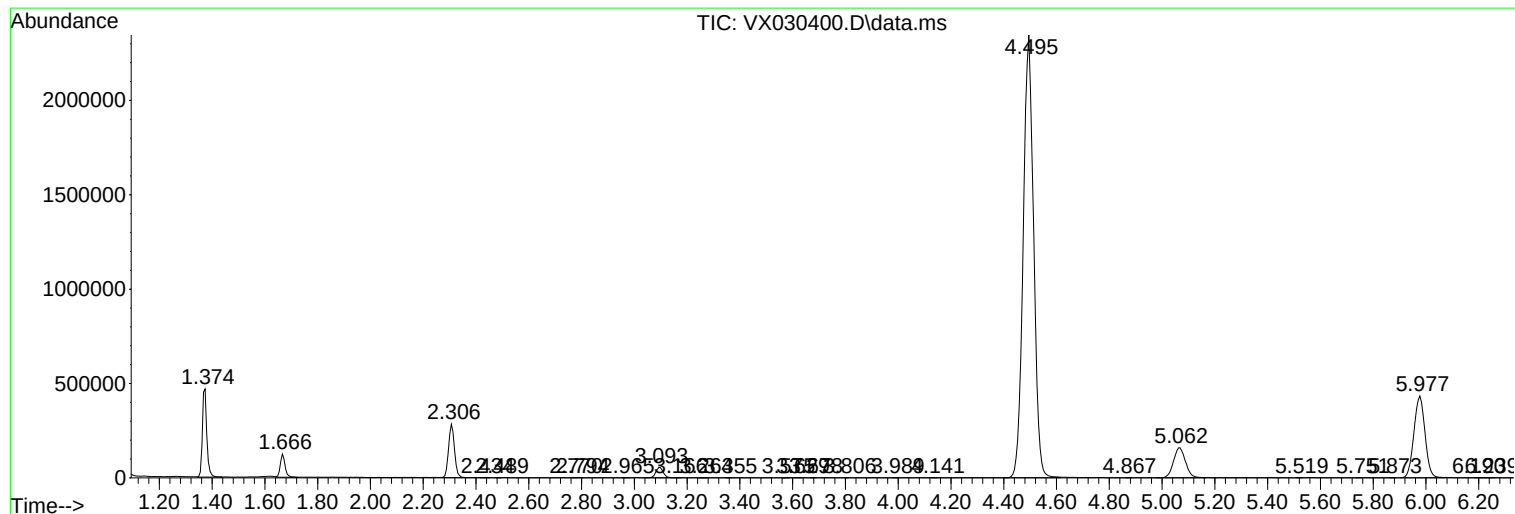

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030400.D
Acq On : 04 Aug 2022 18:37
Operator : JC/MD
Sample : N4003-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030400.D
Acq On : 04 Aug 2022 18:37
Operator : JC/MD
Sample : N4003-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc