

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030401.D
 Acq On : 04 Aug 2022 19:01
 Operator : JC/MD
 Sample : N4003-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	14	rVB	4670	4143	0.27%	0.039%
2	1.367	42	46	56	rVB2	197595	203096	13.08%	1.888%
3	1.666	91	95	103	rVB	136530	162277	10.45%	1.509%
4	2.306	194	200	210	rBV	277869	435759	28.05%	4.052%
5	2.392	210	214	220	rVB	7349	12822	0.83%	0.119%
6	2.508	232	233	237	rVB3	630	587	0.04%	0.005%
7	2.770	274	276	277	rBV2	625	594	0.04%	0.006%
8	2.782	277	278	285	rVV4	1186	2046	0.13%	0.019%
9	2.867	288	292	293	rBV3	536	698	0.04%	0.006%
10	2.886	293	295	298	rVV3	506	596	0.04%	0.006%
11	2.977	306	310	312	rBV3	582	909	0.06%	0.008%
12	3.117	323	333	345	rBV	120257	300992	19.38%	2.799%
13	3.276	357	359	362	rVB	584	426	0.03%	0.004%
14	3.385	376	377	381	rBV2	432	447	0.03%	0.004%
15	3.446	385	387	389	rVV2	512	546	0.04%	0.005%
16	3.501	392	396	399	rBV3	306	498	0.03%	0.005%
17	3.581	406	409	413	rVB3	725	987	0.06%	0.009%
18	3.617	413	415	419	rBV2	455	871	0.06%	0.008%
19	3.654	419	421	424	rVV2	514	517	0.03%	0.005%
20	3.818	445	448	449	rBV2	369	390	0.03%	0.004%
21	3.843	450	452	457	rVB2	439	486	0.03%	0.005%
22	3.898	457	461	465	rBV2	459	825	0.05%	0.008%
23	3.971	470	473	474	rBV	419	410	0.03%	0.004%
24	4.062	486	488	493	rBV2	444	718	0.05%	0.007%
25	4.105	493	495	497	rVV2	451	482	0.03%	0.004%
26	4.324	529	531	534	rVB	451	401	0.03%	0.004%
27	4.495	544	559	578	rBV2	510743	1553280	100.00%	14.443%
28	5.068	639	653	669	rBV	160952	500725	32.24%	4.656%
29	5.330	694	696	700	rVB2	453	502	0.03%	0.005%
30	5.373	700	703	706	rBV3	837	1174	0.08%	0.011%
31	5.397	706	707	709	rVB	740	459	0.03%	0.004%
32	5.665	748	751	753	rVV	323	417	0.03%	0.004%
33	5.824	773	777	779	rBV	440	529	0.03%	0.005%
34	5.976	790	802	816	rBV2	419266	1235924	79.57%	11.492%
35	6.208	837	840	845	rBV2	530	843	0.05%	0.008%
36	6.336	859	861	863	rBV2	659	615	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030401.D
 Acq On : 04 Aug 2022 19:01
 Operator : JC/MD
 Sample : N4003-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.470	880	883	888	rVB2	710	884	0.06%	0.008%
38	6.598	899	904	905	rBV2	421	567	0.04%	0.005%
39	6.769	921	932	945	rBV	266866	640618	41.24%	5.957%
40	7.129	981	991	1002	rBV3	63693	147859	9.52%	1.375%
41	7.312	1012	1021	1036	rBV	256530	560818	36.11%	5.215%
42	7.476	1045	1048	1049	rBV2	682	635	0.04%	0.006%
43	7.592	1066	1067	1069	rBV2	462	426	0.03%	0.004%
44	7.775	1093	1097	1098	rBV	319	421	0.03%	0.004%
45	7.860	1106	1111	1114	rBV3	421	839	0.05%	0.008%
46	8.153	1156	1159	1161	rVB2	596	614	0.04%	0.006%
47	8.330	1180	1188	1198	rBV	174900	287220	18.49%	2.671%
48	8.653	1234	1241	1254	rBV	641764	988364	63.63%	9.190%
49	8.951	1285	1290	1300	rBV	127586	188482	12.13%	1.753%
50	9.055	1305	1307	1309	rVB3	600	486	0.03%	0.005%
51	9.238	1335	1337	1340	rVV2	513	514	0.03%	0.005%
52	9.275	1340	1343	1351	rVB5	7236	11390	0.73%	0.106%
53	9.390	1356	1362	1376	rBV	477323	692302	44.57%	6.437%
54	9.586	1392	1394	1400	rBV2	479	812	0.05%	0.008%
55	9.628	1400	1401	1404	rVB	621	528	0.03%	0.005%
56	9.665	1404	1407	1408	rBV2	552	399	0.03%	0.004%
57	9.683	1408	1410	1412	rVB2	662	504	0.03%	0.005%
58	9.817	1430	1432	1437	rVB2	418	399	0.03%	0.004%
59	9.884	1442	1443	1447	rBV3	445	650	0.04%	0.006%
60	10.055	1465	1471	1483	rBV	541951	728911	46.93%	6.778%
61	10.390	1524	1526	1528	rVV	578	538	0.03%	0.005%
62	10.610	1560	1562	1564	rBV	431	397	0.03%	0.004%
63	10.646	1567	1568	1571	rVB2	746	459	0.03%	0.004%
64	10.695	1574	1576	1578	rVV	581	376	0.02%	0.003%
65	10.762	1585	1587	1589	rBV2	468	409	0.03%	0.004%
66	11.091	1637	1641	1644	rBV2	613	683	0.04%	0.006%
67	11.195	1652	1658	1671	rBV	429360	553151	35.61%	5.143%
68	11.286	1671	1673	1675	rBV	639	443	0.03%	0.004%
69	11.402	1688	1692	1694	rBV2	497	635	0.04%	0.006%
70	11.561	1717	1718	1722	rVB	470	449	0.03%	0.004%
71	11.652	1730	1733	1735	rVV3	396	455	0.03%	0.004%
72	11.738	1746	1747	1749	rBV	403	382	0.02%	0.004%
73	11.756	1749	1750	1753	rVV	674	598	0.04%	0.006%
74	11.945	1779	1781	1785	rVB2	532	742	0.05%	0.007%
75	11.981	1785	1787	1788	rBV	529	389	0.03%	0.004%
76	12.024	1788	1794	1805	rBV	556141	672502	43.30%	6.253%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030401.D
 Acq On : 04 Aug 2022 19:01
 Operator : JC/MD
 Sample : N4003-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.225	1826	1827	1830	rVB	500	418	0.03%	0.004%
78	12.323	1837	1843	1850	rBV	658237	827664	53.28%	7.696%
79	12.469	1865	1867	1870	rVB3	547	489	0.03%	0.005%
80	12.707	1902	1906	1907	rBV	350	393	0.03%	0.004%
81	12.865	1930	1932	1935	rBV	334	417	0.03%	0.004%
82	13.109	1970	1972	1974	rVB2	526	466	0.03%	0.004%
83	13.243	1992	1994	1997	rBV	508	744	0.05%	0.007%
84	13.749	2075	2077	2079	rBV2	596	515	0.03%	0.005%
85	13.816	2086	2088	2090	rBV2	435	400	0.03%	0.004%
86	13.969	2111	2113	2115	rVB	582	394	0.03%	0.004%
87	14.012	2119	2120	2123	rBV2	431	502	0.03%	0.005%
88	14.152	2141	2143	2146	rBV3	428	395	0.03%	0.004%
89	14.243	2156	2158	2160	rVB2	579	395	0.03%	0.004%
90	14.262	2160	2161	2163	rBV	559	378	0.02%	0.004%
91	14.505	2199	2201	2203	rBV	502	384	0.02%	0.004%
92	14.591	2212	2215	2218	rBV3	640	884	0.06%	0.008%
93	14.676	2226	2229	2232	rBV3	572	784	0.05%	0.007%
94	14.792	2246	2248	2253	rBV4	537	903	0.06%	0.008%
95	14.963	2274	2276	2277	rBV2	806	576	0.04%	0.005%
96	15.237	2319	2321	2323	rBV2	507	490	0.03%	0.005%
97	15.993	2444	2445	2451	rVB4	992	1092	0.07%	0.010%
98	16.060	2454	2456	2457	rBV2	677	555	0.04%	0.005%
99	16.542	2533	2535	2536	rBV	710	429	0.03%	0.004%
100	16.755	2568	2570	2572	rBV3	702	603	0.04%	0.006%

Sum of corrected areas: 10754511




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030401.D
Acq On : 04 Aug 2022 19:01
Operator : JC/MD
Sample : N4003-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

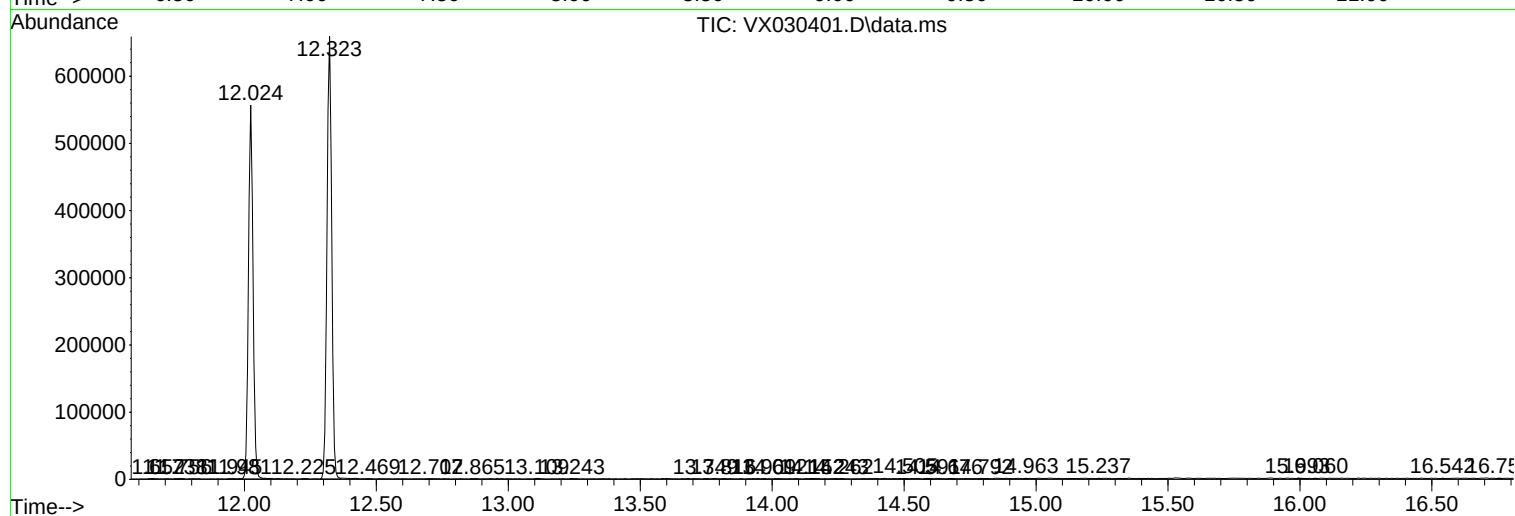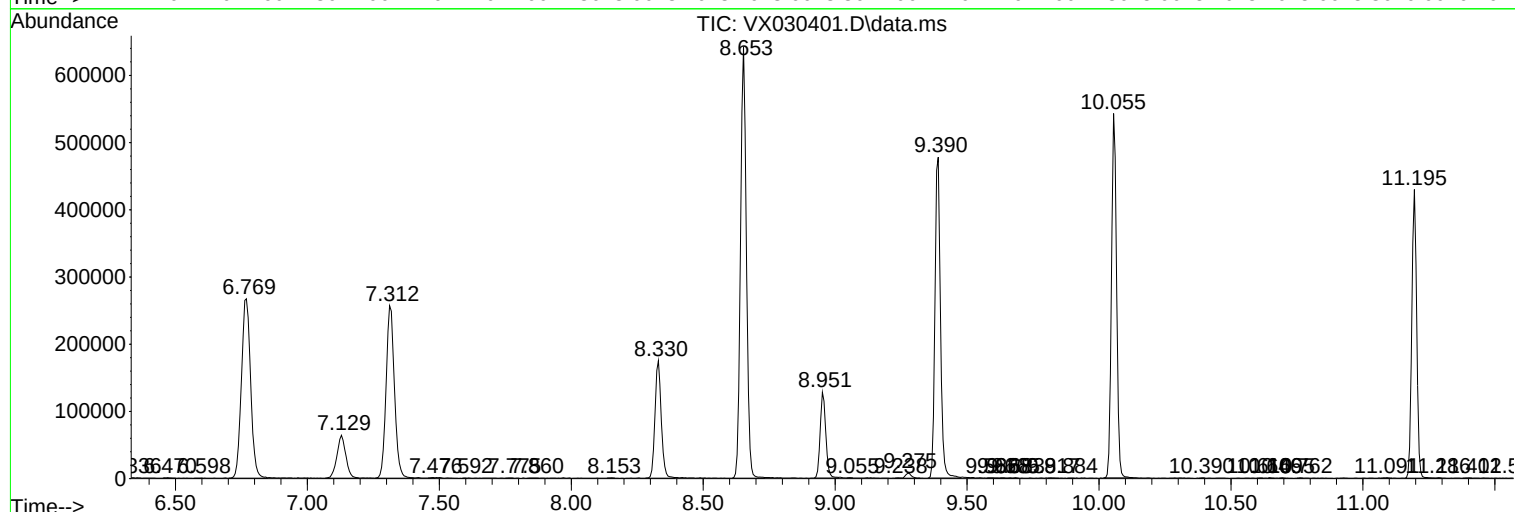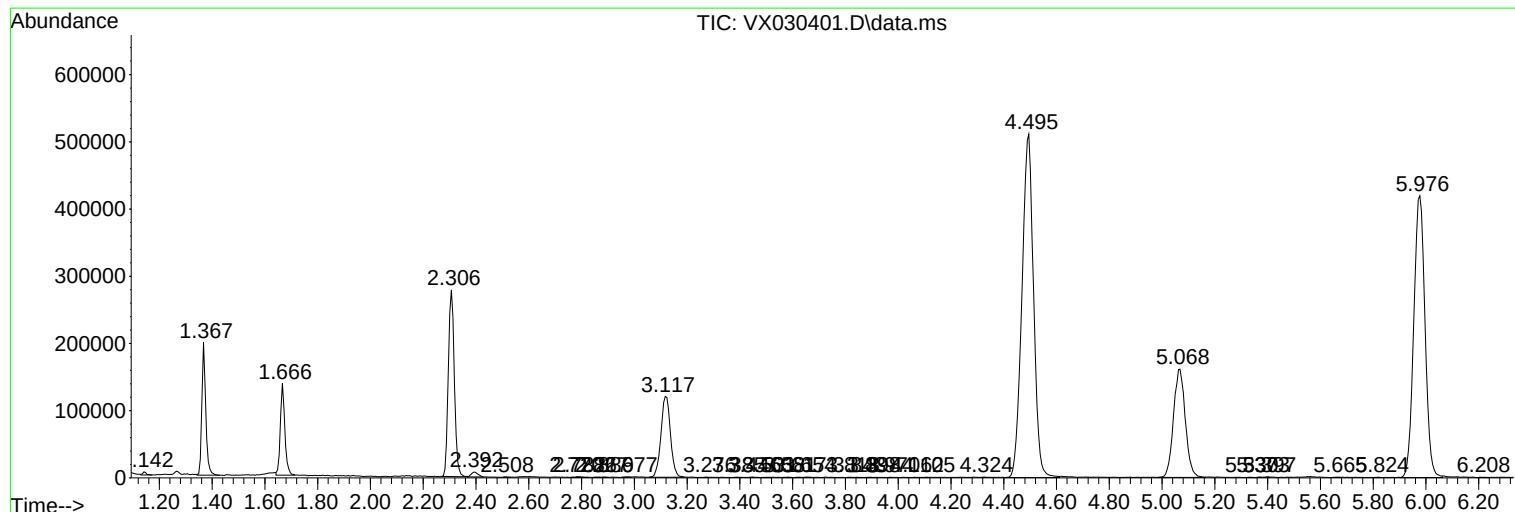

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030401.D
Acq On : 04 Aug 2022 19:01
Operator : JC/MD
Sample : N4003-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030401.D
Acq On : 04 Aug 2022 19:01
Operator : JC/MD
Sample : N4003-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------