

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030403.D
 Acq On : 04 Aug 2022 19:47
 Operator : JC/MD
 Sample : N4003-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	205202	224662	8.80%	1.957%
2	1.666	91	95	104	rVB	125447	153223	6.00%	1.335%
3	2.306	194	200	212	rVB	281515	435853	17.07%	3.797%
4	2.709	264	266	267	rBV2	483	383	0.01%	0.003%
5	2.788	276	279	283	rVB3	1326	1751	0.07%	0.015%
6	2.825	283	285	289	rVB2	416	593	0.02%	0.005%
7	3.099	323	330	337	rVV	28168	55193	2.16%	0.481%
8	3.331	366	368	371	rVV2	443	577	0.02%	0.005%
9	3.440	385	386	388	rBV	446	383	0.01%	0.003%
10	3.837	445	451	454	rBV2	340	616	0.02%	0.005%
11	4.397	536	543	545	rBV4	502	1035	0.04%	0.009%
12	4.489	545	558	576	rBV2	877500	2553949	100.00%	22.249%
13	4.702	591	593	595	rBV	757	481	0.02%	0.004%
14	4.861	614	619	621	rBV3	529	913	0.04%	0.008%
15	4.934	630	631	635	rBV	569	496	0.02%	0.004%
16	5.062	640	652	668	rBV2	161567	506143	19.82%	4.409%
17	5.300	690	691	696	rVB2	492	538	0.02%	0.005%
18	5.355	696	700	702	rBV2	414	440	0.02%	0.004%
19	5.385	702	705	709	rBV3	655	1161	0.05%	0.010%
20	5.483	719	721	724	rBV2	376	443	0.02%	0.004%
21	5.556	728	733	735	rBV5	1208	1460	0.06%	0.013%
22	5.976	786	802	818	rBV2	423720	1249730	48.93%	10.887%
23	6.306	855	856	858	rBV2	456	371	0.01%	0.003%
24	6.361	863	865	870	rVB2	683	583	0.02%	0.005%
25	6.470	879	883	884	rBV2	452	647	0.03%	0.006%
26	6.586	900	902	904	rVB2	431	401	0.02%	0.003%
27	6.617	904	907	910	rBV2	536	733	0.03%	0.006%
28	6.641	910	911	914	rBV2	334	393	0.02%	0.003%
29	6.769	920	932	944	rBV	268469	642831	25.17%	5.600%
30	7.129	981	991	999	rBV7	18676	49146	1.92%	0.428%
31	7.312	1012	1021	1034	rBV	256165	567192	22.21%	4.941%
32	7.482	1047	1049	1053	rBV2	841	1262	0.05%	0.011%
33	7.537	1056	1058	1061	rVB2	368	331	0.01%	0.003%
34	7.562	1061	1062	1065	rBV2	538	480	0.02%	0.004%
35	7.586	1065	1066	1068	rBV2	437	363	0.01%	0.003%
36	7.647	1073	1076	1081	rBV3	582	1033	0.04%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030403.D
 Acq On : 04 Aug 2022 19:47
 Operator : JC/MD
 Sample : N4003-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.763	1093	1095	1100	rVB3	449	483	0.02%	0.004%
38	7.866	1110	1112	1114	rBV	458	382	0.01%	0.003%
39	8.104	1149	1151	1155	rVB	570	480	0.02%	0.004%
40	8.147	1155	1158	1159	rBV2	384	357	0.01%	0.003%
41	8.202	1165	1167	1168	rBV2	401	334	0.01%	0.003%
42	8.226	1168	1171	1174	rVB3	335	424	0.02%	0.004%
43	8.250	1174	1175	1176	rBV	676	328	0.01%	0.003%
44	8.330	1181	1188	1202	rVV	173301	285580	11.18%	2.488%
45	8.543	1221	1223	1224	rVB2	601	355	0.01%	0.003%
46	8.653	1234	1241	1250	rVV	630903	983886	38.52%	8.571%
47	8.952	1284	1290	1301	rBV	124457	186672	7.31%	1.626%
48	9.116	1315	1317	1322	rBV3	549	875	0.03%	0.008%
49	9.281	1339	1344	1348	rVB4	817	1658	0.06%	0.014%
50	9.323	1348	1351	1354	rBV3	308	516	0.02%	0.004%
51	9.390	1356	1362	1377	rBV	476607	689279	26.99%	6.005%
52	9.555	1388	1389	1393	rVB2	757	559	0.02%	0.005%
53	9.640	1401	1403	1405	rBV2	462	467	0.02%	0.004%
54	9.659	1405	1406	1409	rVV2	515	565	0.02%	0.005%
55	9.689	1409	1411	1413	rVB2	725	490	0.02%	0.004%
56	9.714	1413	1415	1417	rBV2	300	338	0.01%	0.003%
57	9.823	1431	1433	1436	rVB3	537	409	0.02%	0.004%
58	9.927	1449	1450	1455	rBV2	715	773	0.03%	0.007%
59	10.000	1458	1462	1463	rBV2	335	357	0.01%	0.003%
60	10.055	1465	1471	1483	rVV	539265	731817	28.65%	6.375%
61	10.189	1491	1493	1496	rBV2	410	369	0.01%	0.003%
62	10.220	1496	1498	1499	rVB	576	346	0.01%	0.003%
63	10.238	1499	1501	1503	rBV2	314	365	0.01%	0.003%
64	10.268	1503	1506	1509	rBV	476	596	0.02%	0.005%
65	10.299	1509	1511	1516	rVB3	1056	1077	0.04%	0.009%
66	10.512	1543	1546	1548	rBV2	517	589	0.02%	0.005%
67	10.640	1565	1567	1569	rBV2	1070	747	0.03%	0.007%
68	10.829	1594	1598	1600	rVB2	300	387	0.02%	0.003%
69	10.866	1600	1604	1608	rVB2	531	933	0.04%	0.008%
70	10.896	1608	1609	1611	rBV	480	408	0.02%	0.004%
71	10.957	1617	1619	1621	rBV	335	387	0.02%	0.003%
72	11.085	1638	1640	1644	rVB3	640	382	0.01%	0.003%
73	11.195	1652	1658	1669	rBV	446516	570716	22.35%	4.972%
74	11.475	1703	1704	1708	rBV3	369	480	0.02%	0.004%
75	11.762	1749	1751	1754	rVB	638	545	0.02%	0.005%
76	11.884	1768	1771	1773	rBV2	426	580	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030403.D
 Acq On : 04 Aug 2022 19:47
 Operator : JC/MD
 Sample : N4003-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1806	rBV	558397	680486	26.64%	5.928%
78	12.323	1837	1843	1849	rBV	691439	863490	33.81%	7.522%
79	12.609	1886	1890	1891	rBV3	456	632	0.02%	0.006%
80	12.701	1904	1905	1907	rBV	455	331	0.01%	0.003%
81	12.847	1926	1929	1933	rVV2	529	697	0.03%	0.006%
82	12.890	1933	1936	1939	rVV	464	639	0.03%	0.006%
83	12.914	1939	1940	1943	rVB2	551	501	0.02%	0.004%
84	12.945	1943	1945	1946	rBV	394	365	0.01%	0.003%
85	12.981	1950	1951	1954	rBV2	453	522	0.02%	0.005%
86	13.231	1989	1992	1997	rBV	690	829	0.03%	0.007%
87	13.365	2012	2014	2016	rBV	381	371	0.01%	0.003%
88	13.481	2030	2033	2036	rBV2	381	512	0.02%	0.004%
89	13.548	2042	2044	2046	rBV2	396	448	0.02%	0.004%
90	13.774	2079	2081	2084	rBV3	610	776	0.03%	0.007%
91	14.103	2132	2135	2137	rBV2	558	713	0.03%	0.006%
92	14.329	2171	2172	2175	rBV2	581	578	0.02%	0.005%
93	14.408	2181	2185	2187	rVB3	574	780	0.03%	0.007%
94	14.481	2195	2197	2198	rBV	492	352	0.01%	0.003%
95	14.548	2206	2208	2214	rBV2	554	737	0.03%	0.006%
96	14.749	2238	2241	2242	rBV2	692	719	0.03%	0.006%
97	14.883	2261	2263	2264	rBV	597	362	0.01%	0.003%
98	15.396	2343	2347	2348	rVB3	897	1022	0.04%	0.009%
99	15.511	2364	2366	2368	rBV2	735	453	0.02%	0.004%
100	16.578	2539	2541	2542	rBV	549	453	0.02%	0.004%




Sum of corrected areas: 11478848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030403.D
Acq On : 04 Aug 2022 19:47
Operator : JC/MD
Sample : N4003-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

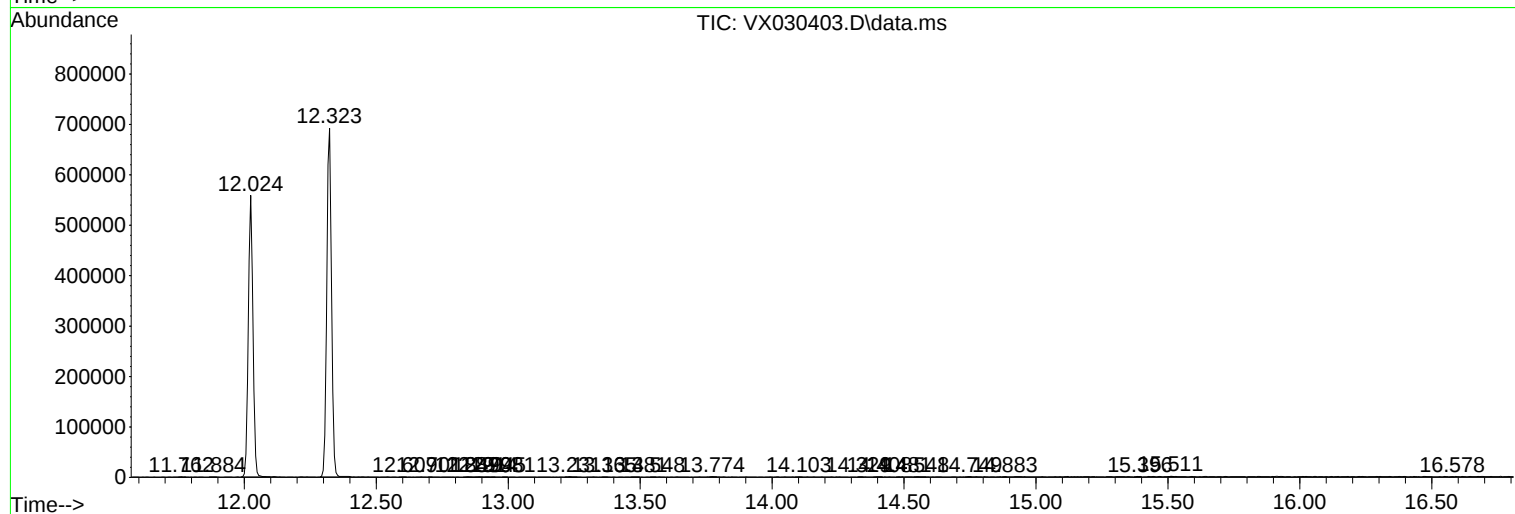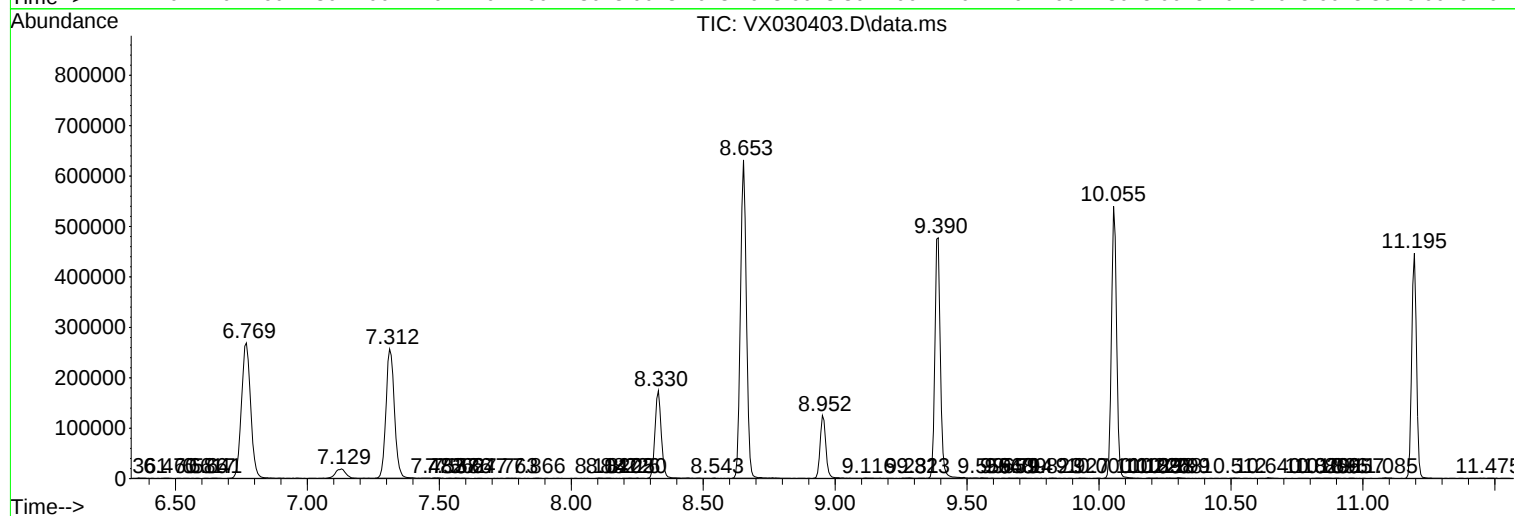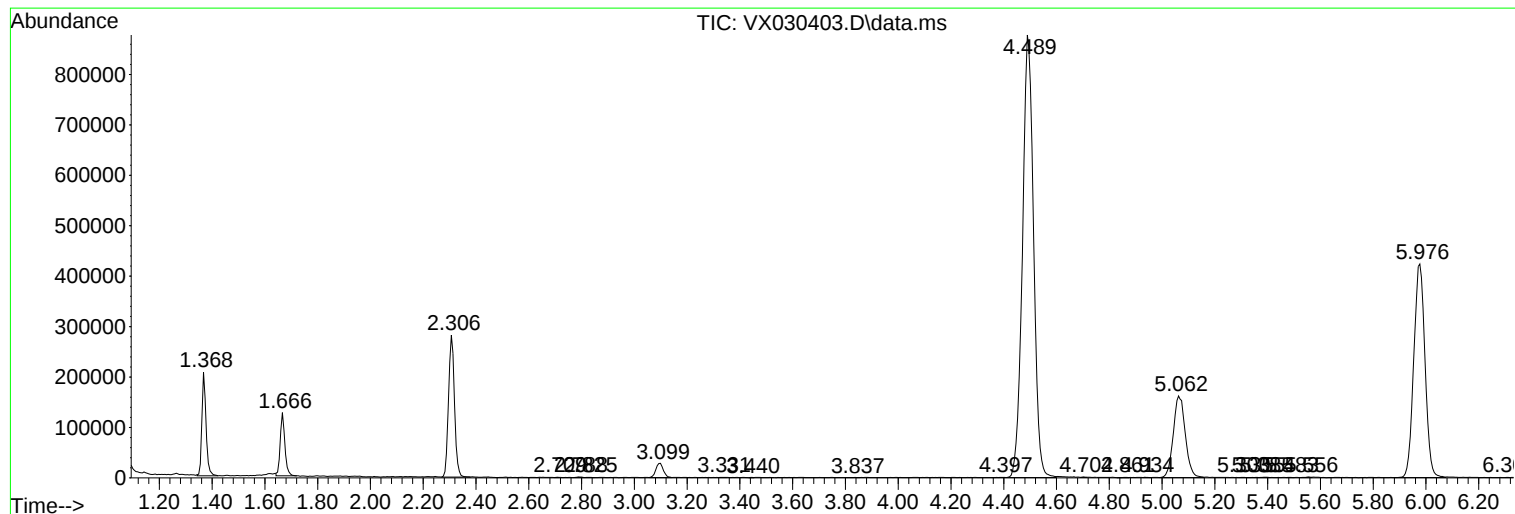

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030403.D
Acq On : 04 Aug 2022 19:47
Operator : JC/MD
Sample : N4003-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030403.D
Acq On : 04 Aug 2022 19:47
Operator : JC/MD
Sample : N4003-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc