

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030404.D
 Acq On : 04 Aug 2022 20:11
 Operator : JC/MD
 Sample : N4003-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB2	211403	230064	8.99%	2.025%
2	1.666	91	95	104	rVB	122229	153248	5.99%	1.349%
3	2.306	194	200	209	rVB	282056	429141	16.77%	3.777%
4	2.501	230	232	236	rBV3	597	834	0.03%	0.007%
5	2.587	244	246	249	rVB2	603	474	0.02%	0.004%
6	2.690	260	263	266	rBV3	546	727	0.03%	0.006%
7	2.794	276	280	282	rBV3	1036	1495	0.06%	0.013%
8	2.849	287	289	291	rBV2	387	414	0.02%	0.004%
9	2.971	307	309	311	rBV	368	366	0.01%	0.003%
10	3.038	316	320	322	rBV2	383	469	0.02%	0.004%
11	3.093	323	329	338	rVB	28073	53533	2.09%	0.471%
12	3.337	366	369	371	rVB2	494	608	0.02%	0.005%
13	3.367	371	374	375	rVB2	488	403	0.02%	0.004%
14	3.385	375	377	380	rBV3	407	560	0.02%	0.005%
15	3.581	405	409	412	rBV	320	379	0.01%	0.003%
16	3.684	423	426	427	rBV2	511	515	0.02%	0.005%
17	3.721	430	432	433	rBV	446	347	0.01%	0.003%
18	3.867	451	456	457	rVB	550	806	0.03%	0.007%
19	3.891	457	460	461	rBV2	485	334	0.01%	0.003%
20	3.916	461	464	468	rBV2	383	561	0.02%	0.005%
21	3.983	471	475	477	rVB2	323	374	0.01%	0.003%
22	4.050	485	486	490	rBV2	416	576	0.02%	0.005%
23	4.160	502	504	507	rVB2	412	388	0.02%	0.003%
24	4.190	507	509	512	rVB3	609	544	0.02%	0.005%
25	4.361	535	537	541	rBV2	454	482	0.02%	0.004%
26	4.397	541	543	545	rVB2	444	381	0.01%	0.003%
27	4.495	545	559	576	rBV2	888993	2559347	100.00%	22.527%
28	4.696	591	592	595	rBV3	707	648	0.03%	0.006%
29	4.782	604	606	610	rVB	605	615	0.02%	0.005%
30	4.842	614	616	618	rBV	646	441	0.02%	0.004%
31	4.971	633	637	638	rBV2	529	623	0.02%	0.005%
32	5.068	640	653	671	rVB	163686	501906	19.61%	4.418%
33	5.269	684	686	687	rBV	737	557	0.02%	0.005%
34	5.373	701	703	704	rBV	389	348	0.01%	0.003%
35	5.397	704	707	708	rVB	513	490	0.02%	0.004%
36	5.854	781	782	785	rVB2	395	333	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030404.D
 Acq On : 04 Aug 2022 20:11
 Operator : JC/MD
 Sample : N4003-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.976	787	802	821	rBV2	428186	1245582	48.67%	10.963%
38	6.452	878	880	881	rBV2	481	425	0.02%	0.004%
39	6.617	905	907	909	rVB	478	334	0.01%	0.003%
40	6.641	909	911	914	rBV	441	571	0.02%	0.005%
41	6.769	919	932	944	rBV	254619	612603	23.94%	5.392%
42	7.129	982	991	999	rVB6	18389	47861	1.87%	0.421%
43	7.312	1013	1021	1038	rVB	260312	562658	21.98%	4.952%
44	7.592	1065	1067	1070	rBV2	491	474	0.02%	0.004%
45	7.714	1084	1087	1089	rVB2	505	584	0.02%	0.005%
46	8.031	1137	1139	1141	rVB2	470	336	0.01%	0.003%
47	8.159	1158	1160	1162	rBV2	331	402	0.02%	0.004%
48	8.330	1181	1188	1200	rBV	181548	287025	11.21%	2.526%
49	8.543	1220	1223	1224	rBV2	422	396	0.02%	0.003%
50	8.561	1224	1226	1228	rVB2	428	379	0.01%	0.003%
51	8.653	1234	1241	1249	rBV	648899	989414	38.66%	8.709%
52	8.854	1272	1274	1276	rVB2	625	386	0.02%	0.003%
53	8.951	1284	1290	1300	rBV	125801	188543	7.37%	1.660%
54	9.080	1309	1311	1315	rBV2	613	761	0.03%	0.007%
55	9.116	1315	1317	1318	rBV2	418	337	0.01%	0.003%
56	9.208	1329	1332	1333	rBV2	447	329	0.01%	0.003%
57	9.384	1356	1361	1375	rBV	464021	687461	26.86%	6.051%
58	9.610	1397	1398	1402	rVB3	500	521	0.02%	0.005%
59	9.915	1444	1448	1449	rBV	302	330	0.01%	0.003%
60	9.933	1449	1451	1455	rVB2	384	380	0.01%	0.003%
61	10.055	1465	1471	1481	rBV	506350	708839	27.70%	6.239%
62	10.305	1509	1512	1515	rBV3	537	720	0.03%	0.006%
63	10.396	1525	1527	1530	rBV	305	354	0.01%	0.003%
64	10.445	1533	1535	1537	rVB	490	353	0.01%	0.003%
65	10.482	1537	1541	1543	rBV	486	663	0.03%	0.006%
66	11.073	1634	1638	1639	rBV	521	483	0.02%	0.004%
67	11.195	1652	1658	1670	rBV	453064	577608	22.57%	5.084%
68	11.366	1682	1686	1687	rVV	359	397	0.02%	0.003%
69	11.427	1693	1696	1697	rBV	503	451	0.02%	0.004%
70	11.488	1700	1706	1707	rBV2	551	817	0.03%	0.007%
71	11.506	1707	1709	1711	rBV2	441	344	0.01%	0.003%
72	11.689	1737	1739	1741	rBV2	403	323	0.01%	0.003%
73	11.707	1741	1742	1744	rBV	566	336	0.01%	0.003%
74	11.774	1749	1753	1755	rBV2	634	751	0.03%	0.007%
75	11.933	1778	1779	1782	rBV2	564	524	0.02%	0.005%
76	12.024	1789	1794	1804	rVB	541324	647720	25.31%	5.701%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030404.D
 Acq On : 04 Aug 2022 20:11
 Operator : JC/MD
 Sample : N4003-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.183	1819	1820	1822	rBV	391	328	0.01%	0.003%
78	12.323	1837	1843	1852	rBV	683066	837975	32.74%	7.376%
79	12.548	1878	1880	1884	rVB2	521	611	0.02%	0.005%
80	12.585	1884	1886	1887	rBV	397	345	0.01%	0.003%
81	12.640	1894	1895	1899	rBV2	483	632	0.02%	0.006%
82	12.731	1907	1910	1912	rBV3	290	382	0.01%	0.003%
83	12.780	1914	1918	1920	rVB2	455	689	0.03%	0.006%
84	12.951	1944	1946	1947	rVB	594	342	0.01%	0.003%
85	13.006	1951	1955	1956	rBV2	381	345	0.01%	0.003%
86	13.054	1960	1963	1964	rBV	405	382	0.01%	0.003%
87	13.109	1970	1972	1974	rBV	688	533	0.02%	0.005%
88	13.195	1982	1986	1988	rVV3	804	733	0.03%	0.006%
89	13.347	2008	2011	2012	rBV2	499	533	0.02%	0.005%
90	13.707	2068	2070	2072	rVB2	563	478	0.02%	0.004%
91	13.853	2092	2094	2097	rBV2	351	358	0.01%	0.003%
92	14.024	2120	2122	2126	rVB2	490	609	0.02%	0.005%
93	14.066	2126	2129	2132	rBV2	527	605	0.02%	0.005%
94	14.335	2171	2173	2175	rBV	625	497	0.02%	0.004%
95	15.542	2369	2371	2372	rBV2	508	333	0.01%	0.003%
96	15.597	2378	2380	2382	rBV	818	583	0.02%	0.005%
97	15.865	2423	2424	2426	rBV	780	527	0.02%	0.005%
98	16.456	2519	2521	2522	rBV	585	363	0.01%	0.003%
99	16.475	2522	2524	2525	rVV	957	516	0.02%	0.005%
100	16.731	2564	2566	2568	rBV2	659	559	0.02%	0.005%

Sum of corrected areas: 11361364




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030404.D
Acq On : 04 Aug 2022 20:11
Operator : JC/MD
Sample : N4003-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

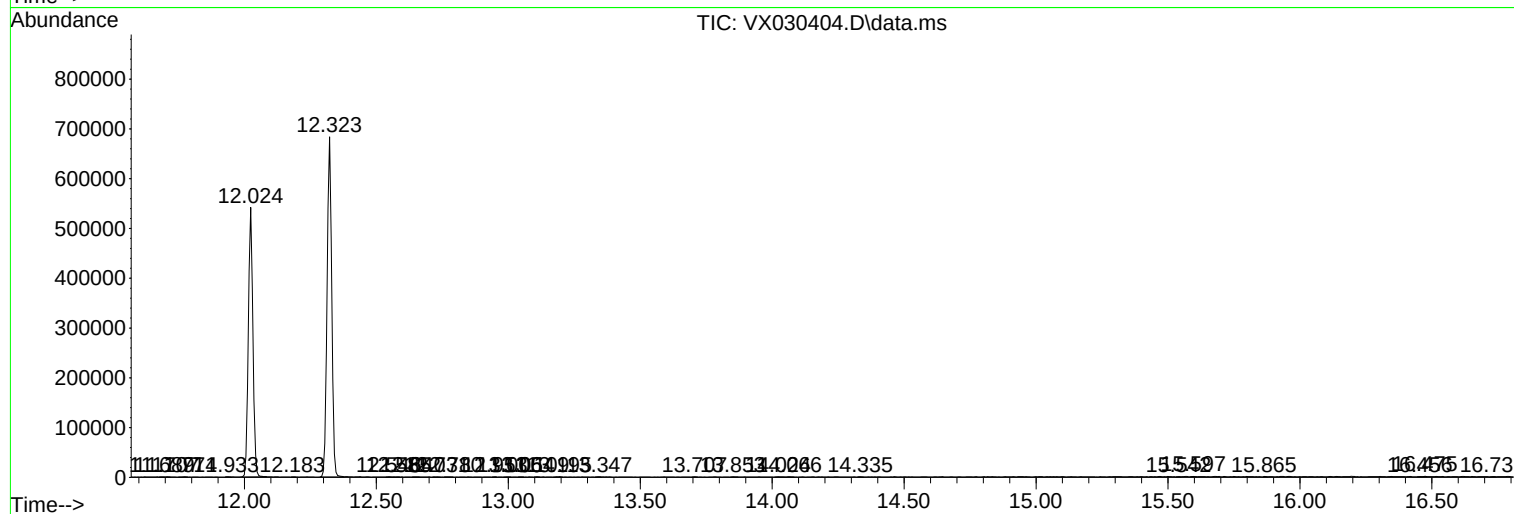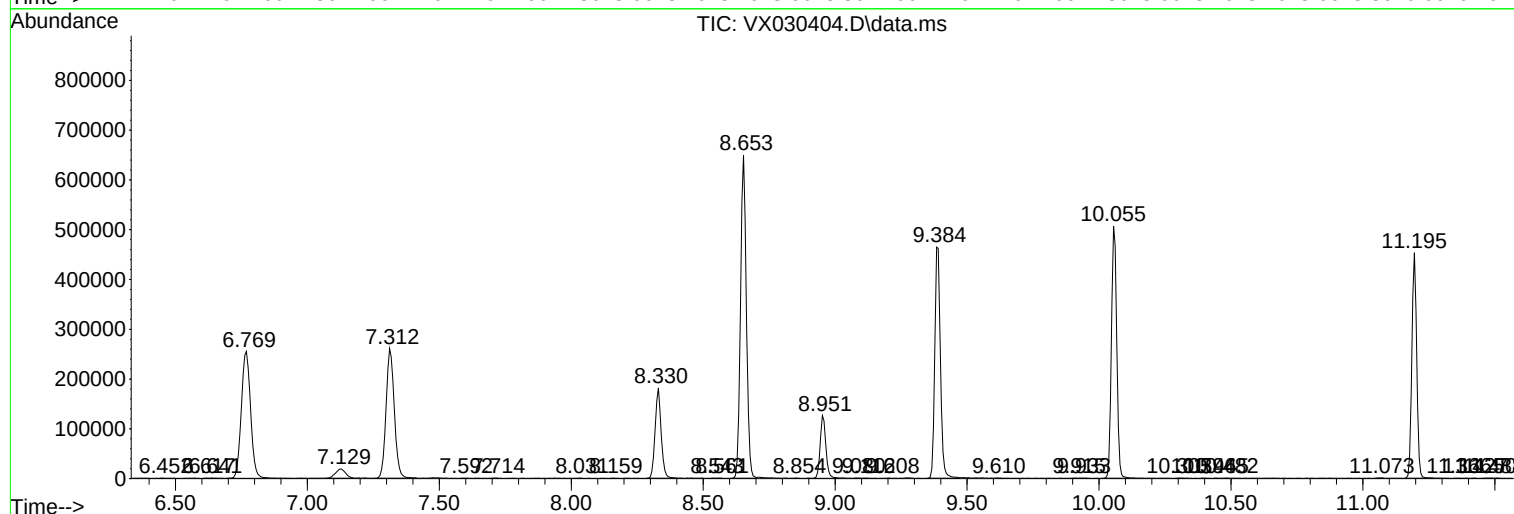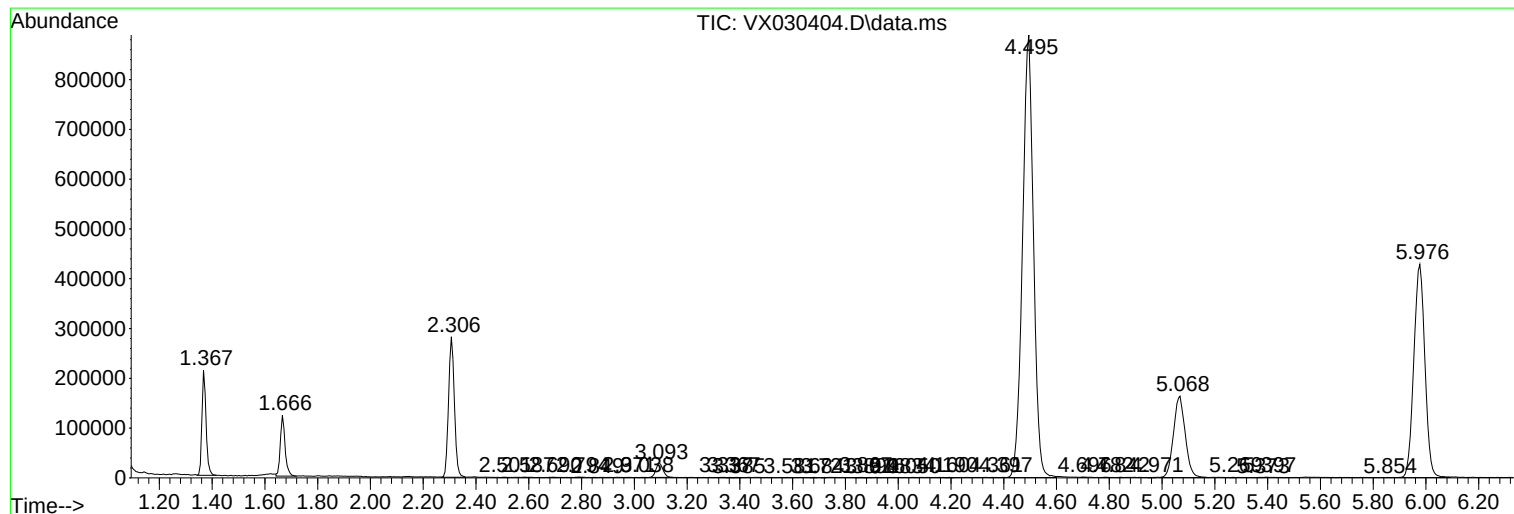

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030404.D
Acq On : 04 Aug 2022 20:11
Operator : JC/MD
Sample : N4003-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030404.D
Acq On : 04 Aug 2022 20:11
Operator : JC/MD
Sample : N4003-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc