

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030408.D
 Acq On : 04 Aug 2022 21:44
 Operator : JC/MD
 Sample : N4003-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rVB	2769305	2965507	20.11%	10.794%
2	1.599	81	84	89	rBV	19036	28208	0.19%	0.103%
3	1.666	91	95	104	rVB	125360	152939	1.04%	0.557%
4	2.313	194	201	212	rVB2	373852	687984	4.67%	2.504%
5	2.703	263	265	266	rBV	456	421	0.00%	0.002%
6	2.782	275	278	279	rBV2	951	954	0.01%	0.003%
7	2.983	309	311	313	rBV	454	560	0.00%	0.002%
8	3.093	319	329	343	rBV	361071	681783	4.62%	2.482%
9	3.257	354	356	358	rVB	565	340	0.00%	0.001%
10	3.282	358	360	363	rBV	453	349	0.00%	0.001%
11	3.398	376	379	380	rBV	751	590	0.00%	0.002%
12	3.416	380	382	385	rVB2	616	595	0.00%	0.002%
13	3.465	385	390	391	rBV	494	733	0.00%	0.003%
14	3.648	418	420	422	rBV	645	631	0.00%	0.002%
15	3.782	439	442	445	rBV	391	593	0.00%	0.002%
16	4.056	484	487	488	rBV2	426	352	0.00%	0.001%
17	4.263	518	521	523	rBV2	558	594	0.00%	0.002%
18	4.361	532	537	545	rVB5	1712	4071	0.03%	0.015%
19	4.495	545	559	581	rBV	5291432	14747414	100.00%	53.677%
20	4.964	634	636	638	rBV2	631	719	0.00%	0.003%
21	5.062	641	652	669	rVB	156654	494374	3.35%	1.799%
22	5.477	717	720	725	rBV	601	984	0.01%	0.004%
23	5.550	728	732	733	rBV2	1014	1214	0.01%	0.004%
24	5.611	740	742	745	rBV	271	363	0.00%	0.001%
25	5.672	751	752	756	rVB	375	340	0.00%	0.001%
26	5.733	758	762	764	rBV2	415	488	0.00%	0.002%
27	5.812	772	775	777	rBV2	321	394	0.00%	0.001%
28	5.861	781	783	787	rBV3	366	382	0.00%	0.001%
29	5.977	789	802	817	rBV2	431194	1245864	8.45%	4.535%
30	6.361	860	865	866	rVV2	956	1338	0.01%	0.005%
31	6.379	866	868	872	rVV4	824	1094	0.01%	0.004%
32	6.470	882	883	885	rVV2	488	438	0.00%	0.002%
33	6.519	888	891	893	rBV3	320	440	0.00%	0.002%
34	6.543	893	895	898	rVB2	740	819	0.01%	0.003%
35	6.574	898	900	902	rBV2	576	575	0.00%	0.002%
36	6.641	910	911	917	rVB2	383	346	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030408.D
 Acq On : 04 Aug 2022 21:44
 Operator : JC/MD
 Sample : N4003-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.763	920	931	944	rBV	282533	677497	4.59%	2.466%
38	7.117	982	989	1000	rVB5	11578	28127	0.19%	0.102%
39	7.312	1011	1021	1033	rBV	273157	609729	4.13%	2.219%
40	7.482	1045	1049	1052	rBV4	1260	1915	0.01%	0.007%
41	7.555	1059	1061	1064	rBV2	580	595	0.00%	0.002%
42	7.671	1077	1080	1084	rBV3	337	624	0.00%	0.002%
43	8.019	1134	1137	1139	rBV	624	593	0.00%	0.002%
44	8.043	1139	1141	1143	rVV2	645	524	0.00%	0.002%
45	8.080	1145	1147	1149	rVV	406	351	0.00%	0.001%
46	8.165	1159	1161	1163	rVB	621	562	0.00%	0.002%
47	8.190	1163	1165	1166	rBV2	489	442	0.00%	0.002%
48	8.330	1181	1188	1199	rBV	169927	283566	1.92%	1.032%
49	8.604	1232	1233	1234	rBV	598	359	0.00%	0.001%
50	8.653	1234	1241	1250	rVV	624072	978486	6.63%	3.561%
51	8.775	1260	1261	1266	rBV2	793	973	0.01%	0.004%
52	8.860	1271	1275	1278	rBV5	511	818	0.01%	0.003%
53	8.952	1284	1290	1298	rBV	126197	188877	1.28%	0.687%
54	9.049	1304	1306	1308	rBV3	494	452	0.00%	0.002%
55	9.208	1330	1332	1338	rVB3	575	805	0.01%	0.003%
56	9.281	1341	1344	1348	rBV4	1383	1842	0.01%	0.007%
57	9.317	1348	1350	1354	rVB2	505	610	0.00%	0.002%
58	9.384	1354	1361	1375	rBV	479307	697063	4.73%	2.537%
59	9.829	1431	1434	1438	rBV3	415	867	0.01%	0.003%
60	10.000	1459	1462	1463	rBV	424	377	0.00%	0.001%
61	10.055	1465	1471	1483	rVV	541940	729088	4.94%	2.654%
62	10.281	1507	1508	1512	rBV2	374	480	0.00%	0.002%
63	10.366	1520	1522	1524	rVV2	396	380	0.00%	0.001%
64	10.476	1538	1540	1543	rBV2	513	498	0.00%	0.002%
65	10.616	1561	1563	1565	rVB2	577	492	0.00%	0.002%
66	10.652	1565	1569	1571	rBV2	378	518	0.00%	0.002%
67	10.768	1587	1588	1591	rVB2	718	458	0.00%	0.002%
68	10.811	1593	1595	1598	rVB2	542	419	0.00%	0.002%
69	10.951	1616	1618	1620	rBV2	499	486	0.00%	0.002%
70	11.079	1637	1639	1644	rVB2	680	1029	0.01%	0.004%
71	11.152	1647	1651	1652	rBV2	357	383	0.00%	0.001%
72	11.195	1652	1658	1665	rBV	459327	574817	3.90%	2.092%
73	11.408	1691	1693	1696	rBV2	427	415	0.00%	0.002%
74	11.494	1704	1707	1708	rVV3	440	342	0.00%	0.001%
75	11.549	1715	1716	1719	rVB2	586	467	0.00%	0.002%
76	11.841	1762	1764	1767	rBV2	506	440	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030408.D
 Acq On : 04 Aug 2022 21:44
 Operator : JC/MD
 Sample : N4003-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.963	1782	1784	1787	rBV2	429	381	0.00%	0.001%
78	12.024	1789	1794	1804	rVV	622565	742364	5.03%	2.702%
79	12.171	1817	1818	1822	rBV2	594	760	0.01%	0.003%
80	12.201	1822	1823	1825	rVB	575	350	0.00%	0.001%
81	12.323	1837	1843	1850	rBV	722204	907643	6.15%	3.304%
82	12.646	1895	1896	1900	rBV	443	548	0.00%	0.002%
83	13.012	1951	1956	1957	rVB3	638	809	0.01%	0.003%
84	13.146	1976	1978	1982	rVB2	282	356	0.00%	0.001%
85	13.311	2002	2005	2007	rVB3	473	478	0.00%	0.002%
86	13.390	2016	2018	2021	rVB3	377	510	0.00%	0.002%
87	13.481	2031	2033	2036	rVV2	693	548	0.00%	0.002%
88	13.536	2040	2042	2043	rVV2	520	400	0.00%	0.001%
89	13.713	2067	2071	2074	rBV2	821	1256	0.01%	0.005%
90	13.786	2080	2083	2089	rVB3	581	991	0.01%	0.004%
91	14.158	2142	2144	2149	rVB2	492	682	0.00%	0.002%
92	14.231	2153	2156	2159	rBV3	450	651	0.00%	0.002%
93	14.579	2211	2213	2216	rVB	648	396	0.00%	0.001%
94	14.603	2216	2217	2219	rBV	987	693	0.00%	0.003%
95	14.640	2221	2223	2224	rVV	576	379	0.00%	0.001%
96	14.676	2228	2229	2232	rBV2	465	423	0.00%	0.002%
97	14.810	2250	2251	2256	rVB2	650	706	0.00%	0.003%
98	15.420	2349	2351	2352	rVB	708	345	0.00%	0.001%
99	15.828	2417	2418	2420	rBV2	743	539	0.00%	0.002%
100	16.194	2476	2478	2481	rBV3	744	529	0.00%	0.002%




Sum of corrected areas: 27474293

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030408.D
Acq On : 04 Aug 2022 21:44
Operator : JC/MD
Sample : N4003-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

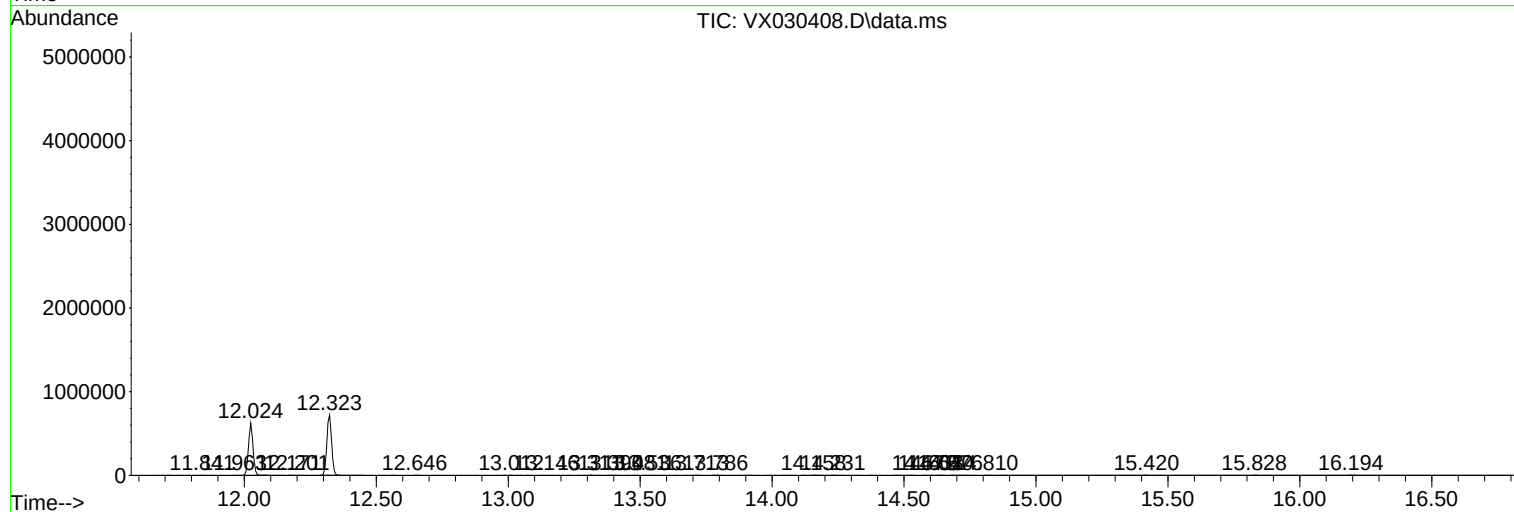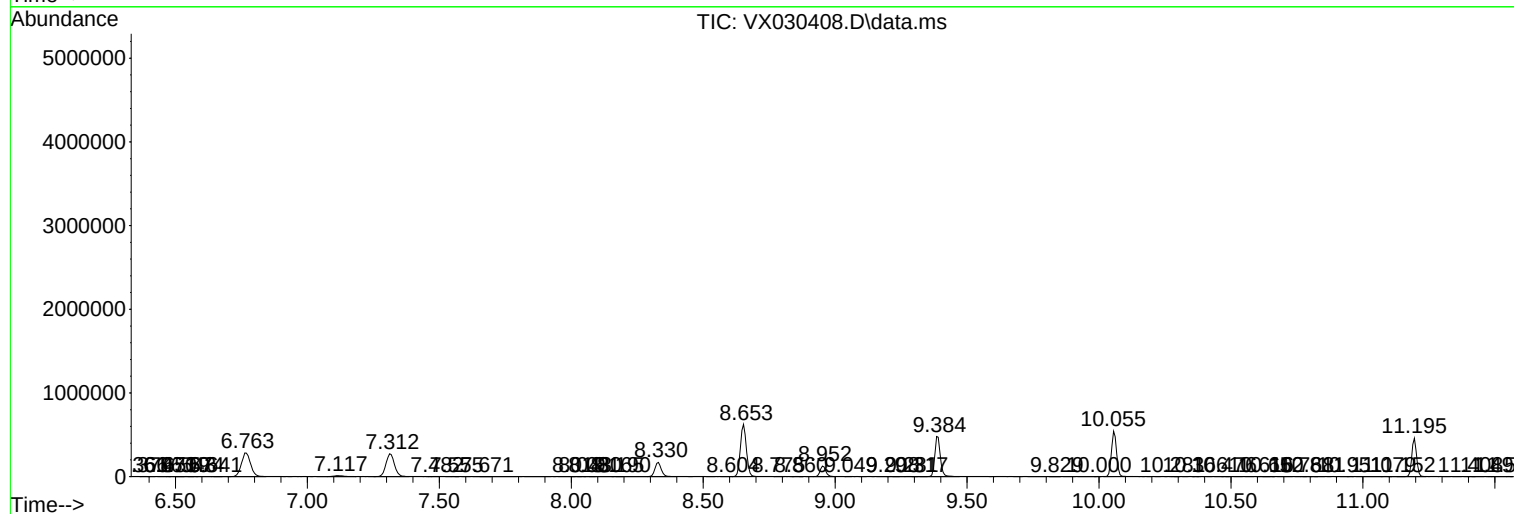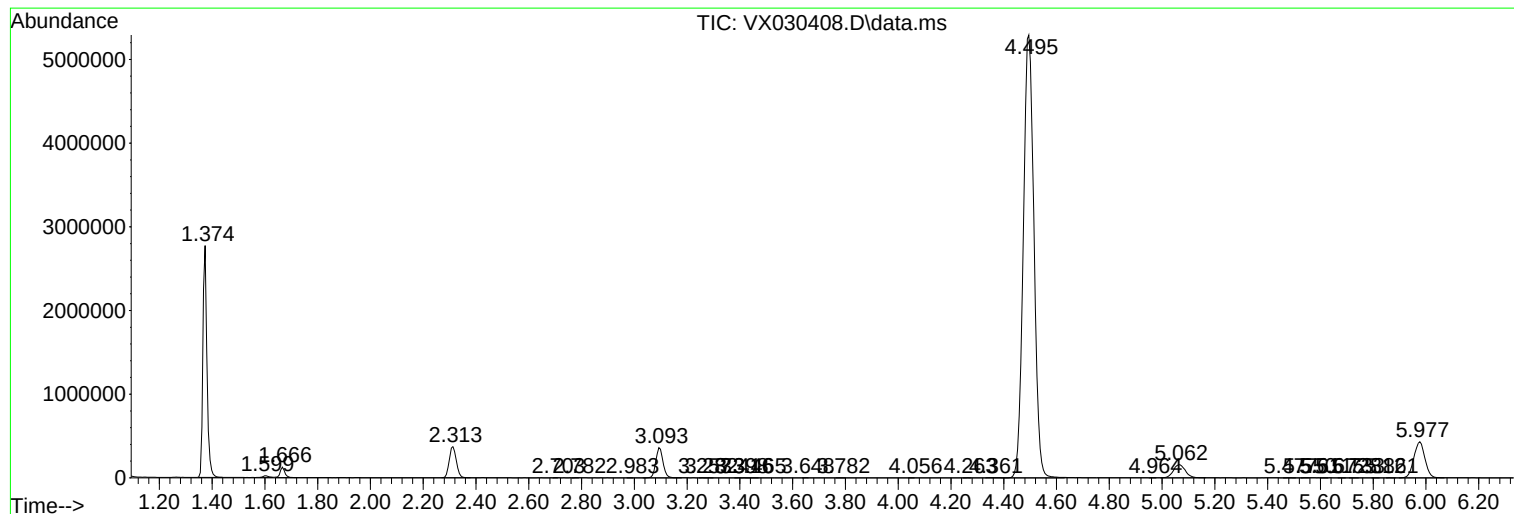

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030408.D
Acq On : 04 Aug 2022 21:44
Operator : JC/MD
Sample : N4003-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030408.D
Acq On : 04 Aug 2022 21:44
Operator : JC/MD
Sample : N4003-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc