

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030410.D
 Acq On : 04 Aug 2022 22:31
 Operator : JC/MD
 Sample : N4021-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	257269	303653	24.65%	3.234%
2	1.666	91	95	103	rVB	130806	156272	12.68%	1.664%
3	2.307	194	200	212	rVB	272038	421636	34.22%	4.490%
4	2.508	231	233	238	rVB2	932	1476	0.12%	0.016%
5	2.624	249	252	253	rBV3	414	405	0.03%	0.004%
6	2.697	260	264	267	rBV3	475	837	0.07%	0.009%
7	2.752	271	273	276	rBV2	356	440	0.04%	0.005%
8	2.782	276	278	281	rBV2	664	739	0.06%	0.008%
9	2.861	290	291	297	rVB3	531	682	0.06%	0.007%
10	2.910	297	299	300	rBV	485	422	0.03%	0.004%
11	2.977	308	310	311	rBV2	421	336	0.03%	0.004%
12	3.093	323	329	335	rBV	10698	18486	1.50%	0.197%
13	3.282	356	360	362	rBV2	297	515	0.04%	0.005%
14	3.556	403	405	408	rVB3	496	393	0.03%	0.004%
15	3.660	421	422	427	rVB3	623	781	0.06%	0.008%
16	3.715	427	431	435	rBV2	664	1081	0.09%	0.012%
17	3.751	435	437	440	rVV2	476	564	0.05%	0.006%
18	3.843	448	452	453	rBV2	590	470	0.04%	0.005%
19	3.861	453	455	457	rVB	555	502	0.04%	0.005%
20	3.879	457	458	460	rBV	384	361	0.03%	0.004%
21	3.922	463	465	467	rBV	374	329	0.03%	0.004%
22	3.977	473	474	476	rVB	711	399	0.03%	0.004%
23	4.196	508	510	513	rVV2	481	442	0.04%	0.005%
24	4.227	513	515	519	rVB2	445	335	0.03%	0.004%
25	4.361	534	537	541	rBV2	388	509	0.04%	0.005%
26	4.483	545	557	574	rBV3	152871	555187	45.06%	5.912%
27	5.068	641	653	668	rVV2	162591	494009	40.10%	5.261%
28	5.196	671	674	676	rVV3	689	577	0.05%	0.006%
29	5.245	678	682	685	rVB	417	698	0.06%	0.007%
30	5.391	704	706	707	rBV	580	411	0.03%	0.004%
31	5.544	728	731	733	rBV3	604	734	0.06%	0.008%
32	5.568	733	735	736	rVB2	804	520	0.04%	0.006%
33	5.641	744	747	749	rBV2	466	690	0.06%	0.007%
34	5.855	780	782	785	rBV2	423	384	0.03%	0.004%
35	5.977	788	802	819	rBV2	423829	1232018	100.00%	13.120%
36	6.245	844	846	849	rVB	545	525	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030410.D
 Acq On : 04 Aug 2022 22:31
 Operator : JC/MD
 Sample : N4021-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	6.379	865	868	871	rBV3	670	738	0.06%	0.008%
38	6.769	922	932	945	rBV	256577	615261	49.94%	6.552%
39	6.976	964	966	969	rVB3	528	464	0.04%	0.005%
40	7.013	970	972	975	rVV	663	494	0.04%	0.005%
41	7.056	977	979	980	rBV	454	456	0.04%	0.005%
42	7.129	982	991	1003	rVV4	57600	140025	11.37%	1.491%
43	7.312	1012	1021	1036	rBV	245824	557723	45.27%	5.939%
44	7.489	1043	1050	1052	rBV3	834	1775	0.14%	0.019%
45	7.635	1071	1074	1077	rBV2	391	613	0.05%	0.007%
46	7.714	1086	1087	1089	rBV2	570	349	0.03%	0.004%
47	7.745	1089	1092	1094	rVB2	552	593	0.05%	0.006%
48	7.769	1094	1096	1097	rVB	516	352	0.03%	0.004%
49	7.787	1097	1099	1102	rBV2	458	643	0.05%	0.007%
50	7.879	1112	1114	1118	rVB2	340	404	0.03%	0.004%
51	7.958	1124	1127	1130	rBV2	487	536	0.04%	0.006%
52	8.275	1176	1179	1181	rBV2	505	632	0.05%	0.007%
53	8.330	1181	1188	1198	rVV	170673	277817	22.55%	2.958%
54	8.525	1218	1220	1223	rVB	705	616	0.05%	0.007%
55	8.653	1234	1241	1252	rBV	626541	970400	78.77%	10.334%
56	8.952	1284	1290	1299	rBV	125341	186528	15.14%	1.986%
57	9.177	1323	1327	1328	rBV3	480	443	0.04%	0.005%
58	9.220	1333	1334	1337	rBV	496	511	0.04%	0.005%
59	9.275	1339	1343	1349	rVB4	4837	7124	0.58%	0.076%
60	9.385	1356	1361	1372	rBV	468928	684515	55.56%	7.289%
61	9.659	1405	1406	1409	rVB	782	557	0.05%	0.006%
62	9.884	1441	1443	1446	rVB	496	464	0.04%	0.005%
63	9.982	1457	1459	1462	rVB2	487	420	0.03%	0.004%
64	10.012	1462	1464	1465	rBV	401	378	0.03%	0.004%
65	10.055	1465	1471	1483	rVV	532681	714054	57.96%	7.604%
66	10.208	1494	1496	1499	rVB3	546	355	0.03%	0.004%
67	10.464	1537	1538	1541	rBV2	559	355	0.03%	0.004%
68	10.653	1567	1569	1570	rVB	537	329	0.03%	0.004%
69	10.787	1589	1591	1595	rBV2	523	693	0.06%	0.007%
70	10.817	1595	1596	1601	rBV2	378	406	0.03%	0.004%
71	11.085	1638	1640	1642	rVB2	634	465	0.04%	0.005%
72	11.110	1642	1644	1648	rBV2	528	472	0.04%	0.005%
73	11.195	1653	1658	1666	rVB	443005	557557	45.26%	5.937%
74	11.293	1673	1674	1676	rBV2	591	362	0.03%	0.004%
75	11.451	1698	1700	1702	rBV	339	346	0.03%	0.004%
76	11.524	1710	1712	1714	rBV2	399	415	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030410.D
 Acq On : 04 Aug 2022 22:31
 Operator : JC/MD
 Sample : N4021-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.549	1714	1716	1718	rVB2	445	389	0.03%	0.004%
78	11.579	1718	1721	1722	rBV2	433	521	0.04%	0.006%
79	11.713	1741	1743	1746	rBV2	646	747	0.06%	0.008%
80	11.805	1756	1758	1760	rBV3	471	511	0.04%	0.005%
81	12.024	1789	1794	1810	rVV	531695	651872	52.91%	6.942%
82	12.158	1814	1816	1818	rVB2	592	411	0.03%	0.004%
83	12.323	1837	1843	1853	rBV	652448	802905	65.17%	8.550%
84	12.622	1889	1892	1894	rBV2	522	670	0.05%	0.007%
85	12.670	1898	1900	1901	rBV	547	478	0.04%	0.005%
86	12.823	1924	1925	1929	rVV3	509	378	0.03%	0.004%
87	12.866	1929	1932	1935	rVV2	627	705	0.06%	0.008%
88	12.975	1948	1950	1952	rBV2	676	536	0.04%	0.006%
89	13.359	2011	2013	2016	rVB	664	562	0.05%	0.006%
90	13.530	2040	2041	2043	rBV	451	345	0.03%	0.004%
91	13.573	2046	2048	2050	rBV2	486	349	0.03%	0.004%
92	13.786	2078	2083	2084	rBV2	757	776	0.06%	0.008%
93	14.000	2116	2118	2122	rVB	656	801	0.07%	0.009%
94	14.036	2122	2124	2125	rBV	626	493	0.04%	0.005%
95	14.566	2208	2211	2213	rBV3	383	363	0.03%	0.004%
96	14.859	2258	2259	2261	rBV2	559	337	0.03%	0.004%
97	14.993	2279	2281	2283	rVB	564	331	0.03%	0.004%
98	15.883	2426	2427	2428	rBV	836	521	0.04%	0.006%
99	16.127	2465	2467	2469	rBV2	751	711	0.06%	0.008%
100	16.523	2530	2532	2534	rVB2	727	399	0.03%	0.004%




Sum of corrected areas: 9390569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030410.D
Acq On : 04 Aug 2022 22:31
Operator : JC/MD
Sample : N4021-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

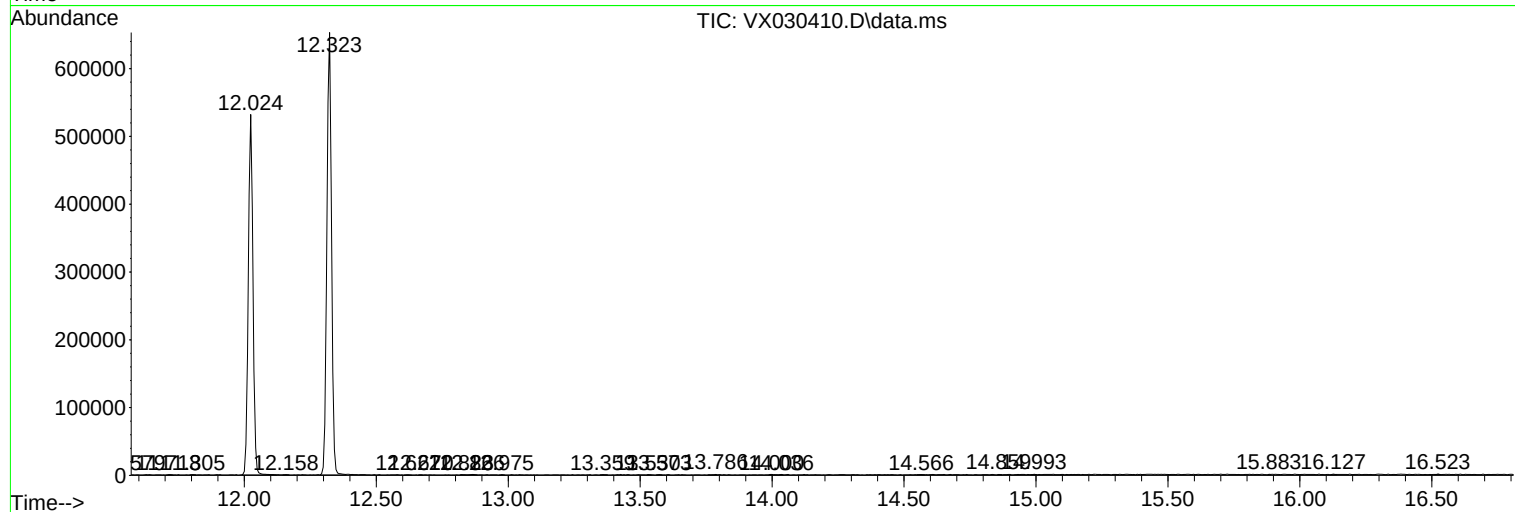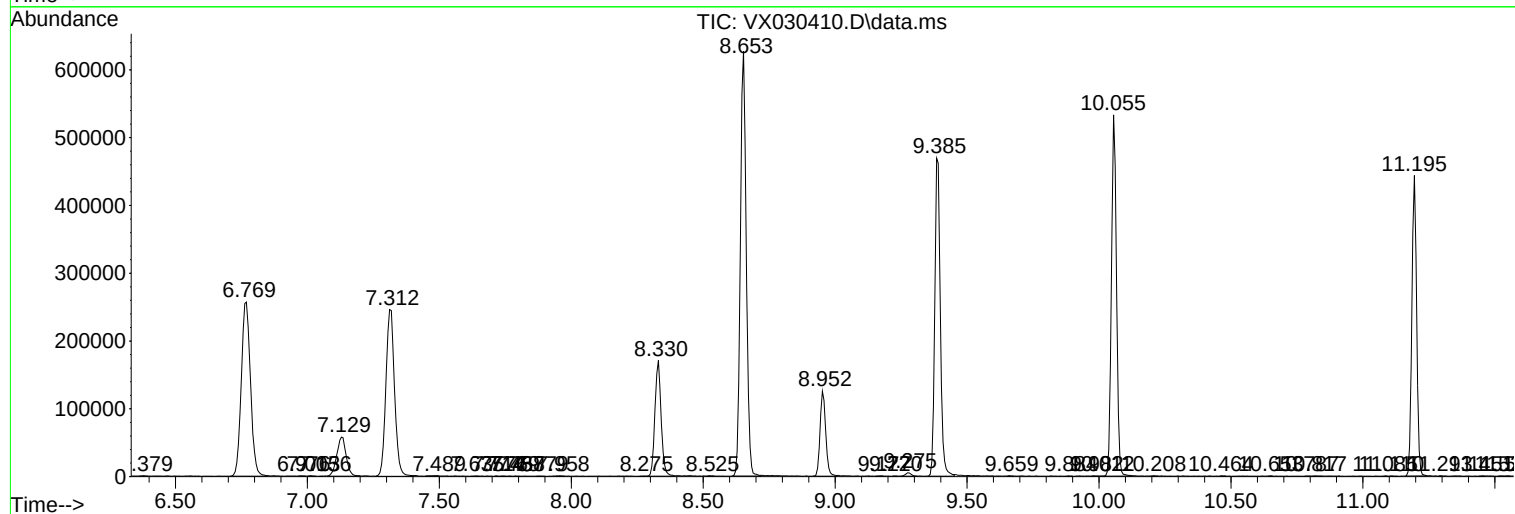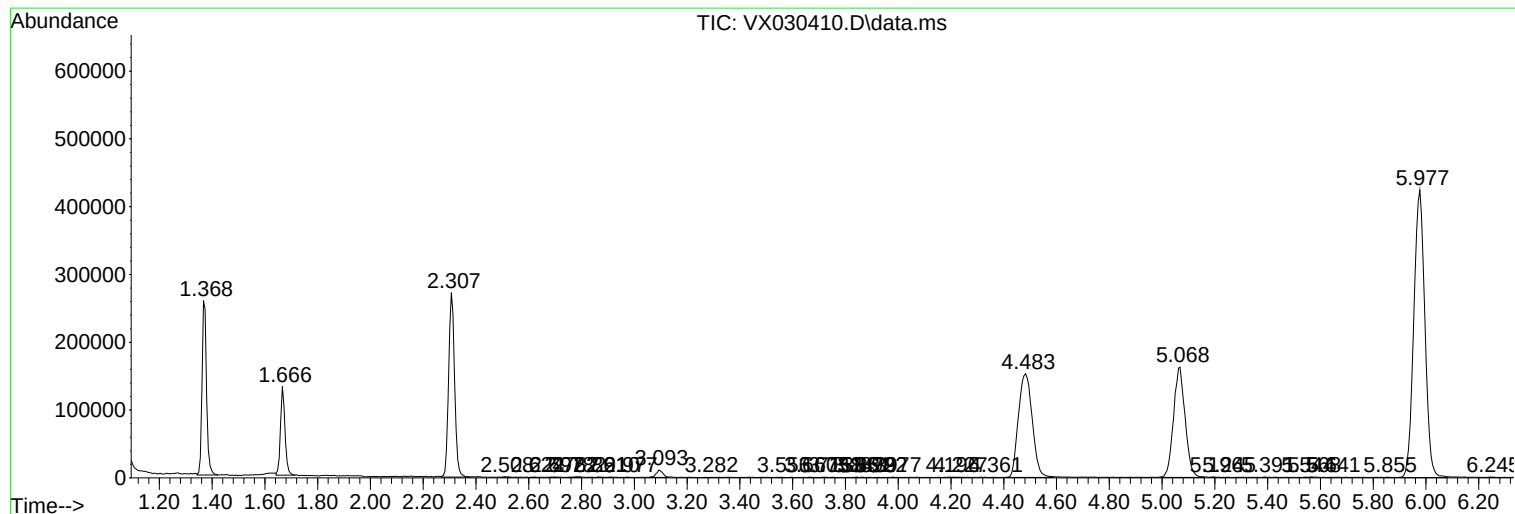

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030410.D
Acq On : 04 Aug 2022 22:31
Operator : JC/MD
Sample : N4021-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030410.D
Acq On : 04 Aug 2022 22:31
Operator : JC/MD
Sample : N4021-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc