

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030411.D
 Acq On : 04 Aug 2022 22:54
 Operator : JC/MD
 Sample : N4021-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	254942	295619	24.02%	3.093%
2	1.666	91	95	105	rVB	121201	149347	12.14%	1.562%
3	2.306	194	200	212	rVB	272654	415516	33.76%	4.347%
4	2.392	212	214	218	rVB5	1068	1238	0.10%	0.013%
5	2.514	232	234	242	rVB4	1180	1596	0.13%	0.017%
6	2.569	242	243	246	rBV	821	601	0.05%	0.006%
7	2.611	248	250	253	rVB	427	437	0.04%	0.005%
8	2.788	277	279	282	rVB3	722	851	0.07%	0.009%
9	2.995	311	313	316	rVB3	464	425	0.03%	0.004%
10	3.093	324	329	339	rVV2	9322	18575	1.51%	0.194%
11	3.251	353	355	358	rVB3	421	411	0.03%	0.004%
12	3.318	364	366	367	rBV2	432	394	0.03%	0.004%
13	3.428	377	384	385	rBV2	500	819	0.07%	0.009%
14	3.446	385	387	392	rVV2	395	665	0.05%	0.007%
15	3.513	396	398	401	rVV2	443	526	0.04%	0.006%
16	3.599	410	412	414	rVV2	477	467	0.04%	0.005%
17	3.635	416	418	420	rVV	325	315	0.03%	0.003%
18	3.709	429	430	432	rVV	468	355	0.03%	0.004%
19	3.818	445	448	451	rVB2	311	366	0.03%	0.004%
20	3.849	451	453	457	rBV2	474	699	0.06%	0.007%
21	3.928	462	466	468	rVB	454	374	0.03%	0.004%
22	3.952	468	470	472	rVB2	386	392	0.03%	0.004%
23	3.995	472	477	478	rBV	312	475	0.04%	0.005%
24	4.099	491	494	497	rBV2	410	501	0.04%	0.005%
25	4.477	545	556	576	rBV3	147242	537267	43.66%	5.621%
26	5.062	640	652	672	rVV	165649	498990	40.55%	5.220%
27	5.385	704	705	708	rBV	561	508	0.04%	0.005%
28	5.556	728	733	734	rBV3	1115	1531	0.12%	0.016%
29	5.781	768	770	773	rBV2	378	399	0.03%	0.004%
30	5.812	773	775	776	rBV	596	348	0.03%	0.004%
31	5.976	789	802	820	rBV2	421020	1230698	100.00%	12.876%
32	6.208	838	840	843	rVB2	453	442	0.04%	0.005%
33	6.312	852	857	859	rBV2	578	884	0.07%	0.009%
34	6.354	862	864	865	rVV	558	478	0.04%	0.005%
35	6.385	868	869	872	rVV2	489	441	0.04%	0.005%
36	6.550	894	896	901	rVB3	550	612	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030411.D
 Acq On : 04 Aug 2022 22:54
 Operator : JC/MD
 Sample : N4021-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	920	932	948	rBV	287145	671926	54.60%	7.030%
38	7.129	982	991	1003	rVB5	55429	131314	10.67%	1.374%
39	7.312	1012	1021	1034	rBV	256658	559517	45.46%	5.854%
40	7.470	1044	1047	1048	rBV2	533	482	0.04%	0.005%
41	7.598	1067	1068	1070	rVB	528	372	0.03%	0.004%
42	7.629	1070	1073	1075	rBV	446	456	0.04%	0.005%
43	7.690	1081	1083	1085	rBV	437	478	0.04%	0.005%
44	8.177	1160	1163	1166	rVB2	496	525	0.04%	0.005%
45	8.244	1171	1174	1176	rBV2	413	525	0.04%	0.005%
46	8.330	1180	1188	1199	rBV	167961	280063	22.76%	2.930%
47	8.488	1210	1214	1217	rBV3	481	609	0.05%	0.006%
48	8.574	1225	1228	1230	rBV2	589	602	0.05%	0.006%
49	8.653	1234	1241	1251	rBV	625769	971651	78.95%	10.165%
50	8.952	1284	1290	1302	rBV	121873	181056	14.71%	1.894%
51	9.281	1340	1344	1349	rVB4	3928	5988	0.49%	0.063%
52	9.384	1356	1361	1375	rBV	473725	692613	56.28%	7.246%
53	9.598	1394	1396	1398	rBV2	295	324	0.03%	0.003%
54	9.622	1398	1400	1402	rVV	452	383	0.03%	0.004%
55	9.817	1431	1432	1435	rVB2	498	410	0.03%	0.004%
56	9.878	1440	1442	1445	rVB	523	445	0.04%	0.005%
57	9.939	1448	1452	1454	rBV2	505	731	0.06%	0.008%
58	9.976	1456	1458	1460	rVB	486	327	0.03%	0.003%
59	10.055	1465	1471	1482	rBV	576683	769957	62.56%	8.055%
60	10.250	1499	1503	1504	rBV	596	696	0.06%	0.007%
61	10.652	1567	1569	1571	rBV3	563	470	0.04%	0.005%
62	10.695	1574	1576	1577	rVB	491	320	0.03%	0.003%
63	10.720	1577	1580	1581	rVB2	494	486	0.04%	0.005%
64	10.744	1581	1584	1587	rBV2	329	456	0.04%	0.005%
65	10.774	1587	1589	1594	rBV2	348	431	0.04%	0.005%
66	11.000	1624	1626	1627	rBV2	454	406	0.03%	0.004%
67	11.195	1652	1658	1665	rBV	442260	564816	45.89%	5.909%
68	11.384	1687	1689	1690	rBV	428	357	0.03%	0.004%
69	11.482	1702	1705	1706	rBV2	387	501	0.04%	0.005%
70	11.573	1717	1720	1723	rVB	402	420	0.03%	0.004%
71	11.640	1729	1731	1733	rVB	651	486	0.04%	0.005%
72	11.689	1738	1739	1742	rBV2	421	344	0.03%	0.004%
73	11.841	1762	1764	1766	rVB2	366	310	0.03%	0.003%
74	12.024	1788	1794	1802	rBV	576203	700608	56.93%	7.330%
75	12.231	1825	1828	1830	rVV2	522	481	0.04%	0.005%
76	12.323	1837	1843	1850	rBV	680368	839687	68.23%	8.785%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030411.D
 Acq On : 04 Aug 2022 22:54
 Operator : JC/MD
 Sample : N4021-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.439	1861	1862	1864	rBV	407	314	0.03%	0.003%
78	12.481	1868	1869	1871	rBV	371	369	0.03%	0.004%
79	12.561	1880	1882	1885	rBV2	316	310	0.03%	0.003%
80	12.603	1887	1889	1891	rVB	536	474	0.04%	0.005%
81	12.646	1895	1896	1899	rBV	468	395	0.03%	0.004%
82	12.683	1899	1902	1904	rBV	431	388	0.03%	0.004%
83	13.085	1967	1968	1972	rVB	617	650	0.05%	0.007%
84	13.408	2019	2021	2023	rBV2	424	369	0.03%	0.004%
85	13.591	2049	2051	2055	rBV2	342	357	0.03%	0.004%
86	13.640	2057	2059	2064	rVB3	545	746	0.06%	0.008%
87	14.207	2150	2152	2153	rBV	678	355	0.03%	0.004%
88	14.237	2153	2157	2161	rVV3	556	691	0.06%	0.007%
89	14.323	2169	2171	2173	rVB	767	569	0.05%	0.006%
90	14.347	2173	2175	2176	rBV2	368	348	0.03%	0.004%
91	14.414	2184	2186	2191	rBV2	579	820	0.07%	0.009%
92	14.457	2191	2193	2195	rBV2	471	462	0.04%	0.005%
93	14.749	2240	2241	2244	rBV2	696	630	0.05%	0.007%
94	15.024	2284	2286	2289	rVB2	754	597	0.05%	0.006%
95	15.871	2424	2425	2428	rVB3	922	612	0.05%	0.006%
96	15.908	2428	2431	2432	rBV2	744	629	0.05%	0.007%
97	16.042	2451	2453	2455	rBV3	642	619	0.05%	0.006%
98	16.438	2517	2518	2521	rVB2	677	371	0.03%	0.004%
99	16.664	2553	2555	2556	rBV2	878	746	0.06%	0.008%
100	16.718	2562	2564	2567	rBV2	932	935	0.08%	0.010%




Sum of corrected areas: 9558347

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030411.D
Acq On : 04 Aug 2022 22:54
Operator : JC/MD
Sample : N4021-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

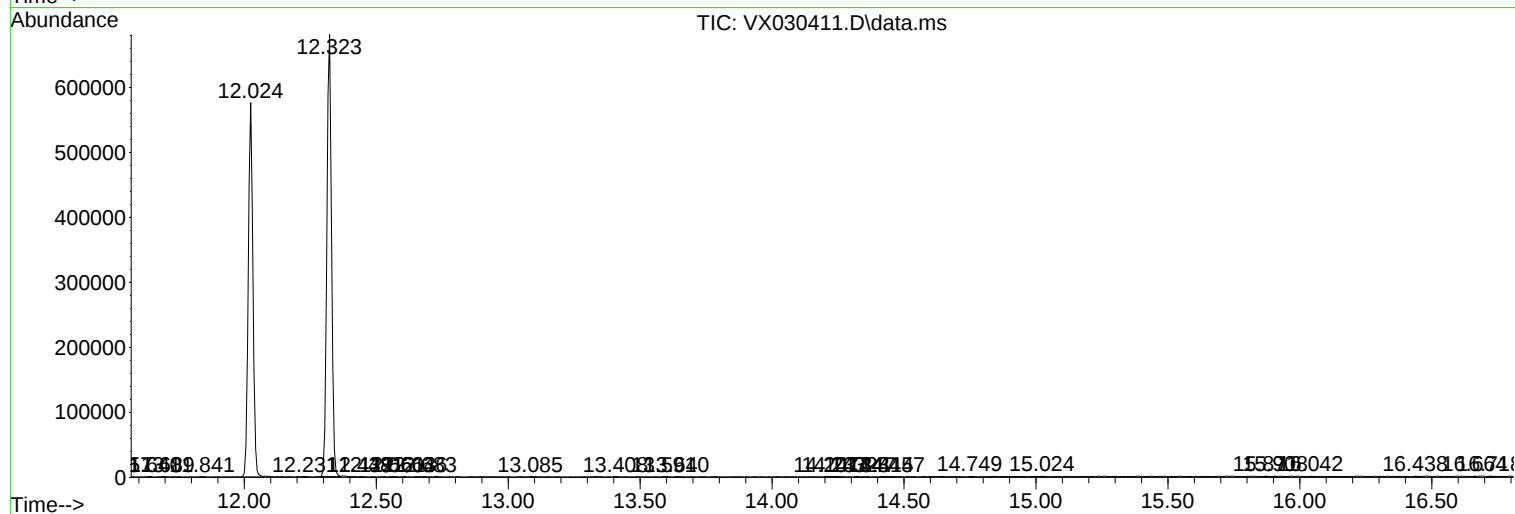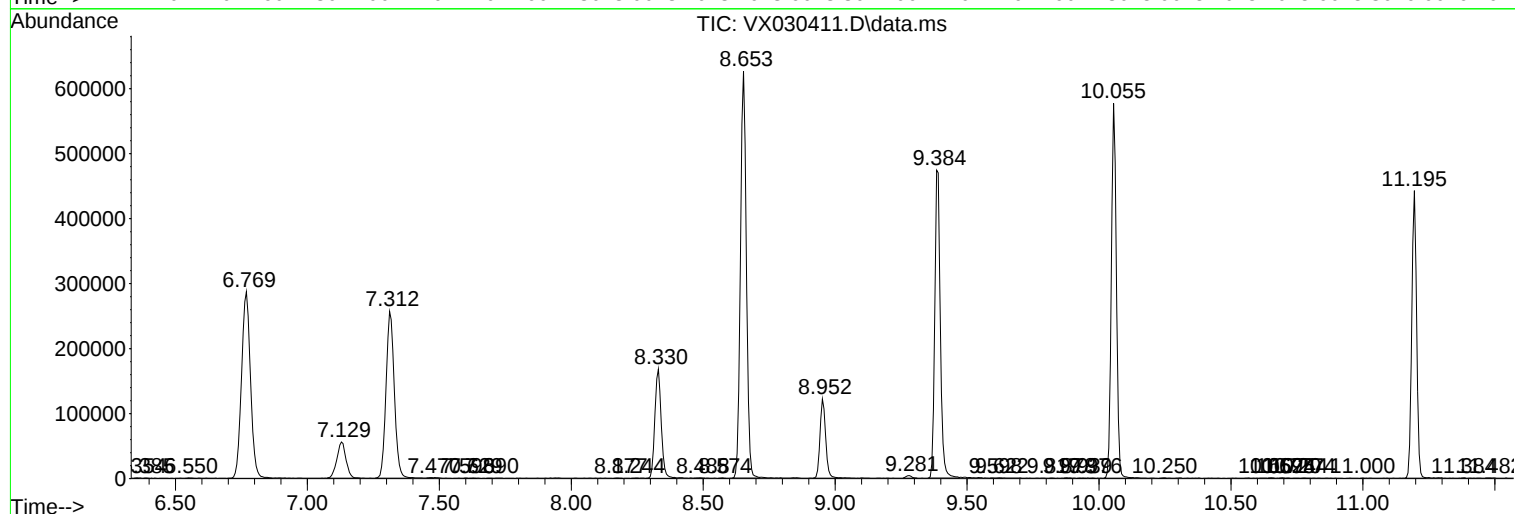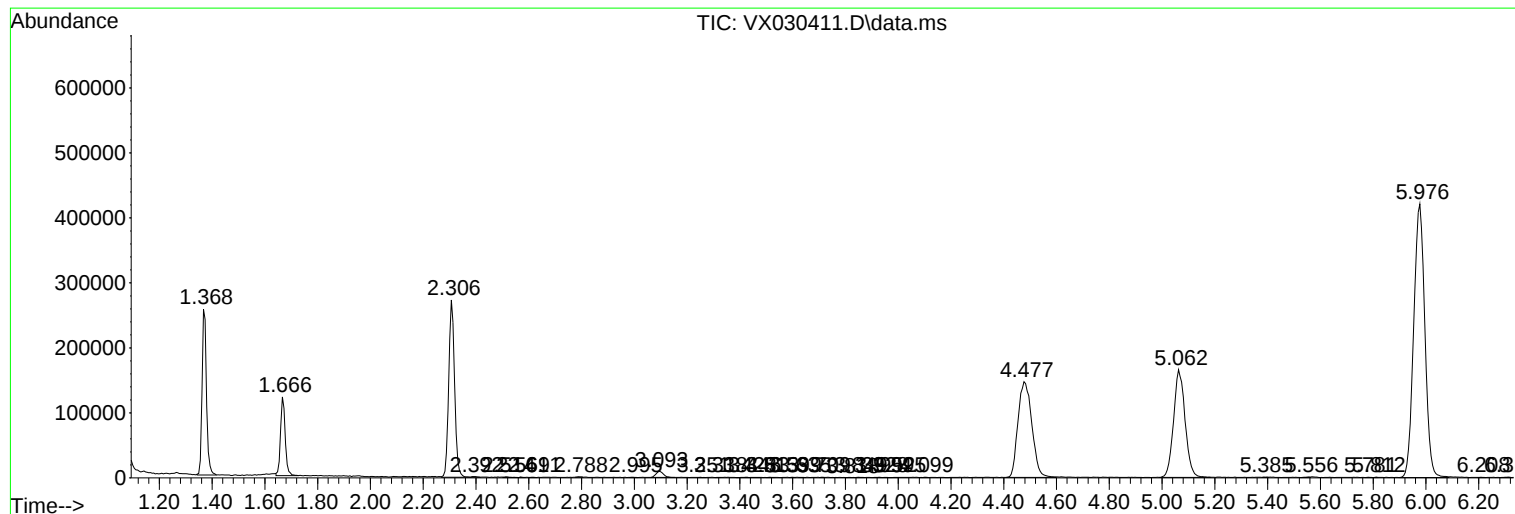

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030411.D
Acq On : 04 Aug 2022 22:54
Operator : JC/MD
Sample : N4021-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030411.D
Acq On : 04 Aug 2022 22:54
Operator : JC/MD
Sample : N4021-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc