

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030412.D
 Acq On : 04 Aug 2022 23:17
 Operator : JC/MD
 Sample : N4021-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	41	46	53	rVB	161531	173425	14.05%	1.891%
2	1.666	91	95	102	rVB	129127	149212	12.09%	1.627%
3	2.069	160	161	164	rBV3	771	648	0.05%	0.007%
4	2.307	194	200	211	rVB	245173	393242	31.85%	4.287%
5	2.520	230	235	238	rVB3	697	1148	0.09%	0.013%
6	2.624	249	252	253	rBV2	461	368	0.03%	0.004%
7	2.666	257	259	261	rVV	531	435	0.04%	0.005%
8	2.788	276	279	281	rVV3	913	1216	0.10%	0.013%
9	2.977	308	310	311	rBV2	795	710	0.06%	0.008%
10	3.093	322	329	339	rVV	70096	137729	11.16%	1.501%
11	3.203	344	347	350	rVB2	432	599	0.05%	0.007%
12	3.501	395	396	399	rBV2	353	320	0.03%	0.003%
13	3.788	442	443	446	rBV	412	421	0.03%	0.005%
14	3.867	454	456	458	rVB3	523	371	0.03%	0.004%
15	3.898	458	461	462	rBV2	415	381	0.03%	0.004%
16	4.300	525	527	530	rVV2	430	457	0.04%	0.005%
17	4.465	545	554	570	rBV	105053	314845	25.50%	3.432%
18	4.666	584	587	588	rBV2	622	608	0.05%	0.007%
19	4.763	601	603	606	rVB	462	455	0.04%	0.005%
20	4.867	617	620	622	rVB	454	419	0.03%	0.005%
21	4.904	622	626	628	rVV2	272	438	0.04%	0.005%
22	5.062	640	652	670	rVV	165106	505115	40.92%	5.507%
23	5.184	670	672	675	rVB2	601	430	0.03%	0.005%
24	5.282	686	688	691	rBV	442	450	0.04%	0.005%
25	5.324	694	695	698	rBV	421	358	0.03%	0.004%
26	5.464	716	718	720	rVB	407	364	0.03%	0.004%
27	5.495	720	723	727	rBV3	495	922	0.07%	0.010%
28	5.556	731	733	735	rBV3	618	449	0.04%	0.005%
29	5.574	735	736	738	rVB2	644	407	0.03%	0.004%
30	5.678	751	753	756	rBV2	308	410	0.03%	0.004%
31	5.751	762	765	766	rBV	356	356	0.03%	0.004%
32	5.977	788	802	815	rBV2	418348	1234524	100.00%	13.458%
33	6.348	860	863	864	rBV	722	708	0.06%	0.008%
34	6.391	864	870	871	rBV5	1590	2292	0.19%	0.025%
35	6.452	878	880	885	rVB2	614	739	0.06%	0.008%
36	6.531	891	893	895	rBV2	455	598	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030412.D
 Acq On : 04 Aug 2022 23:17
 Operator : JC/MD
 Sample : N4021-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.617	905	907	910	rVB	364	417	0.03%	0.005%
38	6.769	922	932	942	rBV	275865	657766	53.28%	7.171%
39	7.001	967	970	973	rBV2	896	921	0.07%	0.010%
40	7.117	981	989	997	rBV5	11426	28336	2.30%	0.309%
41	7.214	1003	1005	1008	rVB2	359	322	0.03%	0.004%
42	7.312	1010	1021	1035	rBV	256441	570154	46.18%	6.216%
43	7.482	1044	1049	1054	rBV5	970	2153	0.17%	0.023%
44	7.598	1065	1068	1072	rBV3	393	660	0.05%	0.007%
45	7.635	1072	1074	1077	rVV2	428	395	0.03%	0.004%
46	7.708	1083	1086	1088	rBV2	364	394	0.03%	0.004%
47	7.775	1095	1097	1100	rVB2	717	485	0.04%	0.005%
48	7.799	1100	1101	1104	rVB	475	404	0.03%	0.004%
49	7.836	1104	1107	1110	rBV2	234	428	0.03%	0.005%
50	7.891	1114	1116	1118	rVV	457	341	0.03%	0.004%
51	7.915	1118	1120	1121	rVV2	452	318	0.03%	0.003%
52	7.946	1121	1125	1126	rVB2	437	437	0.04%	0.005%
53	8.330	1181	1188	1197	rVV	164843	275594	22.32%	3.004%
54	8.494	1213	1215	1218	rVB2	746	647	0.05%	0.007%
55	8.592	1228	1231	1233	rVB2	535	496	0.04%	0.005%
56	8.653	1233	1241	1251	rBV	623311	973732	78.88%	10.615%
57	8.952	1285	1290	1299	rBV	125038	179743	14.56%	1.959%
58	9.275	1342	1343	1346	rVB	1054	684	0.06%	0.007%
59	9.385	1356	1361	1378	rVB	461544	684776	55.47%	7.465%
60	9.671	1406	1408	1410	rVB2	477	388	0.03%	0.004%
61	9.970	1455	1457	1459	rVB2	544	351	0.03%	0.004%
62	10.055	1465	1471	1486	rBV	584789	768112	62.22%	8.374%
63	10.238	1499	1501	1503	rBV2	418	415	0.03%	0.005%
64	10.305	1508	1512	1517	rVV3	899	1562	0.13%	0.017%
65	10.653	1564	1569	1572	rBV3	834	1290	0.10%	0.014%
66	10.695	1575	1576	1579	rBV2	313	342	0.03%	0.004%
67	10.720	1579	1580	1582	rVB2	521	328	0.03%	0.004%
68	10.744	1582	1584	1585	rBV	503	316	0.03%	0.003%
69	10.787	1589	1591	1592	rBV2	426	318	0.03%	0.003%
70	10.805	1592	1594	1596	rBV	508	347	0.03%	0.004%
71	10.988	1622	1624	1625	rVV	427	358	0.03%	0.004%
72	11.031	1629	1631	1634	rVV2	409	428	0.03%	0.005%
73	11.092	1638	1641	1647	rVB4	864	1365	0.11%	0.015%
74	11.195	1652	1658	1668	rVB	447582	566877	45.92%	6.180%
75	11.348	1682	1683	1685	rBV2	661	503	0.04%	0.005%
76	11.390	1688	1690	1693	rVV2	479	388	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030412.D
 Acq On : 04 Aug 2022 23:17
 Operator : JC/MD
 Sample : N4021-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.482	1704	1705	1708	rVB2	519	432	0.03%	0.005%
78	11.591	1720	1723	1725	rVV3	396	470	0.04%	0.005%
79	11.671	1732	1736	1737	rBV2	569	559	0.05%	0.006%
80	11.713	1741	1743	1745	rVB	650	390	0.03%	0.004%
81	11.847	1763	1765	1767	rVB2	497	409	0.03%	0.004%
82	11.884	1767	1771	1775	rBV4	1145	1605	0.13%	0.017%
83	12.024	1788	1794	1803	rBV	580514	693335	56.16%	7.558%
84	12.323	1837	1843	1851	rBV	647541	818110	66.27%	8.919%
85	12.457	1863	1865	1871	rBV2	395	902	0.07%	0.010%
86	12.847	1927	1929	1932	rVB2	886	622	0.05%	0.007%
87	12.945	1940	1945	1948	rVV2	847	1191	0.10%	0.013%
88	13.085	1966	1968	1972	rVB2	440	499	0.04%	0.005%
89	13.122	1972	1974	1975	rBV	437	360	0.03%	0.004%
90	13.817	2087	2088	2092	rBV2	459	441	0.04%	0.005%
91	13.890	2098	2100	2103	rBV	311	333	0.03%	0.004%
92	13.963	2110	2112	2113	rBV	528	470	0.04%	0.005%
93	14.371	2177	2179	2182	rBV3	370	510	0.04%	0.006%
94	14.402	2182	2184	2185	rVV	711	374	0.03%	0.004%
95	14.420	2185	2187	2190	rVV3	598	743	0.06%	0.008%
96	14.451	2190	2192	2194	rVB	764	535	0.04%	0.006%
97	15.194	2313	2314	2317	rVB2	618	472	0.04%	0.005%
98	15.847	2419	2421	2422	rBV2	567	337	0.03%	0.004%
99	16.145	2468	2470	2473	rVB2	809	575	0.05%	0.006%
100	16.365	2504	2506	2508	rBV	597	463	0.04%	0.005%




Sum of corrected areas: 9172997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030412.D
Acq On : 04 Aug 2022 23:17
Operator : JC/MD
Sample : N4021-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

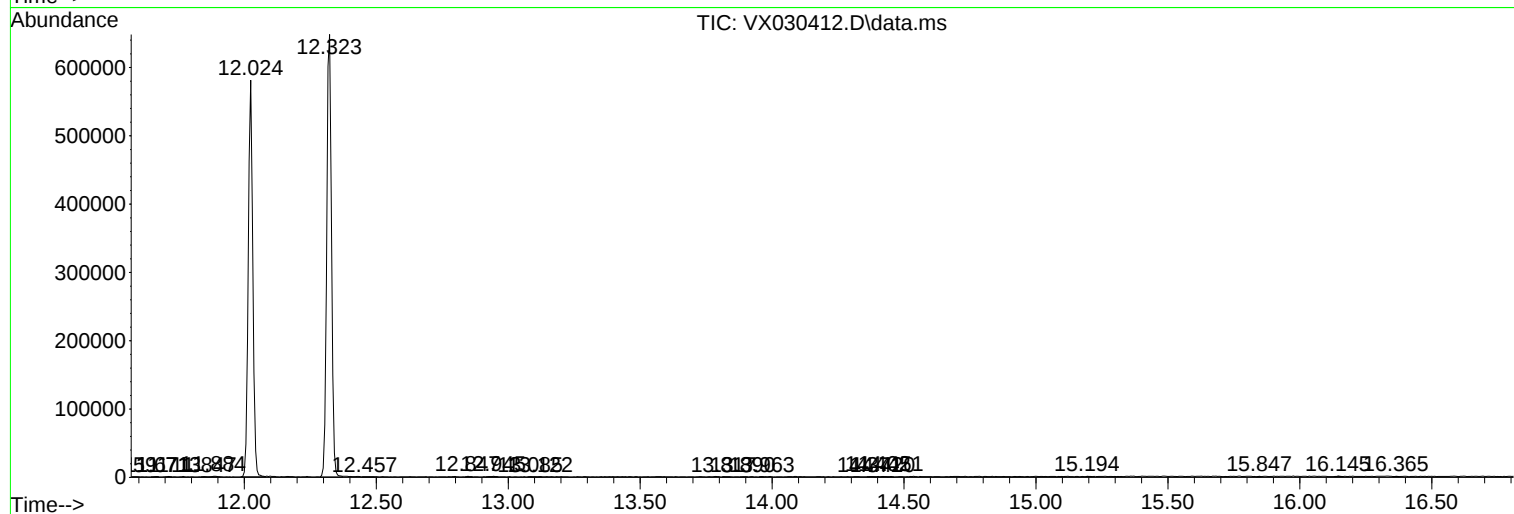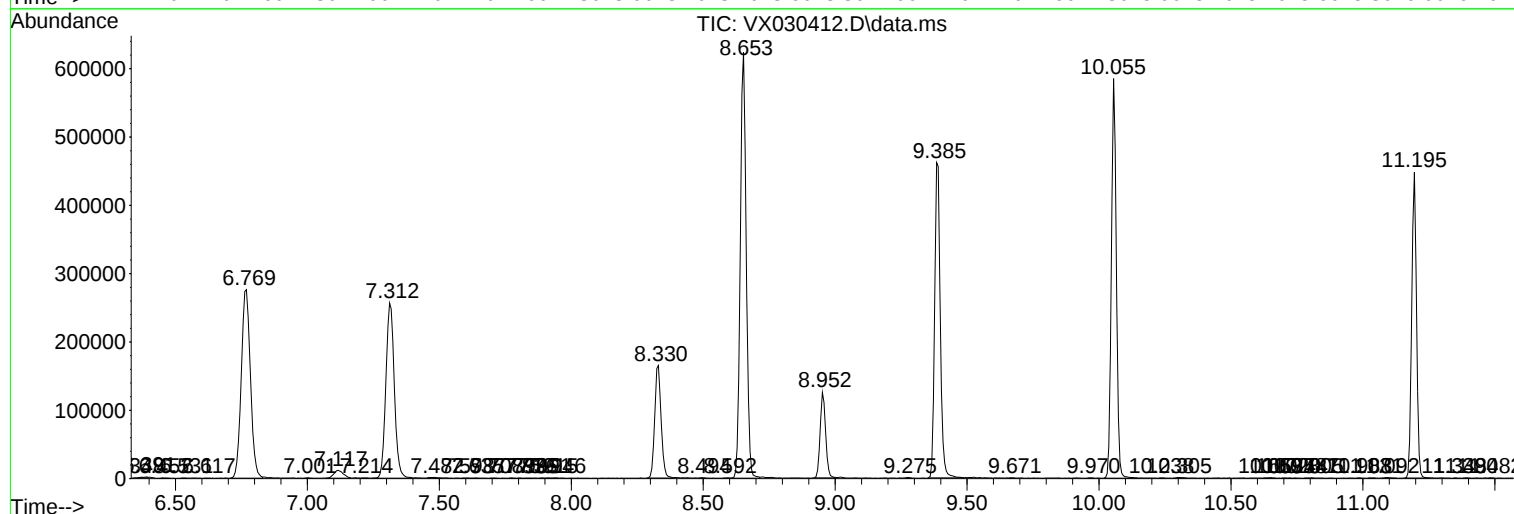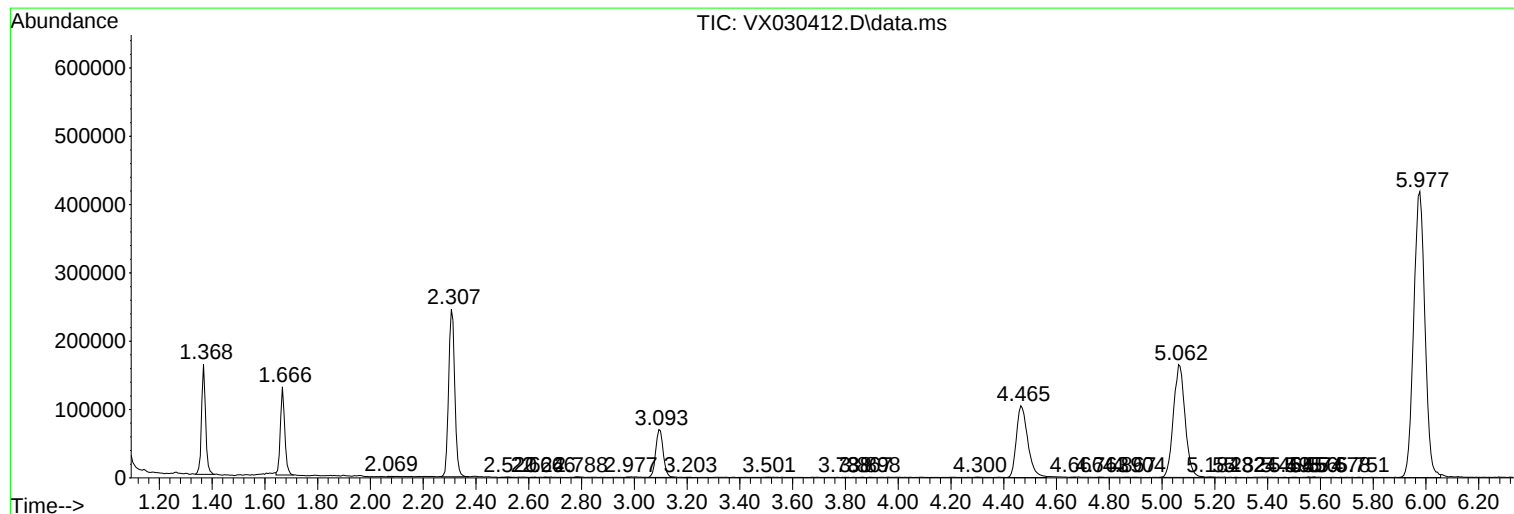

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030412.D
Acq On : 04 Aug 2022 23:17
Operator : JC/MD
Sample : N4021-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030412.D
Acq On : 04 Aug 2022 23:17
Operator : JC/MD
Sample : N4021-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc