

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030413.D
 Acq On : 04 Aug 2022 23:41
 Operator : JC/MD
 Sample : N4021-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	59	rVB2	639311	731452	9.67%	4.232%
2	1.666	91	95	105	rVB	126602	158514	2.10%	0.917%
3	2.306	193	200	212	rBV3	297098	523016	6.92%	3.026%
4	2.471	225	227	229	rVB	607	407	0.01%	0.002%
5	2.489	229	230	233	rBV	448	391	0.01%	0.002%
6	2.520	233	235	237	rVB	489	401	0.01%	0.002%
7	2.721	265	268	274	rBV	789	990	0.01%	0.006%
8	2.794	277	280	284	rVB3	1092	1612	0.02%	0.009%
9	2.837	284	287	289	rBV	423	482	0.01%	0.003%
10	2.916	298	300	303	rVB2	334	367	0.00%	0.002%
11	2.959	303	307	310	rBV2	222	353	0.00%	0.002%
12	3.093	322	329	340	rVB	116712	226870	3.00%	1.313%
13	3.343	366	370	373	rBV	522	739	0.01%	0.004%
14	3.386	373	377	378	rBV	474	511	0.01%	0.003%
15	3.428	382	384	386	rBV2	350	395	0.01%	0.002%
16	3.507	395	397	400	rBV2	317	404	0.01%	0.002%
17	3.544	400	403	406	rBV2	323	428	0.01%	0.002%
18	3.751	435	437	440	rVB2	448	540	0.01%	0.003%
19	3.910	457	463	467	rBV2	320	727	0.01%	0.004%
20	3.965	470	472	476	rVB	386	449	0.01%	0.003%
21	4.020	480	481	485	rBV2	457	391	0.01%	0.002%
22	4.294	523	526	529	rBV2	412	515	0.01%	0.003%
23	4.495	545	559	576	rBV	2756785	7561103	100.00%	43.750%
24	4.873	619	621	622	rBV	576	481	0.01%	0.003%
25	5.062	639	652	668	rBV	161464	507598	6.71%	2.937%
26	5.349	697	699	702	rBV2	360	462	0.01%	0.003%
27	5.385	702	705	706	rBV	503	485	0.01%	0.003%
28	5.403	706	708	710	rVB2	689	466	0.01%	0.003%
29	5.422	710	711	715	rVB2	598	474	0.01%	0.003%
30	5.477	719	720	725	rVB2	431	578	0.01%	0.003%
31	5.556	729	733	738	rVB3	739	1296	0.02%	0.007%
32	5.769	763	768	770	rVB2	306	461	0.01%	0.003%
33	5.836	776	779	782	rBV2	369	479	0.01%	0.003%
34	5.976	789	802	820	rBV2	419594	1239705	16.40%	7.173%
35	6.281	846	852	855	rVB2	259	530	0.01%	0.003%
36	6.342	857	862	864	rBV3	607	763	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030413.D
 Acq On : 04 Aug 2022 23:41
 Operator : JC/MD
 Sample : N4021-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.531	891	893	896	rBV3	407	466	0.01%	0.003%
38	6.769	922	932	950	rVV	254575	613667	8.12%	3.551%
39	6.958	961	963	967	rVB	520	508	0.01%	0.003%
40	7.049	976	978	981	rBV3	471	413	0.01%	0.002%
41	7.129	981	991	1002	rBV2	99817	227602	3.01%	1.317%
42	7.312	1011	1021	1034	rBV	256628	569278	7.53%	3.294%
43	7.458	1043	1045	1046	rBV2	660	580	0.01%	0.003%
44	7.476	1046	1048	1050	rVV2	663	571	0.01%	0.003%
45	7.562	1061	1062	1064	rBV	466	358	0.00%	0.002%
46	7.616	1066	1071	1072	rVV3	484	638	0.01%	0.004%
47	7.909	1117	1119	1120	rBV2	450	358	0.00%	0.002%
48	7.958	1123	1127	1128	rVB3	502	630	0.01%	0.004%
49	8.061	1139	1144	1146	rVV2	478	536	0.01%	0.003%
50	8.244	1169	1174	1175	rBV3	390	665	0.01%	0.004%
51	8.330	1181	1188	1196	rBV	166581	277096	3.66%	1.603%
52	8.500	1214	1216	1218	rVB2	412	356	0.00%	0.002%
53	8.653	1234	1241	1251	rBV	624922	981306	12.98%	5.678%
54	8.952	1285	1290	1304	rBV	125618	185324	2.45%	1.072%
55	9.275	1340	1343	1351	rBV4	3137	4298	0.06%	0.025%
56	9.384	1355	1361	1376	rBV	468637	690067	9.13%	3.993%
57	9.683	1408	1410	1413	rVB3	575	723	0.01%	0.004%
58	9.714	1413	1415	1418	rBV2	496	460	0.01%	0.003%
59	9.750	1420	1421	1424	rVV2	493	358	0.00%	0.002%
60	9.884	1441	1443	1447	rVB2	502	494	0.01%	0.003%
61	10.055	1465	1471	1483	rVV	538891	707800	9.36%	4.096%
62	10.299	1509	1511	1516	rVB2	579	702	0.01%	0.004%
63	10.482	1538	1541	1544	rVB3	577	693	0.01%	0.004%
64	10.555	1550	1553	1555	rBV	371	521	0.01%	0.003%
65	10.982	1621	1623	1625	rBV	320	355	0.00%	0.002%
66	11.037	1631	1632	1634	rBV	540	370	0.00%	0.002%
67	11.091	1636	1641	1642	rBV2	553	758	0.01%	0.004%
68	11.195	1652	1658	1665	rBV	443398	564219	7.46%	3.265%
69	11.476	1703	1704	1710	rVB2	698	749	0.01%	0.004%
70	11.573	1718	1720	1721	rBV	355	359	0.00%	0.002%
71	11.610	1725	1726	1732	rVB2	442	628	0.01%	0.004%
72	11.677	1732	1737	1740	rBV2	541	952	0.01%	0.006%
73	11.841	1762	1764	1765	rBV	550	371	0.00%	0.002%
74	11.878	1768	1770	1773	rVB	438	519	0.01%	0.003%
75	11.982	1784	1787	1788	rBV2	391	357	0.00%	0.002%
76	12.024	1788	1794	1804	rBV	541013	644253	8.52%	3.728%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030413.D
 Acq On : 04 Aug 2022 23:41
 Operator : JC/MD
 Sample : N4021-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.219	1824	1826	1828	rBV3	455	381	0.01%	0.002%
78	12.244	1828	1830	1832	rBV	772	612	0.01%	0.004%
79	12.323	1837	1843	1853	rBV	664776	824720	10.91%	4.772%
80	12.445	1862	1863	1867	rBV3	411	415	0.01%	0.002%
81	12.506	1870	1873	1875	rBV2	328	367	0.00%	0.002%
82	12.616	1890	1891	1893	rBV	459	367	0.00%	0.002%
83	12.780	1914	1918	1920	rBV2	533	489	0.01%	0.003%
84	12.902	1935	1938	1942	rVB2	450	558	0.01%	0.003%
85	13.018	1952	1957	1958	rBV2	459	717	0.01%	0.004%
86	13.054	1961	1963	1967	rVB2	538	404	0.01%	0.002%
87	13.176	1982	1983	1986	rBV	745	602	0.01%	0.003%
88	13.481	2031	2033	2035	rVB	575	390	0.01%	0.002%
89	13.585	2049	2050	2054	rBV2	482	351	0.00%	0.002%
90	13.689	2065	2067	2070	rBV2	366	457	0.01%	0.003%
91	13.749	2074	2077	2080	rVV	362	524	0.01%	0.003%
92	13.792	2080	2084	2086	rVB3	832	1024	0.01%	0.006%
93	14.219	2151	2154	2155	rBV2	380	370	0.00%	0.002%
94	14.249	2158	2159	2162	rVV2	505	576	0.01%	0.003%
95	14.755	2240	2242	2243	rVB	629	361	0.00%	0.002%
96	14.847	2255	2257	2259	rBV2	560	378	0.00%	0.002%
97	15.310	2332	2333	2334	rBV	874	409	0.01%	0.002%
98	15.847	2417	2421	2424	rBV4	607	1209	0.02%	0.007%
99	16.316	2496	2498	2499	rBV	813	780	0.01%	0.005%
100	16.767	2570	2572	2575	rVB	1234	681	0.01%	0.004%




Sum of corrected areas: 17282335

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030413.D
Acq On : 04 Aug 2022 23:41
Operator : JC/MD
Sample : N4021-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

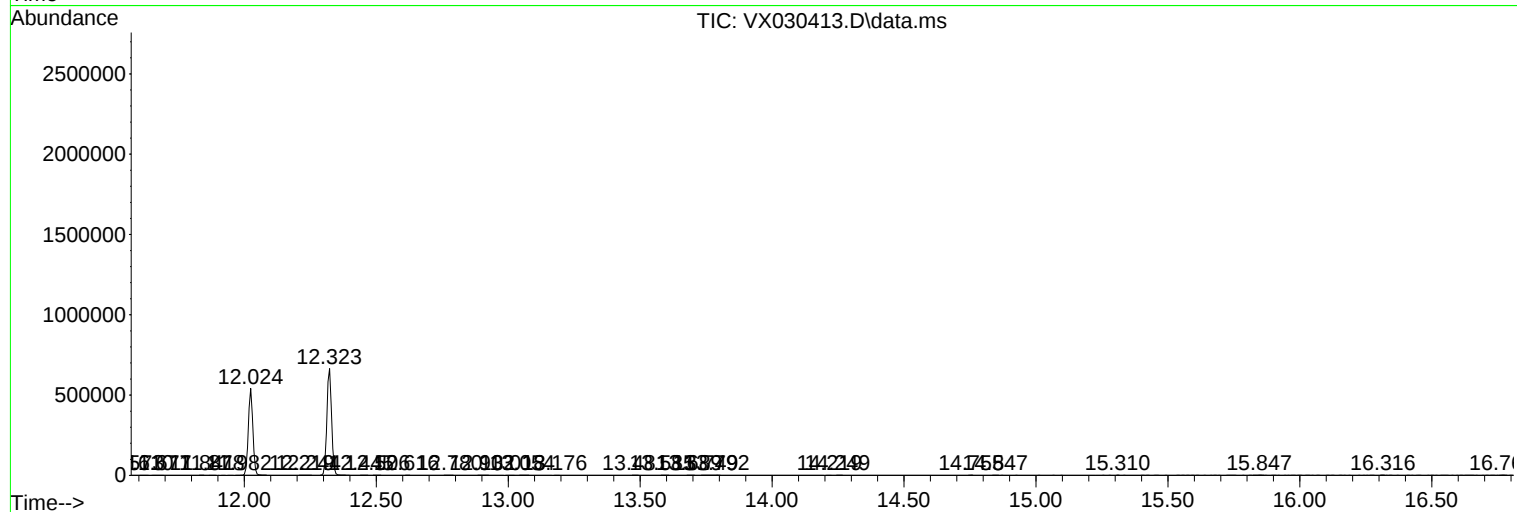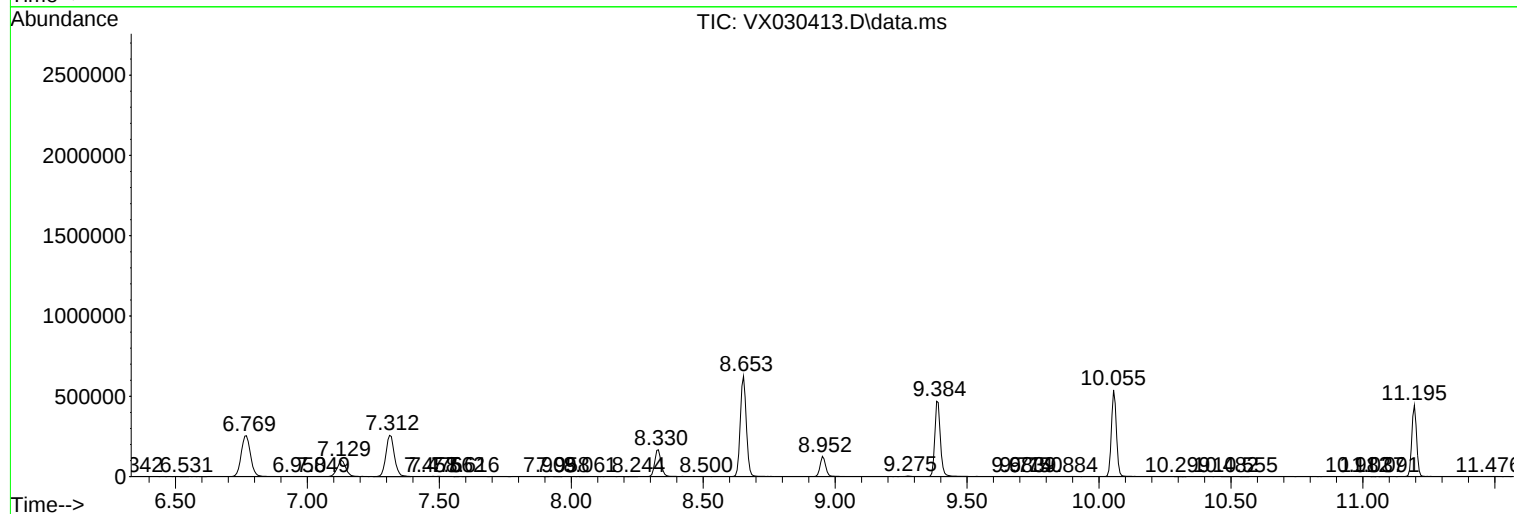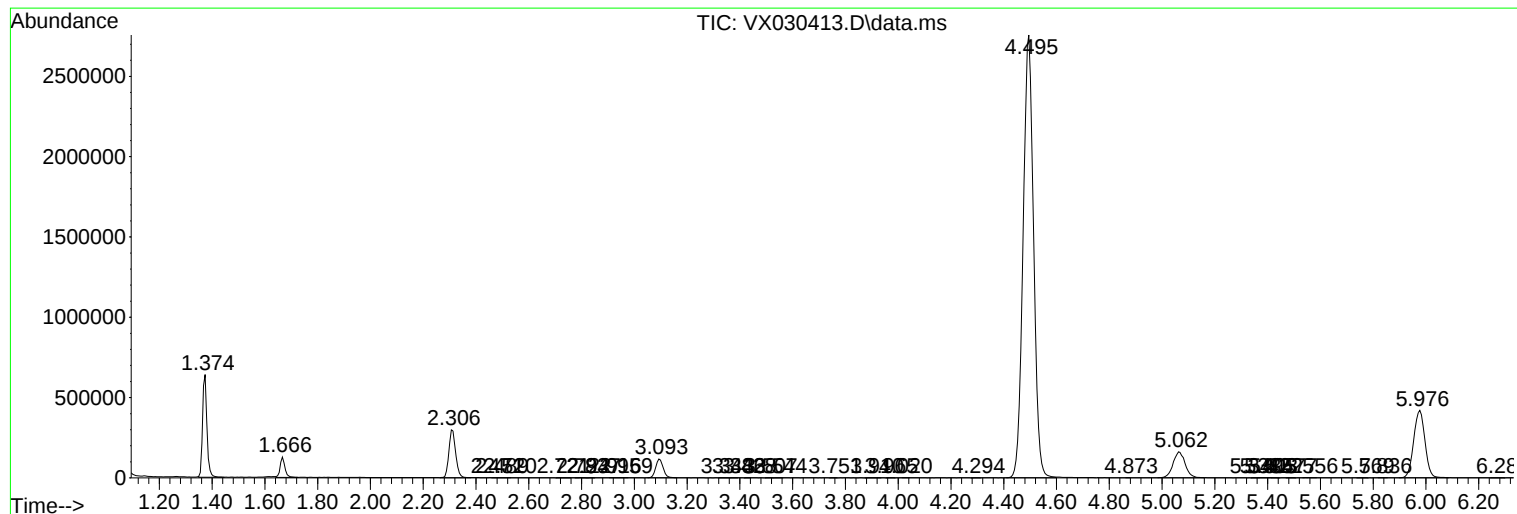

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030413.D
Acq On : 04 Aug 2022 23:41
Operator : JC/MD
Sample : N4021-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
Data File : VX030413.D
Acq On : 04 Aug 2022 23:41
Operator : JC/MD
Sample : N4021-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc