
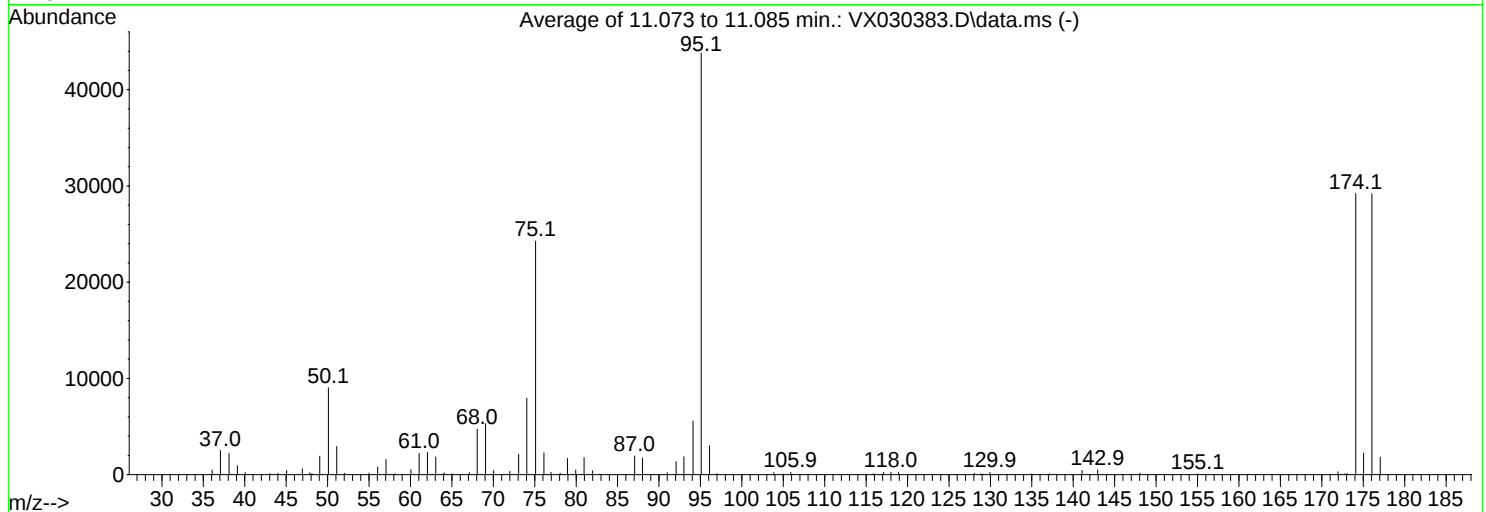


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080422\
 Data File : VX030383.D
 Acq On : 04 Aug 2022 09:12
 Operator : JC/MD
 Sample : BFB670
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB670

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Fri Aug 05 05:25:14 2022

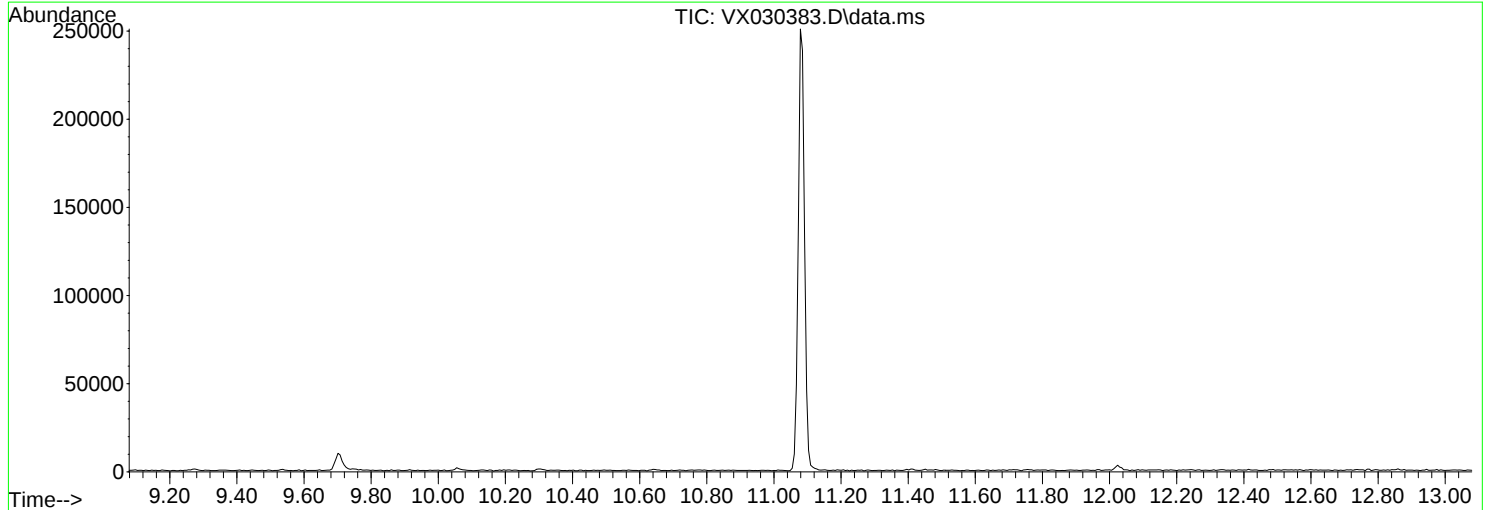

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	9025	PASS
75	95	30	80	55.4	24283	PASS
95	95	100	100	100.0	43829	PASS
96	95	5	9	6.8	3002	PASS
173	174	0.00	2	0.4	114	PASS
174	95	50	120	66.7	29213	PASS
175	174	5	9	7.7	2236	PASS
176	174	95	101	99.9	29195	PASS
177	176	5	9	6.2	1810	PASS

m/z	Abundance
40.10	218.0
44.00	450.0

Instrument :
MSVOA_X
ClientSampleId :
BFB670

m/z	Abundance
36.10	382.0
37.00	1989.0
38.10	1594.0
39.10	654.0
40.10	455.0
43.00	130.0
44.10	614.0
45.00	326.0
46.90	593.0
47.80	212.0
49.10	1631.0
50.10	7075.0
51.10	2317.0
52.00	94.0
55.10	122.0
56.00	771.0
57.00	1258.0
58.10	50.0
60.00	363.0
61.00	1909.0
62.10	1844.0
63.10	1176.0
63.90	189.0
65.00	96.0
67.20	70.0
68.10	3802.0
69.10	3615.0
70.00	333.0
72.00	296.0
73.10	1858.0
74.10	5993.0
75.10	18376.0
76.10	1564.0
76.90	119.0
77.90	120.0
78.90	1052.0
79.90	416.0
80.90	1370.0
82.10	191.0
87.00	1260.0
88.00	1316.0
89.50	56.0
91.10	225.0
92.10	1060.0
93.00	1220.0
94.10	3511.0
95.10	30424.0
96.10	2322.0
103.90	135.0
105.00	57.0
105.90	213.0
115.80	145.0
116.90	144.0
118.00	171.0
119.00	136.0
128.00	93.0
128.80	89.0
130.00	154.0
131.00	63.0
134.90	50.0
141.20	308.0
143.00	331.0
145.00	94.0
145.90	65.0
148.10	109.0
171.90	142.0
173.00	122.0
174.10	16592.0
175.00	1306.0
176.00	15968.0
177.00	1147.0

Instrument :
MSVOA_X
ClientSampleId :
BFB670

m/z	Abundance
35.90	602.0
37.10	3188.0
38.10	2900.0
39.10	1141.0
40.00	436.0
43.00	74.0
44.00	507.0
45.10	434.0
47.00	669.0
47.90	389.0
49.00	2353.0
50.10	11100.0
51.10	3559.0
52.10	165.0
55.10	118.0
56.10	968.0
57.10	1698.0
58.10	112.0
60.00	624.0
61.10	2365.0
62.10	2699.0
63.00	2325.0
64.10	287.0
65.00	191.0
67.10	316.0
68.10	5606.0
69.10	6393.0
70.00	595.0
71.10	64.0
72.00	525.0
73.00	2350.0
74.10	9518.0
75.10	28832.0
76.10	2809.0
76.90	264.0
78.10	179.0
79.00	1987.0
80.00	335.0
81.00	2006.0
81.90	500.0
82.70	59.0
87.10	2321.0
88.00	1925.0
91.00	220.0
92.10	1682.0
93.00	2283.0
94.10	7125.0
95.10	51728.0
96.10	3571.0
97.00	147.0
103.80	309.0
105.90	254.0
107.10	62.0
116.00	194.0
117.10	305.0
117.90	318.0
118.80	289.0
123.90	59.0
128.00	171.0
129.10	157.0
129.90	344.0
135.00	171.0
137.10	141.0
140.00	61.0
141.00	635.0
142.00	110.0
143.00	521.0
145.00	53.0
145.80	91.0
148.10	176.0
149.10	62.0
155.20	83.0
161.10	89.0
172.00	434.0
173.10	220.0
174.10	34600.0
175.10	2706.0
176.10	34088.0
177.10	2136.0
178.10	70.0

Instrument :
MSVOA_X
ClientSampleId :
BFB670

m/z	Abundance
36.10	441.0
37.10	2338.0
38.10	2179.0
39.10	991.0
40.00	414.0
43.10	142.0
44.10	623.0
45.00	554.0
47.00	539.0
48.10	355.0
49.00	1775.0
50.10	8899.0
51.10	2912.0
52.10	132.0
54.90	268.0
56.10	705.0
57.00	1762.0
58.20	115.0
60.10	563.0
61.00	2377.0
62.00	2372.0
63.00	2049.0
64.00	240.0
65.20	102.0
67.10	194.0
68.00	4809.0
69.00	5901.0
70.10	325.0
71.20	62.0
72.00	193.0
73.10	2168.0
74.00	8354.0
75.10	25640.0
76.10	2397.0
77.00	348.0
78.00	291.0
78.90	2004.0
80.00	698.0
81.00	1977.0
82.00	517.0
82.80	110.0
86.00	99.0
87.00	2215.0
88.00	1930.0
90.90	198.0
92.00	1339.0
93.00	2079.0
94.10	6071.0
95.10	49336.0
96.10	3113.0
97.00	152.0
103.80	225.0
105.00	139.0
105.90	234.0
112.80	56.0
115.10	154.0
115.90	122.0
117.10	407.0
118.10	227.0
119.00	220.0
124.00	69.0
128.10	250.0
128.90	139.0
129.90	208.0
135.00	77.0
137.20	98.0
141.00	418.0
142.90	622.0
148.00	180.0
155.00	189.0
159.20	59.0
171.80	324.0
172.80	292.0
174.10	36448.0
175.10	2695.0
176.10	37528.0
177.10	2148.0

Instrument :
MSVOA_X
ClientSampleId :
BFB670