

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080519\
 Data File : VX011321.D
 Acq On : 05 Aug 2019 11:03
 Operator : JC/SP
 Sample : VX0805WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0805WBL01

Quant Time: Aug 06 03:16:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	137308	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	216963	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	200599	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	90489	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	73826	53.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.78%	
35) Dibromofluoromethane	5.49	113	71638	50.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.14%	
50) Toluene-d8	8.71	98	264201	49.41	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.82%	
62) 4-Bromofluorobenzene	11.13	95	87498	45.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.66%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080519\
Data File : VX011321.D
Acq On : 05 Aug 2019 11:03
Operator : JC/SP
Sample : VX0805WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL01

Quant Time: Aug 06 03:16:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

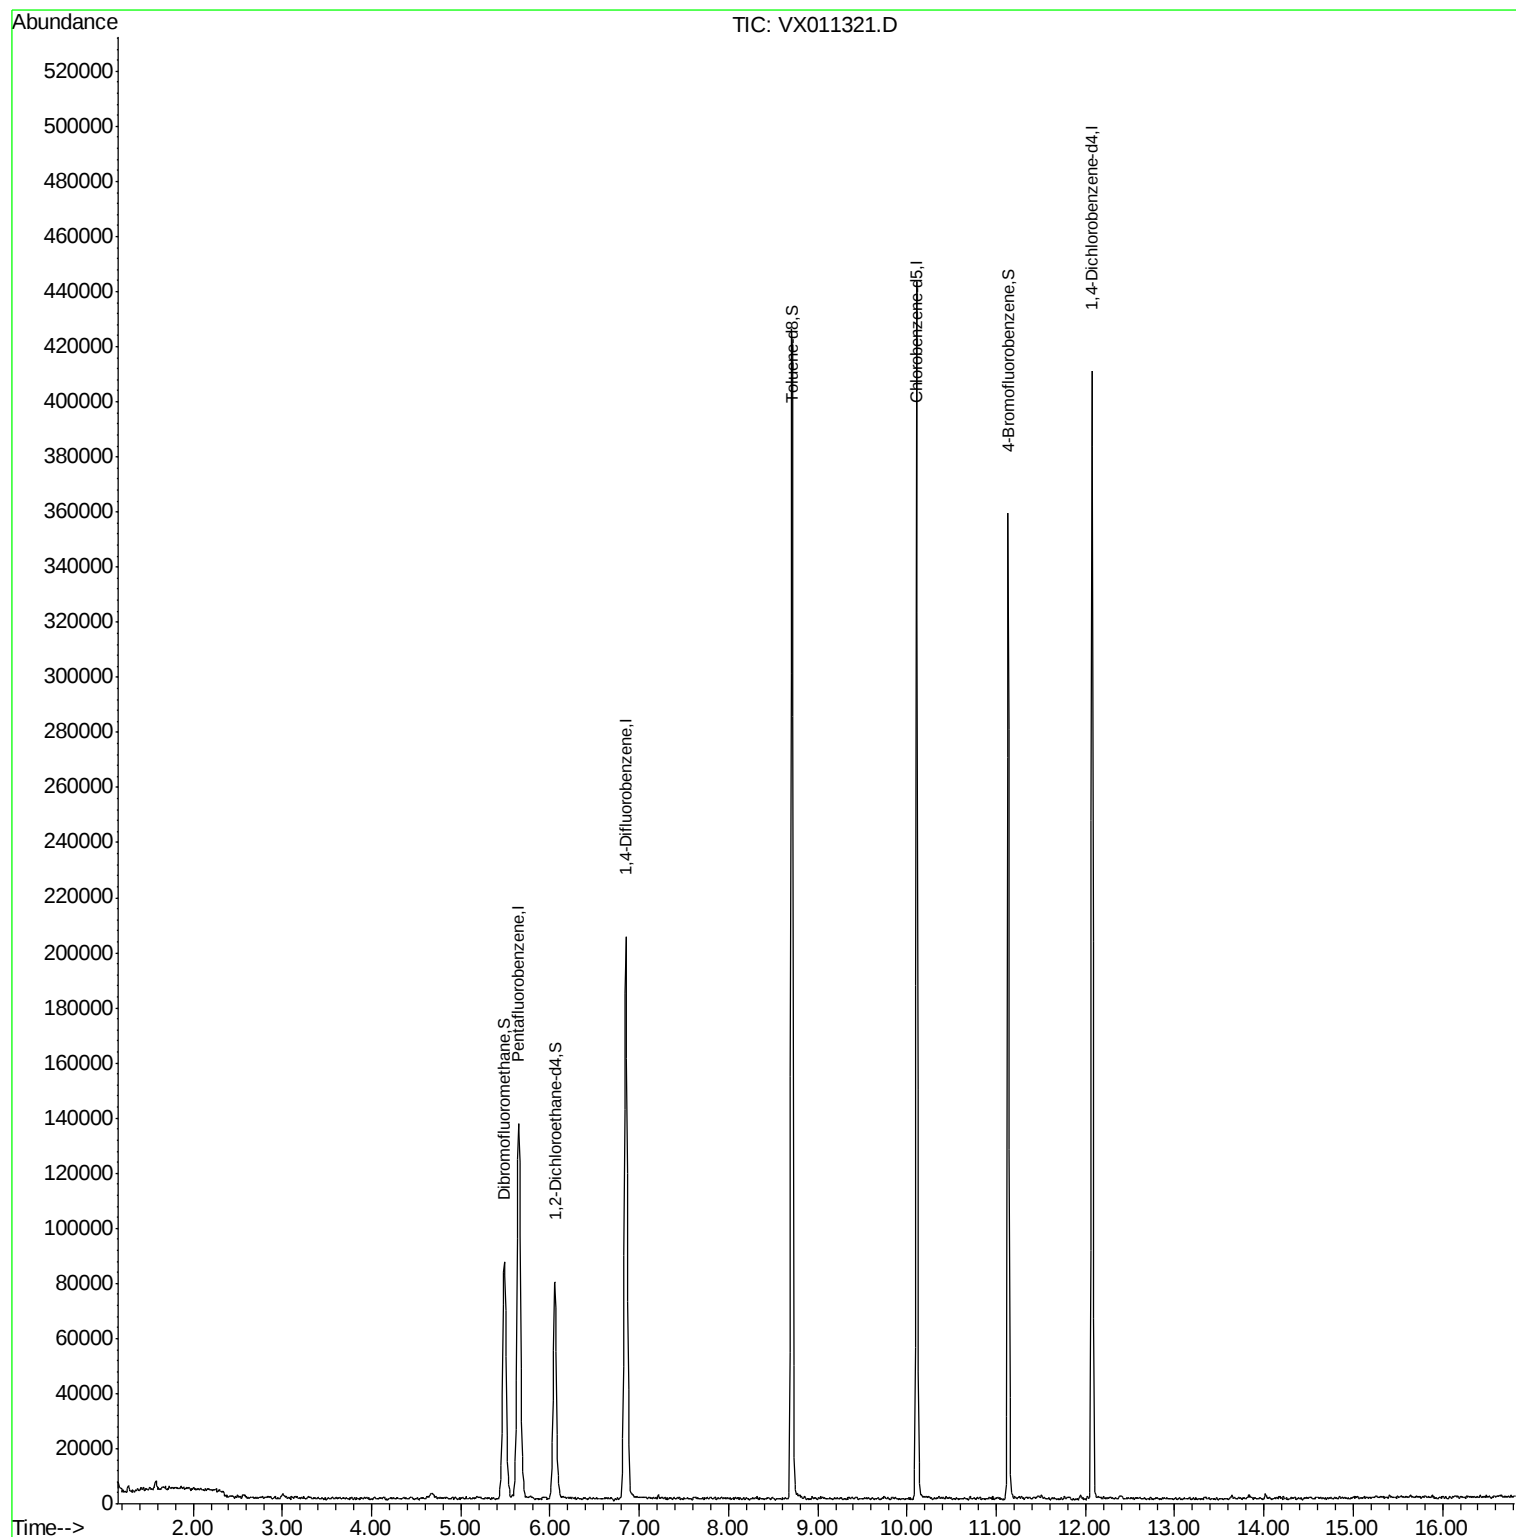

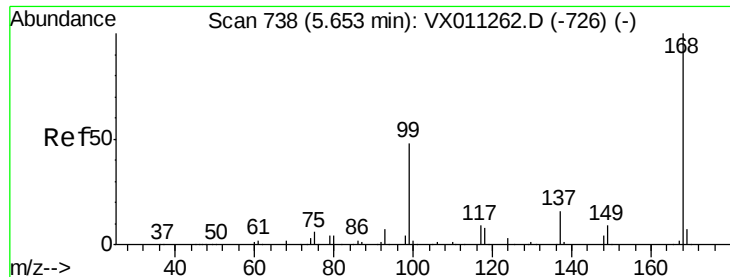

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 737

Delta R.T. -0.01 min

Lab File: VX011321.D

Acq: 05 Aug 2019 11:03

Instrument :

MSVOA_X

ClientSampleId :


VX0805WBL01

Tot Ion:168 Resp: 137308

Ion Ratio Lower Upper




168 100

99 49.6 38.5 57.7

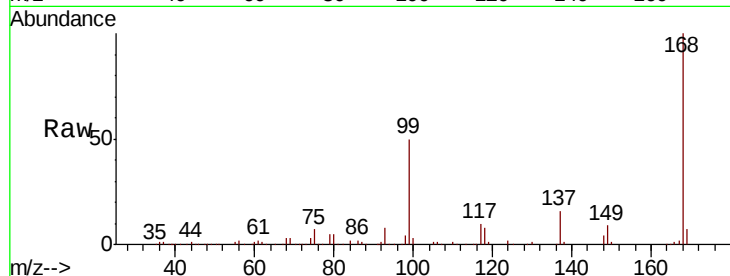

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

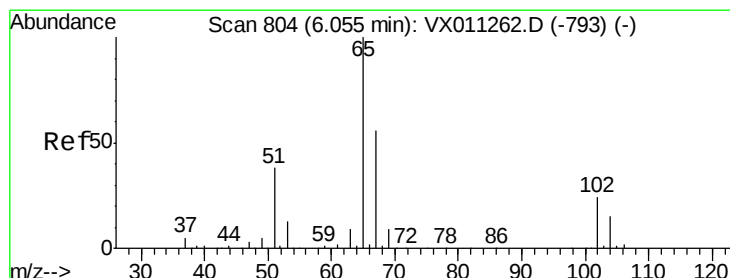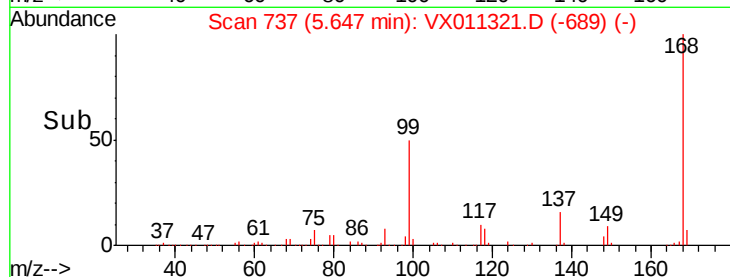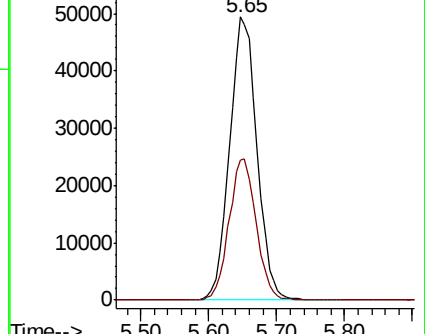

#33

1,2-Dichloroethane-d4

Concen: 53.390 ug/l

RT: 6.05 min Scan# 803

Delta R.T. -0.01 min

Lab File: VX011321.D


Acq: 05 Aug 2019 11:03

Tgt Ion: 65 Resp: 73826

Ion Ratio Lower Upper



65 100


67 54.2 0.0 110.6

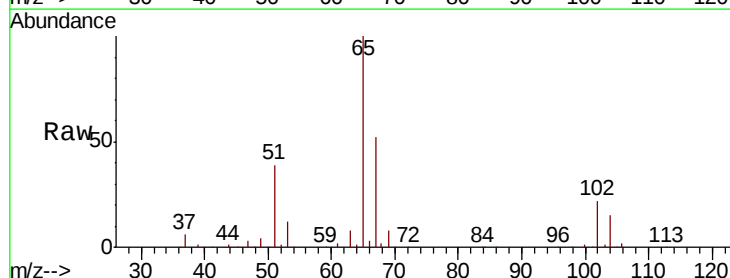

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

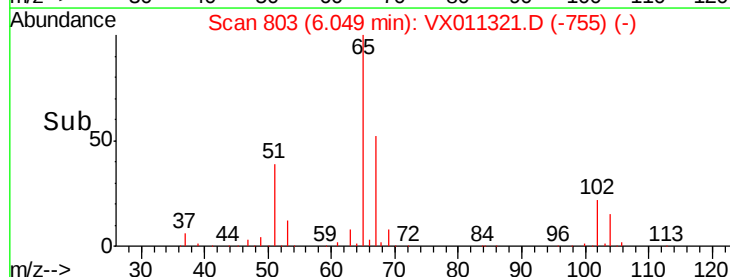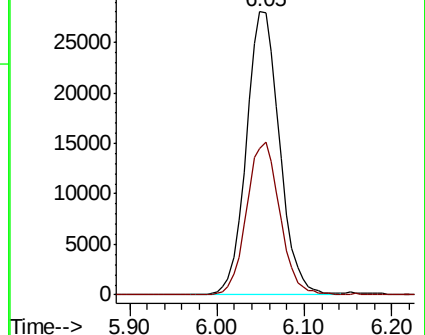

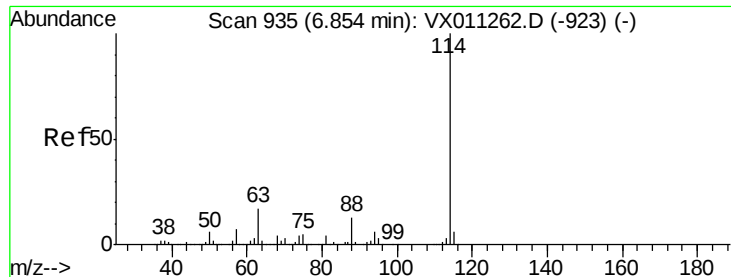

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 934

Delta R.T. -0.01 min

Lab File: VX011321.D

Acq: 05 Aug 2019 11:03

Instrument :

MSVOA_X

ClientSampleId :

VX0805WBL01


Tot Ion:114 Resp: 216963

Ion Ratio Lower Upper

114 100

63 18.0 0.0 34.0




88 14.3 0.0 26.4

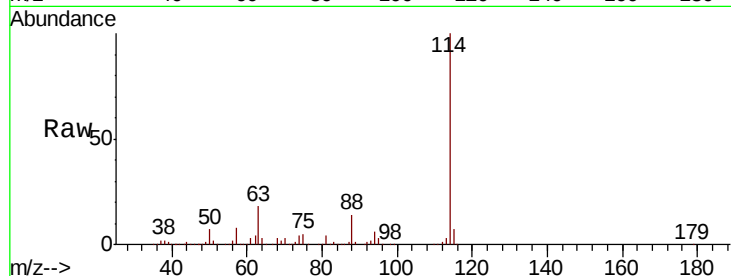

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

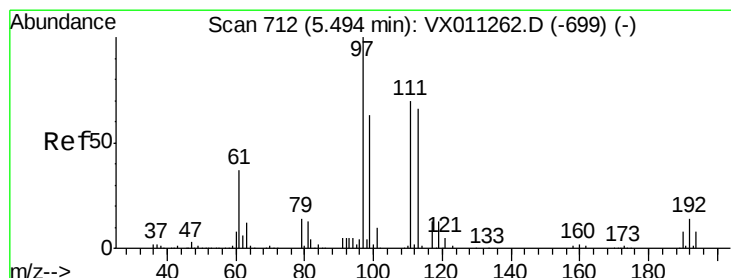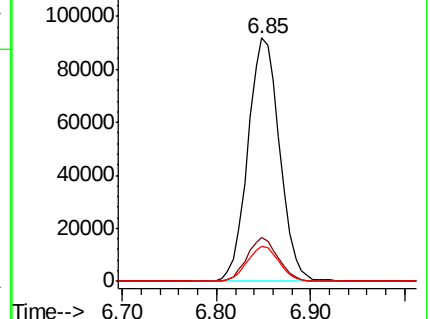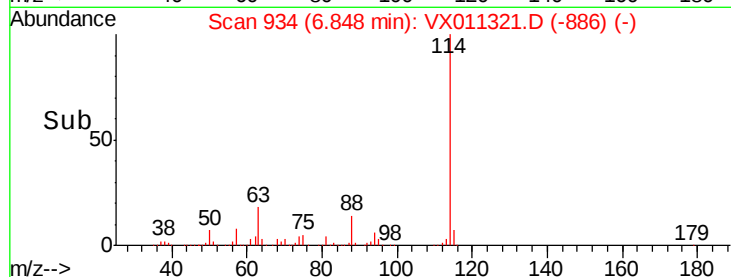

#35

Dibromofluoromethane

Concen: 50.574 ug/l

RT: 5.49 min Scan# 711

Delta R.T. -0.01 min

Lab File: VX011321.D

Acq: 05 Aug 2019 11:03


Tgt Ion:113 Resp: 71638

Ion Ratio Lower Upper

113 100

111 101.6 81.9 122.9



192 22.6 17.8 26.8

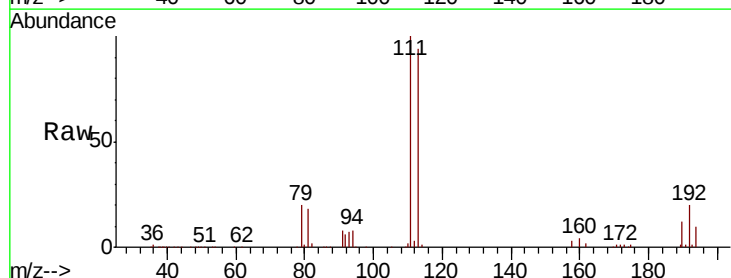


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

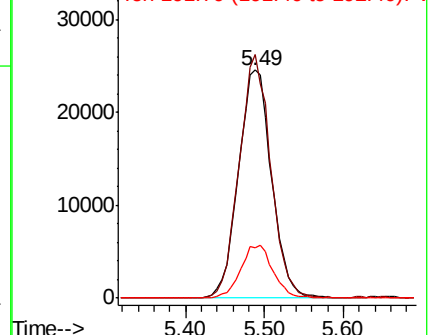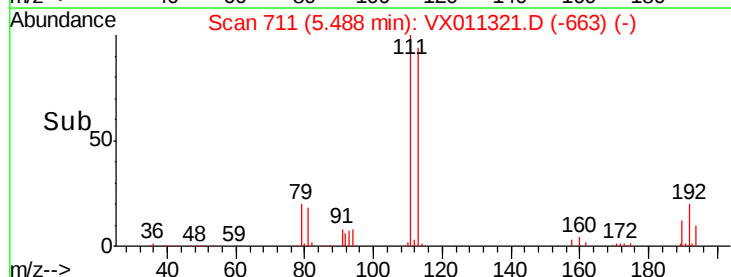

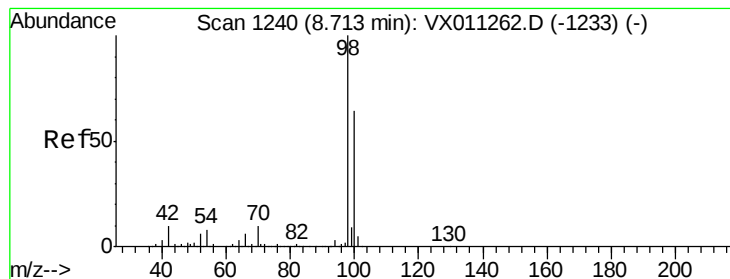

#50

Toluene-d8

Concen: 49.412 ug/l

RT: 8.71 min Scan# 1239

Delta R.T. -0.01 min

Lab File: VX011321.D

Acq: 05 Aug 2019 11:03

Instrument :

MSVOA_X

ClientSampleId :


VX0805WBL01

Tot Ion: 98 Resp: 264201

Ion Ratio Lower Upper

98 100

100 63.2 51.7 77.5

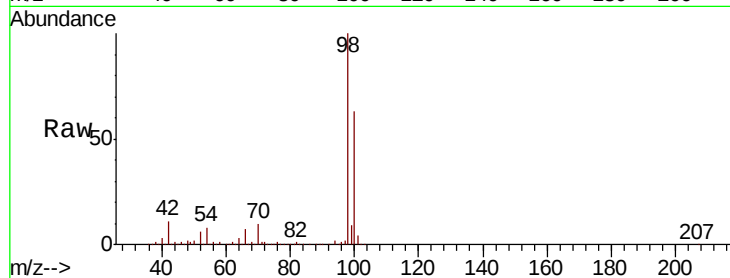

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

8.71

150000



100000

50000

0

8.60 8.70 8.80

Time-->

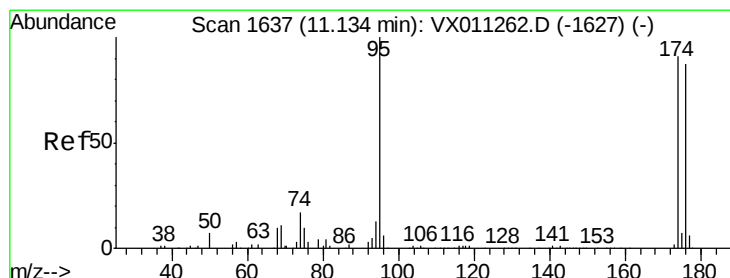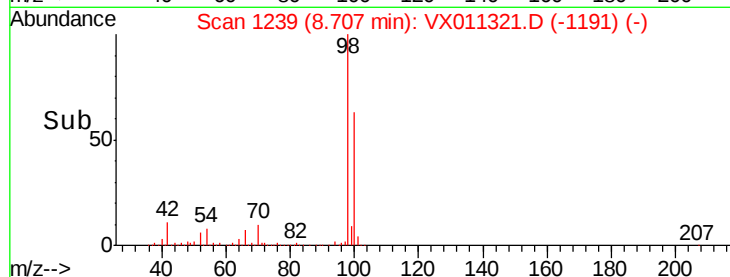

#62

4-Bromofluorobenzene

Concen: 45.835 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX011321.D

Acq: 05 Aug 2019 11:03


Tgt Ion: 95 Resp: 87498

Ion Ratio Lower Upper

95 100

174 93.0 0.0 191.2

176 88.8 0.0 184.8

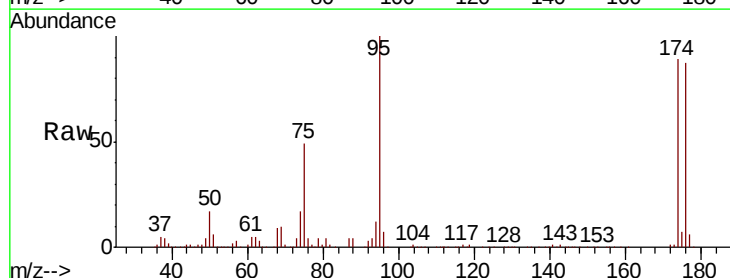

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

11.13

80000

60000


40000


20000

0

11.10 11.20

Time-->

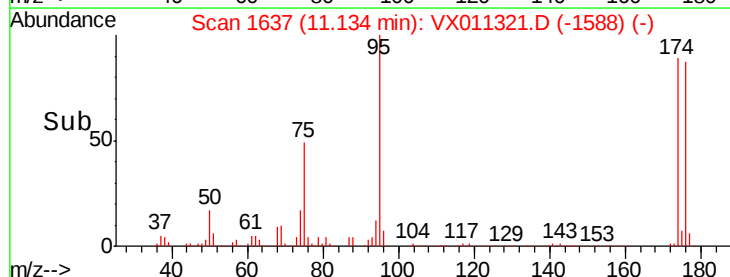


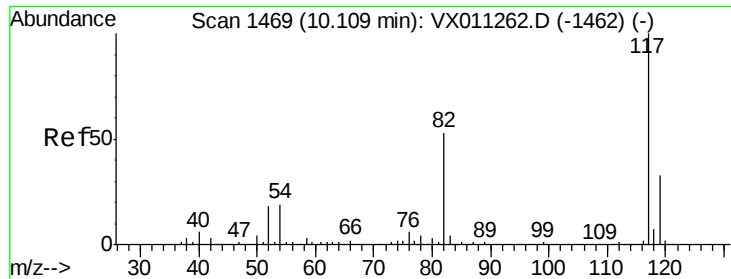




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX011321.D
Acq: 05 Aug 2019 11:03

Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL01

Tot Ion:117 Resp: 200599
Ion Ratio Lower Upper
117 100
82 52.1 42.2 63.2
119 34.5 26.6 39.8

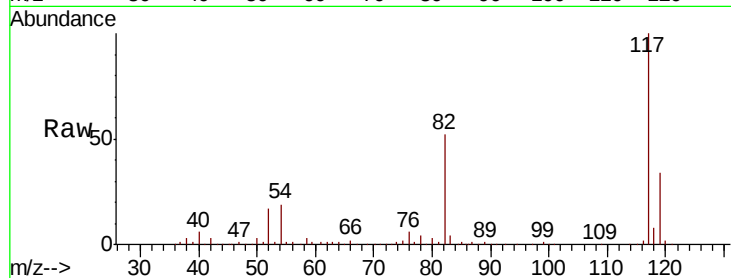


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

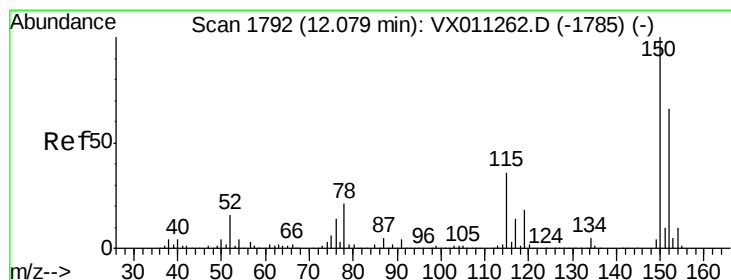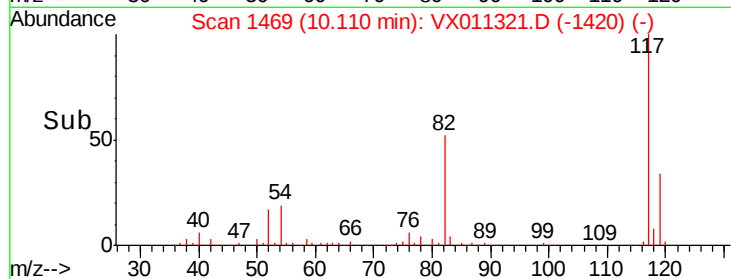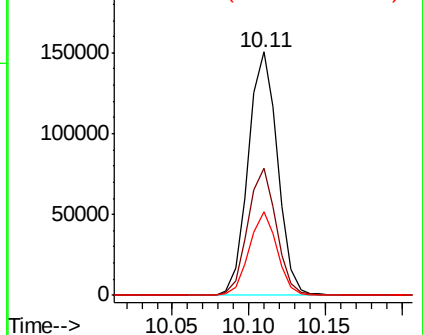

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1791
Delta R.T. -0.01 min
Lab File: VX011321.D
Acq: 05 Aug 2019 11:03

Tgt Ion:152 Resp: 90489
Ion Ratio Lower Upper
152 100
115 53.6 40.0 119.9
150 154.6 0.0 350.4

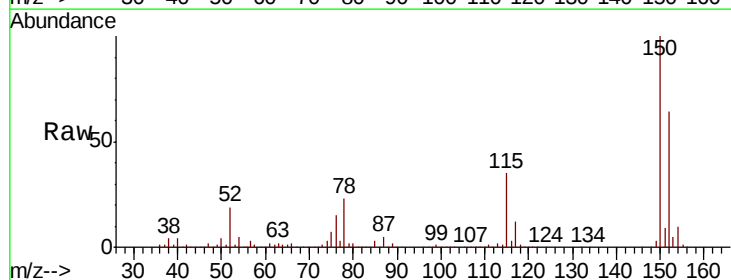

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

