


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080519\
Data File : VX011319.D
Acq On : 05 Aug 2019 09:11
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Title : SW846 8260
Last Update : Fri Aug 02 01:55:00 2019

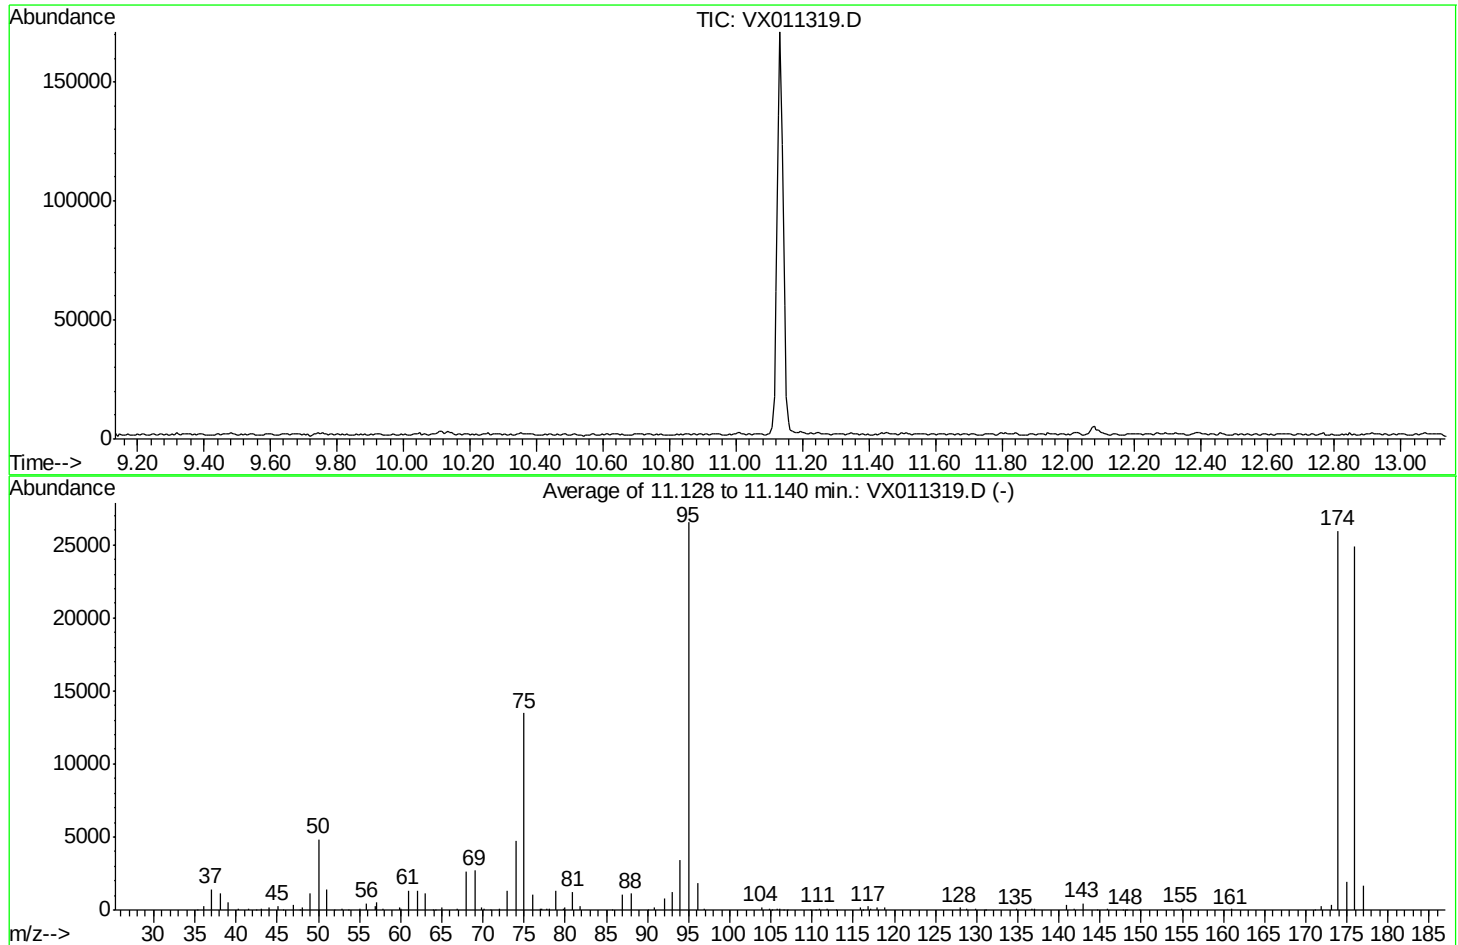

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	4845	PASS
75	95	30	60	50.8	13473	PASS
95	95	100	100	100.0	26533	PASS
96	95	5	9	7.0	1854	PASS
173	174	0.00	2	1.4	360	PASS
174	95	50	100	97.7	25933	PASS
175	174	5	9	7.3	1905	PASS
176	174	95	101	95.9	24861	PASS
177	176	5	9	6.7	1674	PASS