


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080520\
Data File : VX017786.D
Acq On : 05 Aug 2020 09:21
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Title : SW846 8260
Last Update : Fri Jul 24 05:48:09 2020

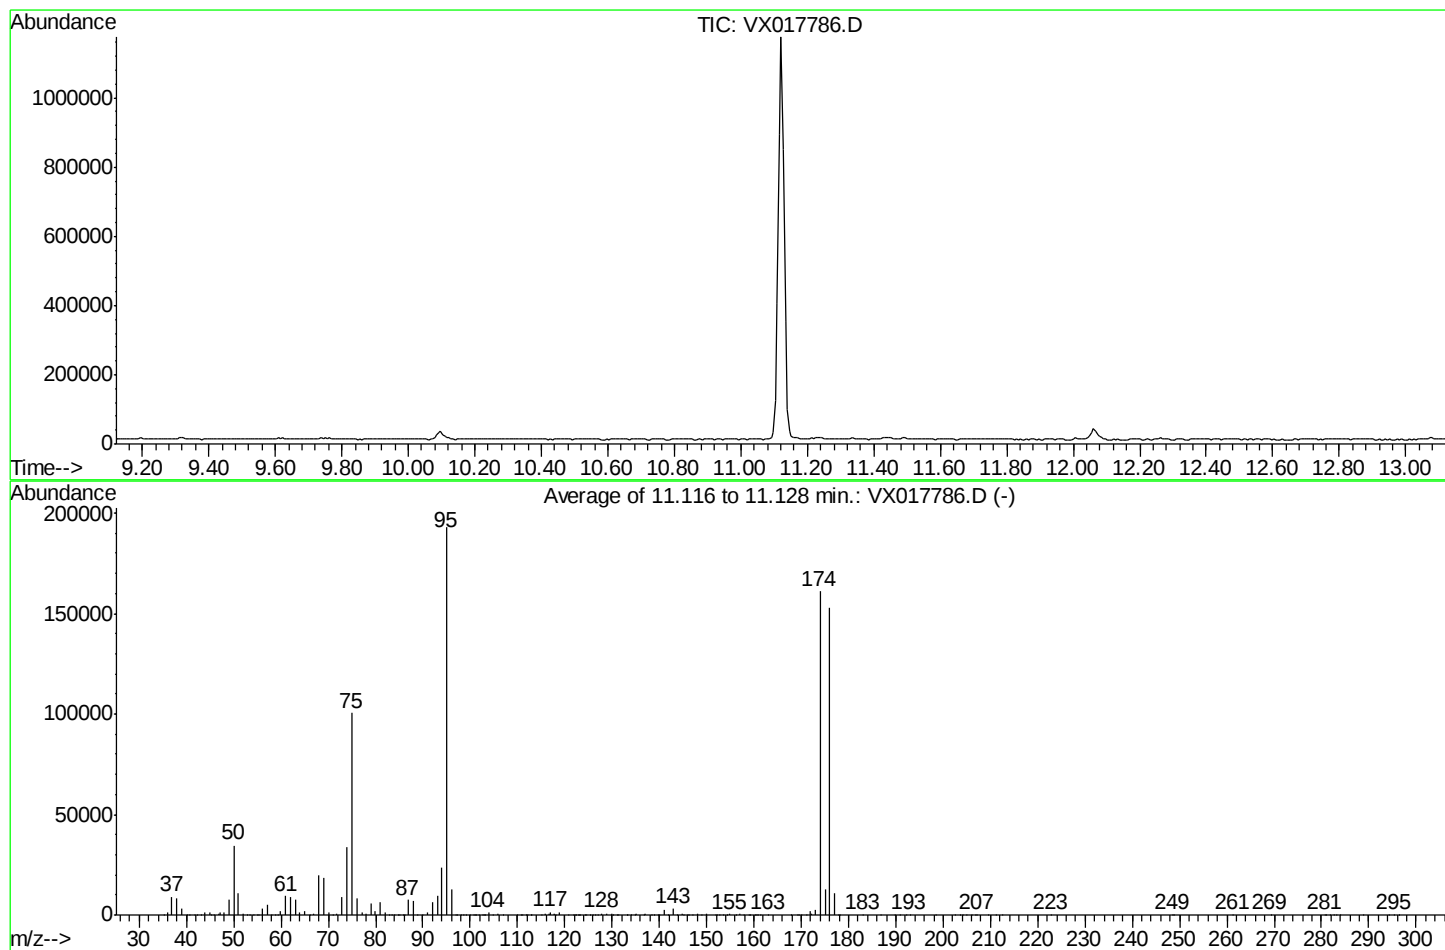

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	34716	PASS
75	95	30	60	52.1	100432	PASS
95	95	100	100	100.0	192938	PASS
96	95	5	9	6.7	12854	PASS
173	174	0.00	2	1.6	2510	PASS
174	95	50	100	83.4	160885	PASS
175	174	5	9	7.9	12719	PASS
176	174	95	101	95.0	152768	PASS
177	176	5	9	7.0	10642	PASS