

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
 Data File : VX023549.D
 Acq On : 04 Aug 2021 18:46
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Aug 05 06:09:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:05:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	167240	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	275184	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	241488	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	90122	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	105906	50.766	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	101.540%
35) Dibromofluoromethane	5.397	113	86657	50.365	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.740%
50) Toluene-d8	8.653	98	328729	52.002	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	104.000%
62) 4-Bromofluorobenzene	11.085	95	103454	48.128	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.260%
Target Compounds						
						Qvalue
20) Methylene Chloride	2.794	84	2548	1.280	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023549.D
Acq On : 04 Aug 2021 18:46
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Aug 05 06:09:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration




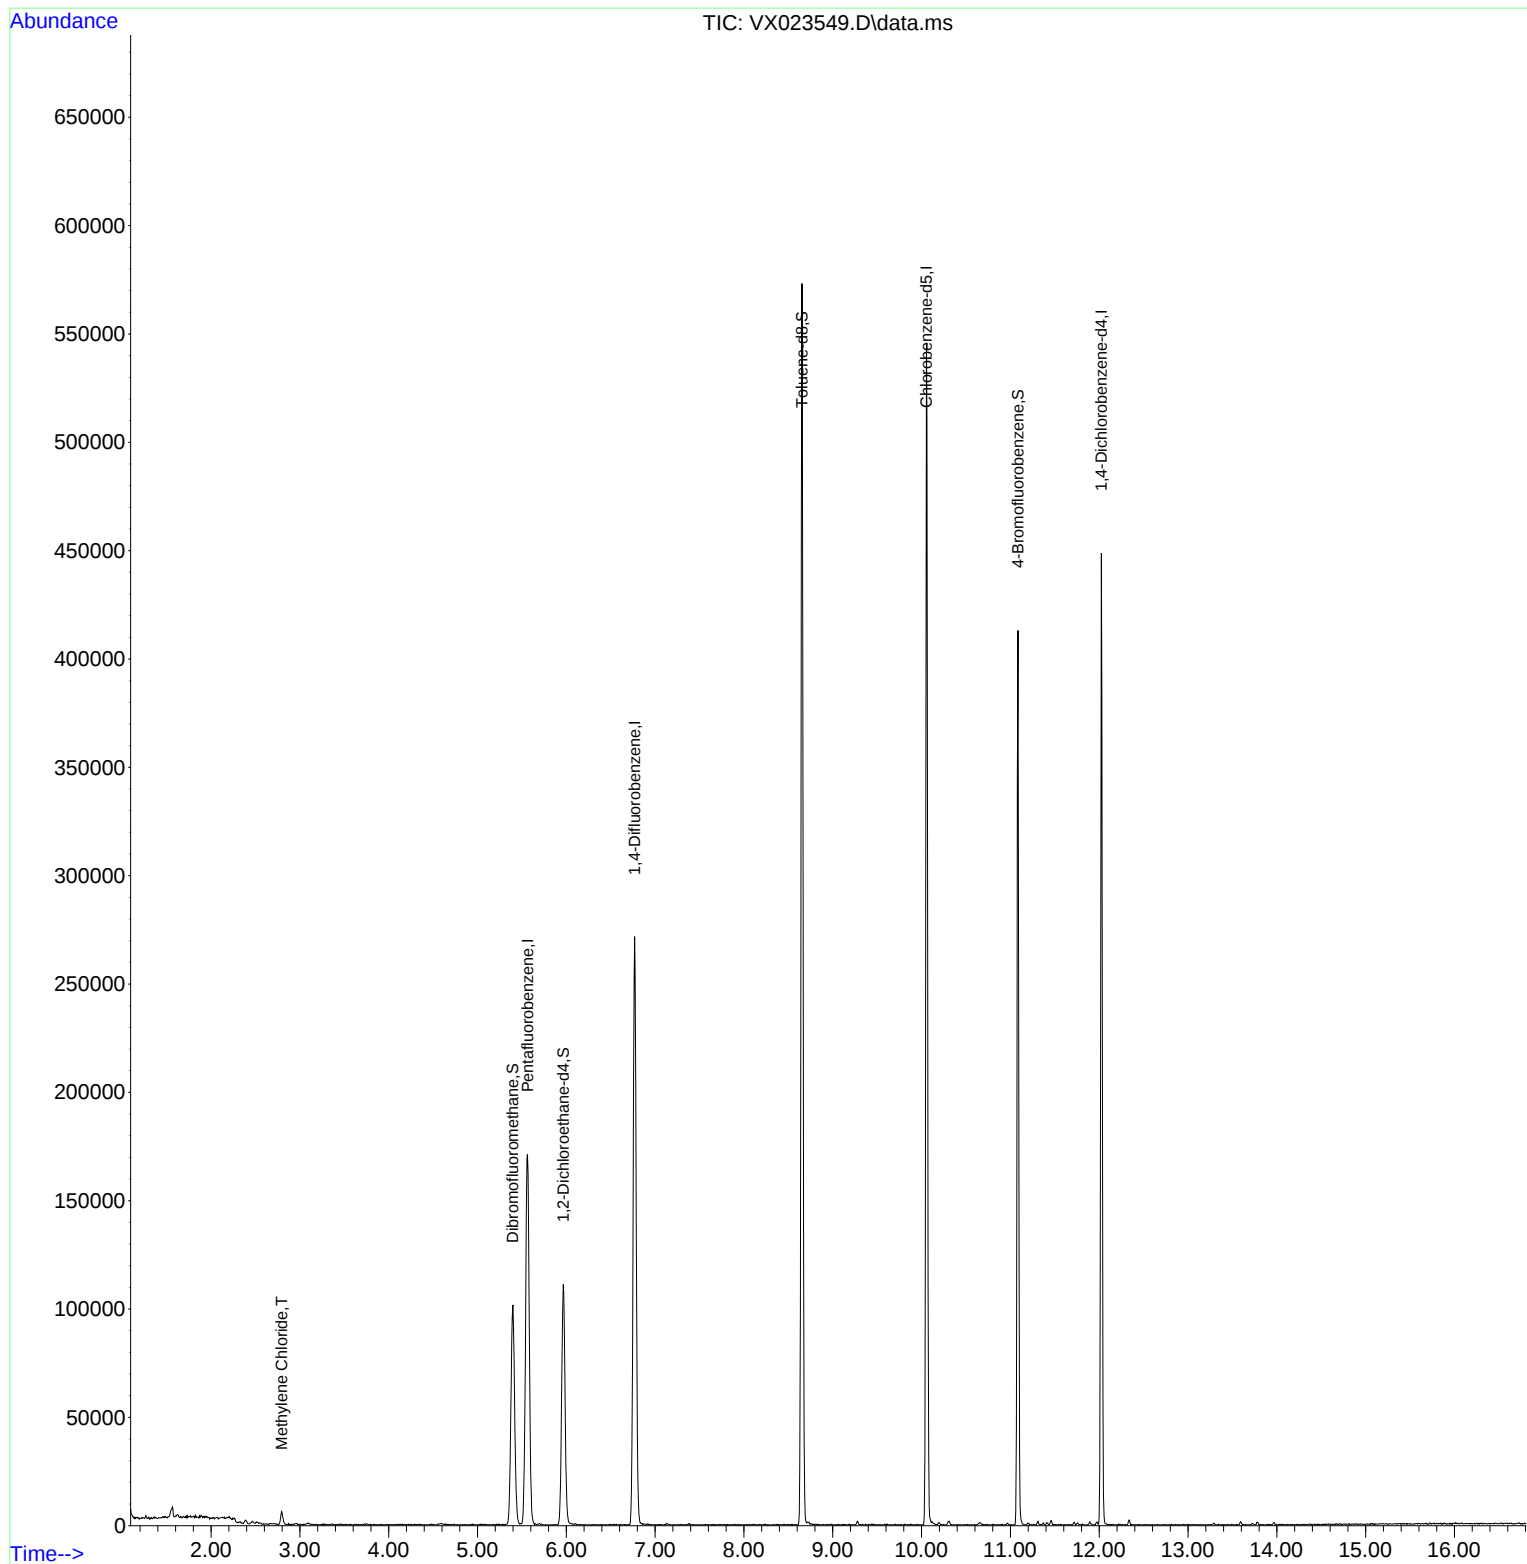


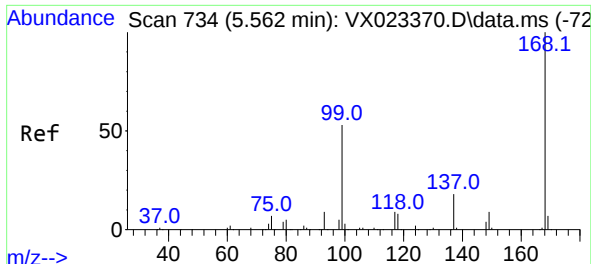

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 167240
Ion Ratio Lower Upper
168 100
99 56.2 45.8 68.6

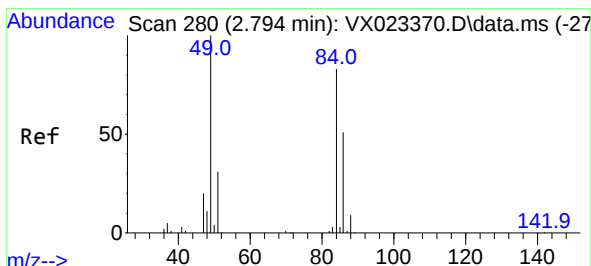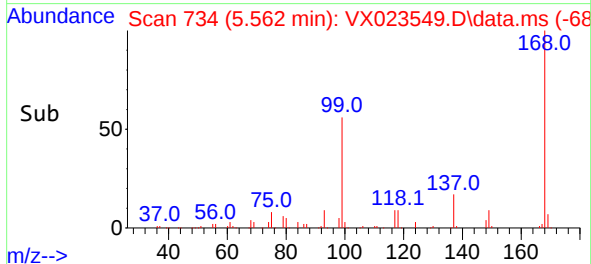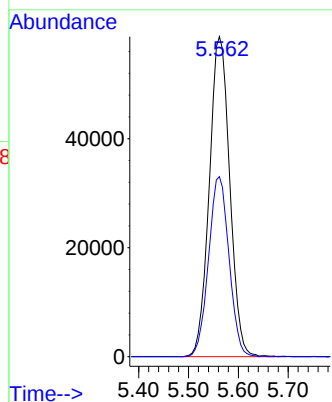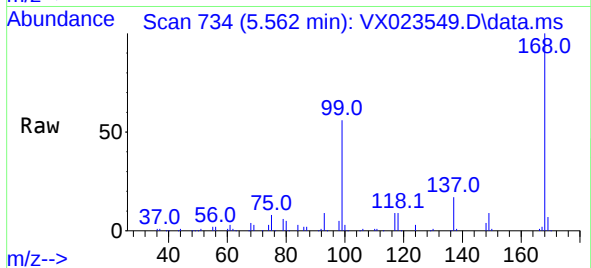

#20
Methylene Chloride
Concen: 1.280 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46

Tgt Ion: 84 Resp: 2548
Ion Ratio Lower Upper
84 100
49 104.2 88.6 132.8
51 45.6 27.0 40.6#
86 67.9 50.3 75.5

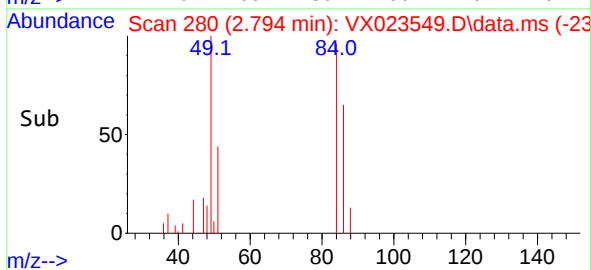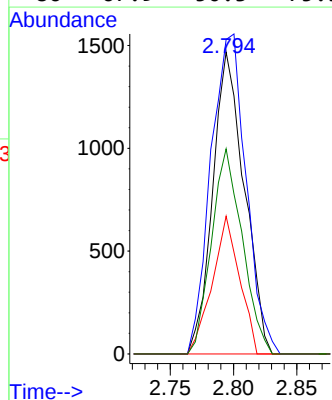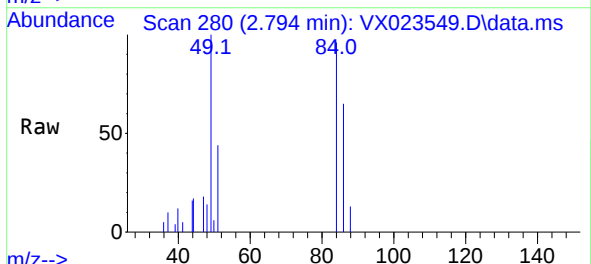




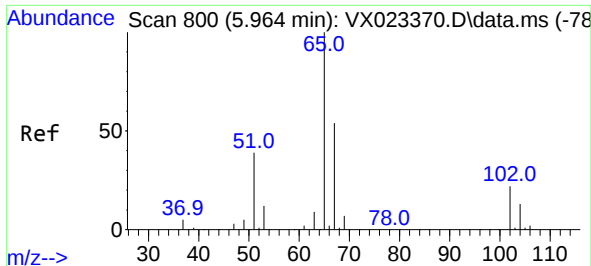


#33

1,2-Dichloroethane-d4
Concen: 50.766 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46

Instrument :
MSVOA_X
ClientSampled :
IBLK




Tgt Ion: 65 Resp: 105906
Ion Ratio Lower Upper
65 100
67 51.9 0.0 105.4

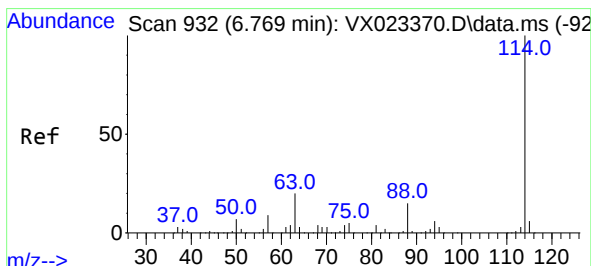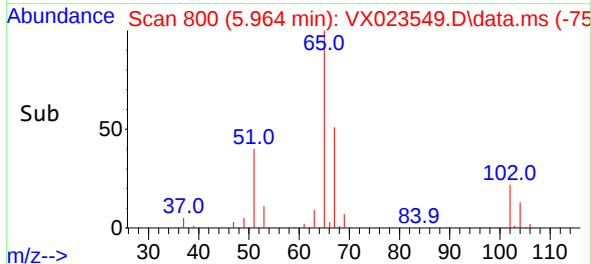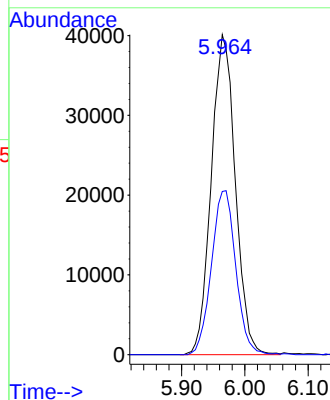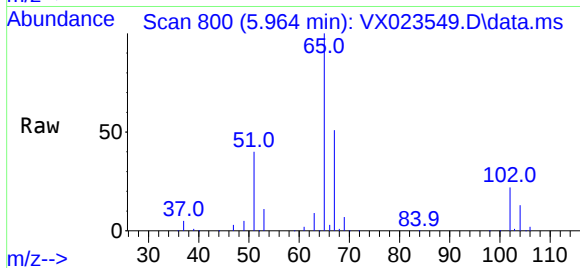


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46

Tgt Ion: 114 Resp: 275184
Ion Ratio Lower Upper
114 100
63 19.8 0.0 40.8
88 16.1 0.0 32.8


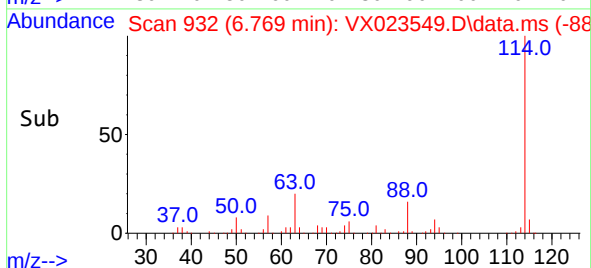
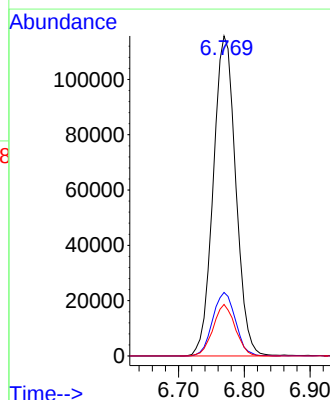
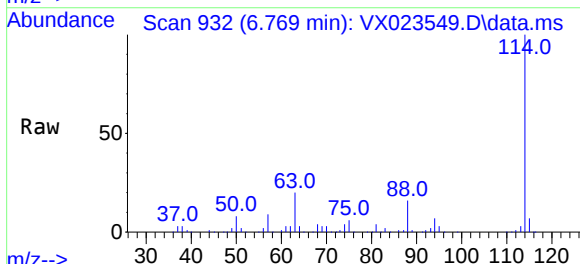


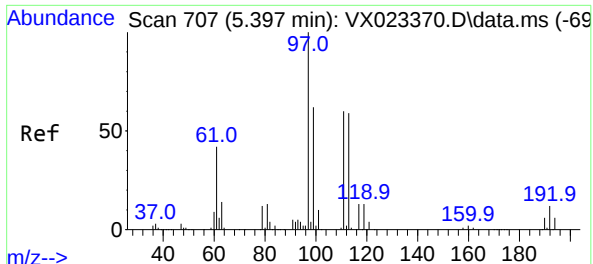

#35
Dibromofluoromethane
Concen: 50.365 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:113 Resp: 86657
Ion Ratio Lower Upper
113 100
111 102.7 81.9 122.9
192 19.7 16.7 25.1

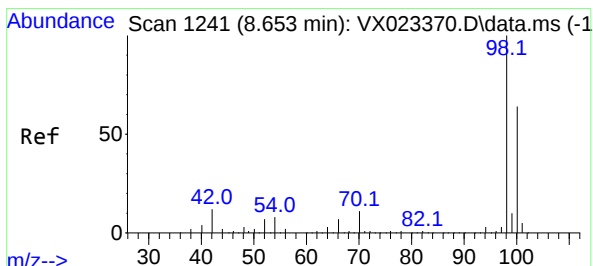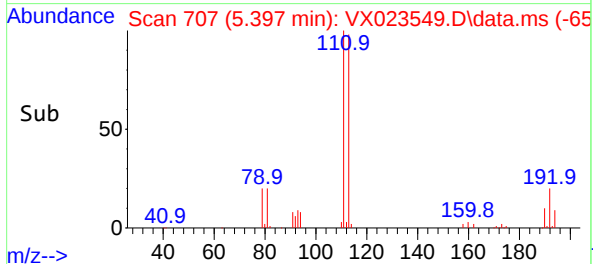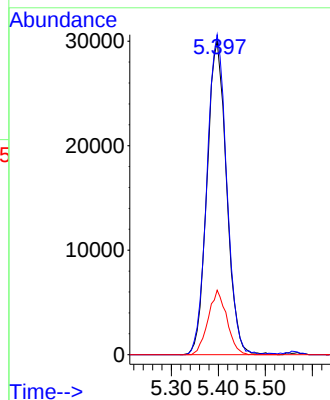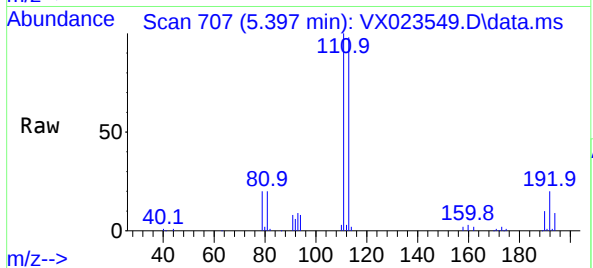

#50
Toluene-d8
Concen: 52.002 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46

Tgt Ion: 98 Resp: 328729
Ion Ratio Lower Upper
98 100
100 64.0 51.9 77.9


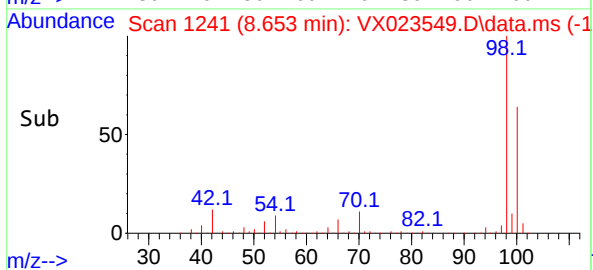
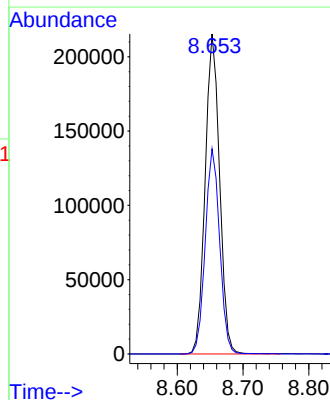
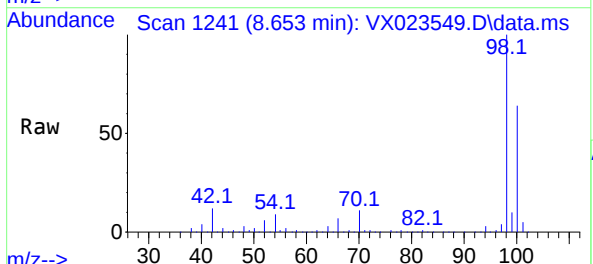


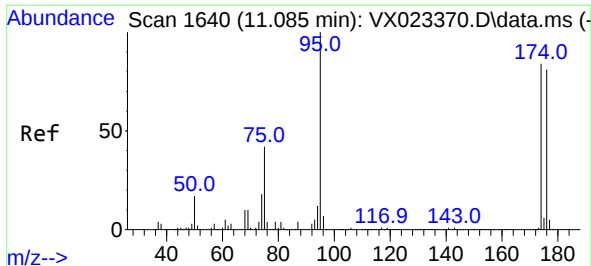

#62
4-Bromofluorobenzene
Concen: 48.128 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46




Instrument :
MSVOA_X
ClientSampled :
IBLK


Tgt Ion: 95 Resp: 103454
Ion Ratio Lower Upper
95 100
174 82.9 0.0 154.6
176 79.5 0.0 155.8

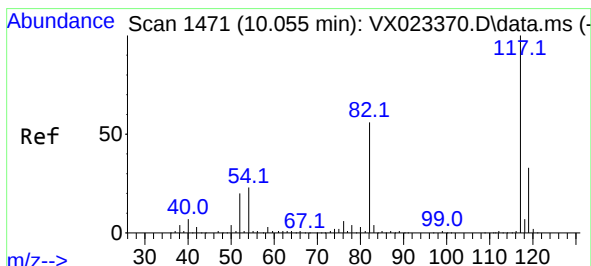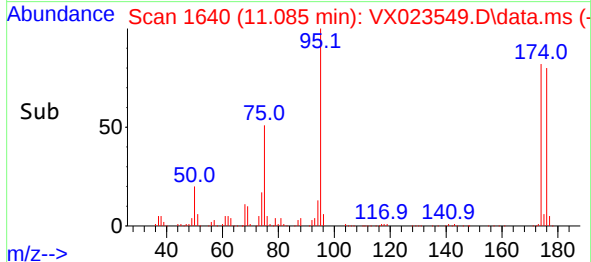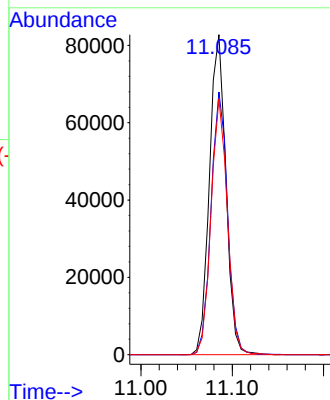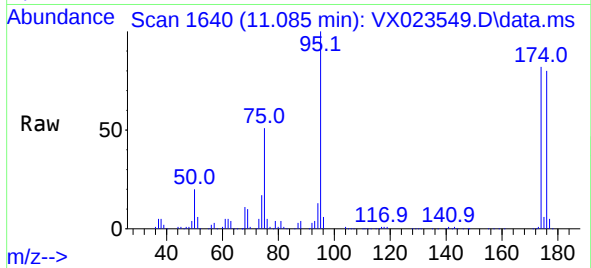

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX023549.D
Acq: 04 Aug 2021 18:46

Tgt Ion: 117 Resp: 241488
Ion Ratio Lower Upper
117 100
82 58.0 47.4 71.2
119 32.6 26.6 39.8

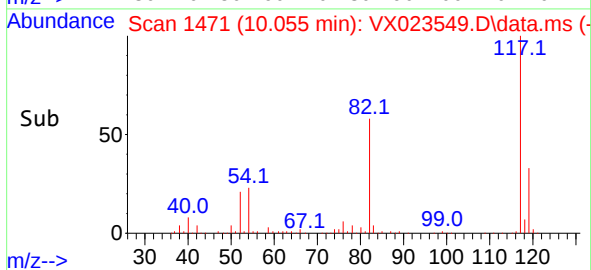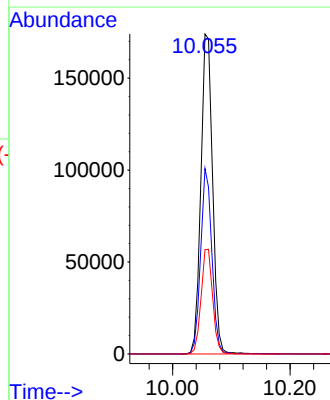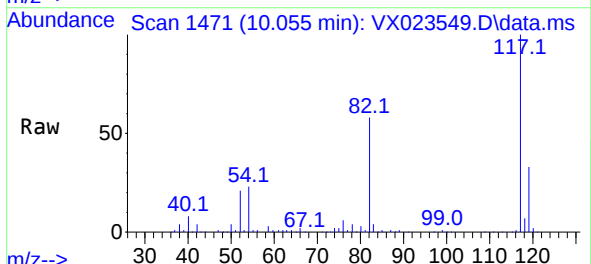

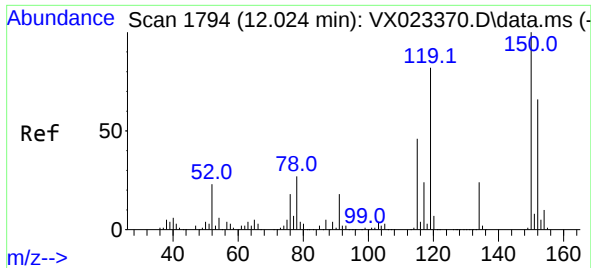

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX023549.D
 Acq: 04 Aug 2021 18:46

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Tgt Ion:152 Resp: 90122
 Ion Ratio Lower Upper
 152 100
 115 59.0 41.1 123.3
 150 159.8 0.0 349.0

