

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
 Data File : VX023562.D
 Acq On : 05 Aug 2021 10:57
 Operator : JC/MD
 Sample : VX0805WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0805WBL02

Quant Time: Aug 06 03:21:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:05:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	159969	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	272385	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	243040	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91409	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	108823	54.535	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	109.060%
35) Dibromofluoromethane	5.391	113	87007	51.088	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.180%
50) Toluene-d8	8.653	98	327719	52.375	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	104.760%
62) 4-Bromofluorobenzene	11.085	95	105106	49.399	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023562.D
Acq On : 05 Aug 2021 10:57
Operator : JC/MD
Sample : VX0805WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL02

Quant Time: Aug 06 03:21:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration




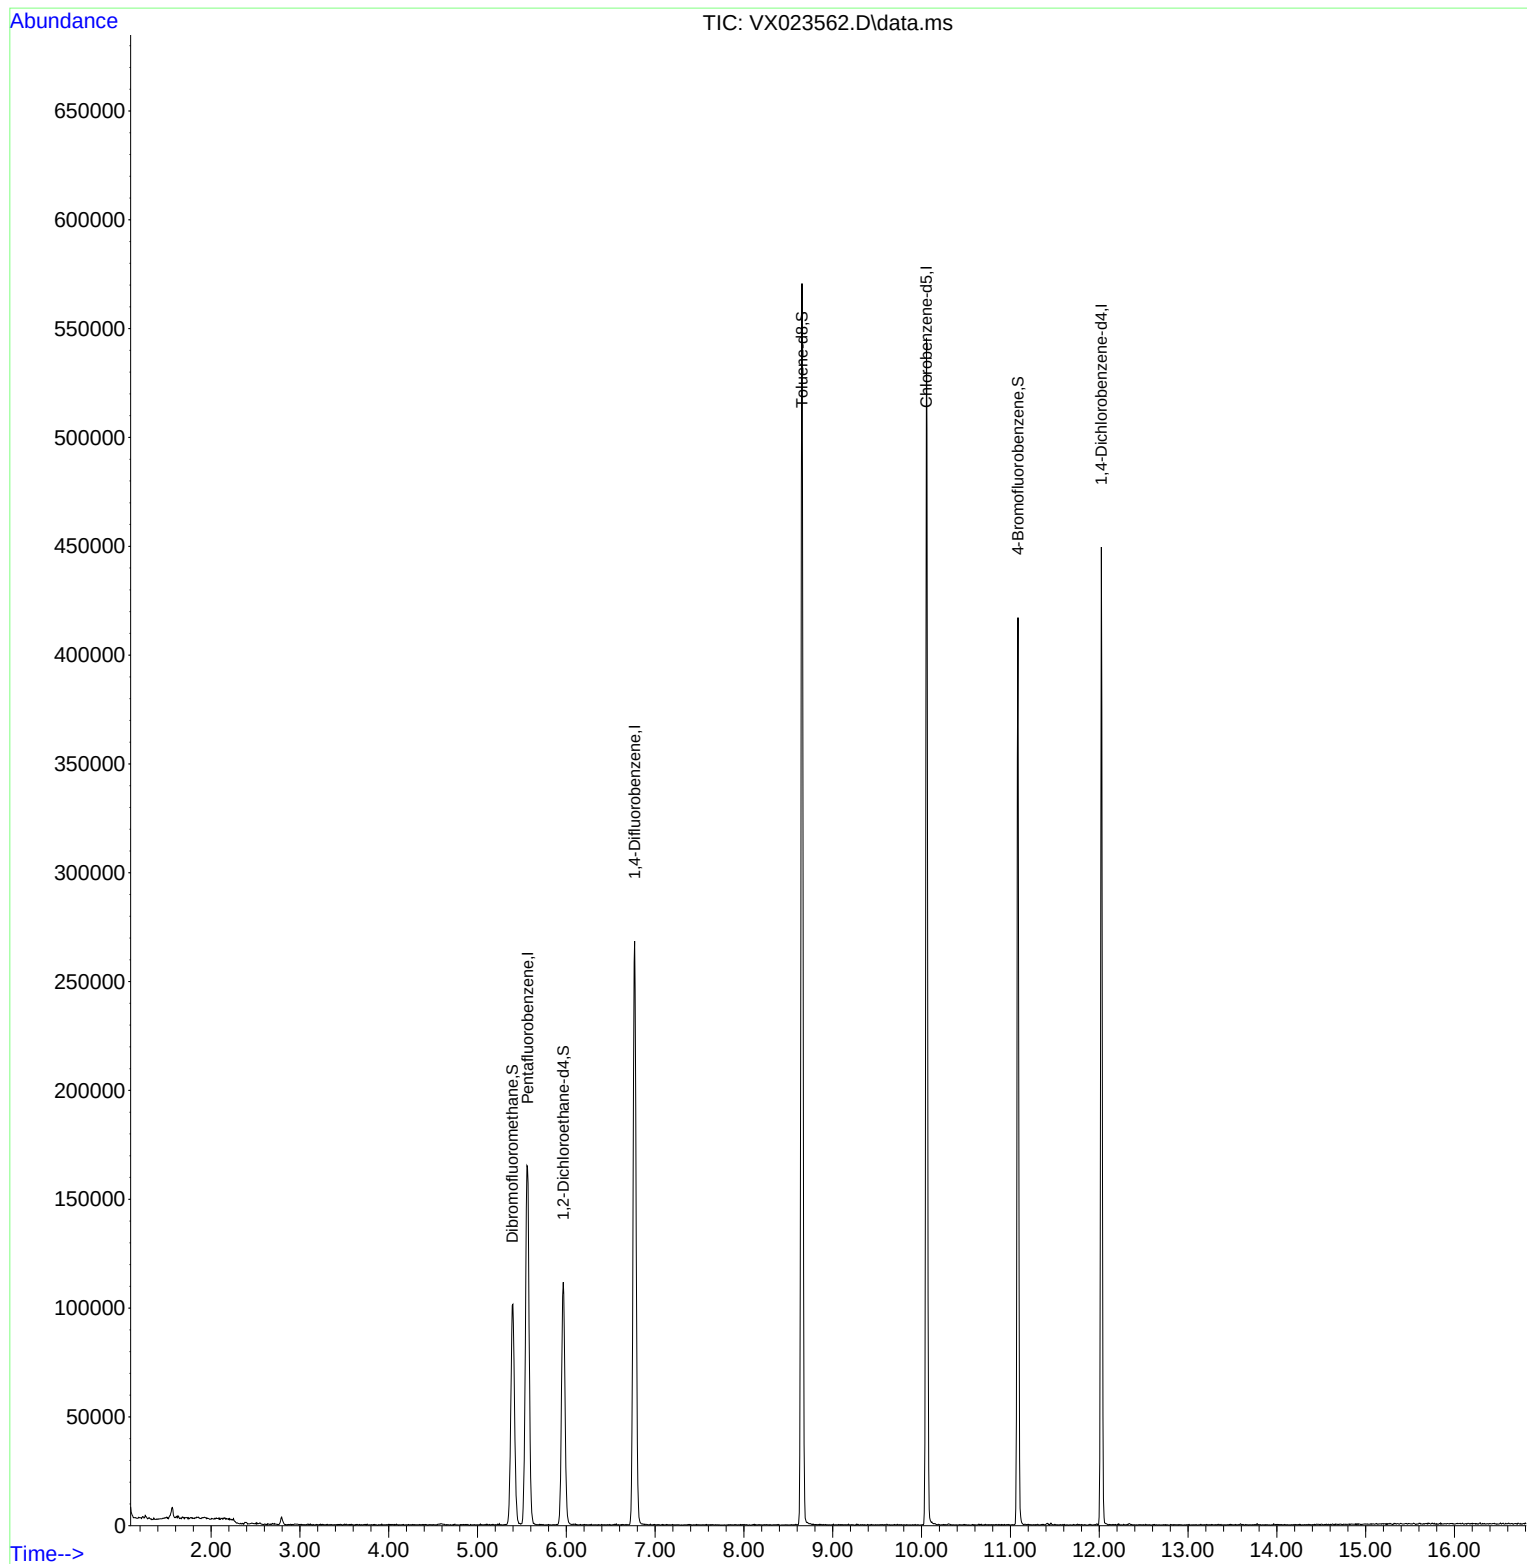


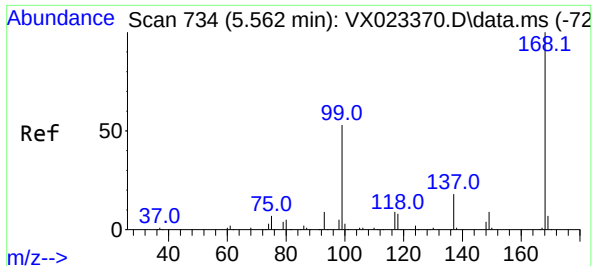

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL02


Tgt Ion:168 Resp: 159969
Ion Ratio Lower Upper
168 100
99 57.2 45.8 68.6

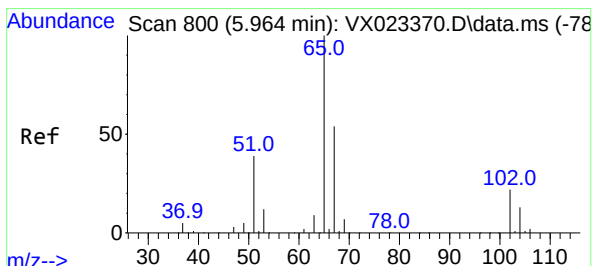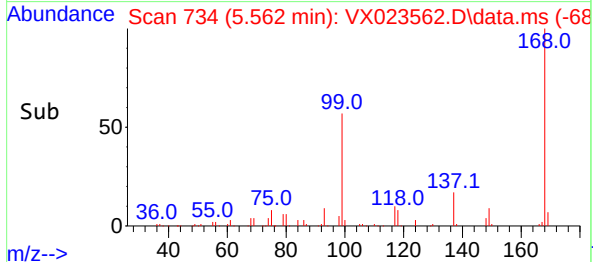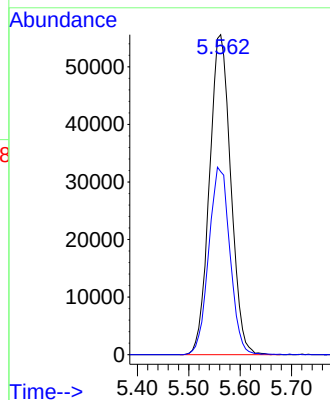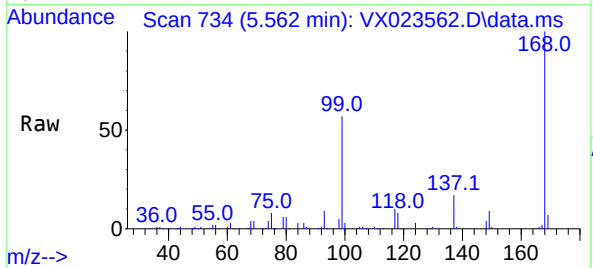

#33
1,2-Dichloroethane-d4
Concen: 54.535 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57

Tgt Ion: 65 Resp: 108823
Ion Ratio Lower Upper
65 100
67 51.7 0.0 105.4


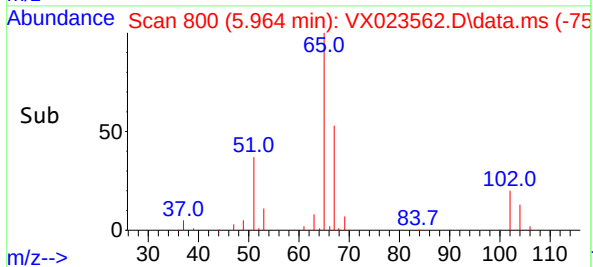
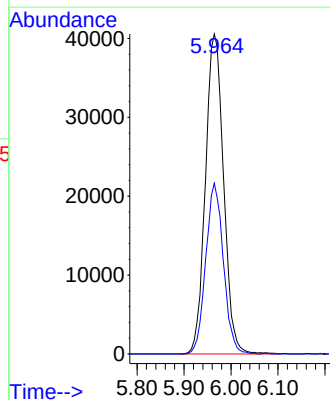
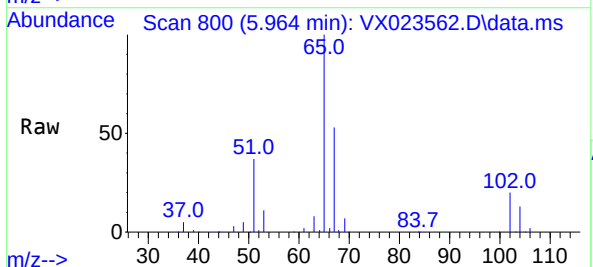


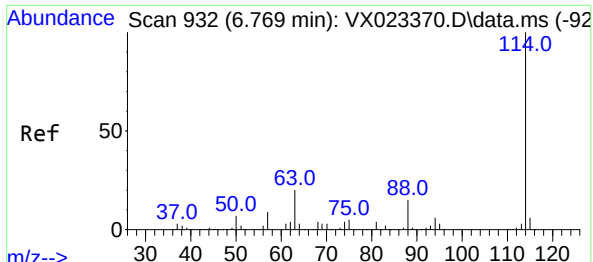

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL02


Tgt Ion:114 Resp: 272385
Ion Ratio Lower Upper
114 100
63 20.6 0.0 40.8
88 16.4 0.0 32.8

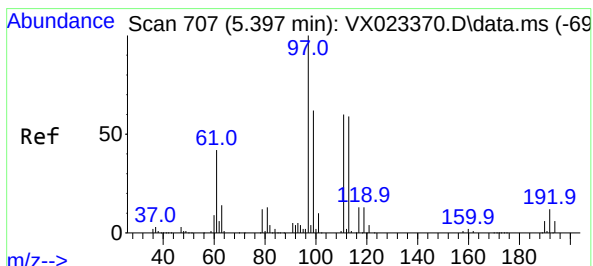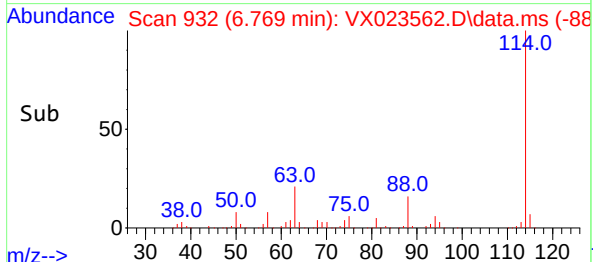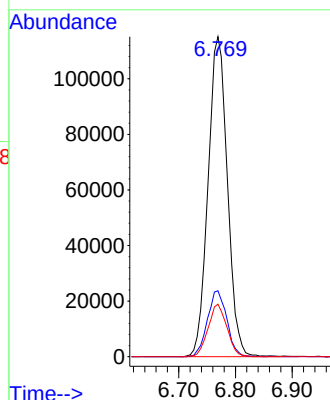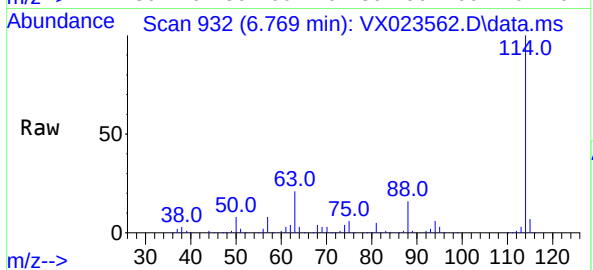

#35
Dibromofluoromethane
Concen: 51.088 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57

Tgt Ion:113 Resp: 87007
Ion Ratio Lower Upper
113 100
111 102.7 81.9 122.9
192 19.7 16.7 25.1


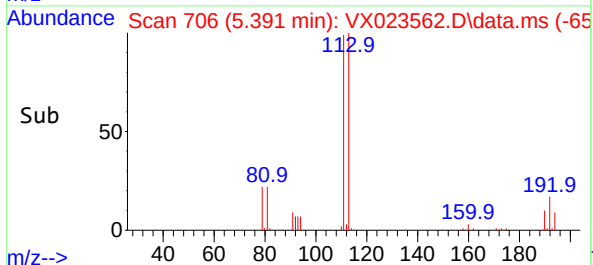
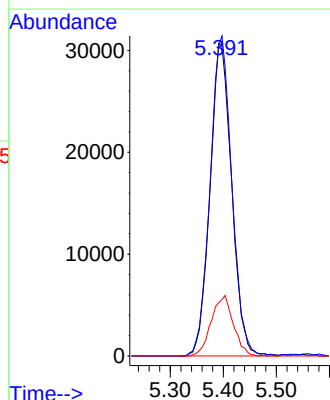
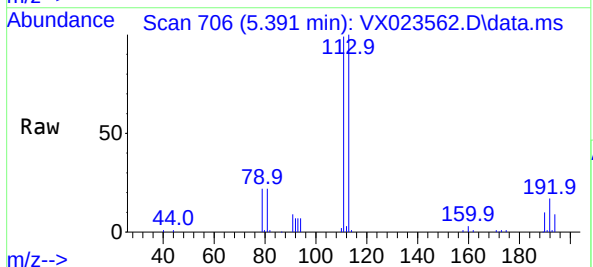


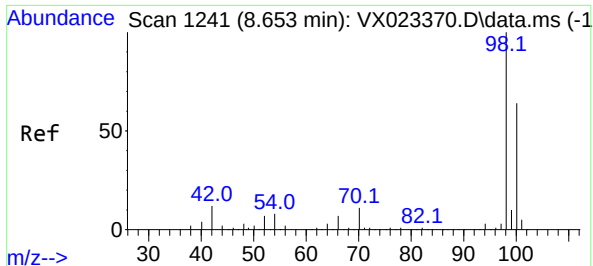

#50
Toluene-d8
Concen: 52.375 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL02


Tgt Ion: 98 Resp: 327719
Ion Ratio Lower Upper
98 100
100 63.7 51.9 77.9

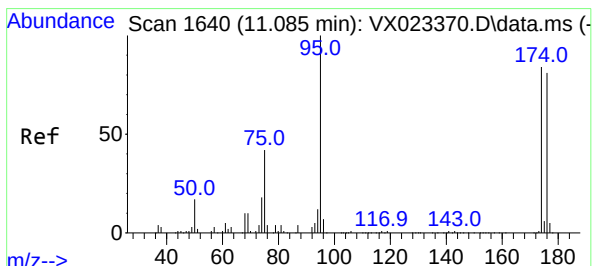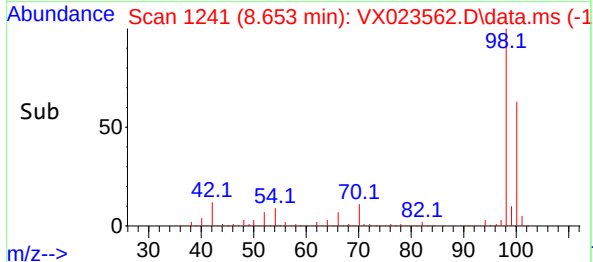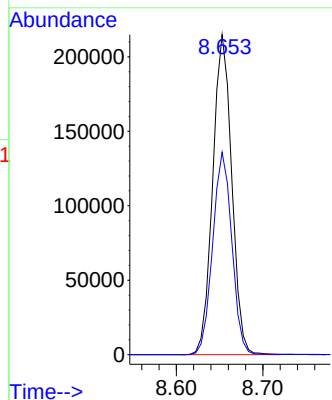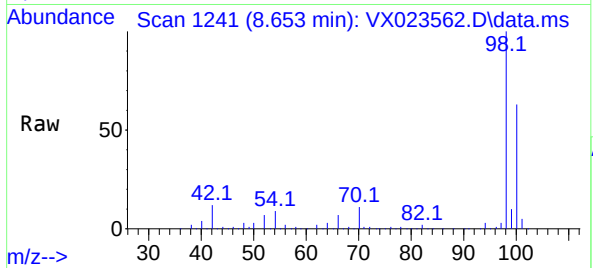

#62
4-Bromofluorobenzene
Concen: 49.399 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57

Tgt Ion: 95 Resp: 105106
Ion Ratio Lower Upper
95 100
174 80.6 0.0 154.6
176 78.7 0.0 155.8


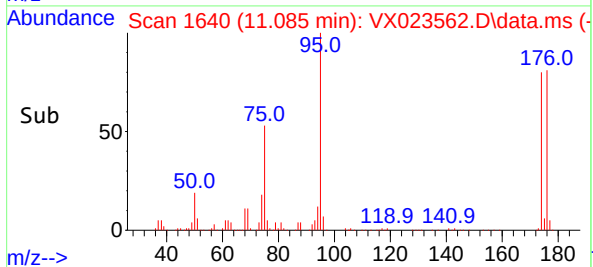
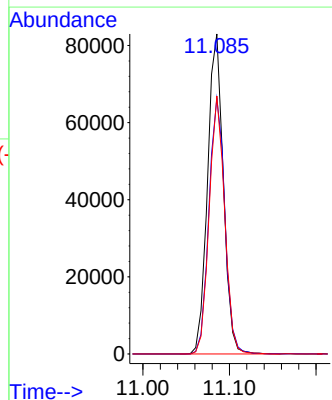
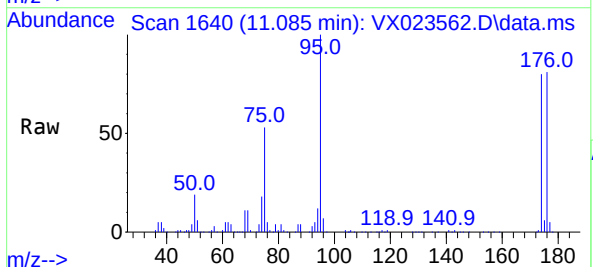


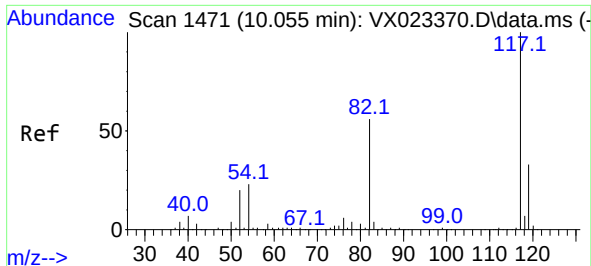

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57

Instrument :
MSVOA_X
ClientSampleId :
VX0805WBL02

Tgt Ion:117 Resp: 243040
Ion Ratio Lower Upper
117 100
82 58.9 47.4 71.2
119 31.0 26.6 39.8

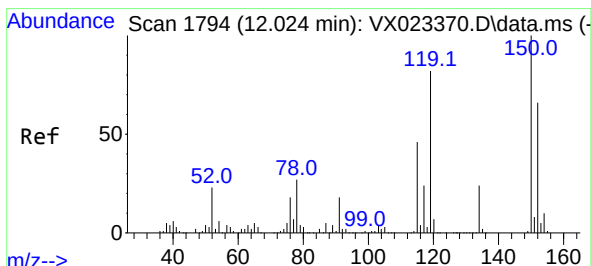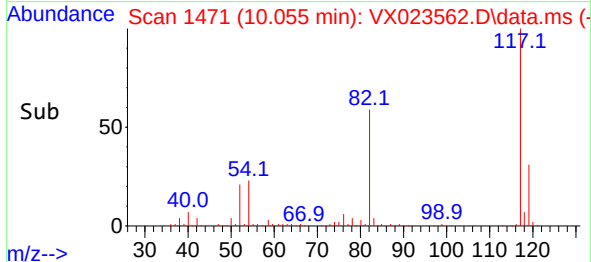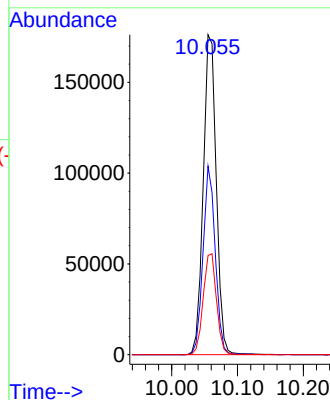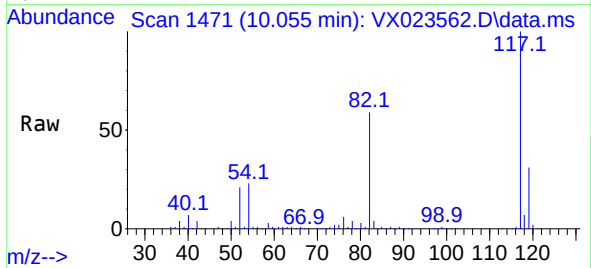

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023562.D
Acq: 05 Aug 2021 10:57

Tgt Ion:152 Resp: 91409
Ion Ratio Lower Upper
152 100
115 58.2 41.1 123.3
150 154.8 0.0 349.0

