

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
 Data File : VX023551.D
 Acq On : 04 Aug 2021 19:33
 Operator : JC/MD
 Sample : M3251-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rBV	168525	150137	16.58%	3.135%
2	1.569	72	79	82	rVB4	5122	9126	1.01%	0.191%
3	2.550	233	240	248	rVB	6202	11890	1.31%	0.248%
4	5.397	695	707	721	rBV2	104383	302551	33.42%	6.318%
5	5.562	723	734	746	rVB	174022	488197	53.92%	10.195%
6	5.964	788	800	818	rBV2	114536	306147	33.81%	6.393%
7	6.769	922	932	946	rBV	281963	655121	72.36%	13.680%
8	8.653	1234	1241	1252	rBV	586842	905380	100.00%	18.906%
9	10.055	1465	1471	1487	rBV	561638	782167	86.39%	16.333%
10	11.085	1634	1640	1652	rBV	443964	557558	61.58%	11.643%
11	12.024	1789	1794	1805	rBV	519829	620461	68.53%	12.957%




Sum of corrected areas: 4788735

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023551.D
Acq On : 04 Aug 2021 19:33
Operator : JC/MD
Sample : M3251-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

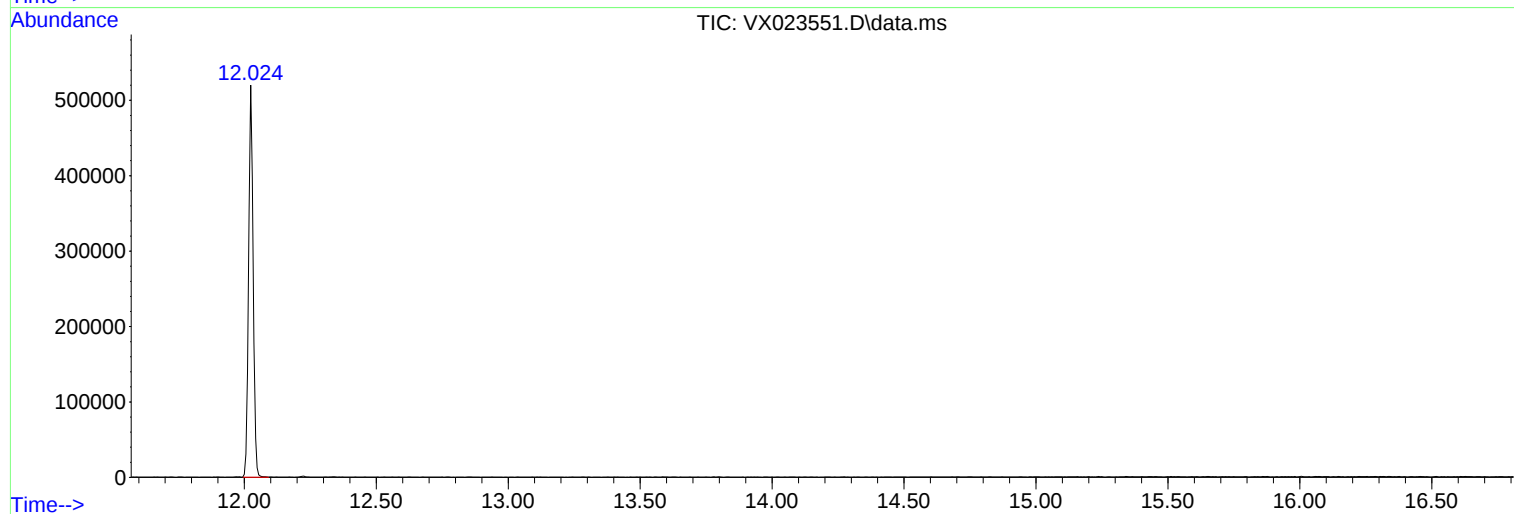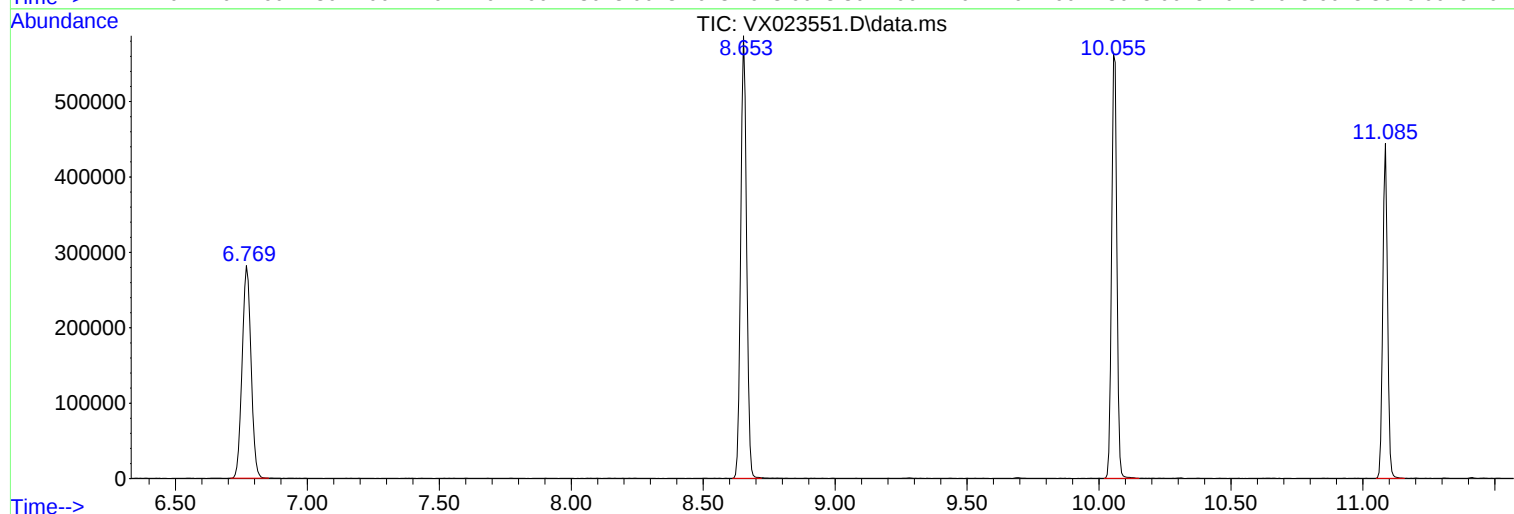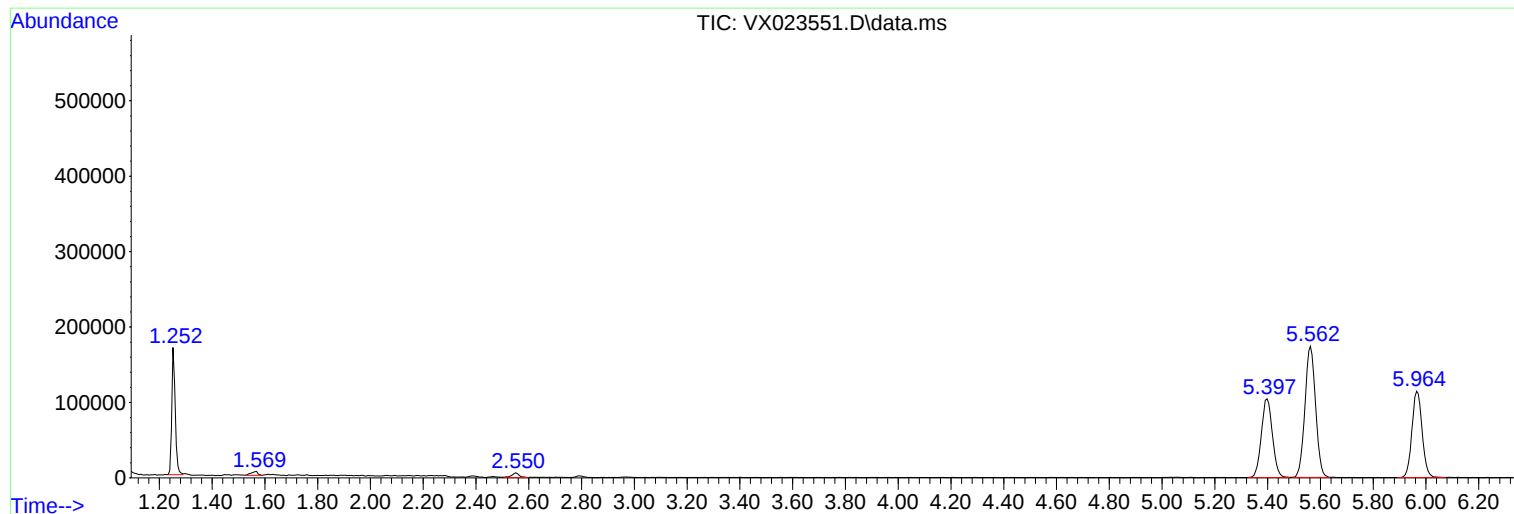

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023551.D
Acq On : 04 Aug 2021 19:33
Operator : JC/MD
Sample : M3251-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023551.D
Acq On : 04 Aug 2021 19:33
Operator : JC/MD
Sample : M3251-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
