

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
 Data File : VX023577.D
 Acq On : 05 Aug 2021 17:00
 Operator : JC/MD
 Sample : M3298-08 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ANTIFREEZE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	71	79	82	rBV2	6376	12429	1.43%	0.272%
2	2.794	274	280	286	rBV	7984	14063	1.61%	0.308%
3	5.397	695	707	722	rBV	97951	281631	32.34%	6.166%
4	5.562	722	734	749	rVB	164074	462647	53.12%	10.129%
5	5.964	787	800	820	rBV	110970	292007	33.53%	6.393%
6	6.769	922	932	945	rBV	263422	619725	71.16%	13.569%
7	8.653	1234	1241	1249	rBV	564273	870907	100.00%	19.068%
8	10.055	1465	1471	1481	rBV	555884	760802	87.36%	16.657%
9	11.085	1634	1640	1651	rBV	462742	580877	66.70%	12.718%
10	12.024	1789	1794	1806	rVB	545977	672241	77.19%	14.718%




Sum of corrected areas: 4567329

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023577.D
Acq On : 05 Aug 2021 17:00
Operator : JC/MD
Sample : M3298-08 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ANTIFREEZE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

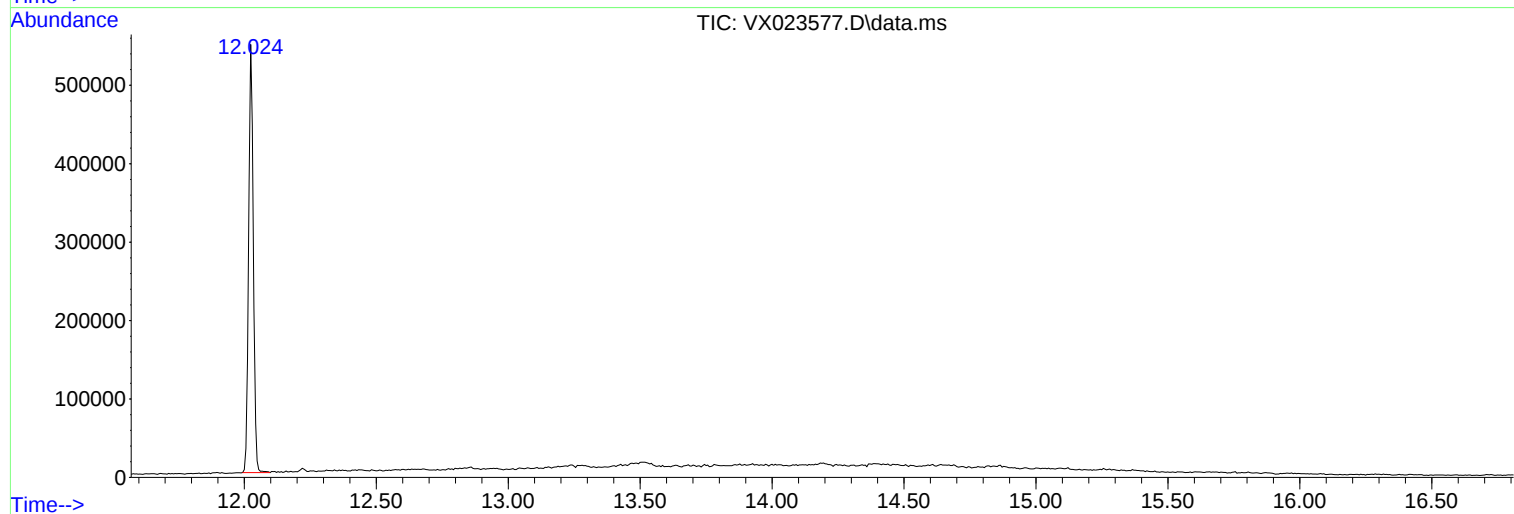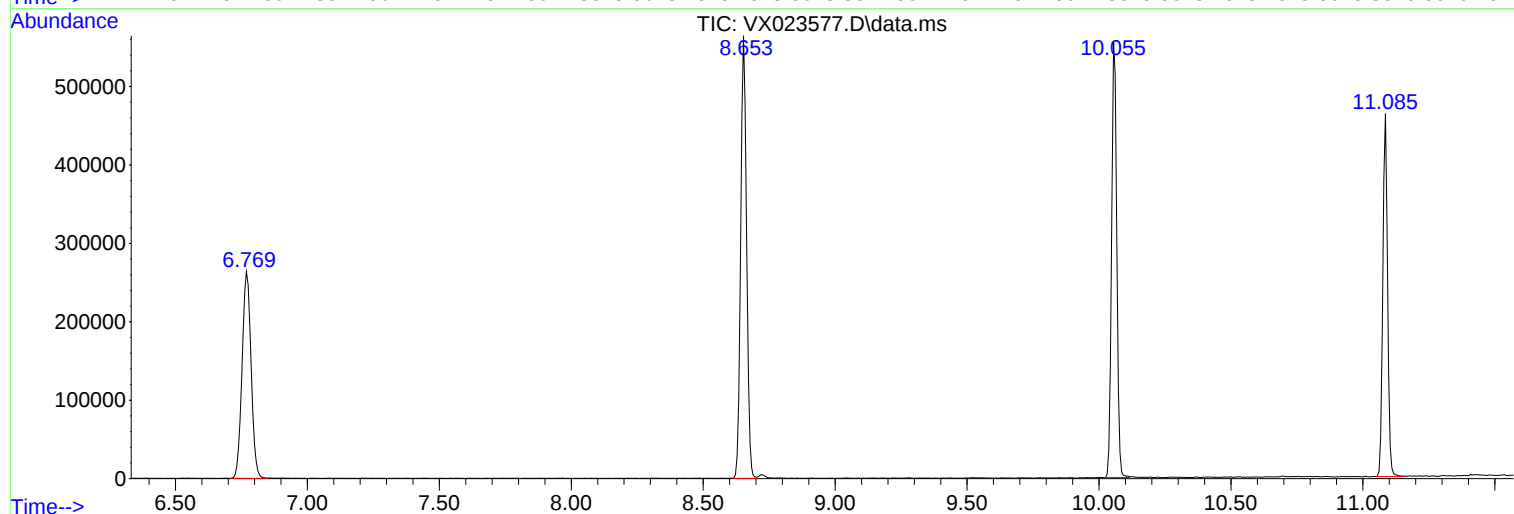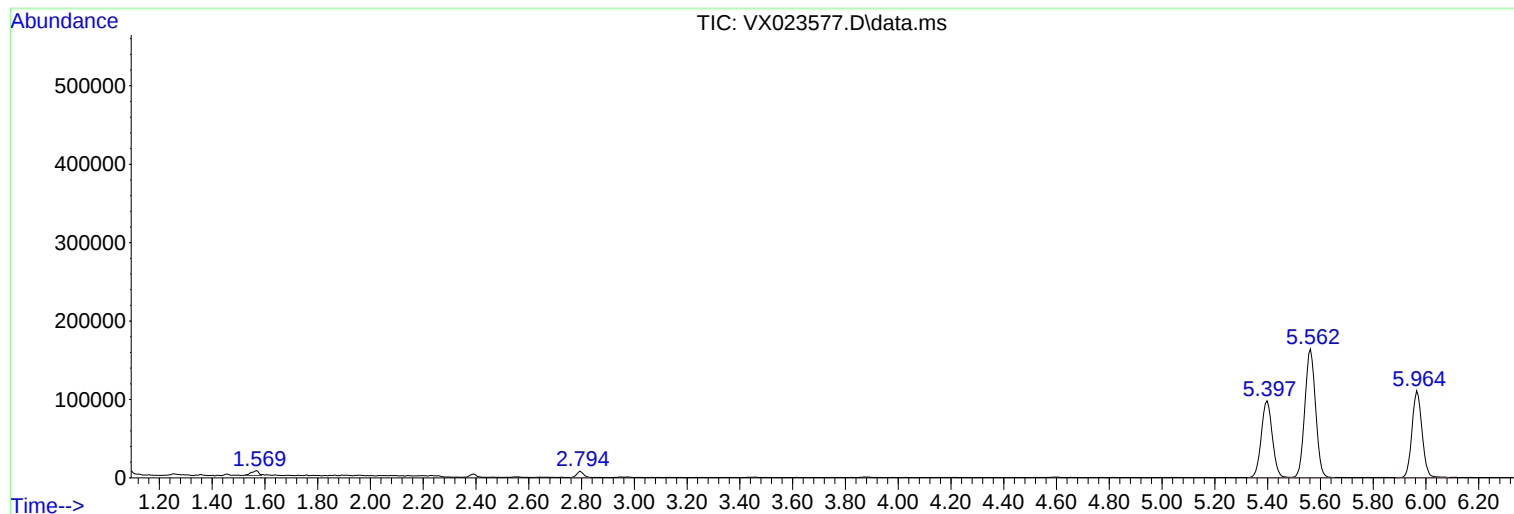

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023577.D
Acq On : 05 Aug 2021 17:00
Operator : JC/MD
Sample : M3298-08 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ANTIFREEZE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023577.D
Acq On : 05 Aug 2021 17:00
Operator : JC/MD
Sample : M3298-08 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ANTIFREEZE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
