


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
 Data File : VX023544.D
 Acq On : 04 Aug 2021 15:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260
 Last Update : Fri Jul 23 06:05:38 2021

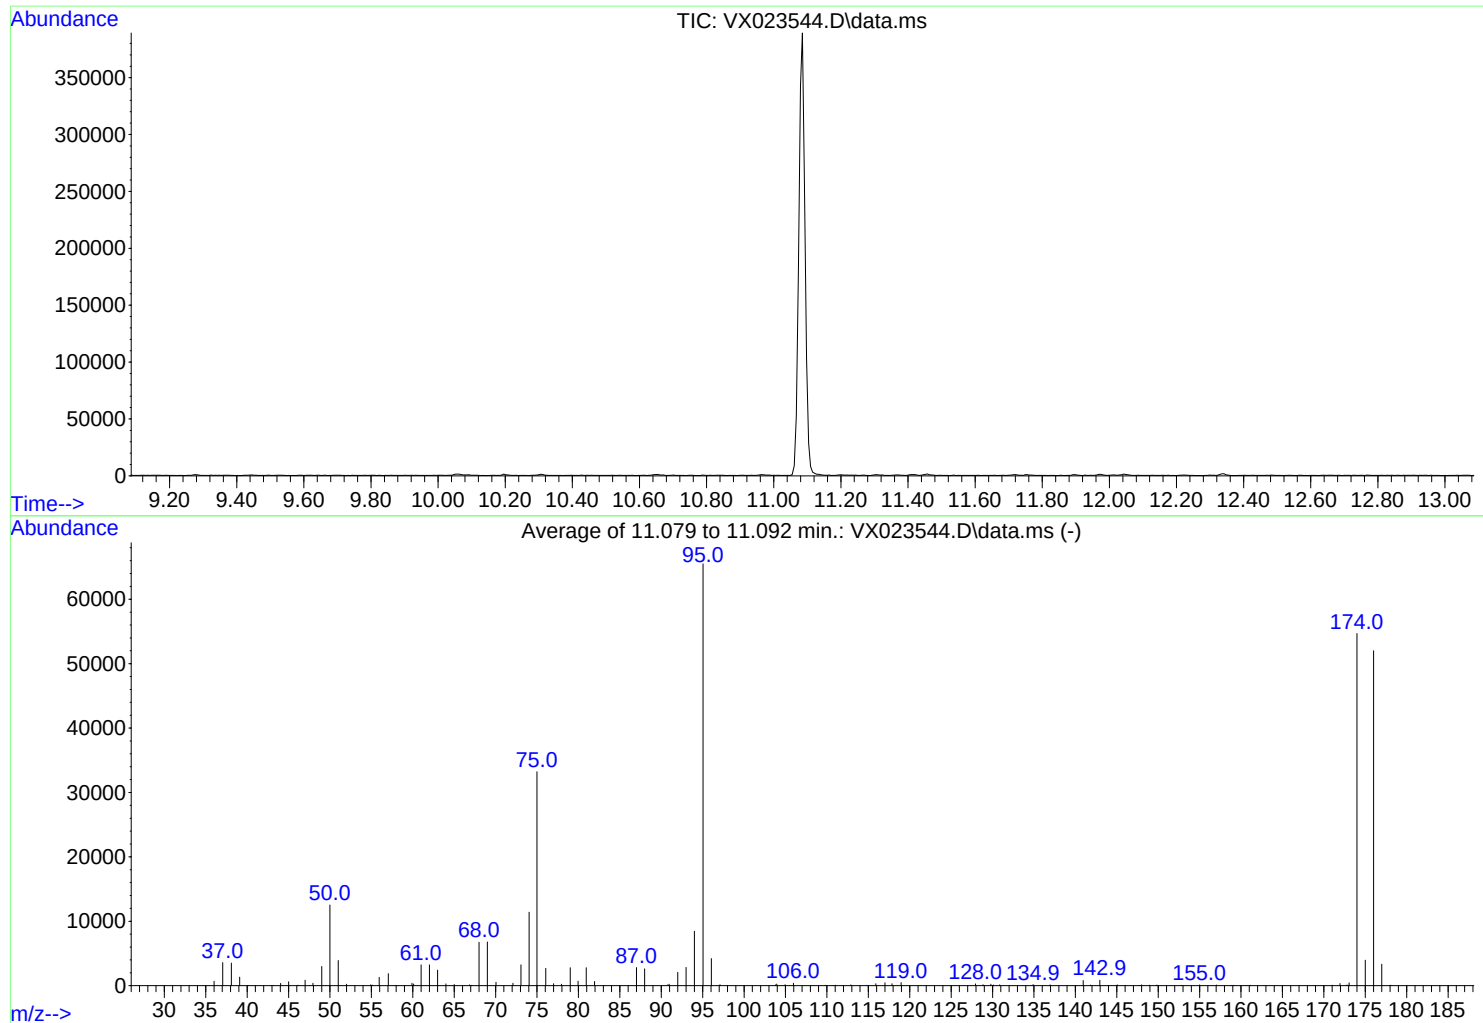

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12528	PASS
75	95	30	60	50.7	33221	PASS
95	95	100	100	100.0	65507	PASS
96	95	5	9	6.4	4213	PASS
173	174	0.00	2	0.8	430	PASS
174	95	50	100	83.5	54699	PASS
175	174	5	9	7.2	3942	PASS
176	174	95	101	95.1	52021	PASS
177	176	5	9	6.4	3323	PASS