
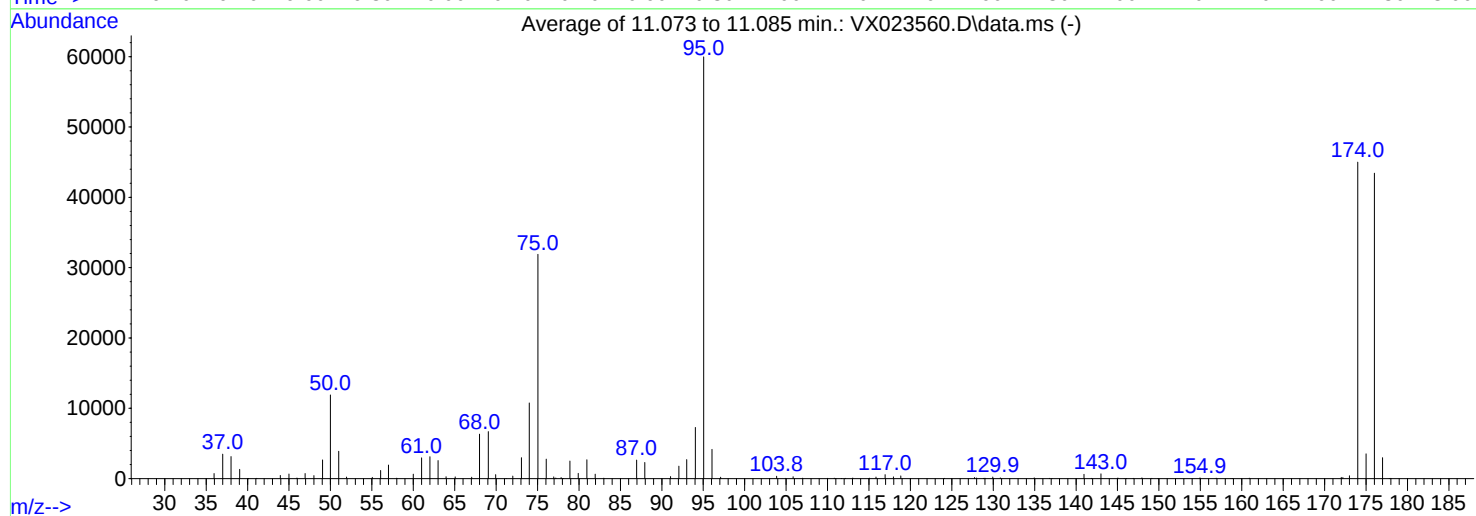


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080521\
Data File : VX023560.D
Acq On : 05 Aug 2021 09:02
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Title : SW846 8260
Last Update : Fri Jul 23 06:05:38 2021

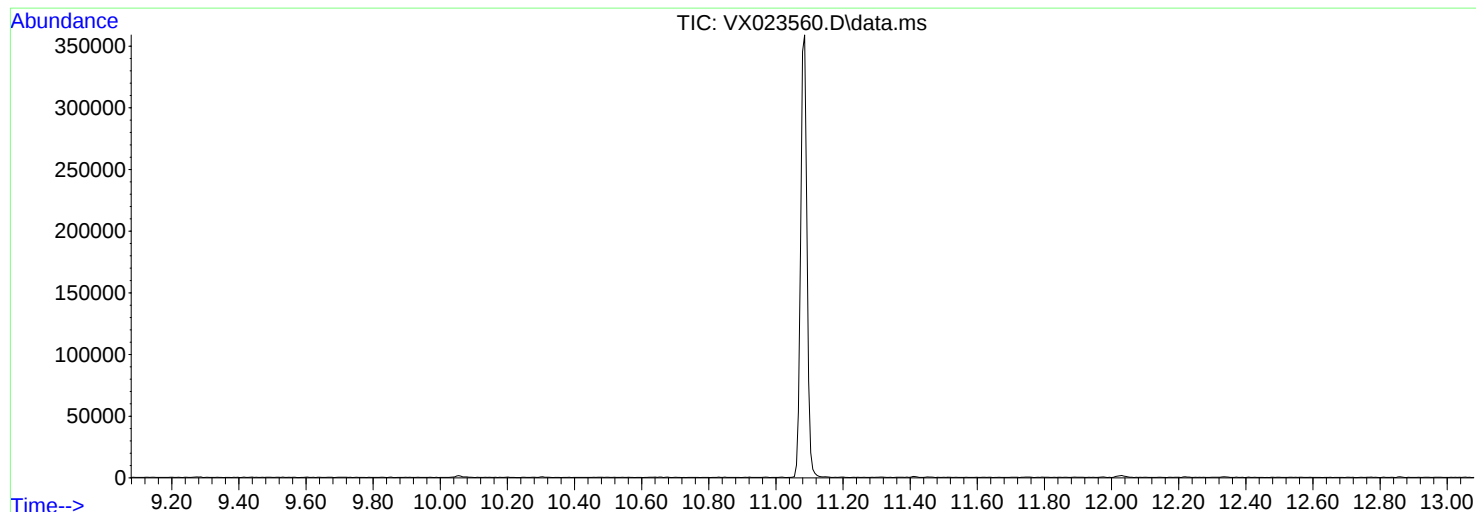

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	11900	PASS
75	95	30	60	53.2	31888	PASS
95	95	100	100	100.0	59973	PASS
96	95	5	9	6.9	4163	PASS
173	174	0.00	2	0.9	417	PASS
174	95	50	100	75.0	44997	PASS
175	174	5	9	7.8	3526	PASS
176	174	95	101	96.5	43440	PASS
177	176	5	9	6.8	2974	PASS