

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030421.D
 Acq On : 05 Aug 2022 11:51
 Operator : JC/MD
 Sample : N4021-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E52

Quant Time: Aug 06 00:55:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 06 00:54:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	275752	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	250649	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	116210	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	85943	48.533	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 97.060%			
7) Chloroethane-d5	1.666	69	69602	55.755	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 111.520%			
11) 1,1-Dichloroethene-d2	2.306	63	129046	38.525	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.040%			
21) 2-Butanone-d5	4.465	46	185711	113.186	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 113.190%			
24) Chloroform-d	5.056	84	183038	50.212	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.420%			
26) 1,2-Dichloroethane-d4	5.958	65	131177	52.997	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.000%			
32) Benzene-d6	5.970	84	367740	51.219	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.440%			
36) 1,2-Dichloropropane-d6	7.312	67	119989	51.510	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 103.020%			
41) Toluene-d8	8.653	98	335323	49.547	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 99.100%			
43) trans-1,3-Dichloroprop...	8.952	79	55201	47.634	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 95.260%			
47) 2-Hexanone-d5	9.384	63	122339	103.035	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 103.030%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	152569	49.857	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 99.720%			
66) 1,2-Dichlorobenzene-d4	12.323	152	117292	52.037	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 104.080%			
Target Compounds					Qvalue	
13) Acetone	2.392	43	2769	2.303	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030421.D
Acq On : 05 Aug 2022 11:51
Operator : JC/MD
Sample : N4021-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E52

Quant Time: Aug 06 00:55:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 06 00:54:06 2022
Response via : Initial Calibration

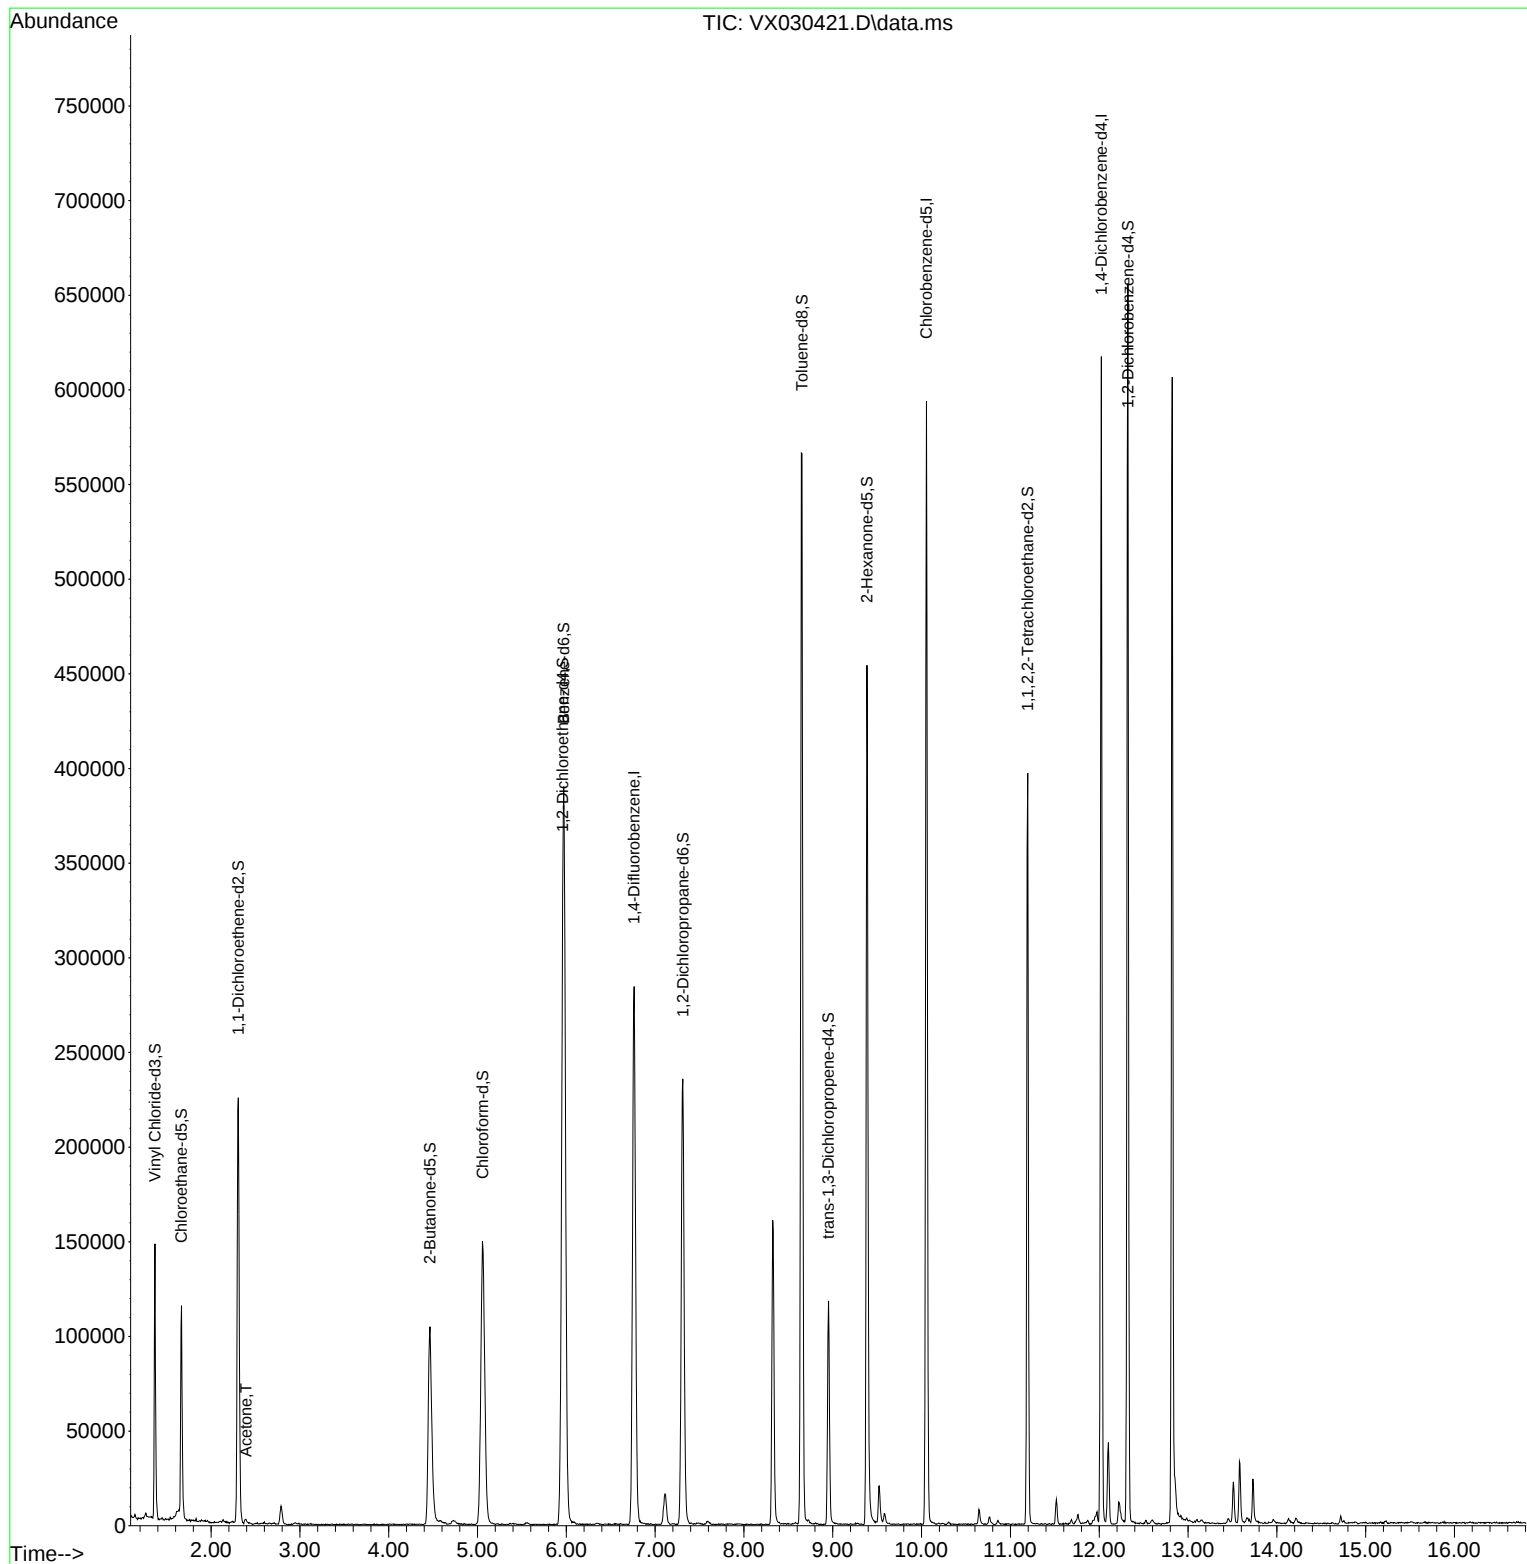

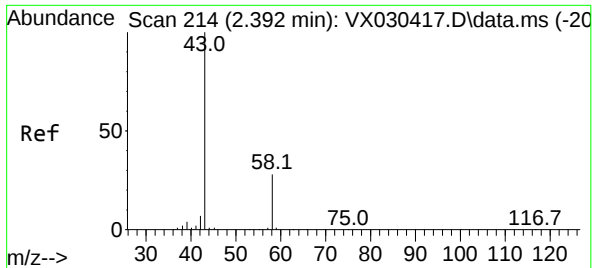

#13
 Acetone
 Concen: 2.303 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX030421.D
 Acq: 05 Aug 2022 11:51

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E52

Tgt Ion: 43 Resp: 2769
 Ion Ratio Lower Upper
 43 100
 58 28.2 0.0 57.8

