

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030418.D
 Acq On : 05 Aug 2022 10:04
 Operator : JC/MD
 Sample : VX0805WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK669

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	143885	145461	12.96%	1.649%
2	1.666	92	95	105	rVB	108644	143107	12.75%	1.622%
3	2.306	194	200	211	rBV	208248	332176	29.61%	3.766%
4	2.788	276	279	286	rVB3	2079	4157	0.37%	0.047%
5	2.873	291	293	295	rVB	620	529	0.05%	0.006%
6	2.953	295	306	312	rBV	9013	19223	1.71%	0.218%
7	3.062	320	324	326	rBV2	472	616	0.05%	0.007%
8	3.209	345	348	350	rBV2	351	400	0.04%	0.005%
9	3.233	350	352	353	rVB	505	284	0.03%	0.003%
10	3.251	353	355	356	rBV	338	253	0.02%	0.003%
11	3.294	359	362	363	rBV2	377	408	0.04%	0.005%
12	3.349	366	371	372	rBV2	296	481	0.04%	0.005%
13	3.373	374	375	378	rVB2	327	295	0.03%	0.003%
14	3.440	384	386	390	rVB2	471	535	0.05%	0.006%
15	3.593	410	411	414	rBV2	348	260	0.02%	0.003%
16	3.617	414	415	417	rVB	398	224	0.02%	0.003%
17	3.672	420	424	427	rBV2	398	592	0.05%	0.007%
18	3.910	460	463	465	rBV2	352	383	0.03%	0.004%
19	3.952	468	470	473	rVB2	393	340	0.03%	0.004%
20	3.989	473	476	477	rBV2	360	382	0.03%	0.004%
21	4.007	477	479	480	rBV	449	271	0.02%	0.003%
22	4.056	483	487	488	rBV2	474	417	0.04%	0.005%
23	4.172	504	506	508	rBV2	260	296	0.03%	0.003%
24	4.471	541	555	567	rBV	105860	308006	27.45%	3.492%
25	4.897	623	625	627	rBV2	492	454	0.04%	0.005%
26	5.068	639	653	670	rBV	153057	464943	41.44%	5.271%
27	5.397	699	707	716	rBV4	1975	5394	0.48%	0.061%
28	5.483	719	721	722	rBV	364	241	0.02%	0.003%
29	5.556	729	733	741	rVB3	2750	6229	0.56%	0.071%
30	5.696	751	756	757	rBV2	402	640	0.06%	0.007%
31	5.794	770	772	775	rVB2	434	327	0.03%	0.004%
32	5.879	785	786	788	rBV2	483	457	0.04%	0.005%
33	5.976	790	802	817	rBV3	380640	1122007	100.00%	12.720%
34	6.281	850	852	853	rVB	490	268	0.02%	0.003%
35	6.452	878	880	882	rBV2	376	468	0.04%	0.005%
36	6.592	901	903	905	rBV	359	300	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030418.D
 Acq On : 05 Aug 2022 10:04
 Operator : JC/MD
 Sample : VX0805WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK669

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.635	908	910	911	rBV2	445	333	0.03%	0.004%
38	6.769	922	932	946	rVV	310922	749836	66.83%	8.501%
39	7.001	968	970	972	rVV	467	272	0.02%	0.003%
40	7.117	980	989	996	rVV2	11988	26538	2.37%	0.301%
41	7.312	1012	1021	1036	rBV	232210	520462	46.39%	5.901%
42	7.488	1044	1050	1052	rBV4	810	1645	0.15%	0.019%
43	7.562	1059	1062	1063	rBV	377	316	0.03%	0.004%
44	7.879	1112	1114	1116	rVB2	368	248	0.02%	0.003%
45	8.019	1135	1137	1139	rBV	427	364	0.03%	0.004%
46	8.068	1144	1145	1148	rBV2	364	414	0.04%	0.005%
47	8.129	1152	1155	1157	rBV	324	450	0.04%	0.005%
48	8.202	1163	1167	1169	rBV	590	866	0.08%	0.010%
49	8.226	1169	1171	1175	rBV2	340	357	0.03%	0.004%
50	8.263	1175	1177	1178	rBV	519	334	0.03%	0.004%
51	8.330	1181	1188	1198	rBV	159069	267153	23.81%	3.029%
52	8.653	1234	1241	1251	rBV	540769	858446	76.51%	9.732%
53	8.848	1271	1273	1274	rBV	388	222	0.02%	0.003%
54	8.952	1284	1290	1301	rBV	117848	175401	15.63%	1.989%
55	9.092	1312	1313	1318	rVB2	731	734	0.07%	0.008%
56	9.134	1318	1320	1323	rBV2	491	515	0.05%	0.006%
57	9.275	1339	1343	1348	rVB3	1607	2745	0.24%	0.031%
58	9.311	1348	1349	1352	rBV	337	425	0.04%	0.005%
59	9.384	1356	1361	1374	rBV	463227	673063	59.99%	7.631%
60	9.677	1408	1409	1411	rBV2	285	241	0.02%	0.003%
61	9.708	1411	1414	1417	rVV3	1134	1346	0.12%	0.015%
62	9.915	1445	1448	1449	rVB2	640	484	0.04%	0.005%
63	9.976	1456	1458	1461	rBV2	334	255	0.02%	0.003%
64	10.055	1465	1471	1481	rBV	652451	859555	76.61%	9.745%
65	10.287	1506	1509	1510	rBV2	314	374	0.03%	0.004%
66	10.384	1521	1525	1526	rVB2	512	547	0.05%	0.006%
67	10.403	1526	1528	1530	rBV2	490	483	0.04%	0.005%
68	10.610	1558	1562	1563	rBV	353	399	0.04%	0.005%
69	10.720	1579	1580	1582	rBV2	341	227	0.02%	0.003%
70	10.738	1582	1583	1585	rVV	501	289	0.03%	0.003%
71	10.787	1589	1591	1594	rVB2	421	418	0.04%	0.005%
72	10.915	1609	1612	1613	rBV	340	286	0.03%	0.003%
73	10.951	1616	1618	1620	rBV	507	485	0.04%	0.005%
74	11.116	1643	1645	1646	rBV2	287	227	0.02%	0.003%
75	11.146	1647	1650	1652	rBV	385	375	0.03%	0.004%
76	11.195	1652	1658	1665	rBV	431027	546124	48.67%	6.191%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
 Data File : VX030418.D
 Acq On : 05 Aug 2022 10:04
 Operator : JC/MD
 Sample : VX0805WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK669

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.396	1690	1691	1695	rBV3	586	849	0.08%	0.010%
78	11.457	1699	1701	1703	rVV	565	420	0.04%	0.005%
79	11.591	1722	1723	1725	rBV	597	367	0.03%	0.004%
80	11.853	1764	1766	1769	rVB2	342	289	0.03%	0.003%
81	12.024	1788	1794	1803	rBV	648177	784596	69.93%	8.895%
82	12.323	1837	1843	1851	rBV	620977	770033	68.63%	8.730%
83	12.506	1871	1873	1876	rBV2	481	509	0.05%	0.006%
84	12.622	1890	1892	1894	rBV2	549	490	0.04%	0.006%
85	12.987	1950	1952	1954	rBV	401	410	0.04%	0.005%
86	13.115	1970	1973	1975	rBV2	597	715	0.06%	0.008%
87	13.152	1977	1979	1980	rBV	350	333	0.03%	0.004%
88	13.207	1986	1988	1989	rBV	434	353	0.03%	0.004%
89	13.347	2010	2011	2013	rBV	328	270	0.02%	0.003%
90	13.518	2037	2039	2041	rBV2	451	356	0.03%	0.004%
91	13.591	2048	2051	2053	rBV3	1039	1183	0.11%	0.013%
92	13.676	2063	2065	2068	rVB	411	296	0.03%	0.003%
93	13.774	2079	2081	2088	rVB2	1253	2025	0.18%	0.023%
94	13.829	2088	2090	2094	rBV2	387	558	0.05%	0.006%
95	13.957	2110	2111	2112	rBV	445	309	0.03%	0.004%
96	13.999	2115	2118	2123	rVV2	463	771	0.07%	0.009%
97	14.140	2139	2141	2143	rVB	601	399	0.04%	0.005%
98	14.286	2164	2165	2167	rBV2	391	253	0.02%	0.003%
99	14.579	2211	2213	2216	rBV2	430	346	0.03%	0.004%
100	16.359	2504	2505	2507	rBV	638	397	0.04%	0.005%




Sum of corrected areas: 8820605

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030418.D
Acq On : 05 Aug 2022 10:04
Operator : JC/MD
Sample : VX0805WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK669

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

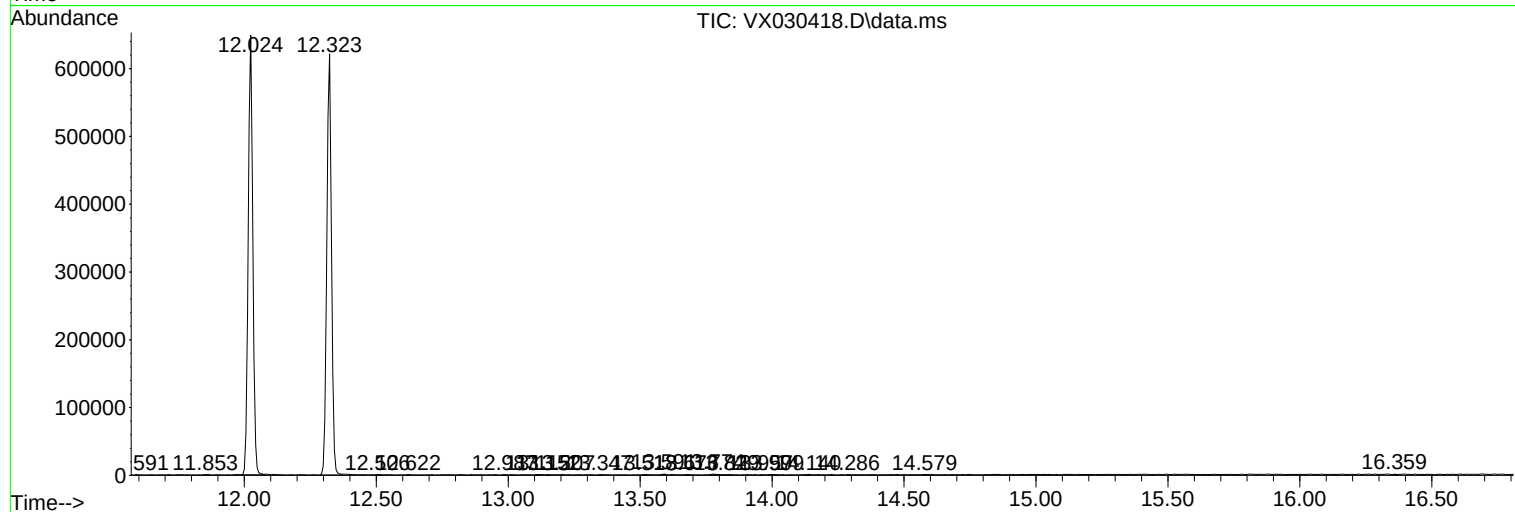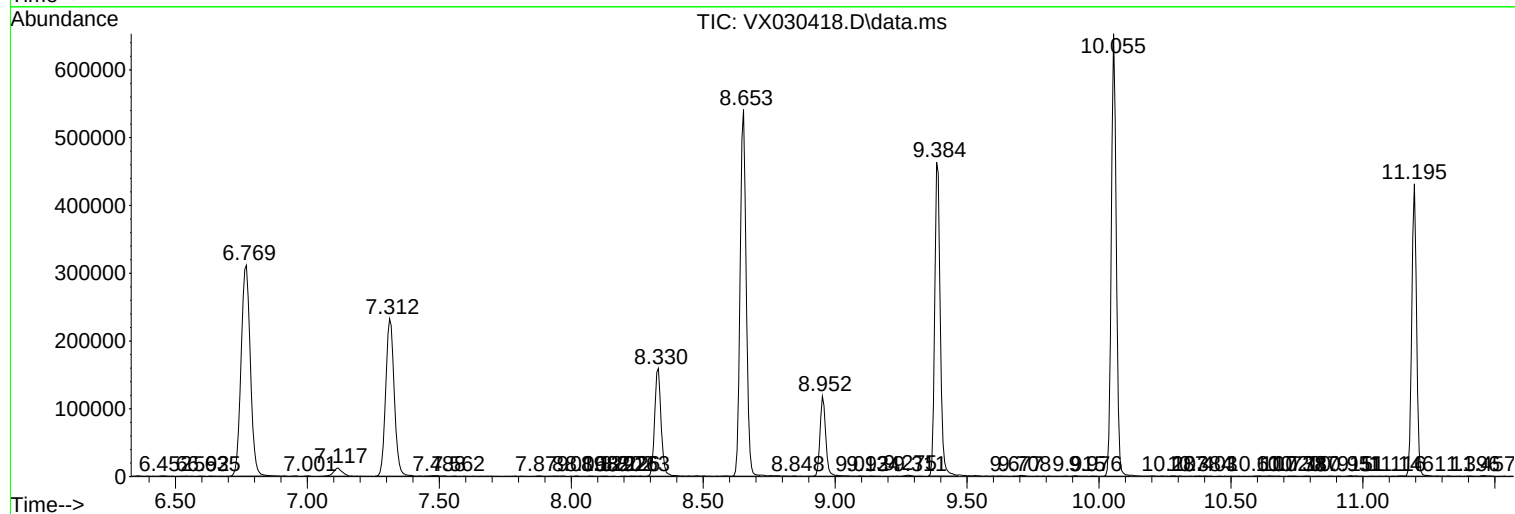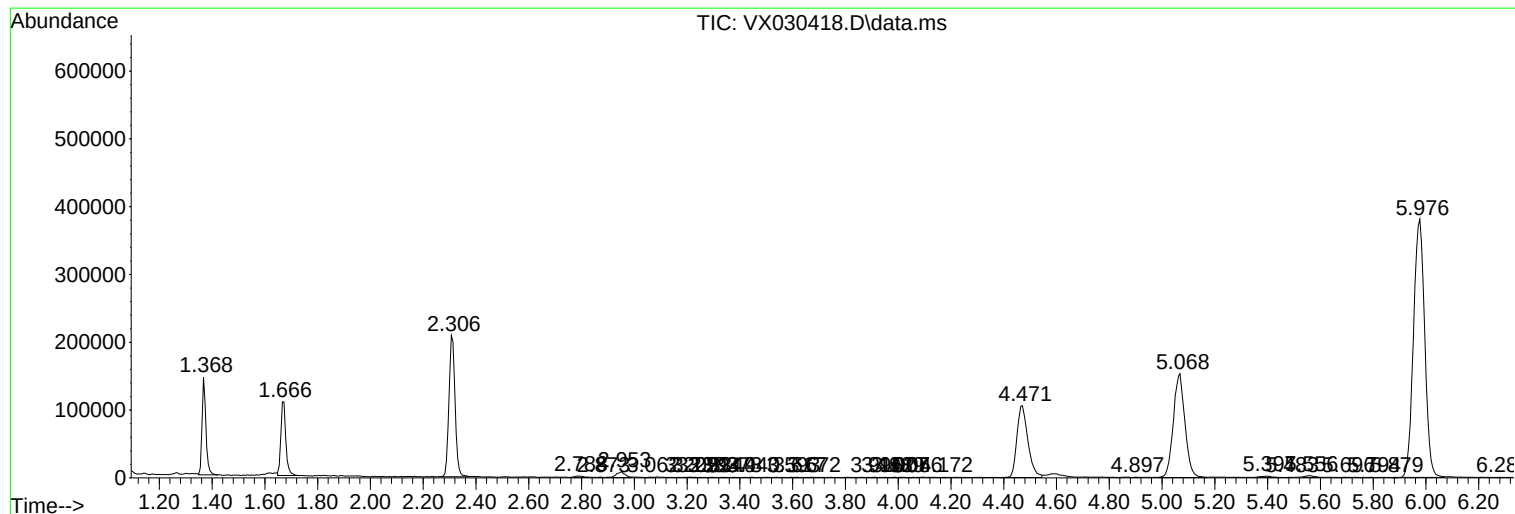

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030418.D
Acq On : 05 Aug 2022 10:04
Operator : JC/MD
Sample : VX0805WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK669

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080522\
Data File : VX030418.D
Acq On : 05 Aug 2022 10:04
Operator : JC/MD
Sample : VX0805WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK669

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc